

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061121\
 Data File : PD063759.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2021 17:43
 Operator : AR\AJ
 Sample : M2649-13MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 B0AA7MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 00:13:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.971	22834818	234.3E6	16.636	16.642
27)	SA Decachlor...	8.195	9.026	48392771	404.6E6	29.786	27.574
Target Compounds							
2)	A alpha-BHC	3.875	4.358	103.5E6	1012.5E6	50.692	45.815
3)	MA gamma-BHC...	4.157	4.643	97793698	935.7E6	48.575	45.798
4)	MA Heptachlor	4.458	5.150	86220096	852.1E6	44.308	41.009
5)	MB Aldrin	4.706	5.454	87683889	878.1E6	46.680	42.667
6)	B beta-BHC	4.409	4.814	40798567	380.3E6	43.859	42.508
7)	B delta-BHC	4.612	5.030	96813021	905.6E6	49.607	41.052
8)	B Heptachlo...	5.149	5.840	84742764	827.1E6	48.174	41.557
9)	A Endosulfan I	5.488	6.197	78313333	772.0E6	47.632	43.226
10)	B trans-Chl...	5.376	6.074	86386176	836.1E6	47.256	41.955
11)	B cis-Chlor...	5.434	6.147	83205865	798.4E6	46.913	42.238
12)	B 4,4'-DDE	5.599	6.304	175.8E6	1617.6E6	97.383	85.485
13)	MA Dieldrin	5.732	6.454	182.9E6	1662.2E6	97.661	86.871
14)	MA Endrin	5.989	6.671	144.4E6	1256.1E6	89.352	79.325
15)	B Endosulfa...	6.262	6.880	137.9E6	1332.0E6	91.788	87.994
16)	A 4,4'-DDD	6.115	6.794	152.1E6	1378.9E6	102.957	90.765
17)	MA 4,4'-DDT	6.356	7.092	132.8E6	1175.1E6	87.471	76.454
18)	B Endrin al...	6.431	7.004	127.8E6	1136.7E6	98.096	86.120
19)	B Endosulfa...	6.645	7.227	117.1E6	1300.0E6	81.533	83.424
20)	A Methoxychlor	6.904	7.551	337.6E6	2630.6E6	409.134	364.603
21)	B Endrin ke...	7.137	7.698	181.1E6	1290.4E6	102.644	83.739

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061121\
Data File : PD063759.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2021 17:43
Operator : AR\AJ
Sample : M2649-13MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 00:13:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

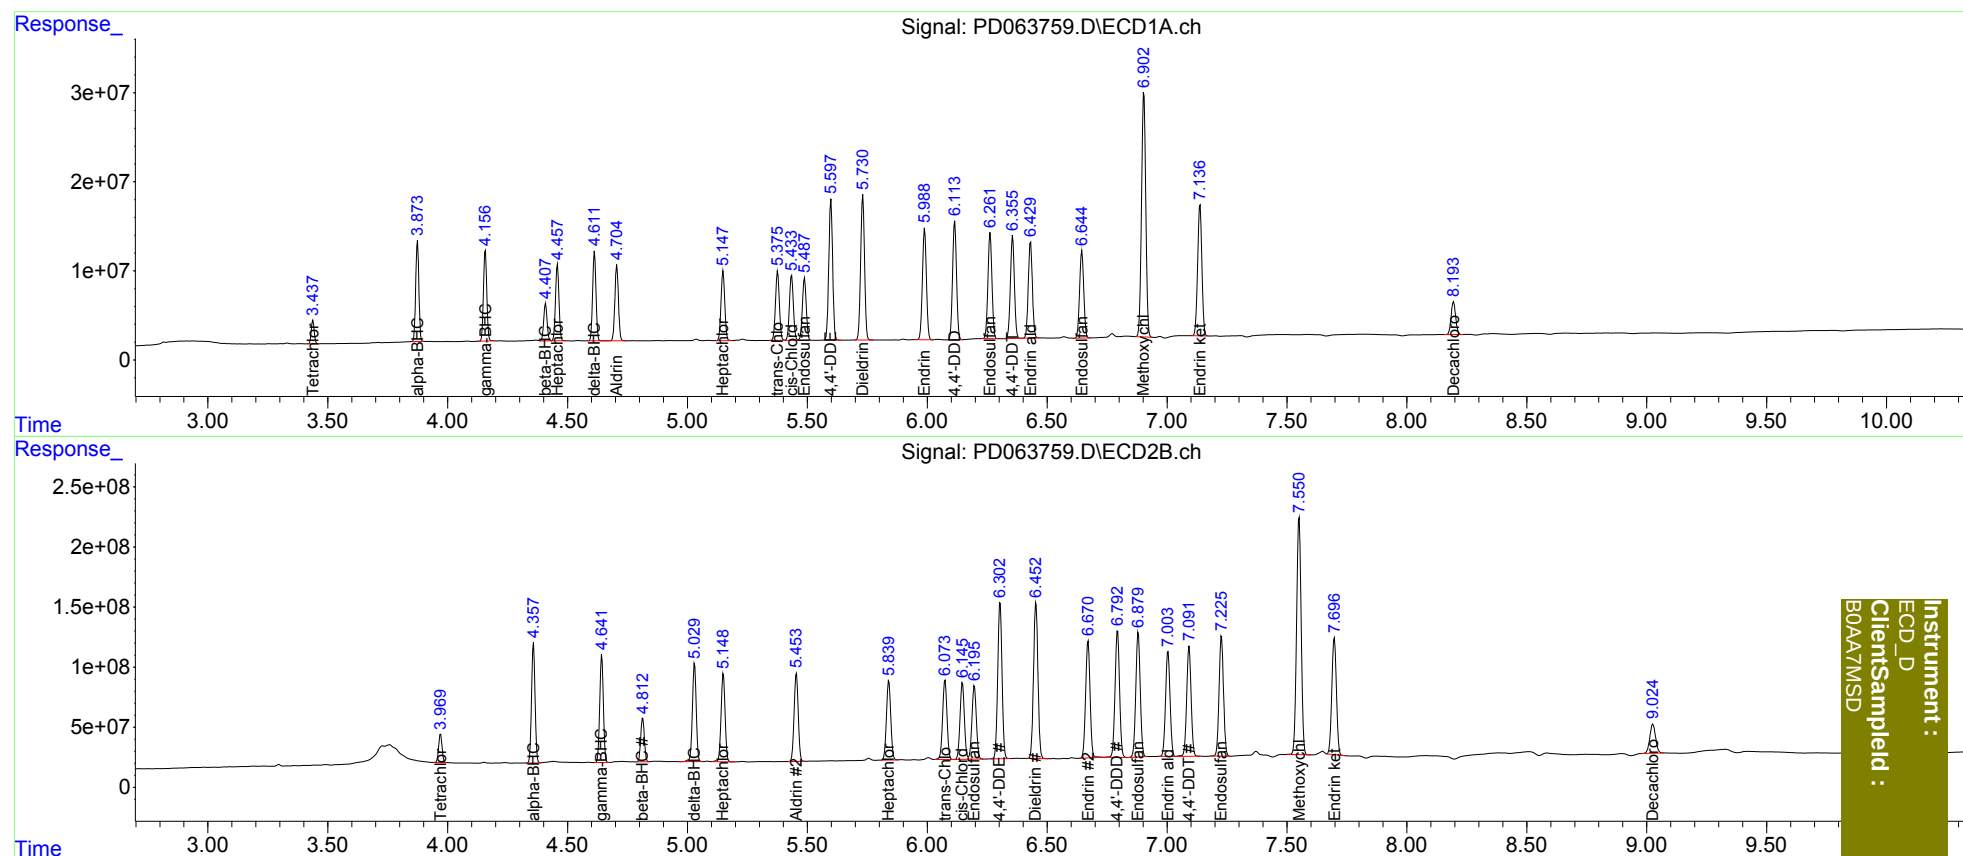

Instrument :
ECD_D
Client Sampled :
B0AA7MSD