

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061121\
 Data File : PD063758.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2021 17:30
 Operator : AR\AJ
 Sample : M2649-12MS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 B0AA7MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 00:12:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.970	23362580	239.4E6	17.020	17.010
27)	SA Decachlor...	8.195	9.026	48552674	402.5E6	29.884	27.430
Target Compounds							
2)	A alpha-BHC	3.875	4.358	102.8E6	1015.5E6	50.345	45.950
3)	MA gamma-BHC...	4.158	4.643	96848215	938.9E6	48.105	45.959
4)	MA Heptachlor	4.459	5.150	85375294	862.9E6	43.874	41.530
5)	MB Aldrin	4.707	5.454	86422516	872.6E6	46.008	42.397
6)	B beta-BHC	4.409	4.813	40131149	380.0E6	43.141	42.480
7)	B delta-BHC	4.614	5.030	95902624	906.0E6	49.140	41.069
8)	B Heptachlo...	5.150	5.840	83830452	827.6E6	47.655	41.585
9)	A Endosulfan I	5.489	6.197	77089054	764.2E6	46.888	42.790
10)	B trans-Chl...	5.377	6.074	84610868	832.4E6	46.285	41.773
11)	B cis-Chlor...	5.435	6.147	81743766	795.4E6	46.089	42.083
12)	B 4,4'-DDE	5.599	6.303	173.4E6	1605.0E6	96.027	84.817
13)	MA Dieldrin	5.732	6.453	180.9E6	1674.3E6	96.581	87.502
14)	MA Endrin	5.990	6.671	142.2E6	1269.0E6	87.959	80.140
15)	B Endosulfa...	6.263	6.881	144.5E6	1332.0E6	96.181	87.997
16)	A 4,4'-DDD	6.115	6.794	149.3E6	1371.5E6	101.015	90.284
17)	MA 4,4'-DDT	6.356	7.093	131.6E6	1166.2E6	86.679	75.875
18)	B Endrin al...	6.432	7.005	126.6E6	1140.9E6	97.145	86.437
19)	B Endosulfa...	6.646	7.228	130.2E6	1309.7E6	90.684	84.042
20)	A Methoxychlor	6.904	7.551	333.7E6	2659.9E6	404.351	368.667
21)	B Endrin ke...	7.138	7.698	180.5E6	1322.2E6	102.335	85.806

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061121\
Data File : PD063758.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2021 17:30
Operator : AR\AJ
Sample : M2649-12MS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 00:12:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

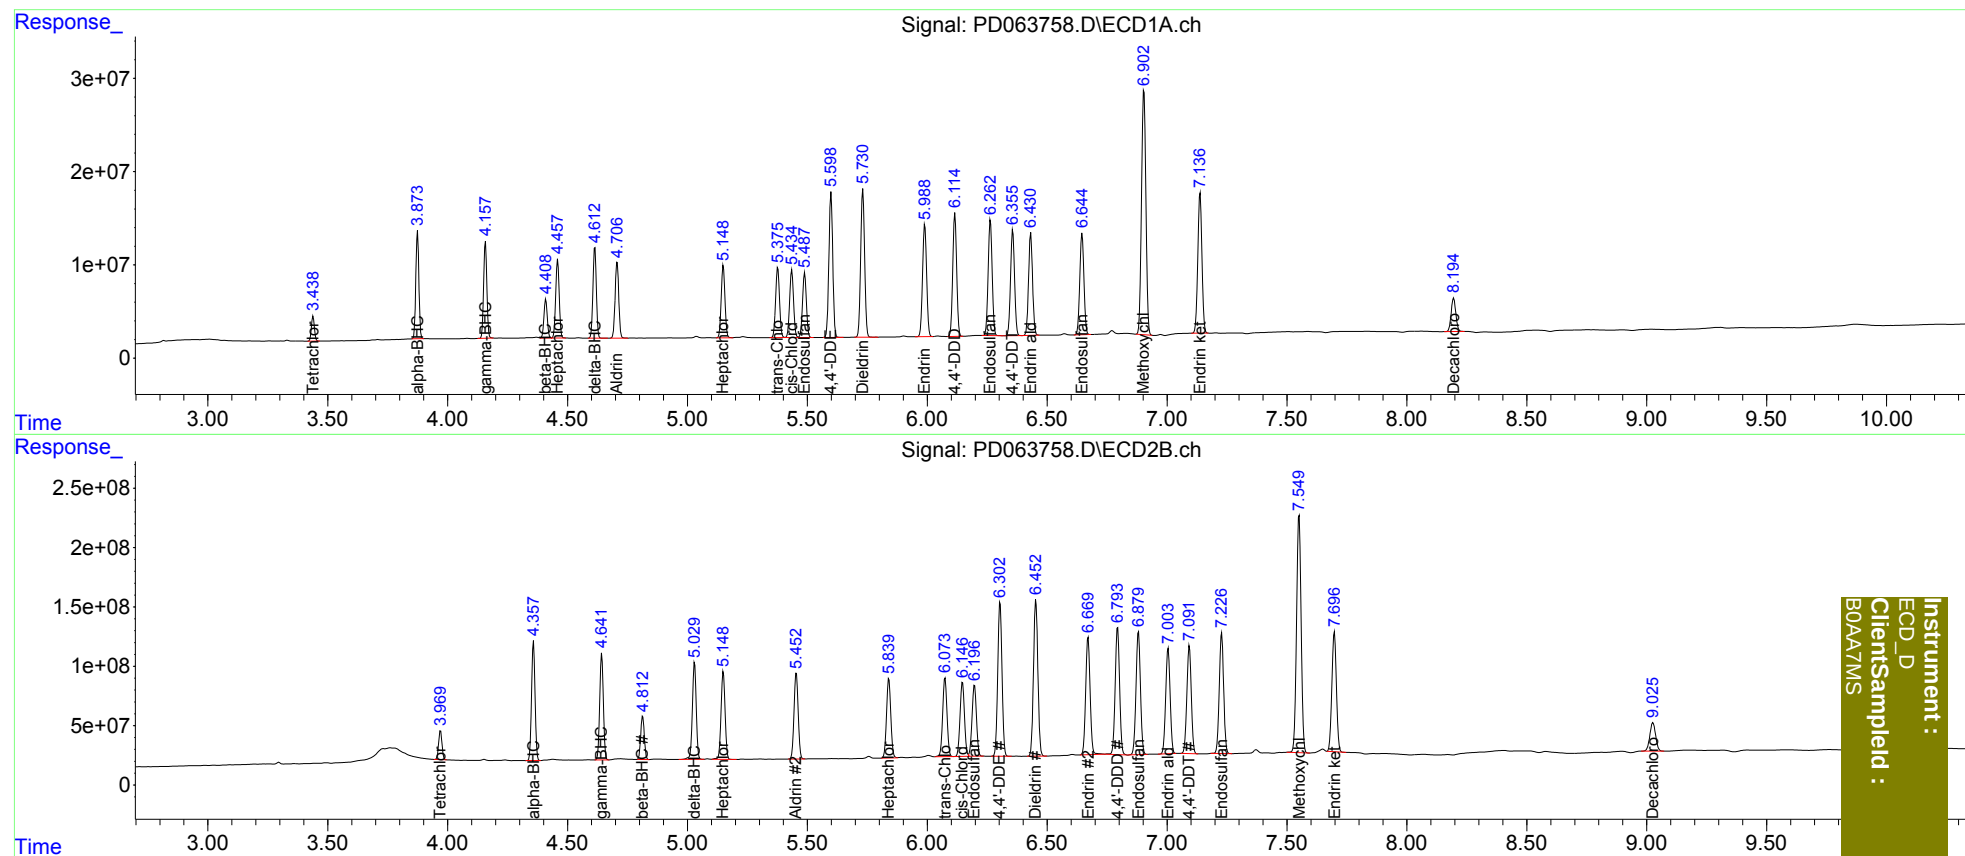

Instrument :
ECD_D
ClientSampled :
B0AA7MS