

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061121\
 Data File : PD063763.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2021 18:38
 Operator : AR\AJ
 Sample : INDA347
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3047

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 00:15:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.971	30333683	299.9E6	22.099	21.307
27)	SA Decachlor...	8.195	9.025	66323380	534.2E6	40.822	36.406
Target Compounds							
2)	A alpha-BHC	3.875	4.359	45151750	475.6E6	22.114	21.518
3)	MA gamma-BHC...	4.158	4.643	42706442	436.5E6	21.213	21.365
4)	MA Heptachlor	4.459	5.150	39740378	416.6E6	20.422	20.048
9)	A Endosulfan I	5.489	6.197	36261935	365.7E6	22.055	20.480
13)	MA Dieldrin	5.732	6.453	81450915	781.1E6	43.481	40.825
14)	MA Endrin	5.989	6.671	61685681	558.9E6	38.168	35.294
16)	A 4,4'-DDD	6.116	6.794	66596914	634.0E6	45.067	41.736
17)	MA 4,4'-DDT	6.355	7.092	56412898	552.0E6	37.157	35.913
20)	A Methoxychlor	6.903	7.550	155.8E6	1249.5E6	188.782	173.174

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061121\
Data File : PD063763.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2021 18:38
Operator : AR\AJ
Sample : INDA347
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 00:15:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

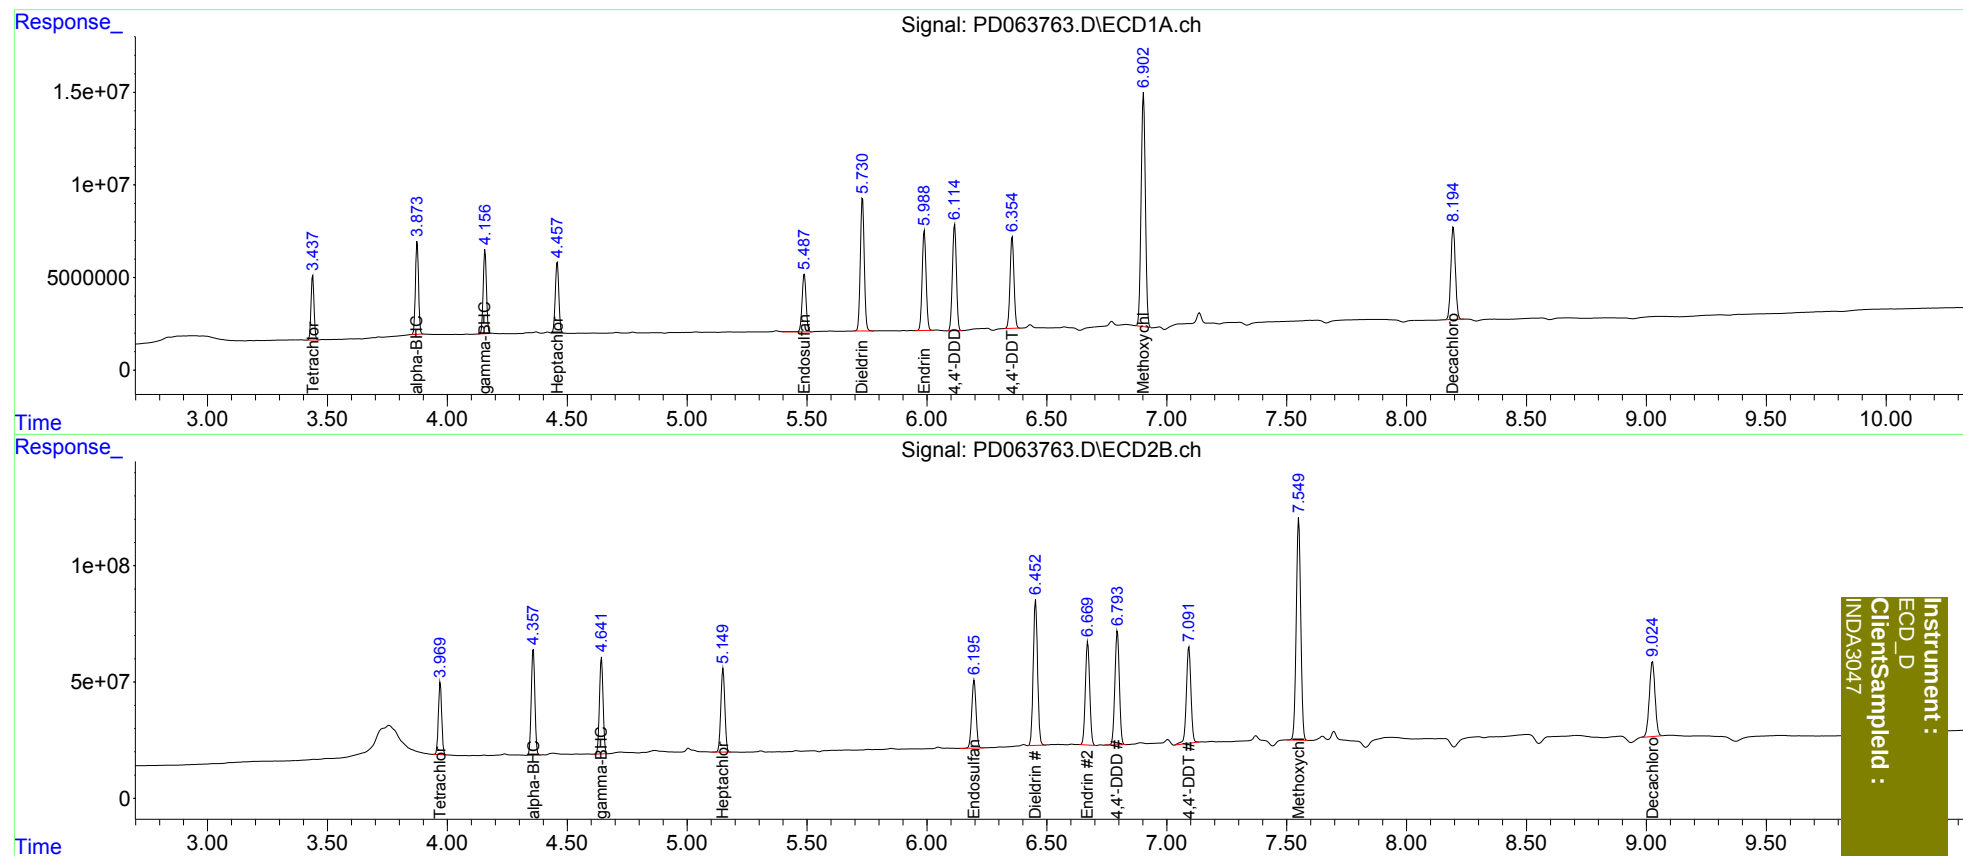

Instrument :
ECD_D
ClientSampled :
INDA3047