

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061124\
 Data File : PD083635.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2024 15:02
 Operator : AR\AJ
 Sample : PIBLK180
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 10:06:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.563	2.771	23270708	106.0E6	17.828	19.446
2) SA Decachlor...	9.123	7.899	40546582	142.5E6	20.852	23.467
Target Compounds						
7) B delta-BHC	4.792	0.000	1039188	0	0.396	N.D. #
8) B Heptachlo...	5.714	0.000	1913964	0	0.927	N.D. #
13) MA Dieldrin	0.000	5.336	0	4391068	N.D.	0.603


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061124\
Data File : PD083635.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2024 15:02
Operator : AR\AJ
Sample : PIBLK180
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 10:06:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

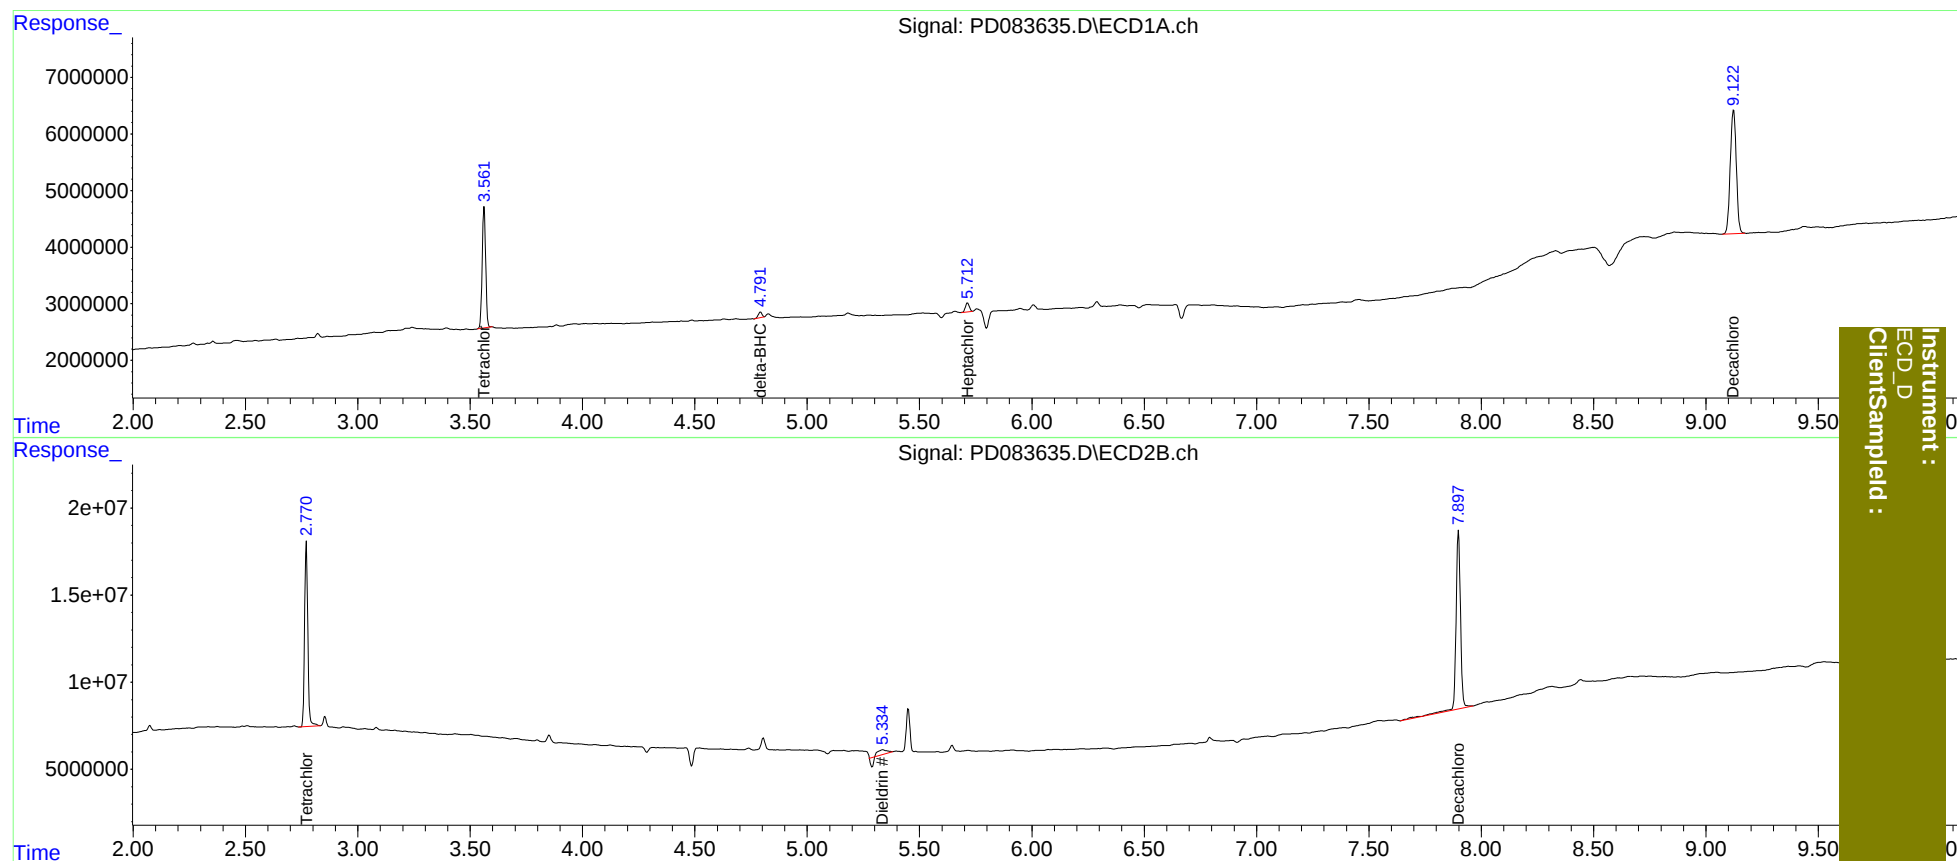


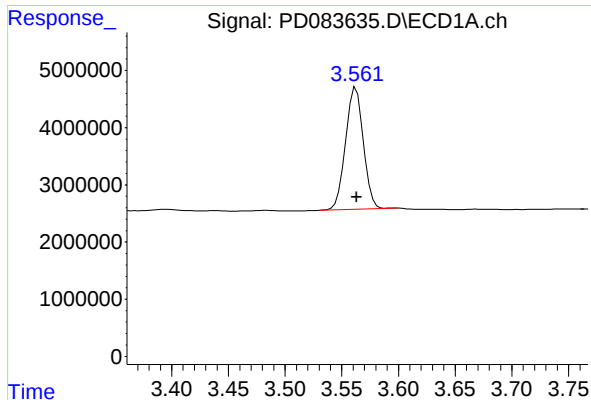

#1 Tetrachloro-m-xylene


R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 23270708
Conc: 17.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

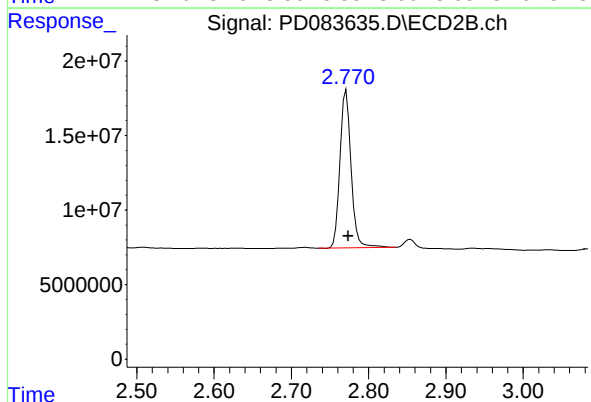


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: -0.002 min
Response: 106001614
Conc: 19.45 ng/ml

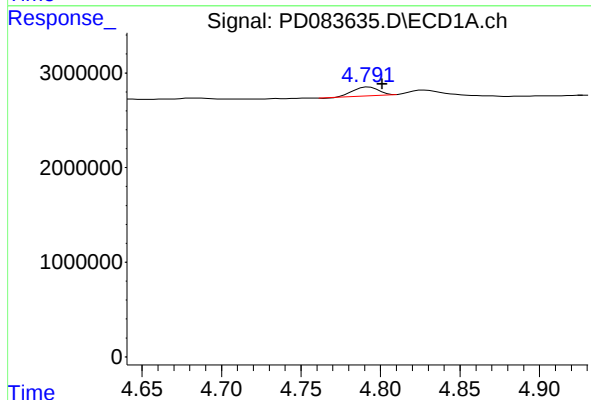


#7 delta-BHC

R.T.: 4.792 min
Delta R.T.: -0.009 min
Response: 1039188
Conc: 0.40 ng/ml

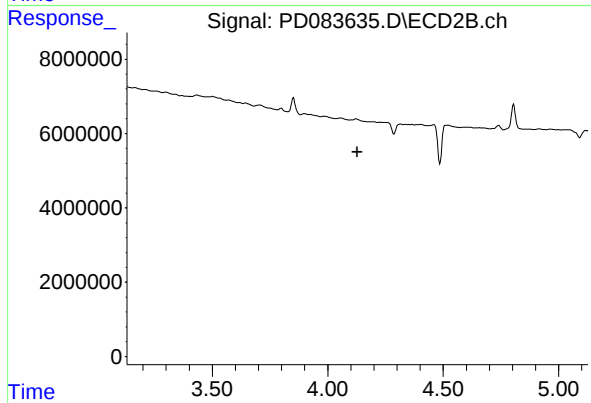

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.128 min
Response: 0
Conc: N.D.

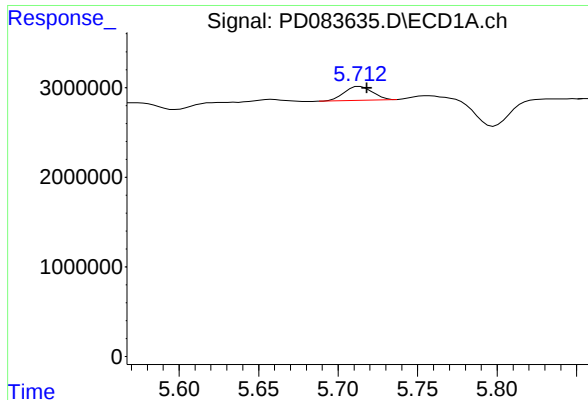

#8 Heptachlor epoxide


R.T.: 5.714 min
Delta R.T.: -0.004 min
Response: 1913964
Conc: 0.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

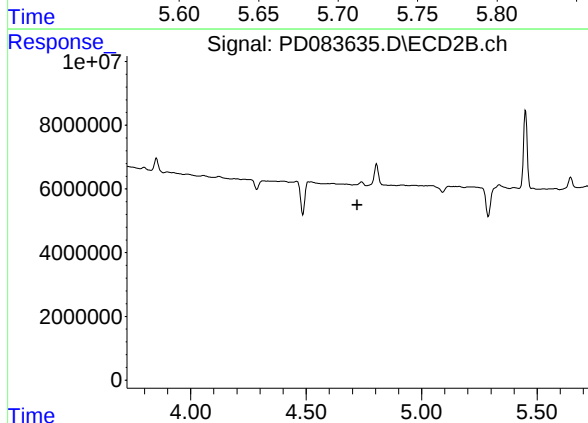


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.721 min
Response: 0
Conc: N.D.

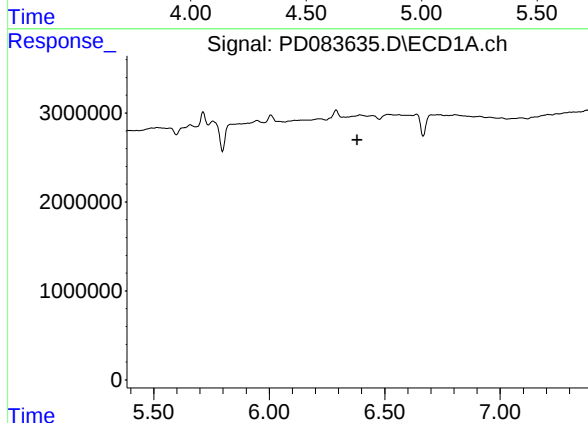


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.381 min
Response: 0
Conc: N.D.

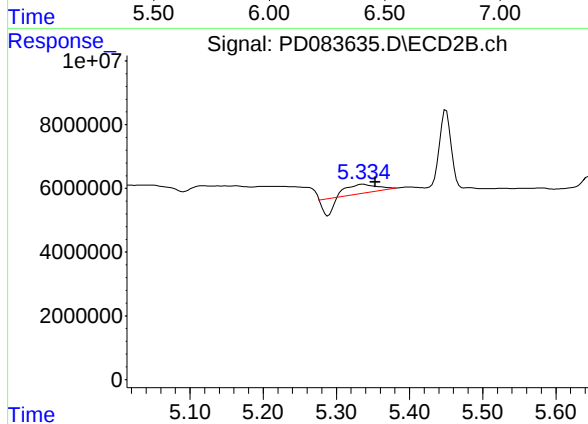

#13 Dieldrin


R.T.: 5.336 min
Delta R.T.: -0.018 min
Response: 4391068
Conc: 0.60 ng/ml

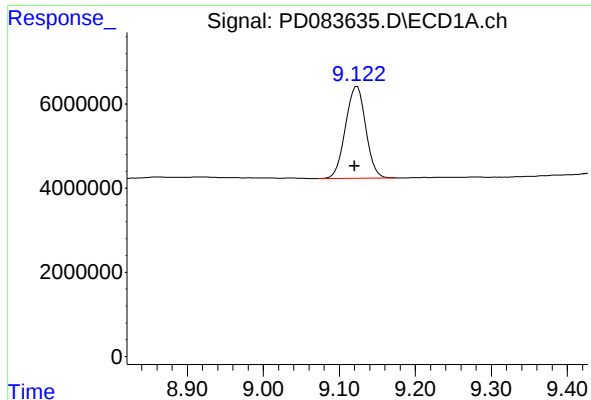

#27 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: 0.003 min
Response: 40546582
Conc: 20.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

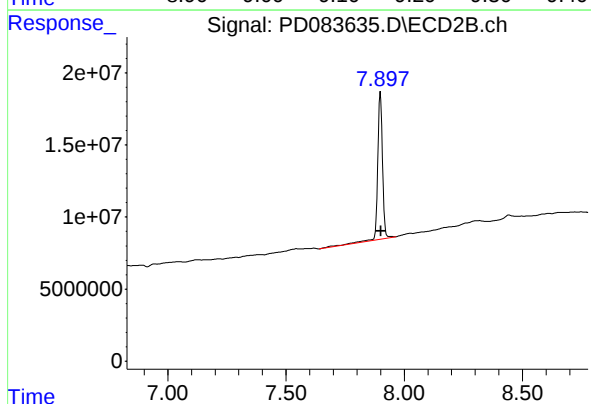

#27 Decachlorobiphenyl

R.T.: 7.899 min
Delta R.T.: -0.002 min
Response: 142495782
Conc: 23.47 ng/ml