

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD061218\
Data File : PD048120.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jun 2018 11:52
Operator : UA/AJ
Sample : J3407-15
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampled :
FLOP2591

Manual Integrations
APPROVED

ugo
6/14/2018 3:39:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 00:51:24 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_D\Method\PD060818CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jun 09 01:14:15 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

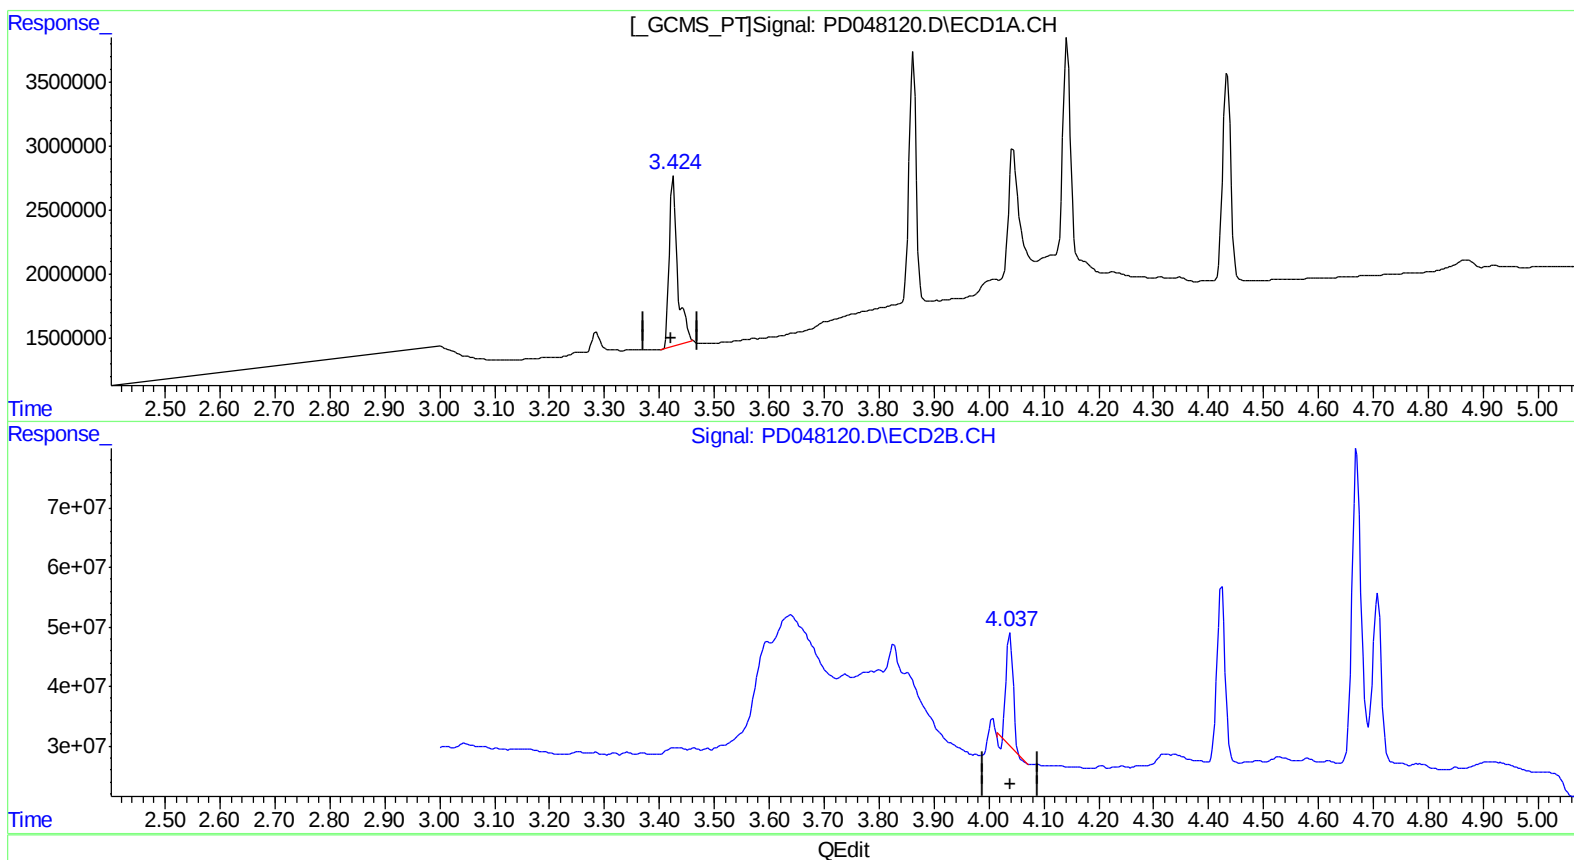

(1) Tetrachloro-m-xylene (SA)

3.426min 11.581 ng/ml

response 13646334

(1) Tetrachloro-m-xylene #2 (SA)

4.038min 7.334 ng/ml

response 147422381

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD061218\
Data File : PD048120.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jun 2018 11:52
Operator : UA/AJ
Sample : J3407-15
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
FLOP2591

Manual Integrations
APPROVED

ugo
6/14/2018 3:39:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 00:51:24 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_D\Method\PD060818CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jun 09 01:14:15 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

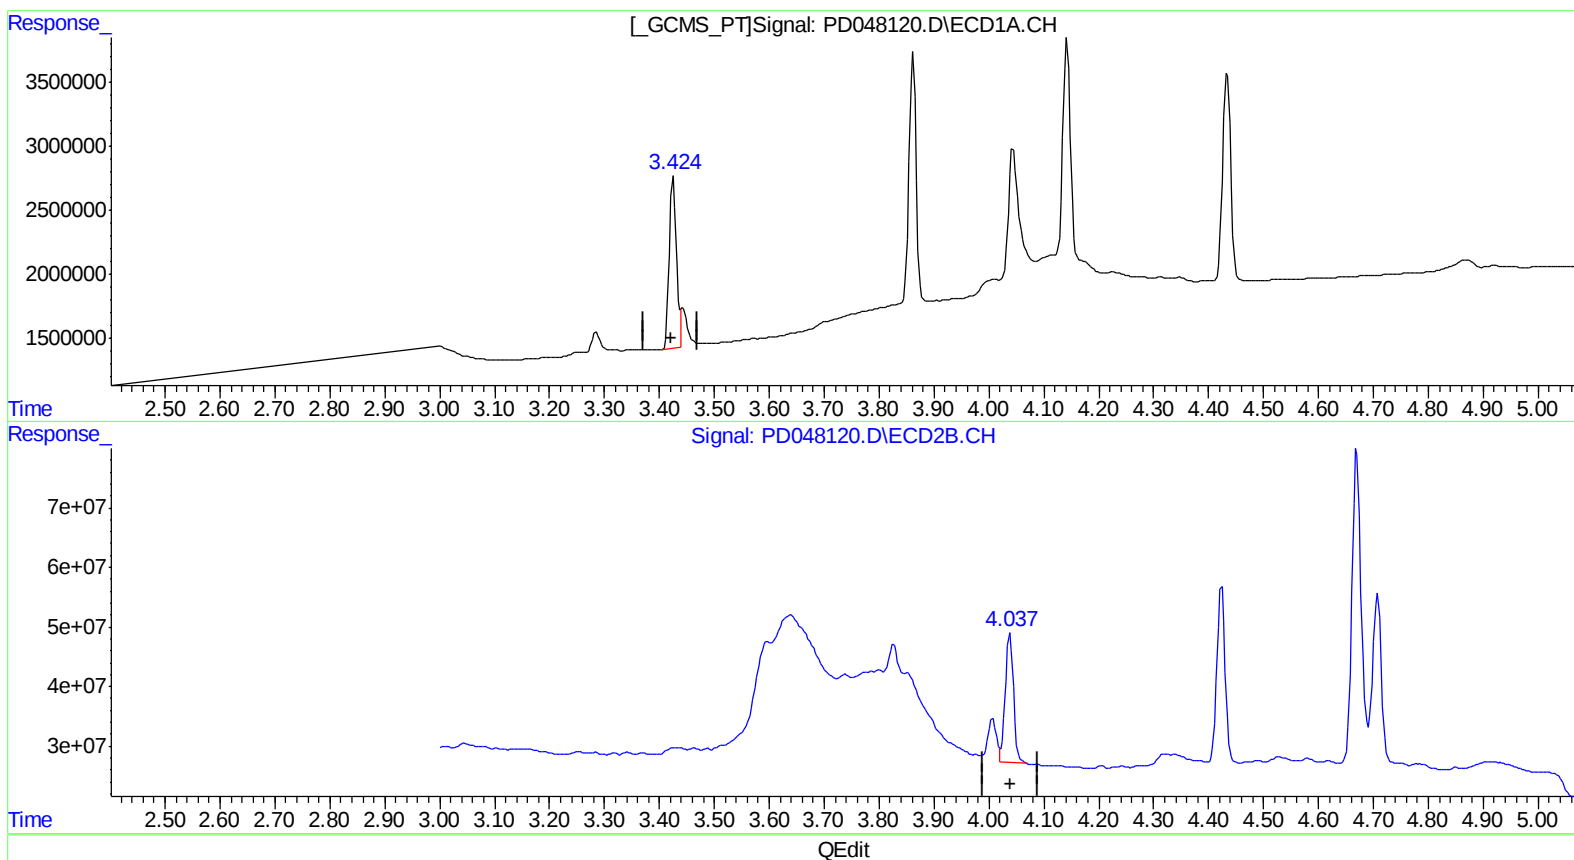

(1) Tetrachloro-m-xylene (SA)

3.424min 10.185 ng/ml m

response 12001734

(1) Tetrachloro-m-xylene #2 (SA)

4.037min 11.284 ng/ml m

response 226801707

(+) = Expected Retention Time

PD060818CLP.M Wed Jun 13 01:10:30 2018

Page: 1

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD061218\
Data File : PD048120.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jun 2018 11:52
Operator : UA/AJ
Sample : J3407-15
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
FLOP2591

Manual Integrations
APPROVED

ugo
6/14/2018 3:39:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 00:51:24 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_D\Method\PD060818CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jun 09 01:14:15 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

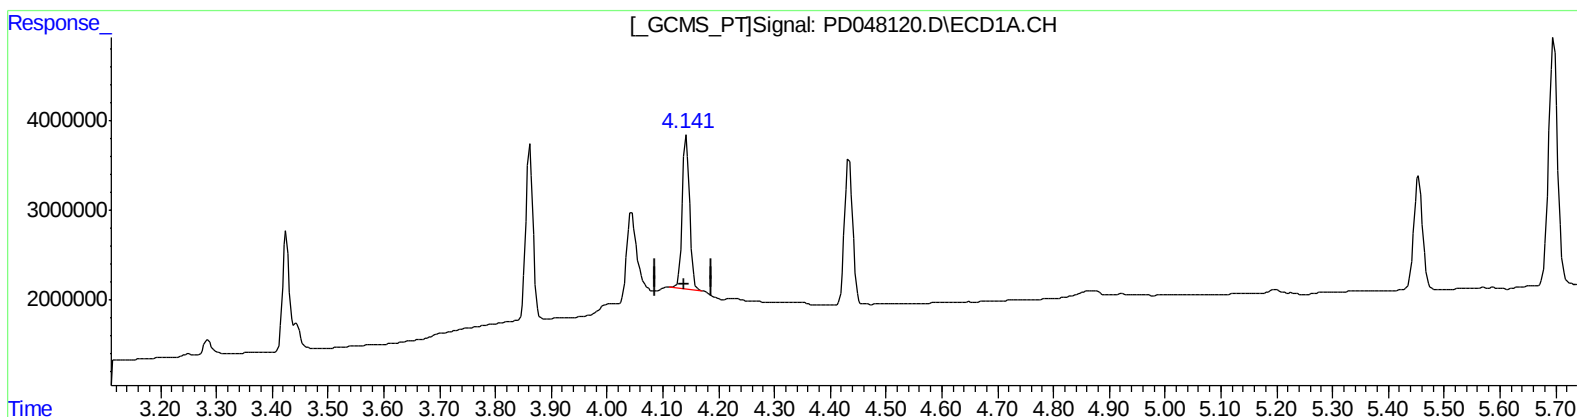

(3) gamma-BHC (Lindane) (MA)

4.143min 8.768 ng/ml

response 15850793

(3) gamma-BHC (Lindane) #2 (MA)

4.708min 0.858 ng/ml

response 23951343

(+) = Expected Retention Time

PD060818CLP.M Wed Jun 13 01:10:38 2018

Page: 1

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD D\Data\PD061218\
Data File : PD048120.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jun 2018 11:52
Operator : UA/AJ
Sample : J3407-15
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
FLOP2591

Manual Integrations
APPROVED

ugo
6/14/2018 3:39:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 00:51:24 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_D\Method\PD060818CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jun 09 01:14:15 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Ini. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

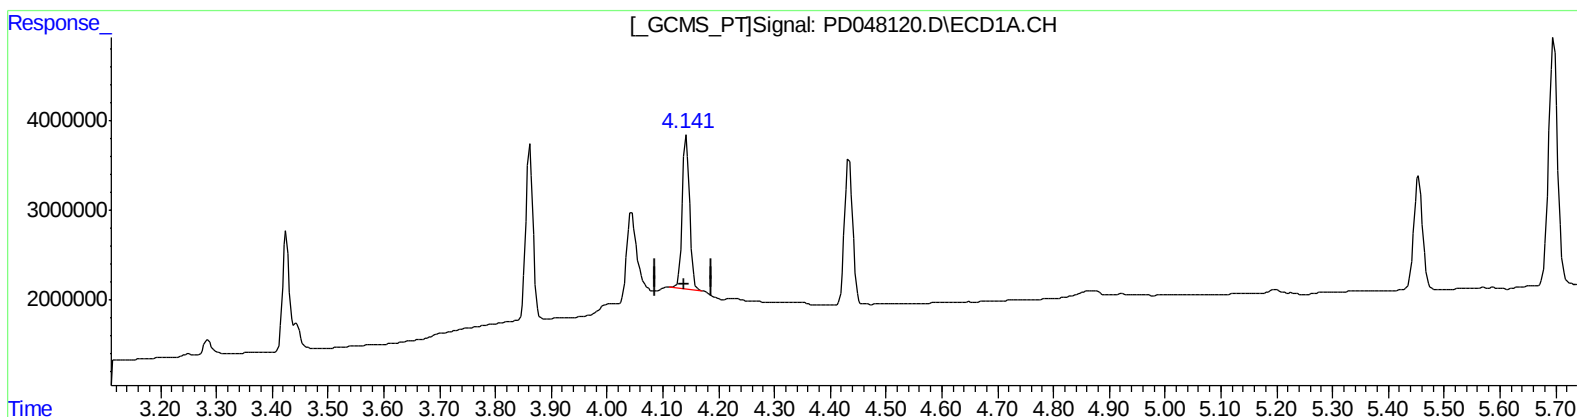

(3) gamma-BHC (Lindane) (MA)

4.143min 8.768 ng/ml

response 15850793

(3) gamma-BHC (Lindane) #2 (MA)

4.707min 11.262 ng/ml m

response 314376461

(+) = Expected Retention Time

PD060818CLP.M Wed Jun 13 01:10:47 2018