

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061218\
Data File : PD048125.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jun 2018 13:04
Operator : UA/AJ
Sample : PIBLK50
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK98

Manual Integrations
APPROVED

ugo
6/14/2018 3:39:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 01:18:03 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_D\Method\PD060818CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jun 09 01:14:15 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.425	4.037	25030715	415.9E6	21.243	20.692m
27)	SA Decachlor...	8.139	9.112	51871946	744.7E6	38.580	37.388

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061218\
Data File : PD048125.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jun 2018 13:04
Operator : UA/AJ
Sample : PIBLK50
Misc :
ALS Vial : 2 Sample Multiplier: 1


Instrument :
ECD_D
ClientSampleId :
PIBLK98


Manual Integrations
APPROVED

ugo
6/14/2018 3:39:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 01:18:03 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_D\Method\PD060818CLP.M
Quant Title : GC Extractables
QLast Update : Sat Jun 09 01:14:15 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

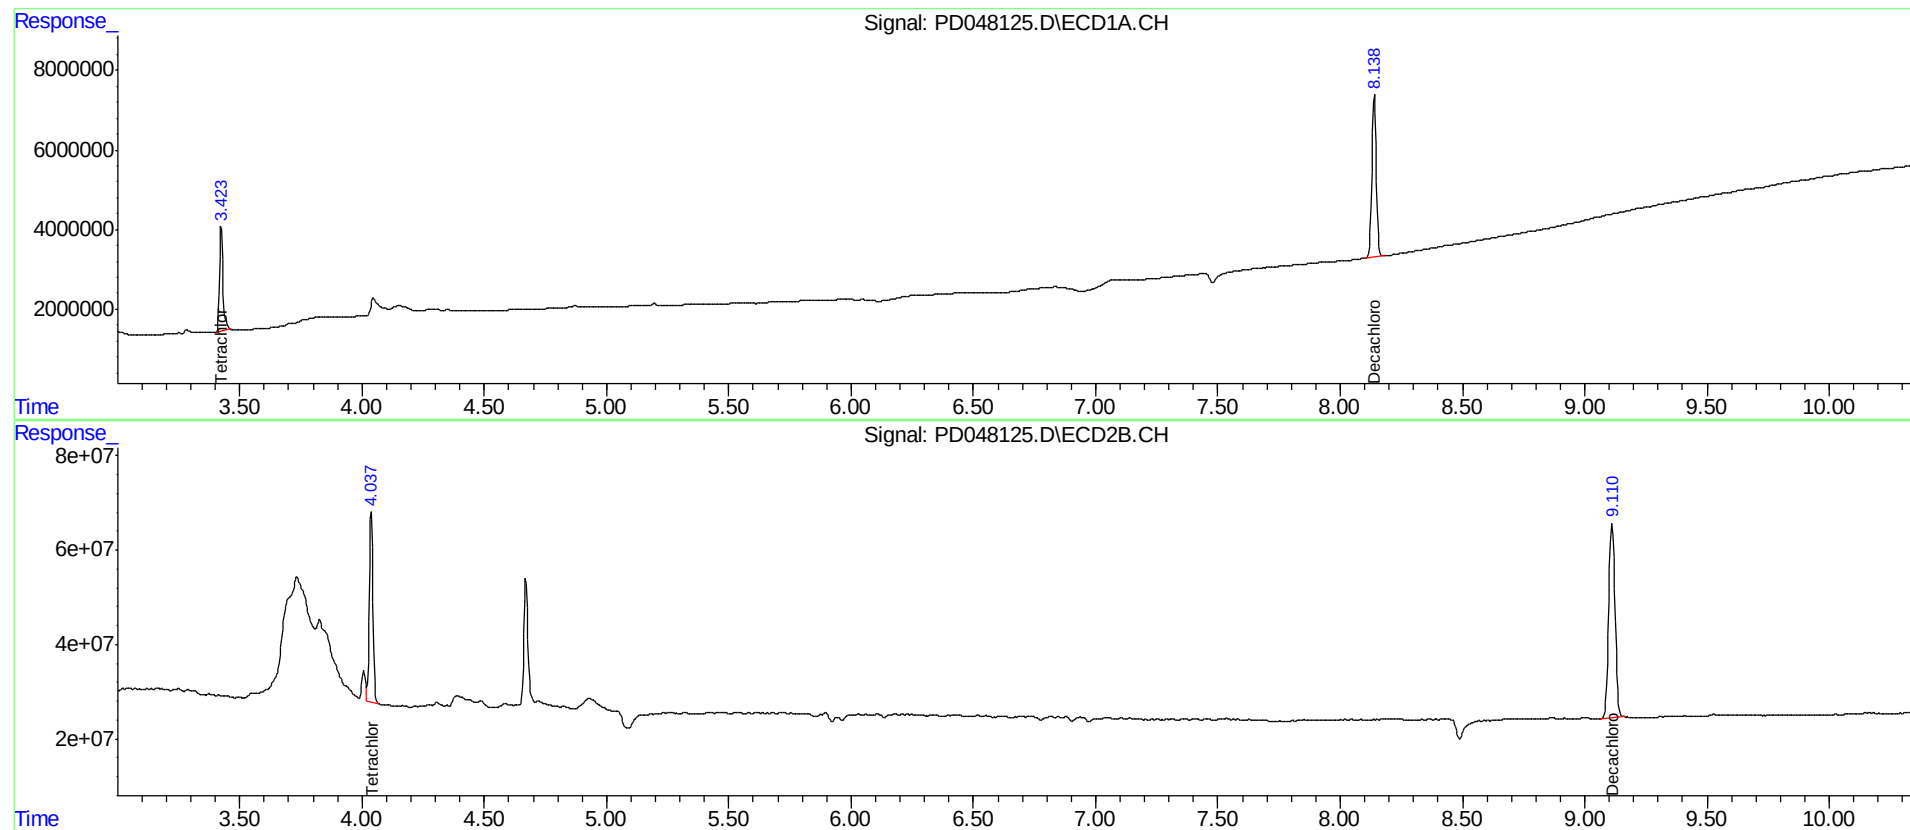

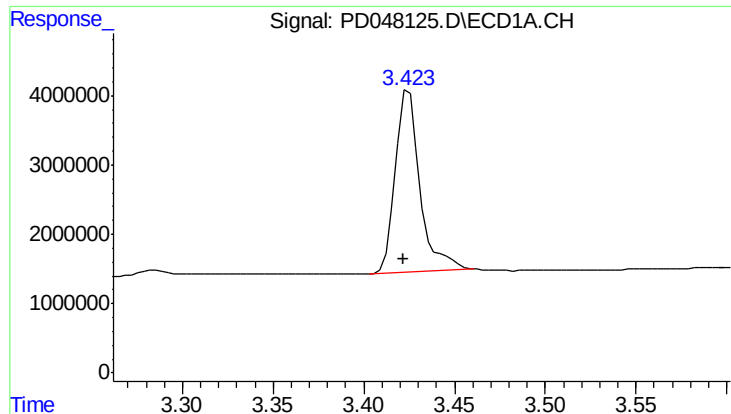


#1 Tetrachloro-m-xylene

R.T.: 3.425 min
Delta R.T.: 0.003 min
Response: 25030715
Conc: 21.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK98


Manual Integrations
APPROVED

ugo
6/14/2018 3:39:33 PM

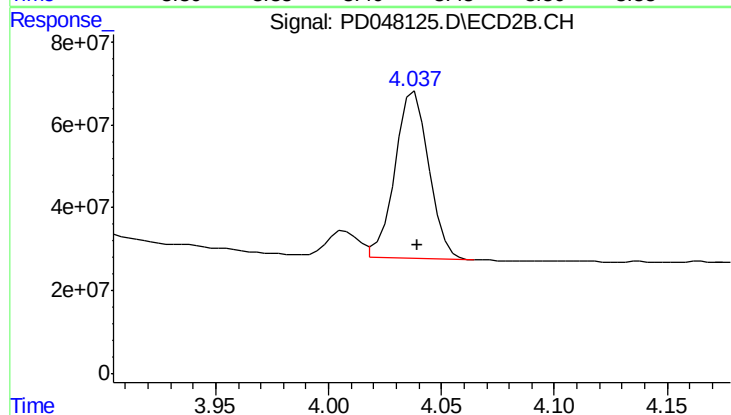


#1 Tetrachloro-m-xylene

R.T.: 4.037 min
Delta R.T.: -0.003 min
Response: 415914983
Conc: 20.69 ng/ml m

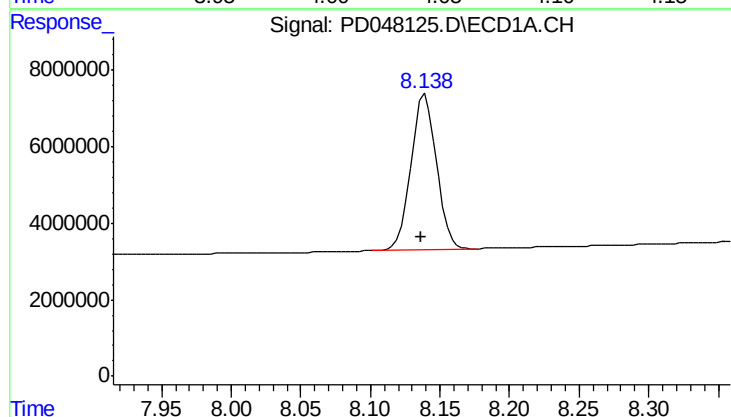

#27 Decachlorobiphenyl

R.T.: 8.139 min
Delta R.T.: 0.003 min
Response: 51871946
Conc: 38.58 ng/ml

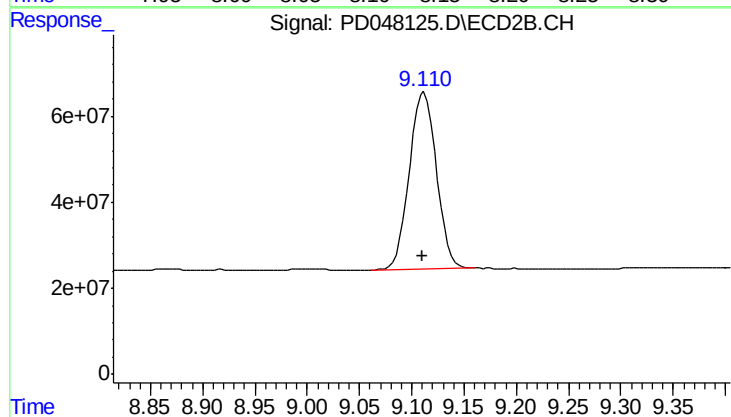

#27 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.002 min
Response: 744695466
Conc: 37.39 ng/ml