

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061219\
 Data File : PD053576.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jun 2019 8:32
 Operator : SM\AJ
 Sample : PIBLK43
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK43

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 01:20:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052119CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed May 22 06:53:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.315	3.983	14515940	22350573	19.812	22.701
27) SA Decachlor...	8.010	9.025	25350537	38895012	38.322	37.654
Target Compounds						
6) B beta-BHC	0.000	4.869f	0	1467638	N.D.	2.502


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061219\
Data File : PD053576.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jun 2019 8:32
Operator : SM\AJ
Sample : PIBLK43
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK43

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 01:20:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052119CLP.M
Quant Title : GC Extractables
QLast Update : Wed May 22 06:53:42 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

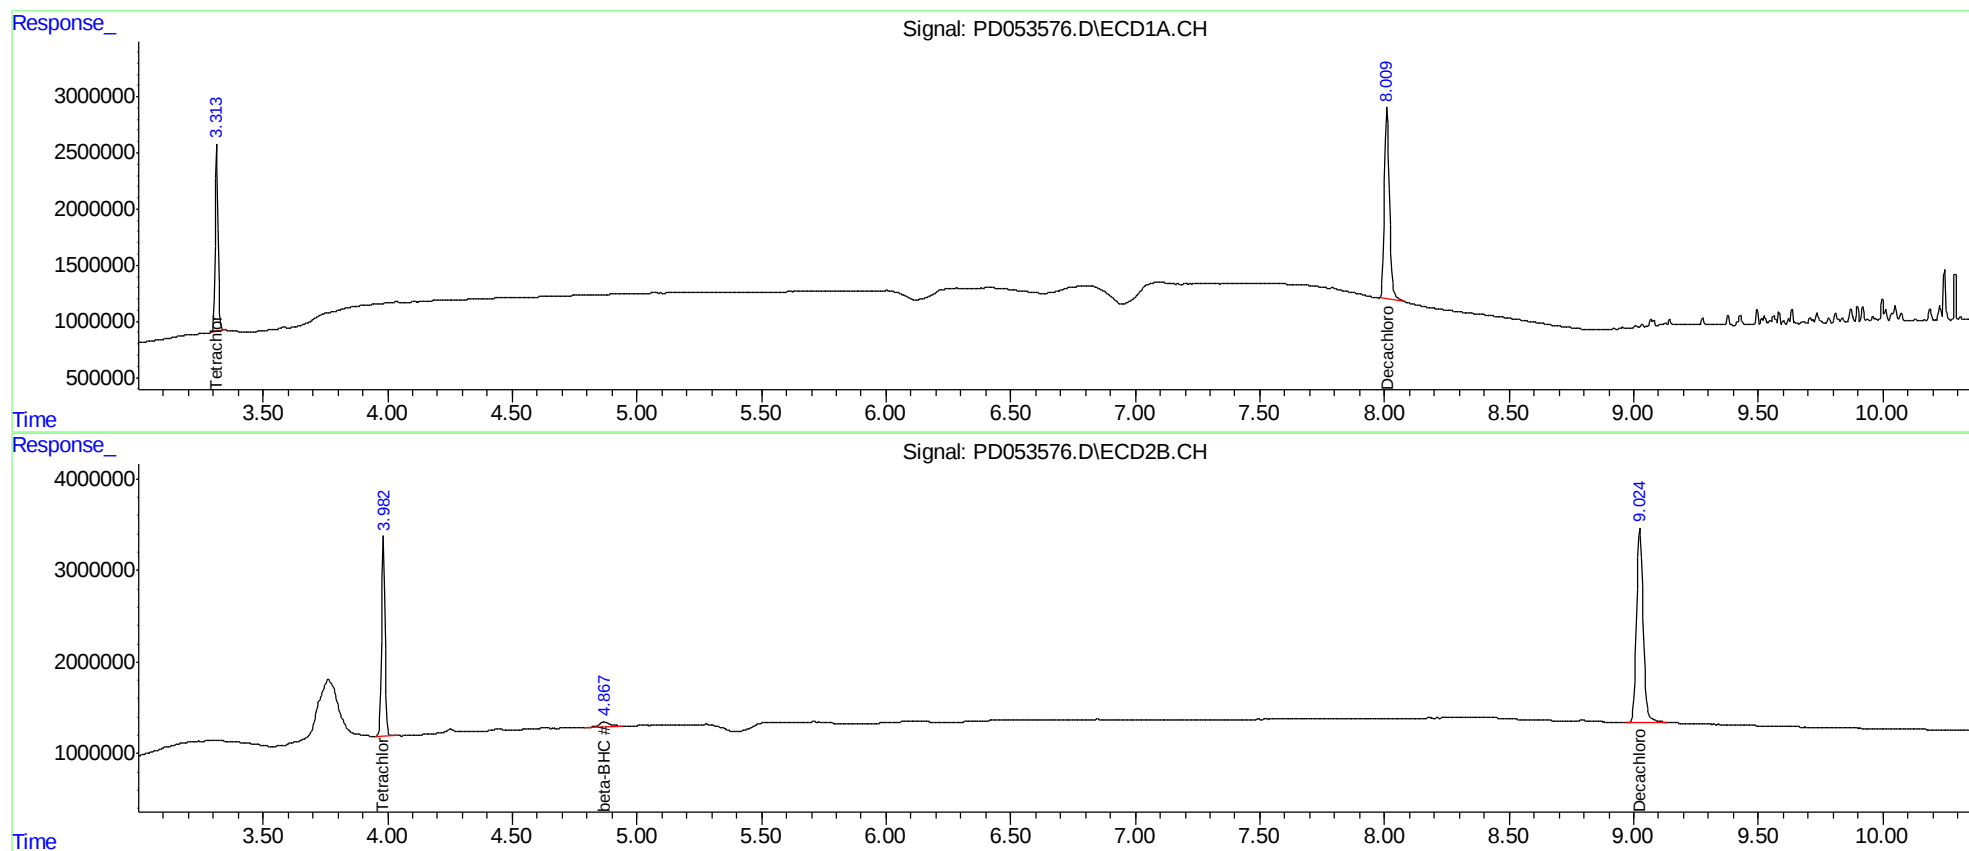


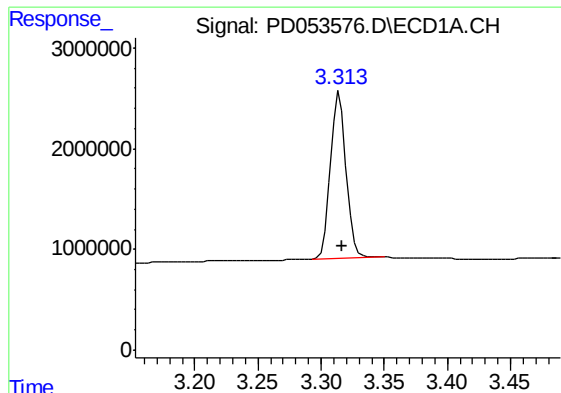

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: -0.002 min
Response: 14515940
Conc: 19.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK43

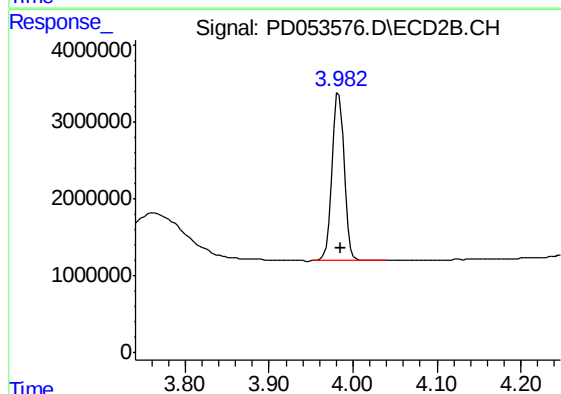


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: -0.002 min
Response: 22350573
Conc: 22.70 ng/ml

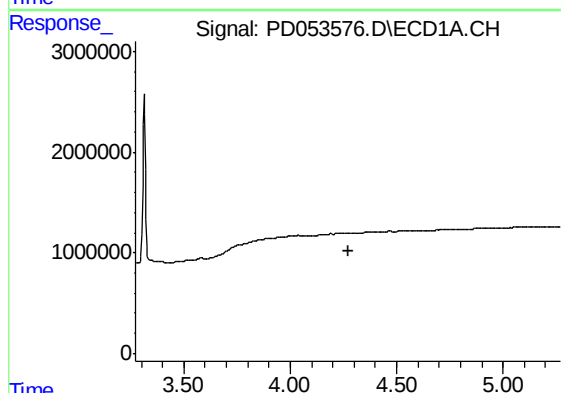


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.272 min
Response: 0
Conc: N.D.

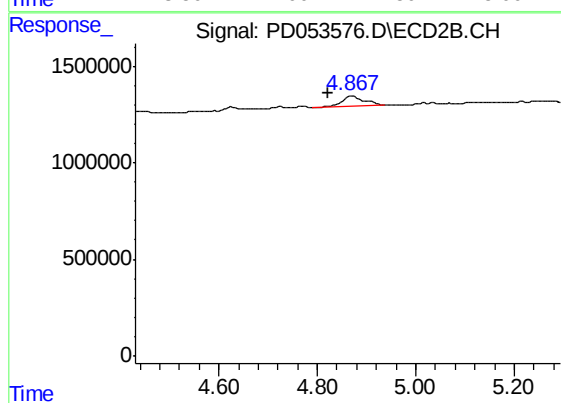

#6 beta-BHC


R.T.: 4.869 min
Delta R.T.: 0.048 min
Response: 1467638
Conc: 2.50 ng/ml

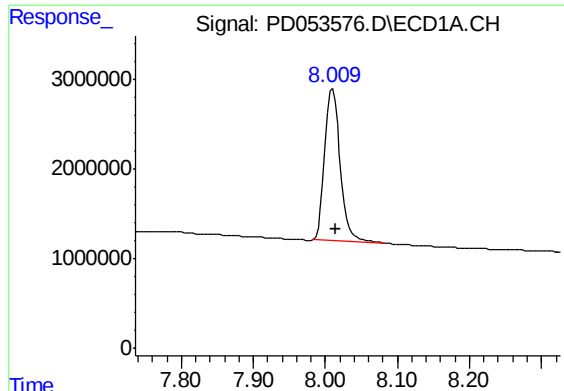

#27 Decachlorobiphenyl

R.T.: 8.010 min
Delta R.T.: -0.005 min
Response: 25350537
Conc: 38.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK43

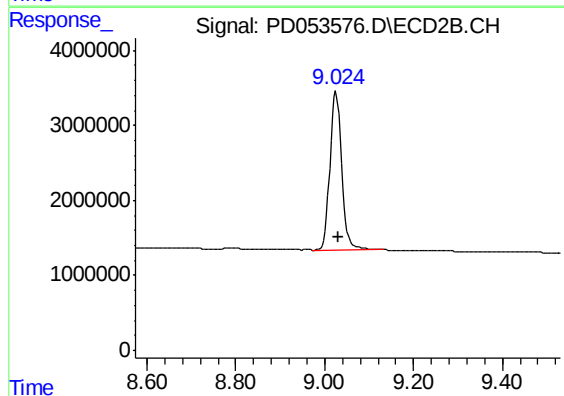

#27 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: -0.004 min
Response: 38895012
Conc: 37.65 ng/ml