

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061219\
 Data File : PD053597.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jun 2019 14:49
 Operator : SM\AJ
 Sample : PIBLK44
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK44

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 01:26:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052119CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed May 22 06:53:42 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.984	14694694	21714833	20.055	22.055
27)	SA Decachlor...	8.010	9.026	25542156	37166053	38.612	35.980
Target Compounds							
6)	B beta-BHC	0.000	4.868f	0	846645	N.D.	1.443
10)	B trans-Chl...	0.000	6.105	0	266012	N.D.	0.208
11)	B cis-Chlor...	0.000	6.105f	0	266012	N.D.	0.211
14)	MA Endrin	0.000	6.683	0	571218	N.D.	0.636
15)	B Endosulfa...	0.000	6.875	0	385890	N.D.	0.367
19)	B Endosulfa...	0.000	7.204	0	5375151	N.D.	5.113
20)	A Methoxychlor	0.000	7.518f	0	1031300	N.D.	2.400
23)	Toxaphene-2	0.000	6.683	0	571218	N.D.	80.052
26)	Toxaphene-5	0.000	7.629	0	224709	N.D.	17.815


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061219\
Data File : PD053597.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jun 2019 14:49
Operator : SM\AJ
Sample : PIBLK44
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK44

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 01:26:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052119CLP.M
Quant Title : GC Extractables
QLast Update : Wed May 22 06:53:42 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

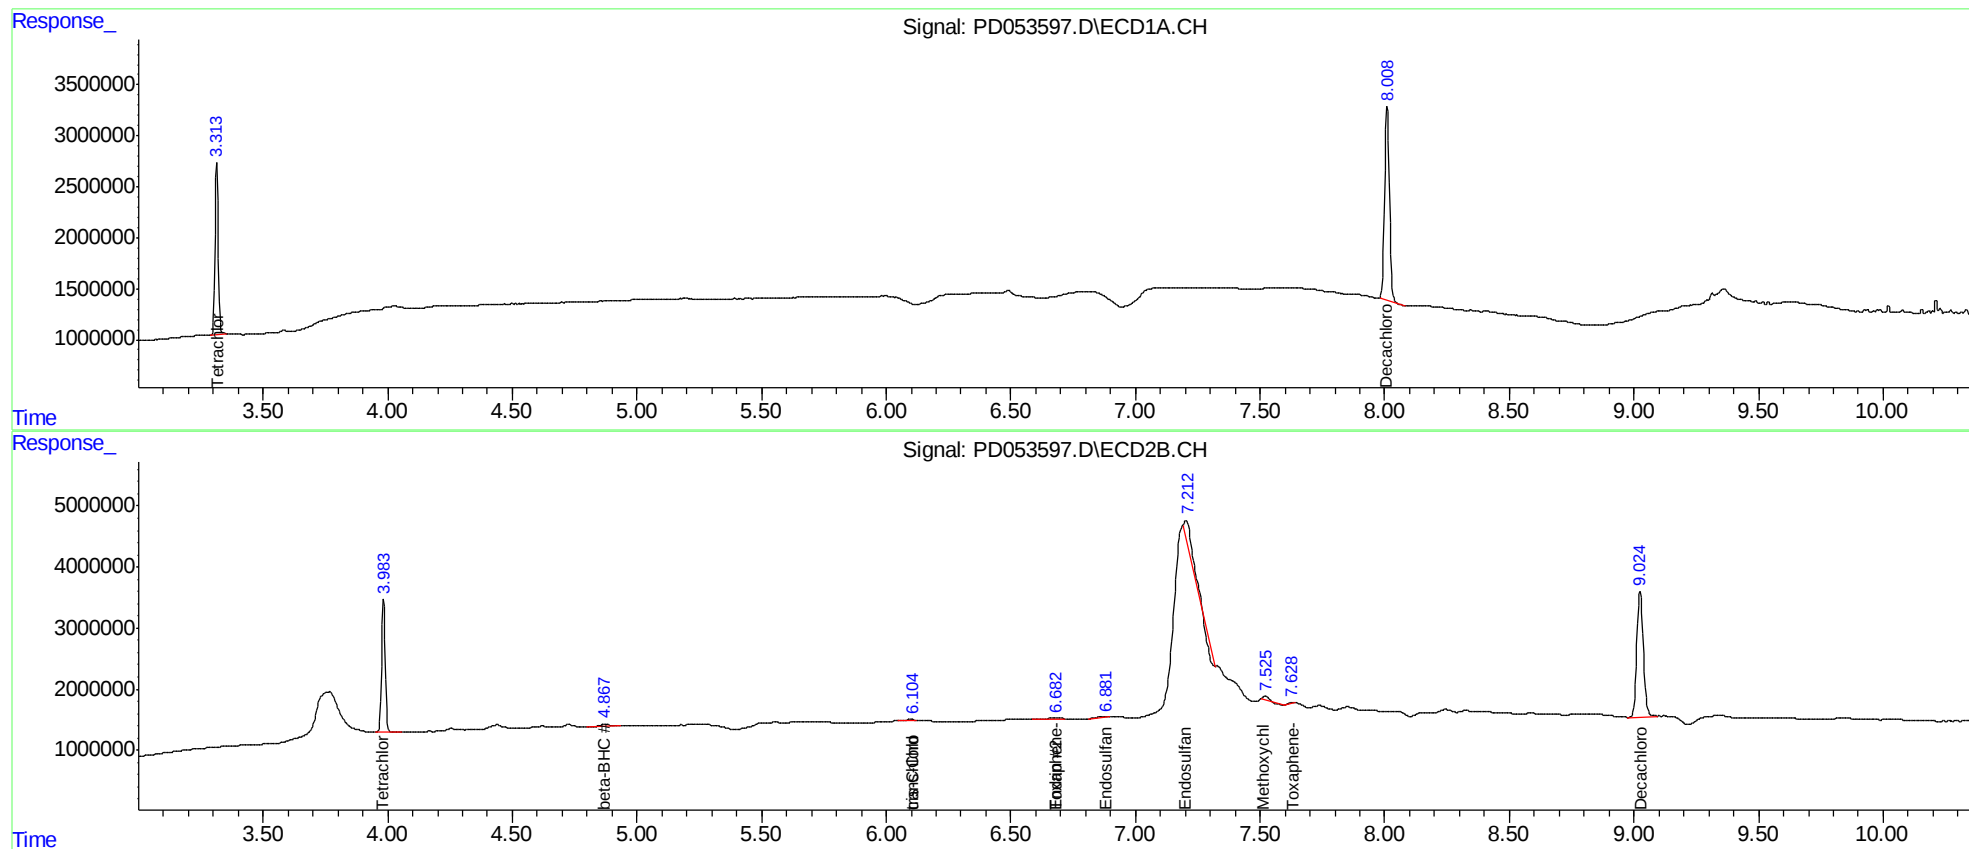


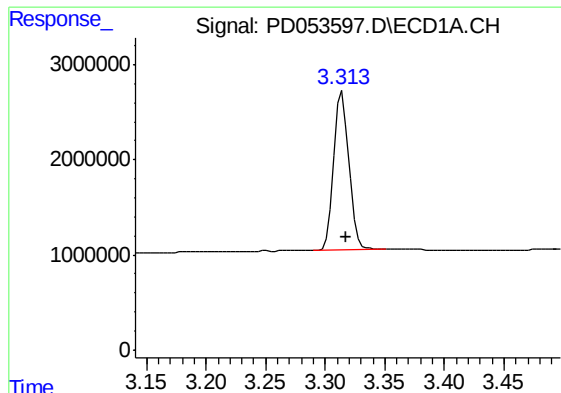

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: -0.002 min
Response: 14694694
Conc: 20.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK44

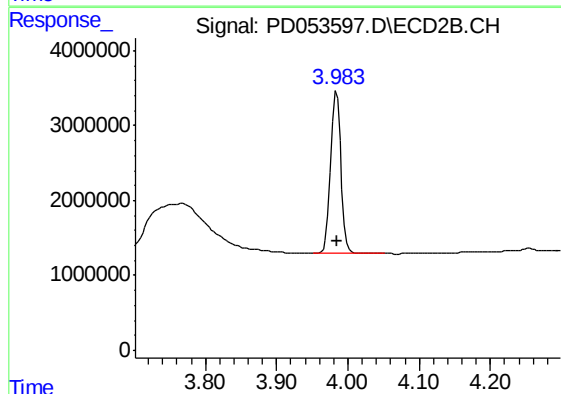


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: -0.001 min
Response: 21714833
Conc: 22.06 ng/ml

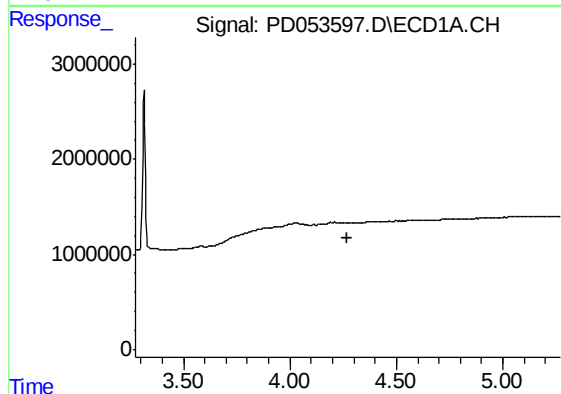


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.272 min
Response: 0
Conc: N.D.

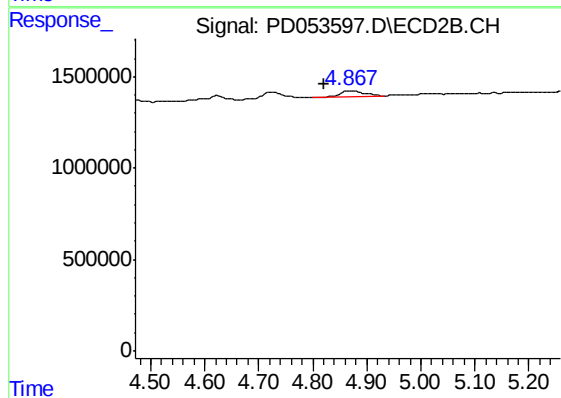

#6 beta-BHC


R.T.: 4.868 min
Delta R.T.: 0.047 min
Response: 846645
Conc: 1.44 ng/ml

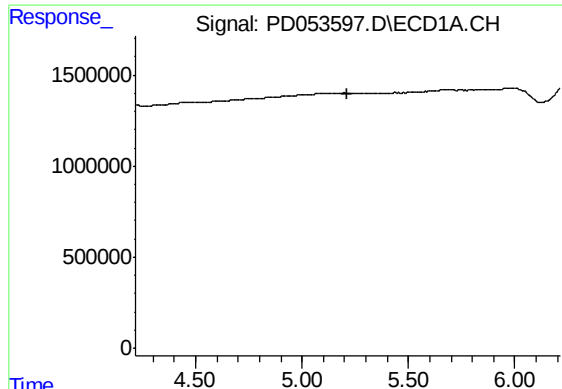

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.215 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK44

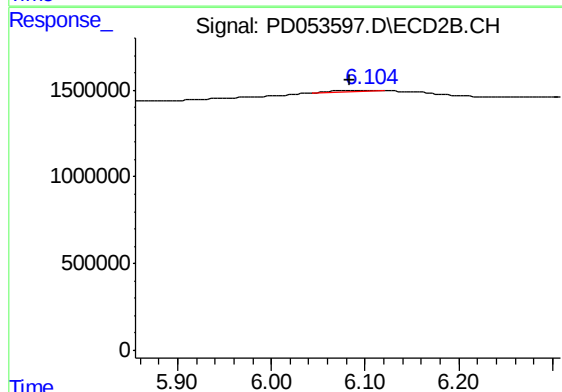


#10 trans-Chlordane

R.T.: 6.105 min
Delta R.T.: 0.021 min
Response: 266012
Conc: 0.21 ng/ml

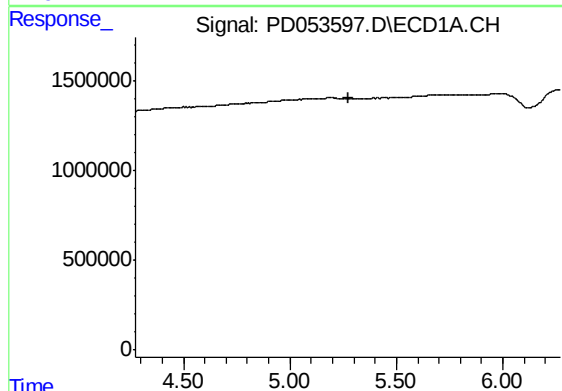


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.273 min
Response: 0
Conc: N.D.

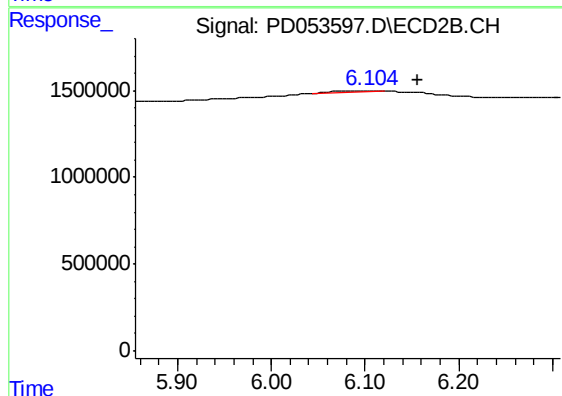

#11 cis-Chlordane


R.T.: 6.105 min
Delta R.T.: -0.052 min
Response: 266012
Conc: 0.21 ng/ml

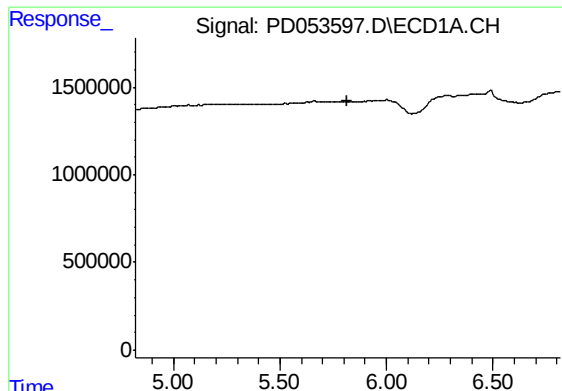

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 5.819 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK44

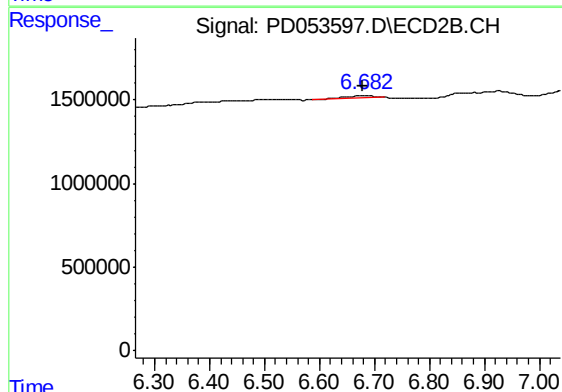


#14 Endrin

R.T.: 6.683 min
Delta R.T.: 0.004 min
Response: 571218
Conc: 0.64 ng/ml

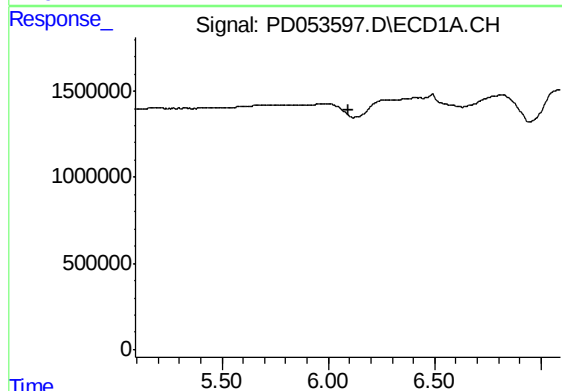


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.093 min
Response: 0
Conc: N.D.

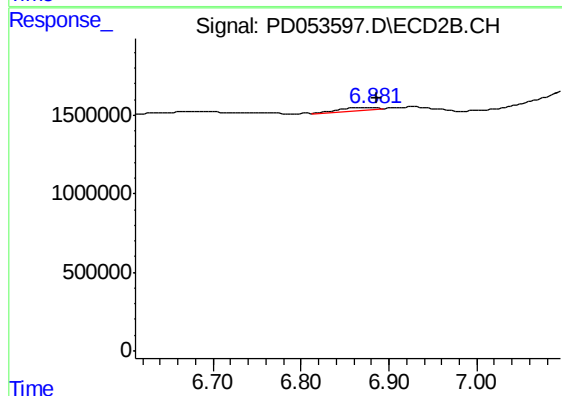

#15 Endosulfan II


R.T.: 6.875 min
Delta R.T.: -0.012 min
Response: 385890
Conc: 0.37 ng/ml

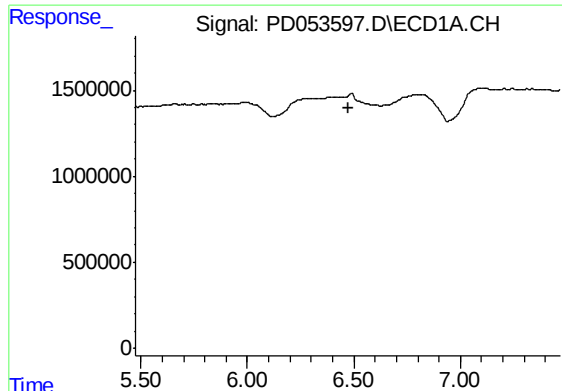

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.473 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK44

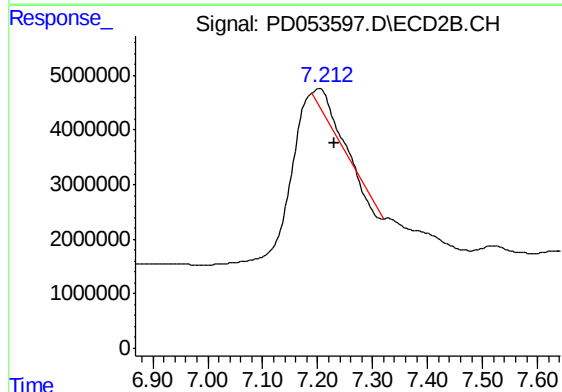


#19 Endosulfan Sulfate

R.T.: 7.204 min
Delta R.T.: -0.027 min
Response: 5375151
Conc: 5.11 ng/ml

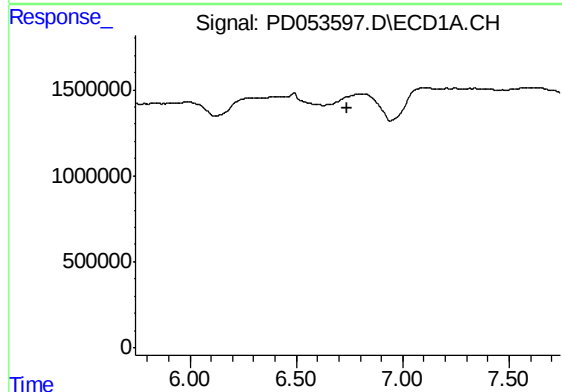


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.741 min
Response: 0
Conc: N.D.

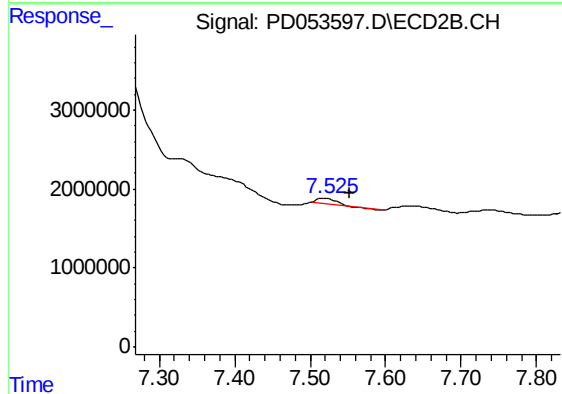

#20 Methoxychlor


R.T.: 7.518 min
Delta R.T.: -0.035 min
Response: 1031300
Conc: 2.40 ng/ml

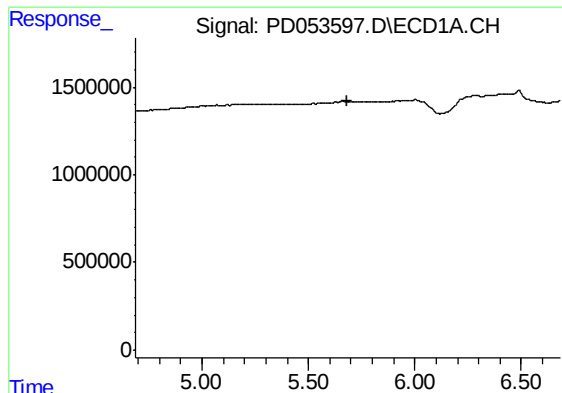

#23 Toxaphene-2


R.T.: 0.000 min
Exp R.T.: 5.684 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK44

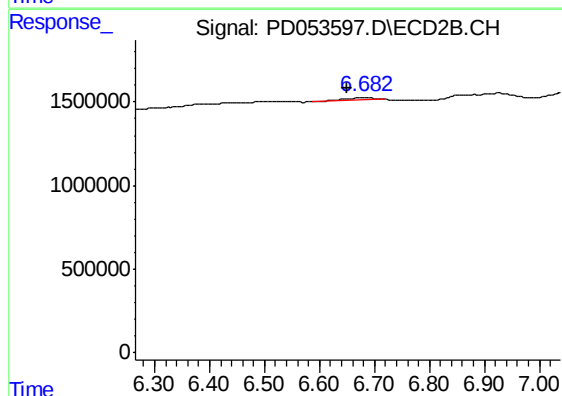


#23 Toxaphene-2

R.T.: 6.683 min
Delta R.T.: 0.032 min
Response: 571218
Conc: 80.05 ng/ml

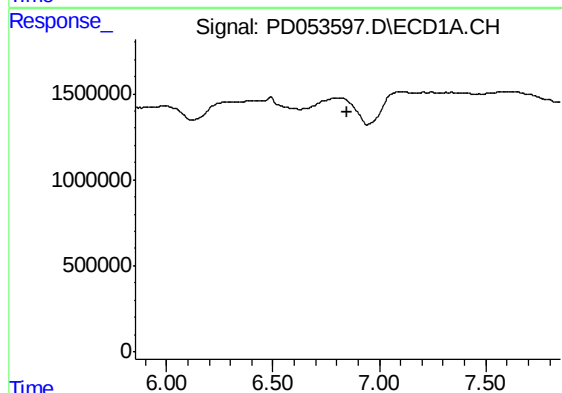


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T.: 6.851 min
Response: 0
Conc: N.D.

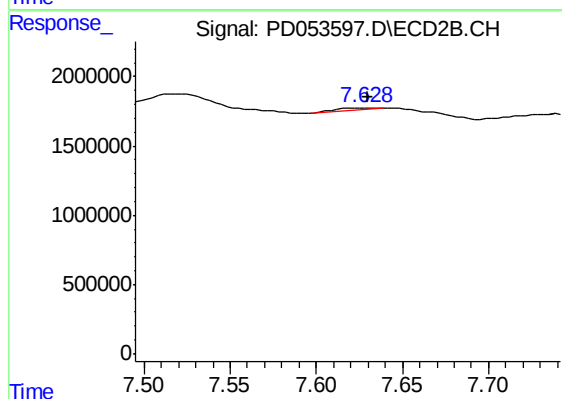

#26 Toxaphene-5


R.T.: 7.629 min
Delta R.T.: 0.000 min
Response: 224709
Conc: 17.81 ng/ml

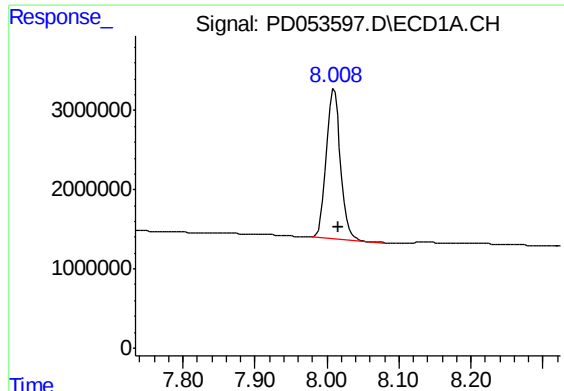

#27 Decachlorobiphenyl

R.T.: 8.010 min
Delta R.T.: -0.005 min
Response: 25542156
Conc: 38.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK44

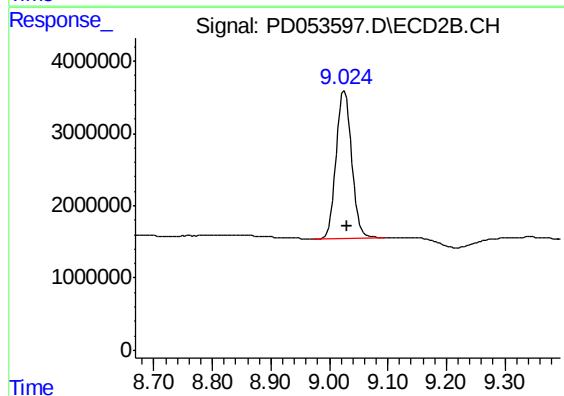

#27 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: -0.004 min
Response: 37166053
Conc: 35.98 ng/ml