

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061221\
 Data File : PD063768.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2021 11:41
 Operator : AR\AJ
 Sample : PB137032BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK032

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 00:21:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	3.971	27313682	278.1E6	19.899	19.753
27)	SA Decachlor...	8.203	9.030	61811580	473.0E6	38.045	32.235
Target Compounds							
2)	A alpha-BHC	0.000	4.346	0	22869433	N.D.	1.035
6)	B beta-BHC	4.380f	4.830	1962964	29814888	2.110	3.333 #
7)	B delta-BHC	0.000	5.025	0	36098252	N.D.	1.636
8)	B Heptachlo...	0.000	5.852	0	31465361	N.D.	1.581
16)	A 4,4'-DDD	0.000	6.754f	0	12500667	N.D.	0.823
19)	B Endosulfa...	0.000	7.254	0	4631977	N.D.	0.297
20)	A Methoxychlor	0.000	7.484f	0	10877377	N.D.	1.508
26)	Toxaphene-5	7.060	0.000	2291123	0	66.876	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061221\
Data File : PD063768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2021 11:41
Operator : AR\AJ
Sample : PB137032BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PBLK032

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 00:21:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

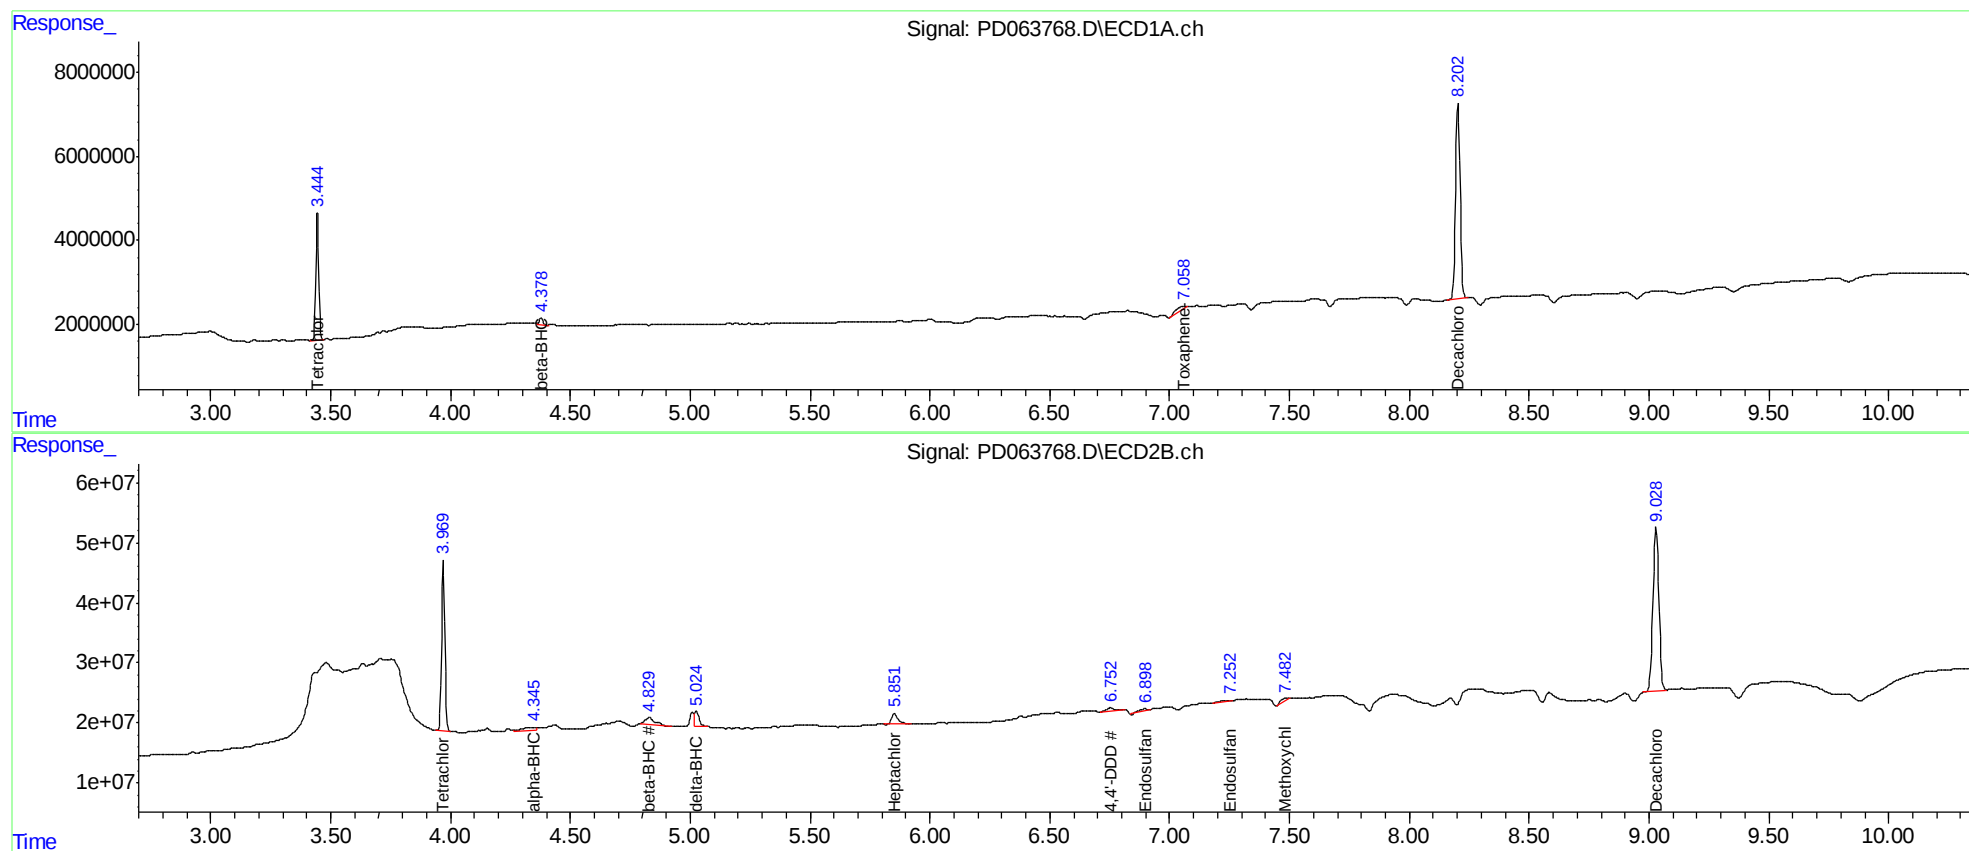


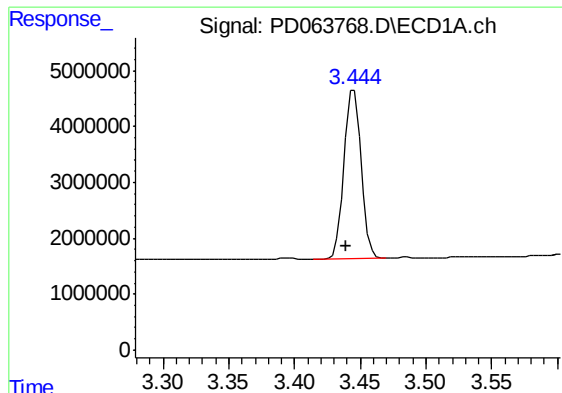

#1 Tetrachloro-m-xylene


R.T.: 3.445 min
Delta R.T.: 0.006 min
Response: 27313682
Conc: 19.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK032

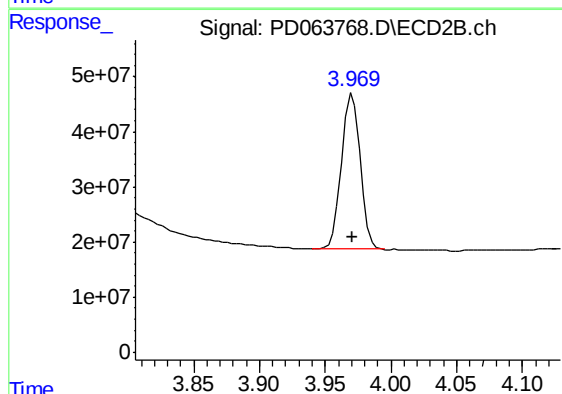


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 278054973
Conc: 19.75 ng/ml

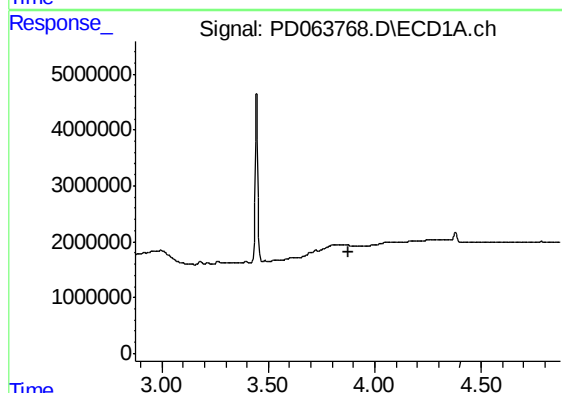


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.875 min
Response: 0
Conc: N.D.

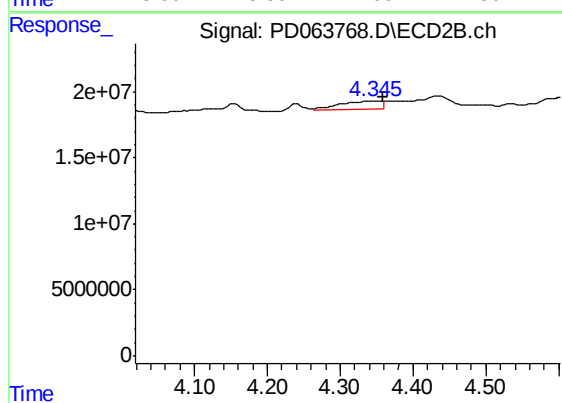

#2 alpha-BHC


R.T.: 4.346 min
Delta R.T.: -0.012 min
Response: 22869433
Conc: 1.03 ng/ml

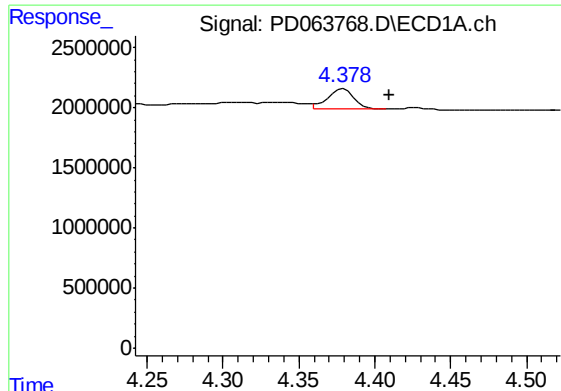

#6 beta-BHC


R.T.: 4.380 min
Delta R.T.: -0.030 min
Response: 1962964
Conc: 2.11 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK032

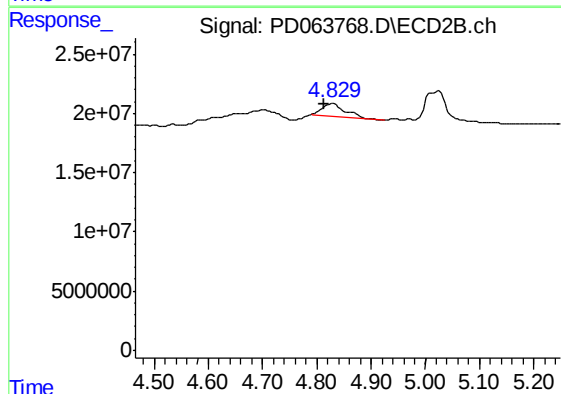


#6 beta-BHC

R.T.: 4.830 min
Delta R.T.: 0.016 min
Response: 29814888
Conc: 3.33 ng/ml

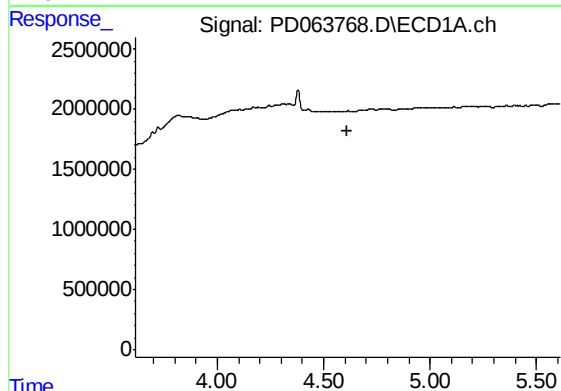


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.613 min
Response: 0
Conc: N.D.

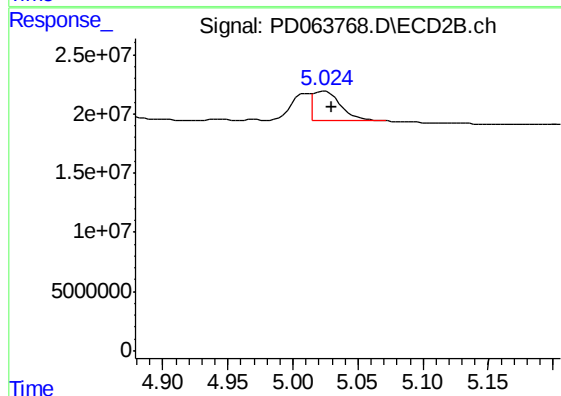

#7 delta-BHC


R.T.: 5.025 min
Delta R.T.: -0.005 min
Response: 36098252
Conc: 1.64 ng/ml

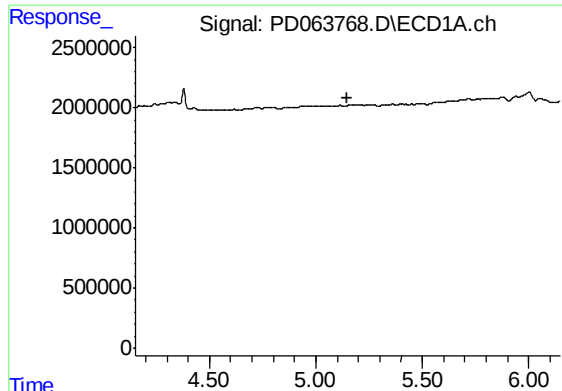

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.150 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PBLK032

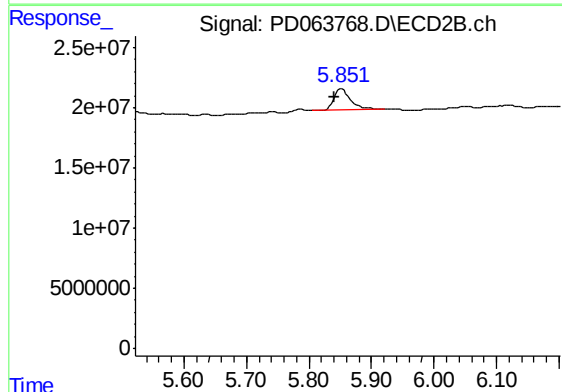


#8 Heptachlor epoxide

R.T.: 5.852 min
Delta R.T.: 0.011 min
Response: 31465361
Conc: 1.58 ng/ml

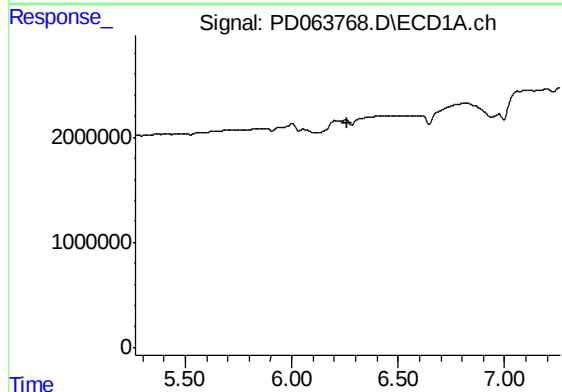


#15 Endosulfan II

R.T.: 6.200 min
Delta R.T.: -0.063 min
Response: -951053
Conc: N.D.

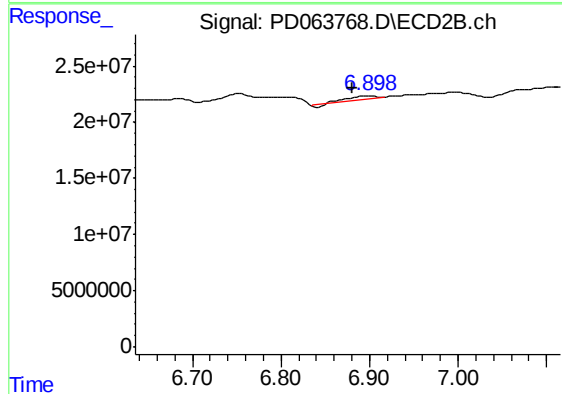

#15 Endosulfan II


R.T.: 6.898 min
Delta R.T.: 0.018 min
Response: 5130735
Conc: 0.34 ng/ml

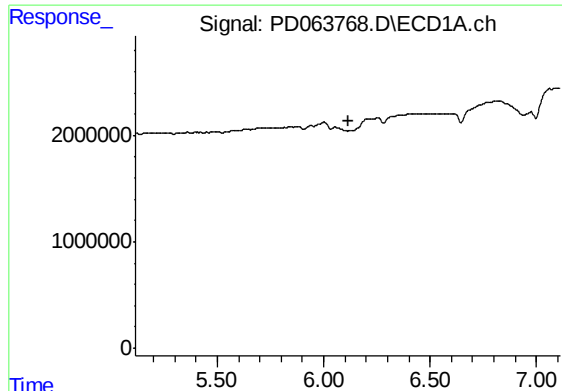

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 6.115 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PBLK032

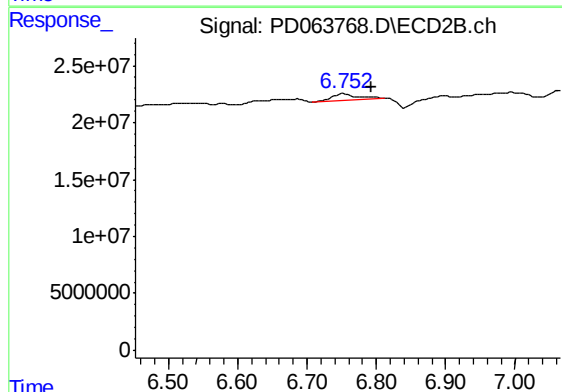


#16 4,4'-DDD

R.T.: 6.754 min
Delta R.T.: -0.039 min
Response: 12500667
Conc: 0.82 ng/ml

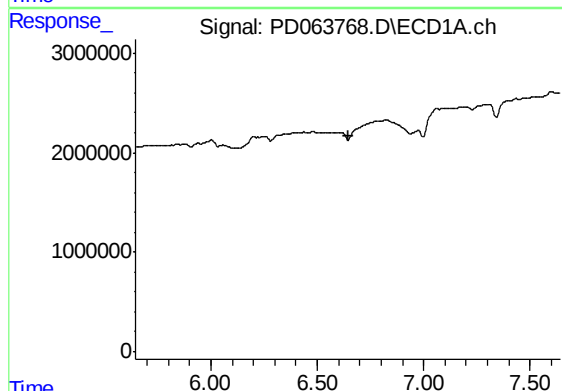


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.645 min
Response: 0
Conc: N.D.

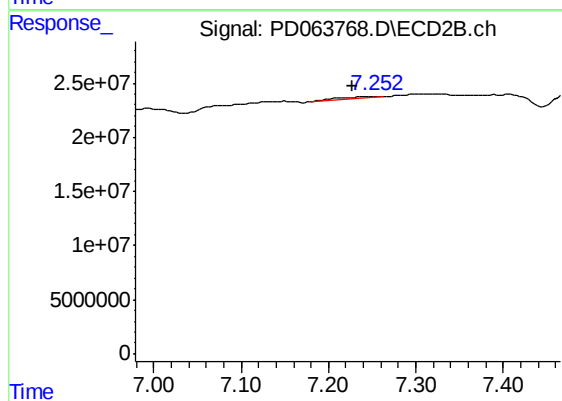

#19 Endosulfan Sulfate


R.T.: 7.254 min
Delta R.T.: 0.027 min
Response: 4631977
Conc: 0.30 ng/ml

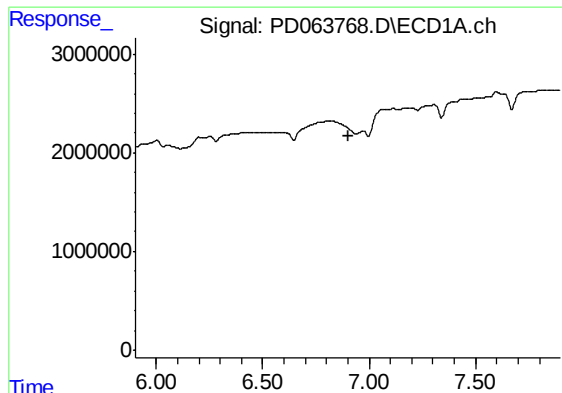

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.902 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PBLK032

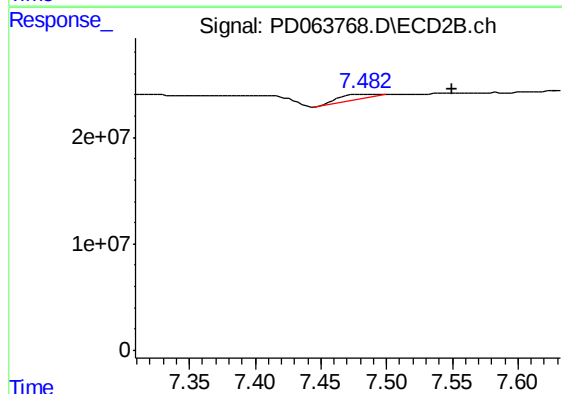


#20 Methoxychlor

R.T.: 7.484 min
Delta R.T.: -0.066 min
Response: 10877377
Conc: 1.51 ng/ml

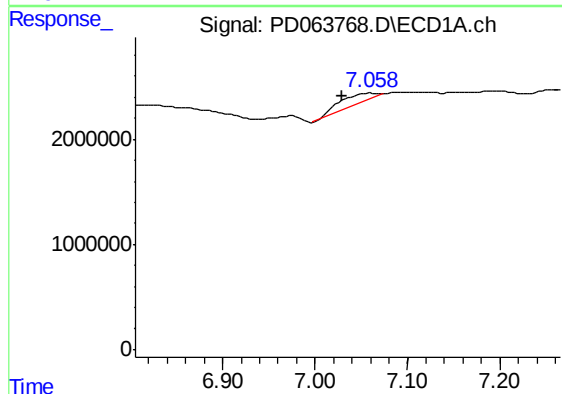


#26 Toxaphene-5

R.T.: 7.060 min
Delta R.T.: 0.030 min
Response: 2291123
Conc: 66.88 ng/ml

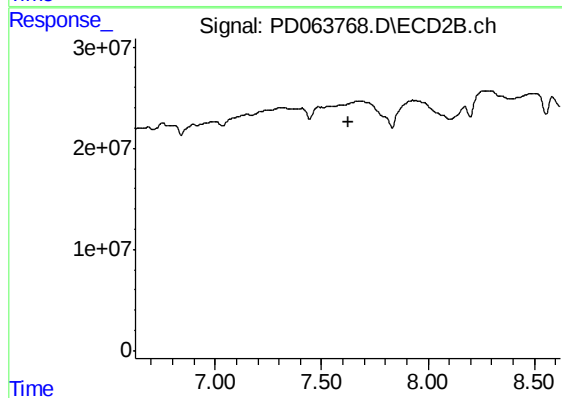

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T. : 7.625 min
Response: 0
Conc: N.D.

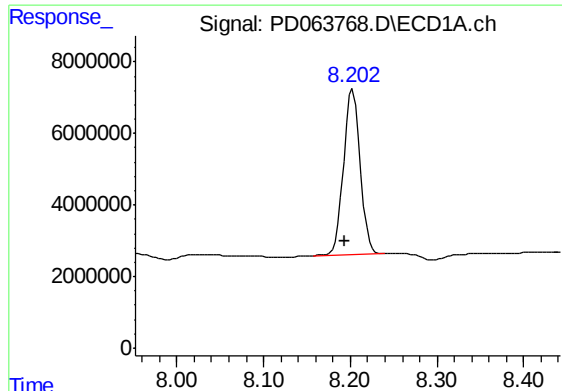

#27 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: 0.009 min
Response: 61811580
Conc: 38.04 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK032

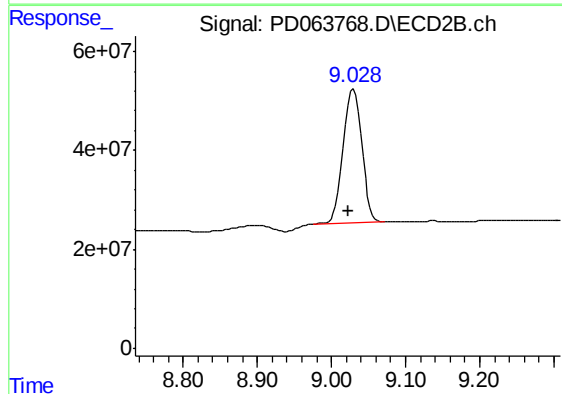

#27 Decachlorobiphenyl

R.T.: 9.030 min
Delta R.T.: 0.006 min
Response: 472979153
Conc: 32.24 ng/ml