

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061221\
 Data File : PD063778.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2021 14:49
 Operator : AR\AJ
 Sample : M2618-06MSD
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BG5R7MSD

Manual Integrations
 APPROVED

Ankita
 6/14/2021 4:57:32 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 00:25:08 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.971	16039839	148.6E6	11.686	10.556
2)	SA Decachlor...	8.194	9.026	84700718	614.6E6	52.133	41.890m
Target Compounds							
2)	A alpha-BHC	3.875	4.359	90150304	814.9E6	44.153	36.873
3)	MA gamma-BHC...	4.159	4.641	98329710	764.2E6	48.841	37.406m
4)	MA Heptachlor	4.459	5.150	81244230	626.0E6	41.751	30.127 #
5)	MB Aldrin	4.706	5.454	74647900	581.9E6	39.740	28.273 #
6)	B beta-BHC	4.409	4.814	34038633	258.0E6	36.592	28.845m
7)	B delta-BHC	4.613	5.030	82333842	626.7E6	42.188	28.410 #
8)	B Heptachlo...	5.149	5.840	62487156	487.7E6	35.522	24.503 #
9)	A Endosulfan I	5.490	6.197	51230490	367.6E6	31.160	20.586 #
10)	B trans-Chl...	5.376	6.067	102.8E6	1197.9E6	56.212	60.113
11)	B cis-Chlor...	5.435	6.147	80717782	630.3E6	45.511	33.344 #
12)	B 4,4'-DDE	5.599	6.303	148.2E6	1108.7E6	82.047	58.588 #
13)	MA Dieldrin	5.731	6.452	179.2E6	1107.1E6	95.688m	57.861m#
14)	MA Endrin	5.989	6.670	134.2E6	817.1E6	83.064	51.601m#
15)	B Endosulfa...	6.264	6.880	126.7E6	927.8E6	84.355	61.291m#
16)	A 4,4'-DDD	6.116	6.794	110.9E6	976.0E6	75.023	64.248
17)	MA 4,4'-DDT	6.357	7.092	287.2E6	2234.4E6	189.154	145.379
18)	B Endrin al...	6.432	7.003	76232458	610.9E6	58.503	46.284m
19)	B Endosulfa...	6.645	7.228	114.5E6	794.2E6	79.708	50.962 #
20)	A Methoxychlor	6.903	7.550	261.3E6	2093.7E6	316.618	290.192
21)	B Endrin ke...	7.137	7.699	100.8E6	663.0E6	57.161m	43.024

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061221\
Data File : PD063778.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2021 14:49
Operator : AR\AJ
Sample : M2618-06MSD
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 00:25:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

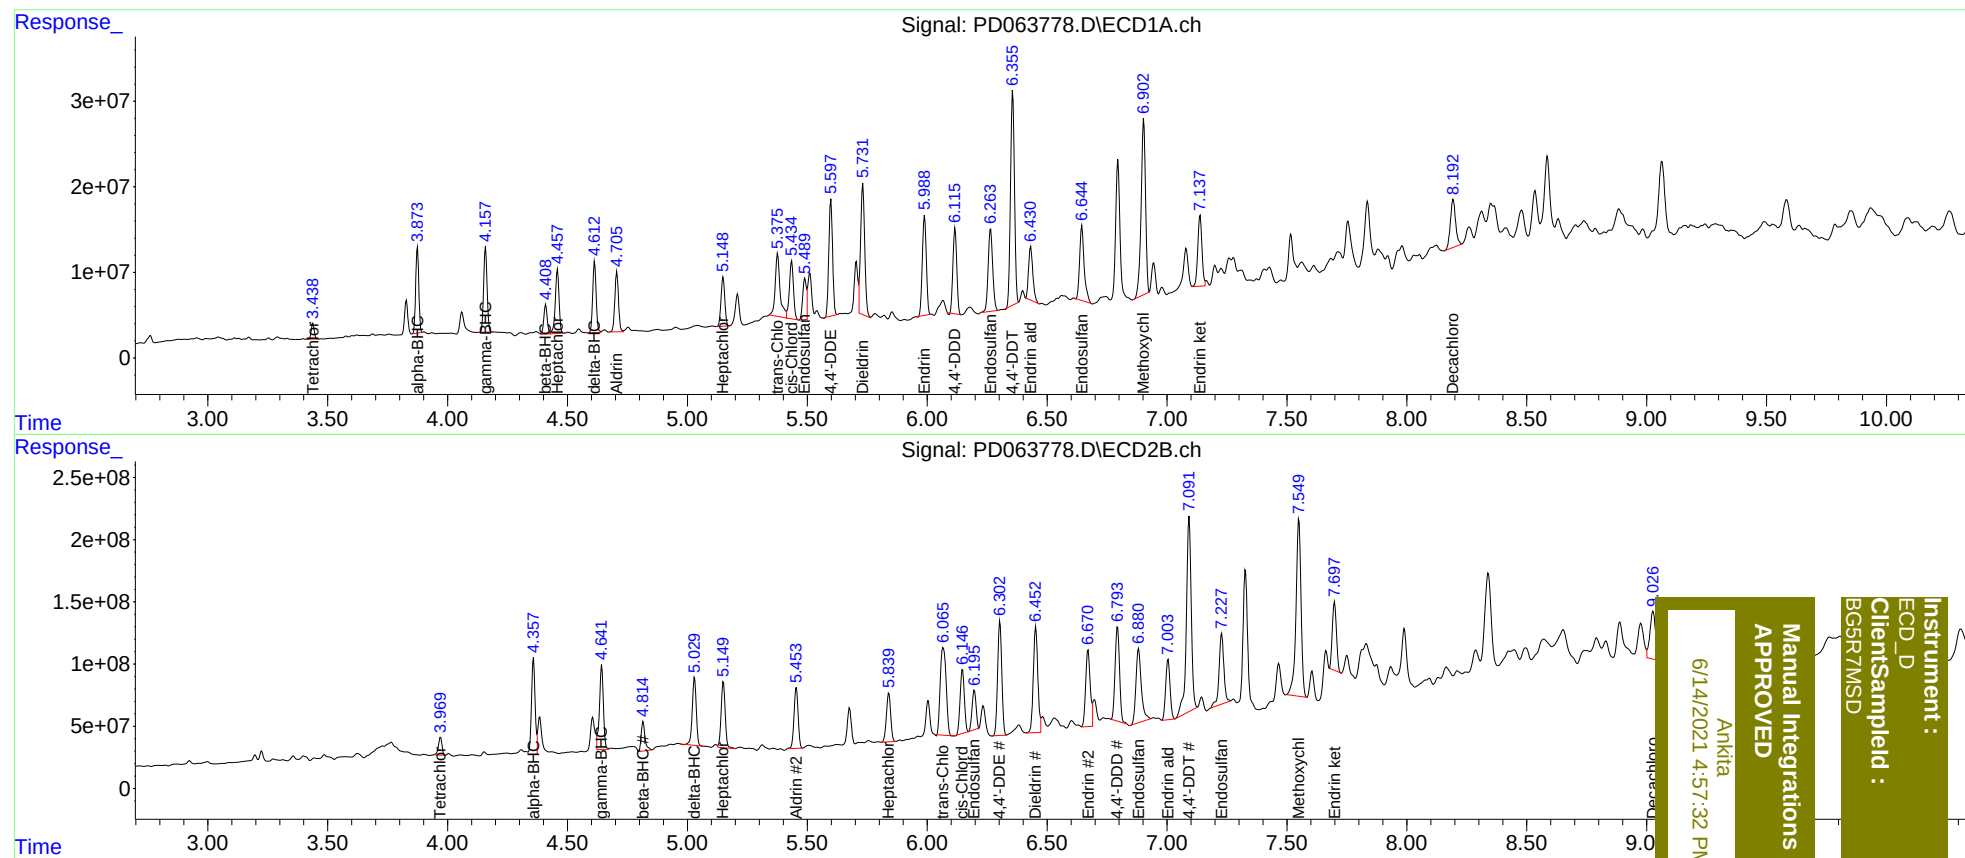

Manual Integrations
APPROVED

6/14/2021 4:57:32 PM

Ankita

Instrument :
ECD_D
ClientSampled :
BG5RTMSD