

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD061221\  
 Data File : PD063771.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 12 Jun 2021 13:09  
 Operator : AR\AJ  
 Sample : INDA348  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 INDA3048

Manual Integrations  
 APPROVED

Ankita  
 6/14/2021 4:57:20 PM

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jun 14 00:22:21 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD060321CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Jun 03 06:08:10 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm


|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml   |
|-----------------------------|-----------------|-------|-------|----------|----------|---------|---------|
| -----                       |                 |       |       |          |          |         |         |
| System Monitoring Compounds |                 |       |       |          |          |         |         |
| 1)                          | SA Tetrachlo... | 3.439 | 3.971 | 31121768 | 311.8E6  | 22.673  | 22.149  |
| 27)                         | SA Decachlor... | 8.197 | 9.026 | 69251367 | 562.6E6  | 42.624  | 38.340  |
| Target Compounds            |                 |       |       |          |          |         |         |
| 2)                          | A alpha-BHC     | 3.875 | 4.359 | 46754541 | 504.7E6  | 22.899  | 22.836  |
| 3)                          | MA gamma-BHC... | 4.158 | 4.643 | 44066224 | 459.4E6  | 21.888  | 22.489  |
| 4)                          | MA Heptachlor   | 4.460 | 5.150 | 42090329 | 458.3E6  | 21.630  | 22.056  |
| 9)                          | A Endosulfan I  | 5.489 | 6.197 | 36703027 | 403.5E6  | 22.324  | 22.596  |
| 13)                         | MA Dieldrin     | 5.733 | 6.454 | 82288567 | 830.0E6  | 43.929  | 43.380  |
| 14)                         | MA Endrin       | 5.991 | 6.671 | 73343828 | 683.8E6  | 45.381  | 43.185  |
| 16)                         | A 4,4'-DDD      | 6.117 | 6.793 | 68549080 | 663.5E6  | 46.388  | 43.675m |
| 17)                         | MA 4,4'-DDT     | 6.357 | 7.093 | 59962533 | 621.3E6  | 39.495  | 40.422  |
| 20)                         | A Methoxychlor  | 6.905 | 7.551 | 165.0E6  | 1366.9E6 | 199.923 | 189.451 |
| -----                       |                 |       |       |          |          |         |         |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD061221\  
Data File : PD063771.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 12 Jun 2021 13:09  
Operator : AR\AJ  
Sample : INDA348  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jun 14 00:22:21 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD060321CLP.M  
Quant Title : GC Extractables  
QLast Update : Thu Jun 03 06:08:10 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

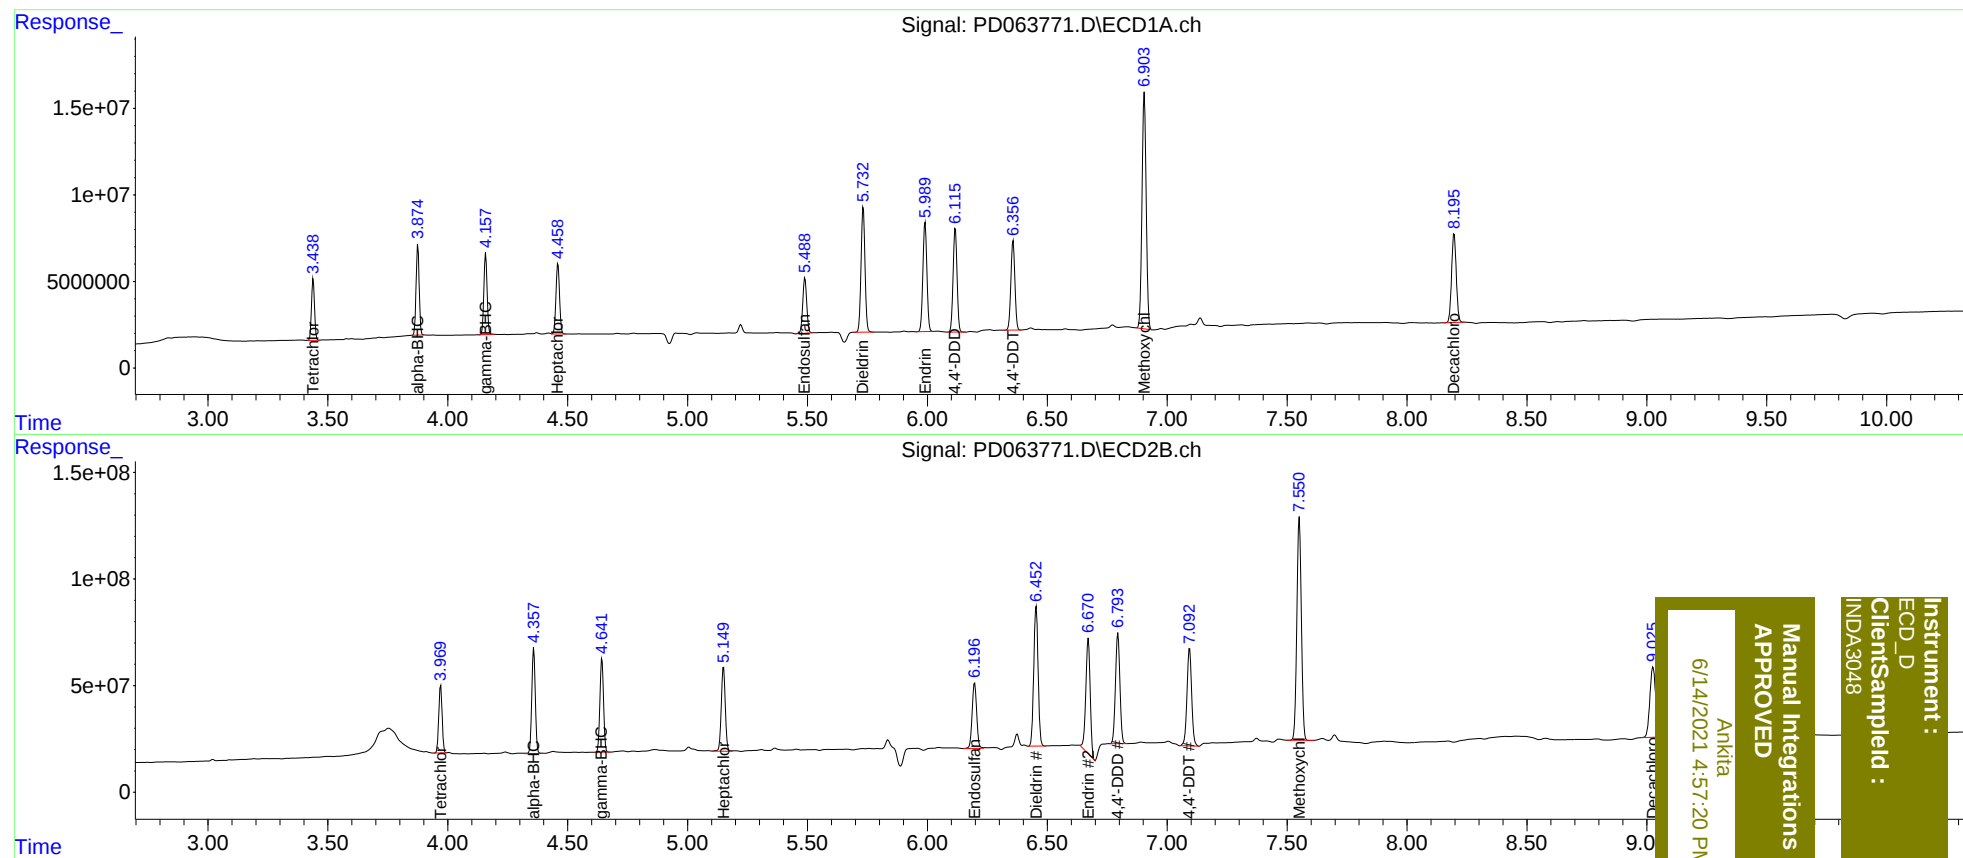

Manual Integrations  
APPROVED

Ankita  
6/14/2021 4:57:20 PM

Instrument :  
ECD\_D  
ClientSampled :  
INDA3048