

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061223\
 Data File : PD075757.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2023 08:53
 Operator : AR\AJ
 Sample : PIBLK163
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 22:19:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.769	48328220	24077223	24.175	23.748
2)	SA Decachlor...	9.092	7.915	117.0E6	49151004	51.019	52.338
Target Compounds							
4)	MA Heptachlor	4.945	0.000	2737076	0	0.844	N.D. #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061223\
Data File : PD075757.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2023 08:53
Operator : AR\AJ
Sample : PIBLK163
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 22:19:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

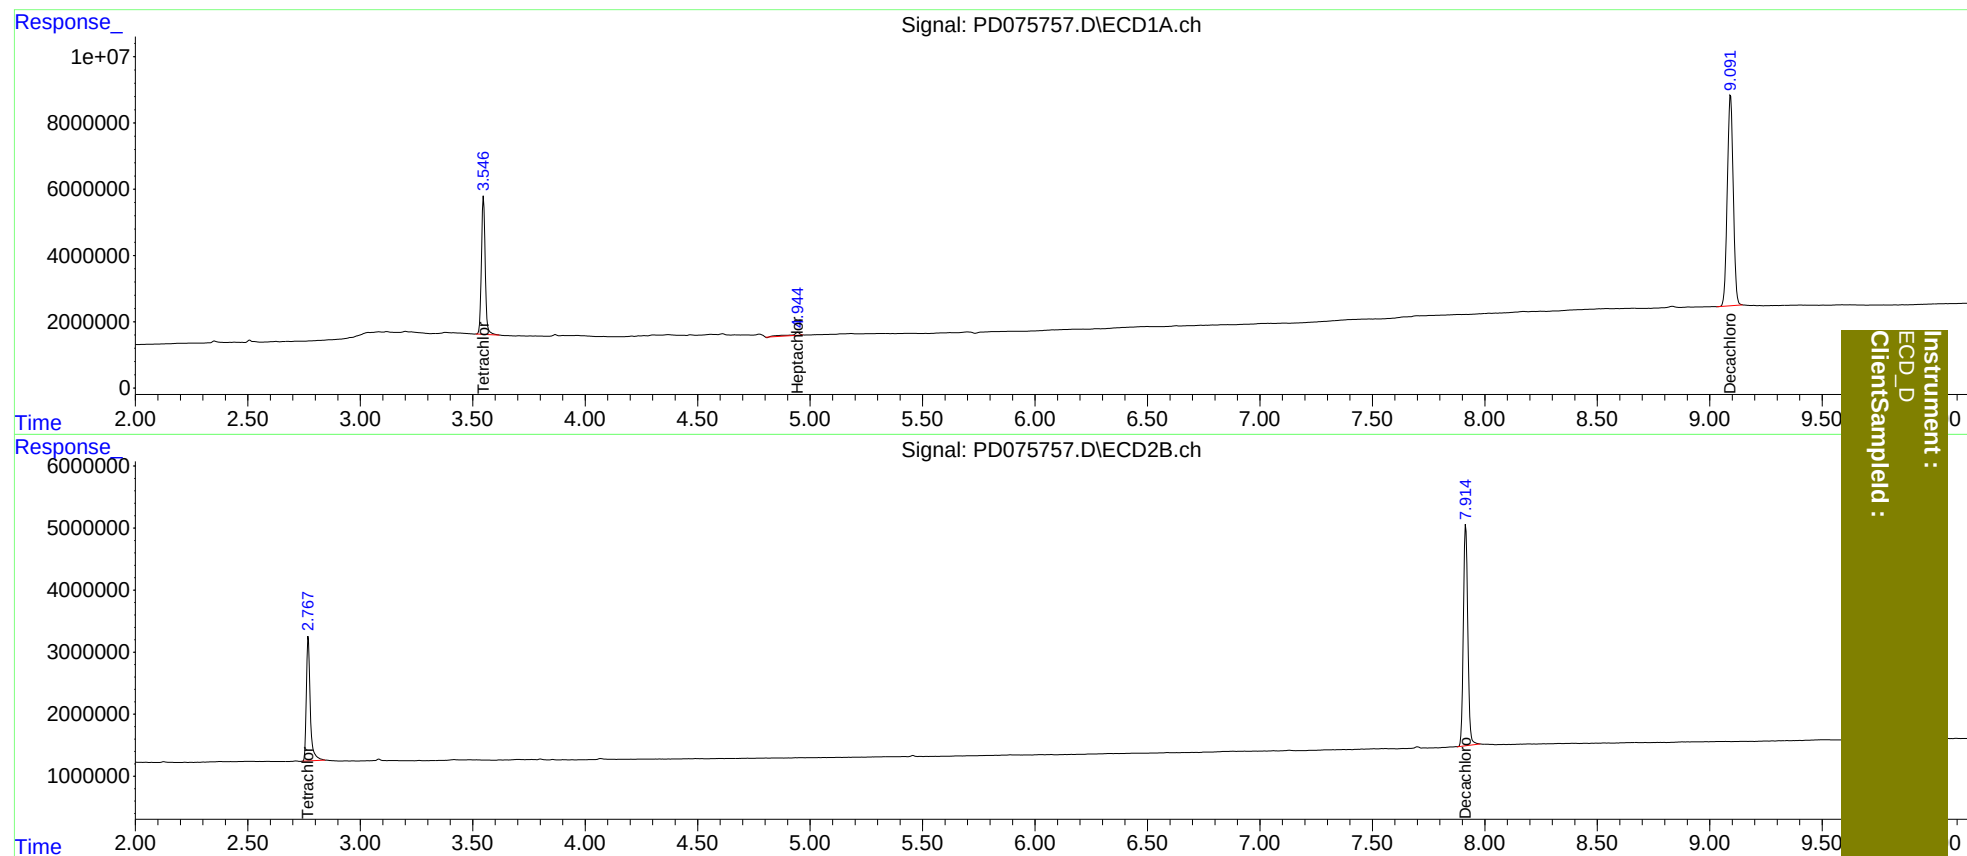


Instrument :
ECD_D
ClientSampled :
0

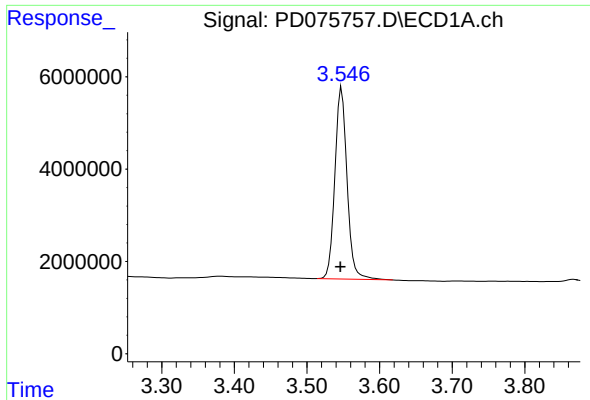

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.002 min
Response: 48328220
Conc: 24.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

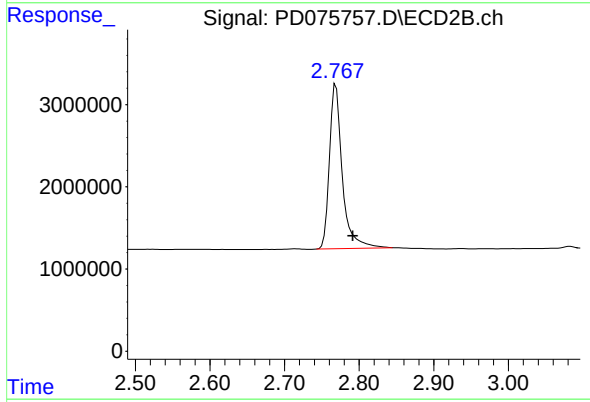


#1 Tetrachloro-m-xylene

R.T.: 2.769 min
Delta R.T.: -0.023 min
Response: 24077223
Conc: 23.75 ng/ml

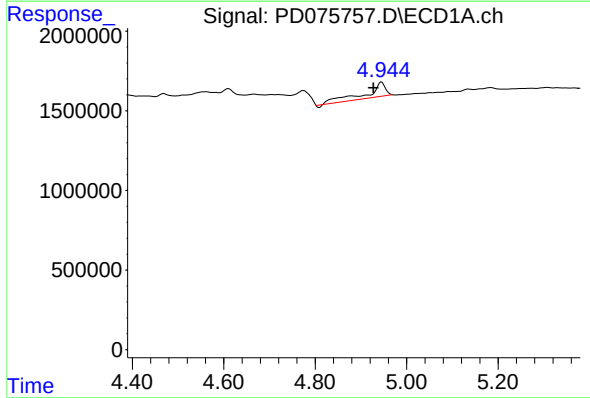


#4 Heptachlor

R.T.: 4.945 min
Delta R.T.: 0.018 min
Response: 2737076
Conc: 0.84 ng/ml

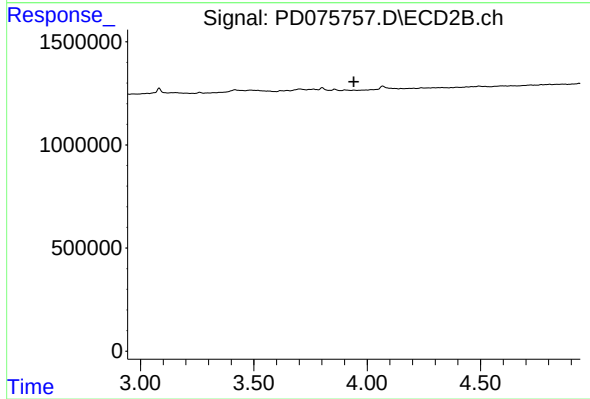

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.941 min
Response: 0
Conc: N.D.

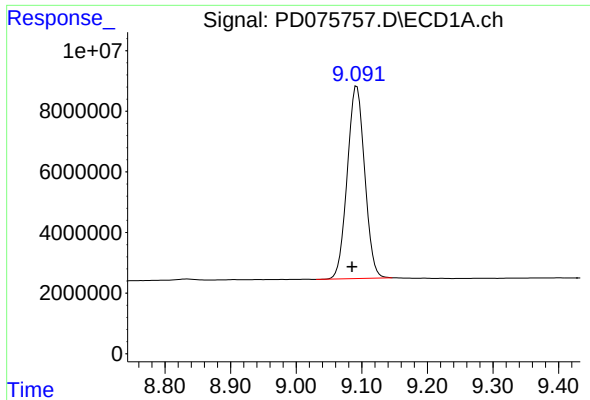

#27 Decachlorobiphenyl

R.T.: 9.092 min
Delta R.T.: 0.007 min
Response: 117014970
Conc: 51.02 ng/ml

Instrument :
ECD_D
ClientSampleId :

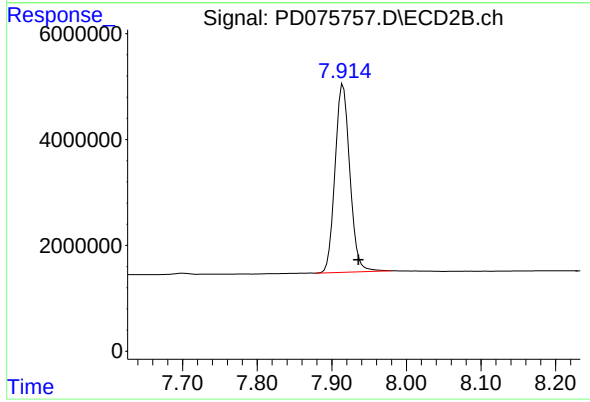

#27 Decachlorobiphenyl

R.T.: 7.915 min
Delta R.T.: -0.020 min
Response: 49151004
Conc: 52.34 ng/ml