

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061223\
 Data File : PD075766.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2023 16:28
 Operator : AR\AJ
 Sample : 03098-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 22:29:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.769	41177115	19142783	20.598	18.881
27)	SA Decachlor...	9.092	7.916	73576379	27343682	32.080	29.117
Target Compounds							
3)	MA gamma-BHC...	0.000	3.622	0	82824	N.D.	<MDL
4)	MA Heptachlor	4.943	0.000	545105	0	0.168	N.D. #
5)	MB Aldrin	0.000	4.247	0	183099	N.D.	0.130
9)	A Endosulfan I	6.083	0.000	1410868	0	0.532	N.D. #
10)	B trans-Chl...	0.000	4.927f	0	99139	N.D.	<MDL
11)	B cis-Chlor...	6.040	0.000	1387658	0	0.461	N.D. #
12)	B 4,4'-DDE	0.000	5.216	0	542005	N.D.	0.477

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061223\
Data File : PD075766.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2023 16:28
Operator : AR\AJ
Sample : 03098-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 22:29:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

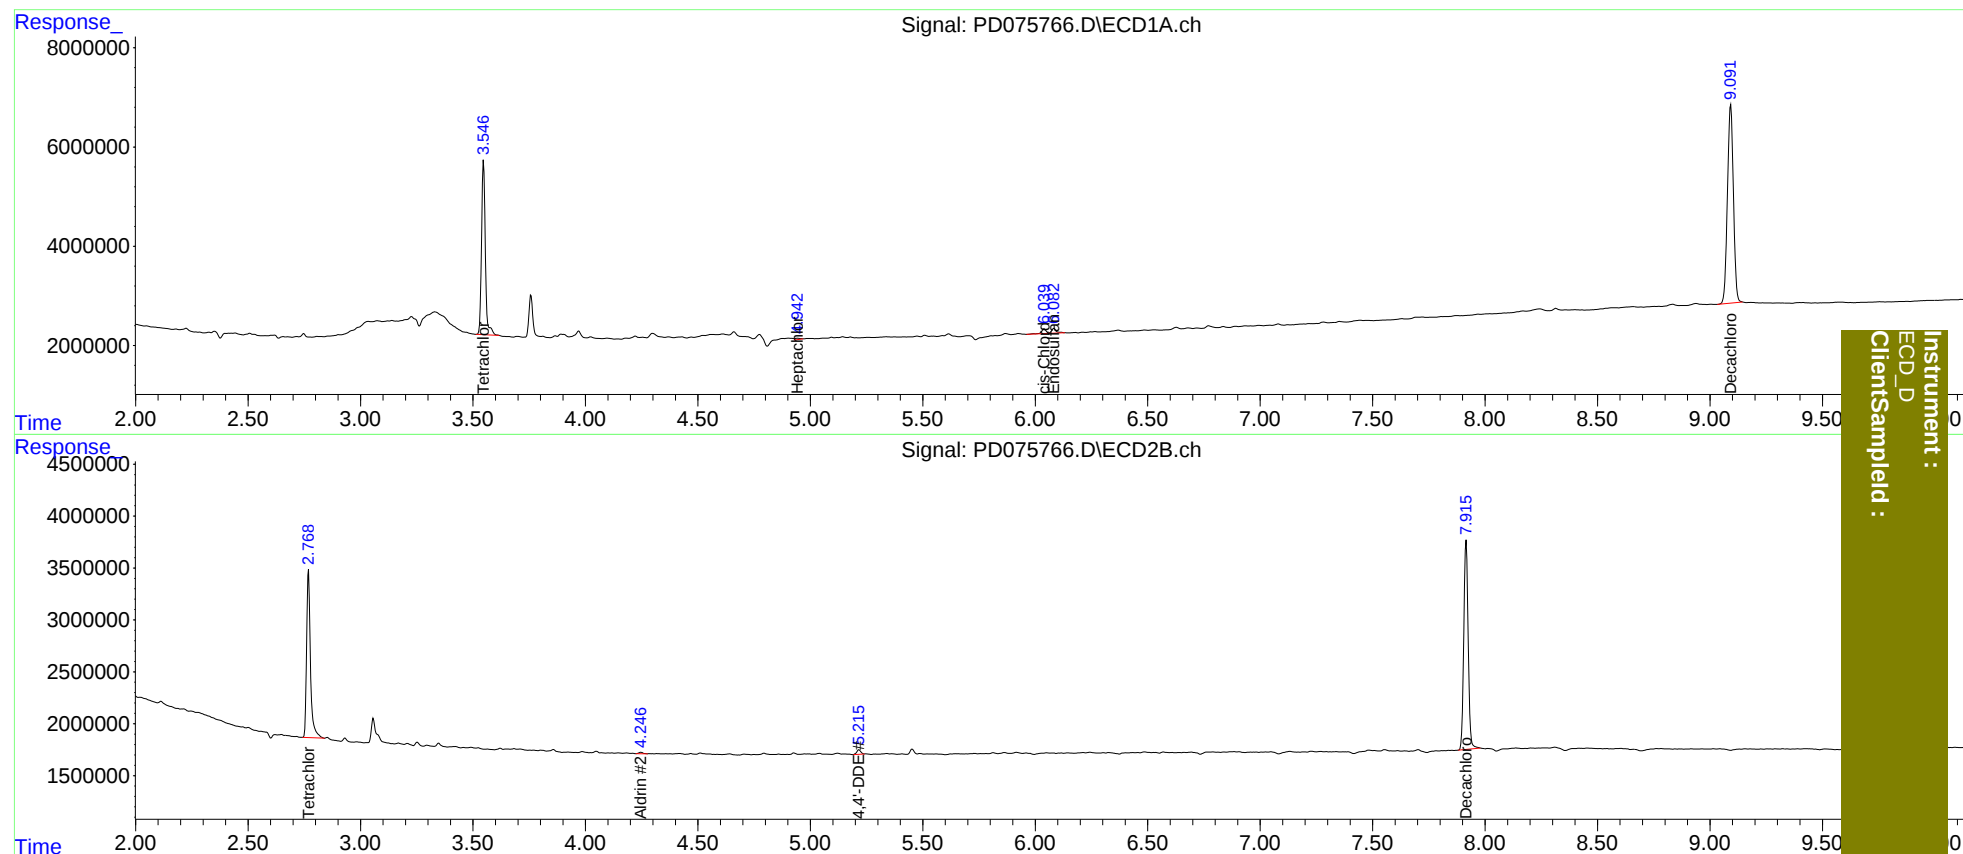


Instrument :
ECD_D
ClientSampled :
0

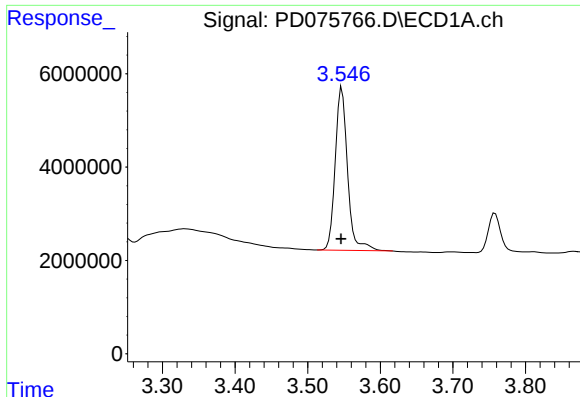

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: 0.001 min
Response: 41177115
Conc: 20.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

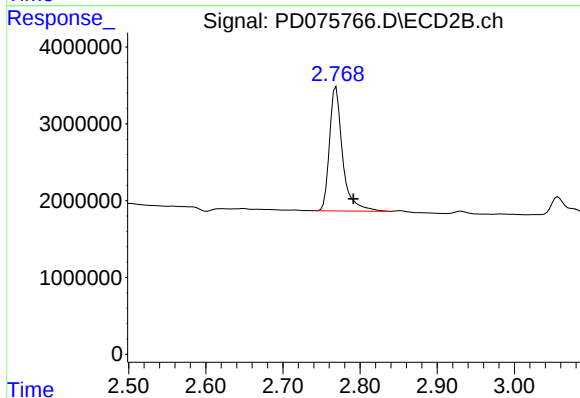


#1 Tetrachloro-m-xylene

R.T.: 2.769 min
Delta R.T.: -0.022 min
Response: 19142783
Conc: 18.88 ng/ml

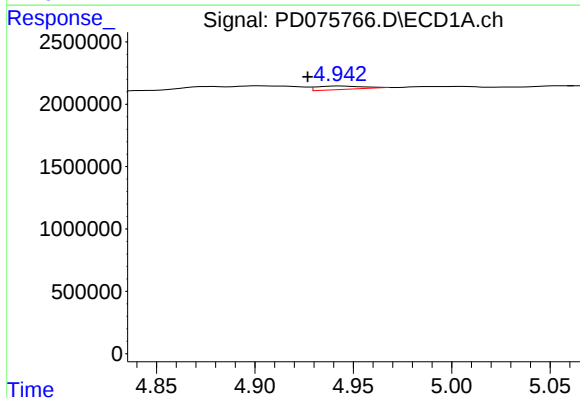


#4 Heptachlor

R.T.: 4.943 min
Delta R.T.: 0.017 min
Response: 545105
Conc: 0.17 ng/ml

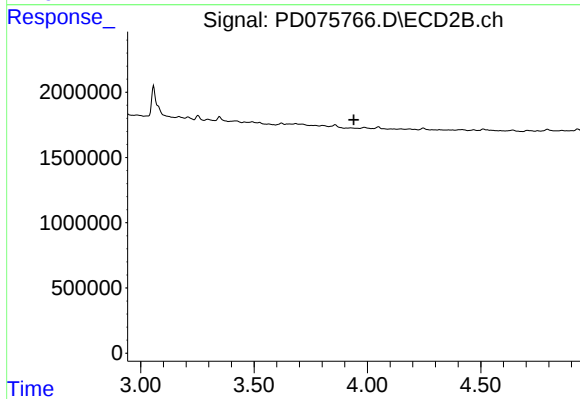

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.941 min
Response: 0
Conc: N.D.

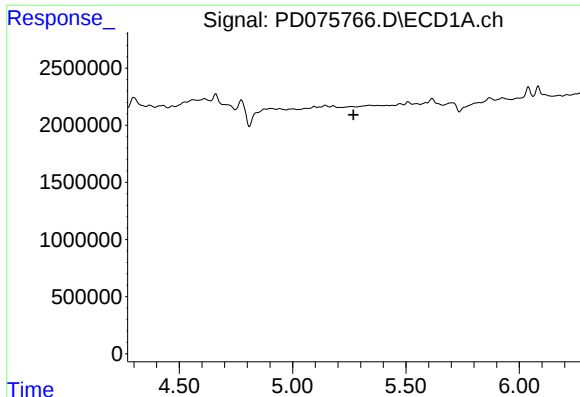

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

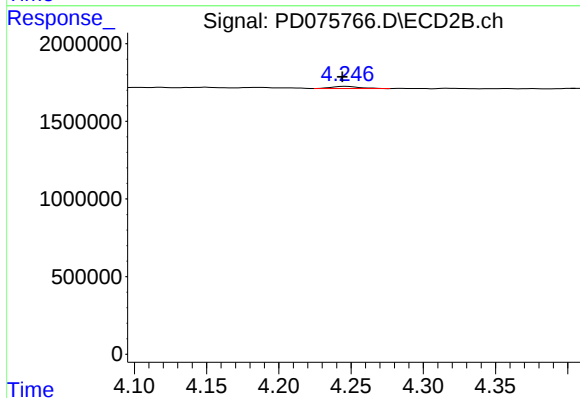


#5 Aldrin

R.T.: 4.247 min
Delta R.T.: 0.003 min
Response: 183099
Conc: 0.13 ng/ml

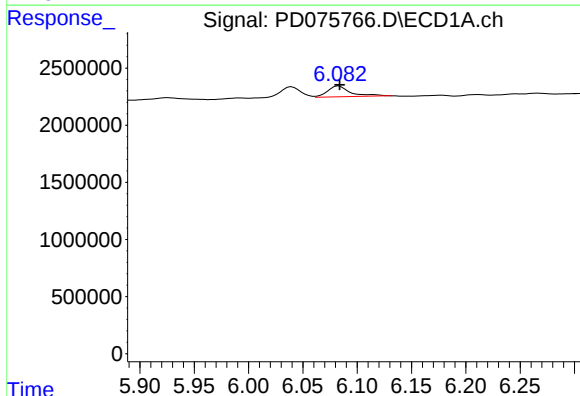


#9 Endosulfan I

R.T.: 6.083 min
Delta R.T.: 0.000 min
Response: 1410868
Conc: 0.53 ng/ml

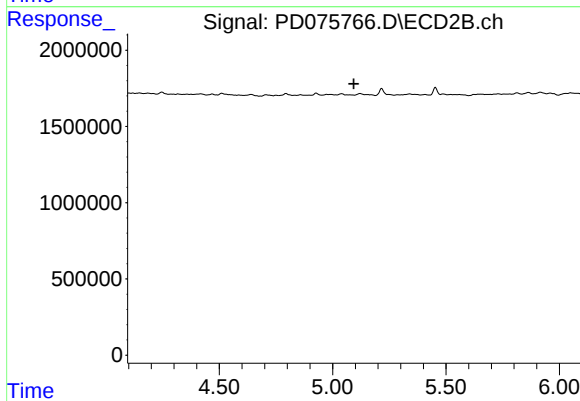

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.093 min
Response: 0
Conc: N.D.

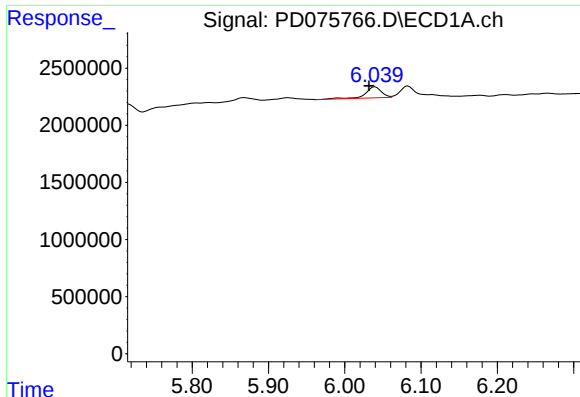

#11 cis-Chlordane


R.T.: 6.040 min
Delta R.T.: 0.008 min
Response: 1387658
Conc: 0.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

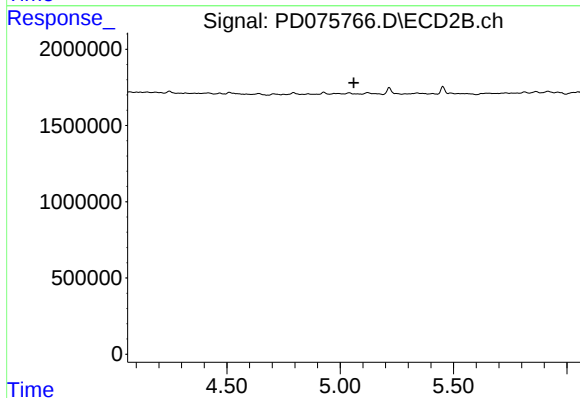


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.060 min
Response: 0
Conc: N.D.

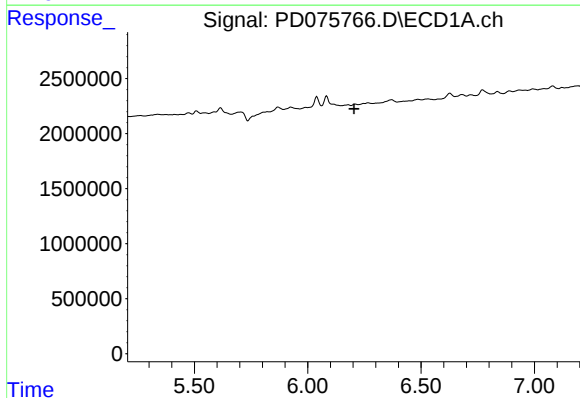


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.204 min
Response: 0
Conc: N.D.

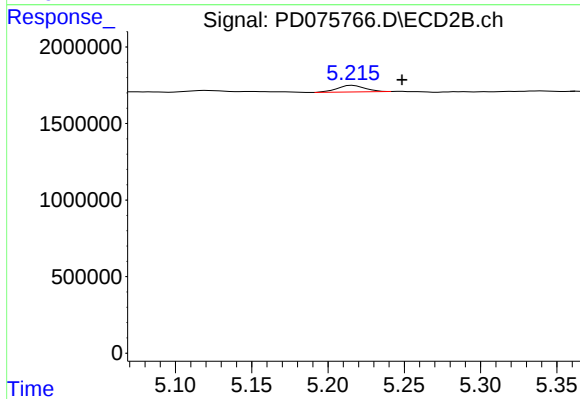

#12 4,4'-DDE


R.T.: 5.216 min
Delta R.T.: -0.032 min
Response: 542005
Conc: 0.48 ng/ml

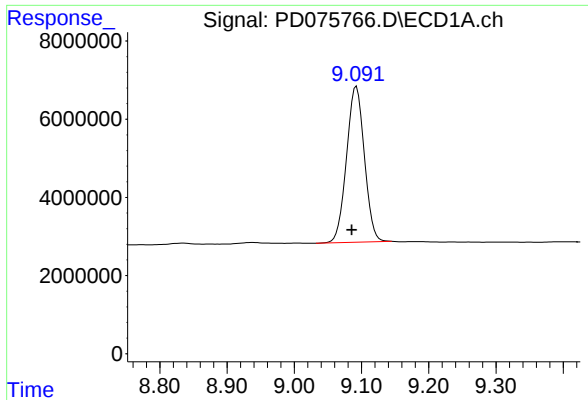

#27 Decachlorobiphenyl

R.T.: 9.092 min
Delta R.T.: 0.007 min
Response: 73576379
Conc: 32.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

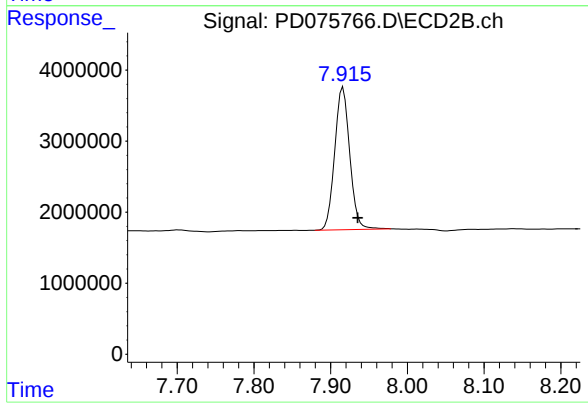

#27 Decachlorobiphenyl

R.T.: 7.916 min
Delta R.T.: -0.019 min
Response: 27343682
Conc: 29.12 ng/ml