

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061223\
 Data File : PD075762.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2023 15:34
 Operator : AR\AJ
 Sample : 03098-02MS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZEP9MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/13/2023
 Supervised By :Ankita Jodhani 06/13/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 22:24:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.769	43189823	20643955	21.605	20.362
27)	SA Decachlor...	9.094	7.917	75468580	30913664	32.905	32.918
Target Compounds							
2)	A alpha-BHC	4.005	3.271	189.6E6	81003618	56.931	54.155
3)	MA gamma-BHC...	4.338	3.601	172.3E6	71631008	55.106	51.603
4)	MA Heptachlor	4.930	3.942	169.3E6	67008385	52.188	48.946
5)	MB Aldrin	5.273	4.222	176.9E6	72039570	54.600	50.976
6)	B beta-BHC	4.535	3.897	71280943	30247723	50.441	44.046m
7)	B delta-BHC	4.782	4.128	169.4E6	70384852	53.409m	48.553
8)	B Heptachlo...	5.700	4.725	154.9E6	63414945	50.670	48.198
9)	A Endosulfan I	6.088	5.095	142.3E6	58483252	53.684	50.641
10)	B trans-Chl...	5.957	4.976	151.1E6	63043331	51.712	49.576
11)	B cis-Chlor...	6.037	5.039	154.2E6	63619254	51.218	48.811
12)	B 4,4'-DDE	6.209	5.229	298.2E6	117.0E6	106.502	102.861
13)	MA Dieldrin	6.364	5.360	329.7E6	135.8E6	110.770	104.207
14)	MA Endrin	6.594	5.636	269.6E6	114.2E6	107.310	99.468
15)	B Endosulfa...	6.814	5.930	266.1E6	112.2E6	103.985	99.850
16)	A 4,4'-DDD	6.728	5.784	235.3E6	92103827	110.877	104.818
17)	MA 4,4'-DDT	7.043	6.035	247.6E6	92577181	120.629	113.782
18)	B Endrin al...	6.944	6.110	187.9E6	78752518	90.890	87.138
19)	B Endosulfa...	7.179	6.333	242.7E6	103.0E6	101.585	98.233
20)	A Methoxychlor	7.519	6.611	633.9E6	219.9E6	508.324	455.544
21)	B Endrin ke...	7.666	6.840	278.9E6	123.2E6	105.355	105.388

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061223\
Data File : PD075762.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2023 15:34
Operator : AR\AJ
Sample : 03098-02MS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 22:24:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

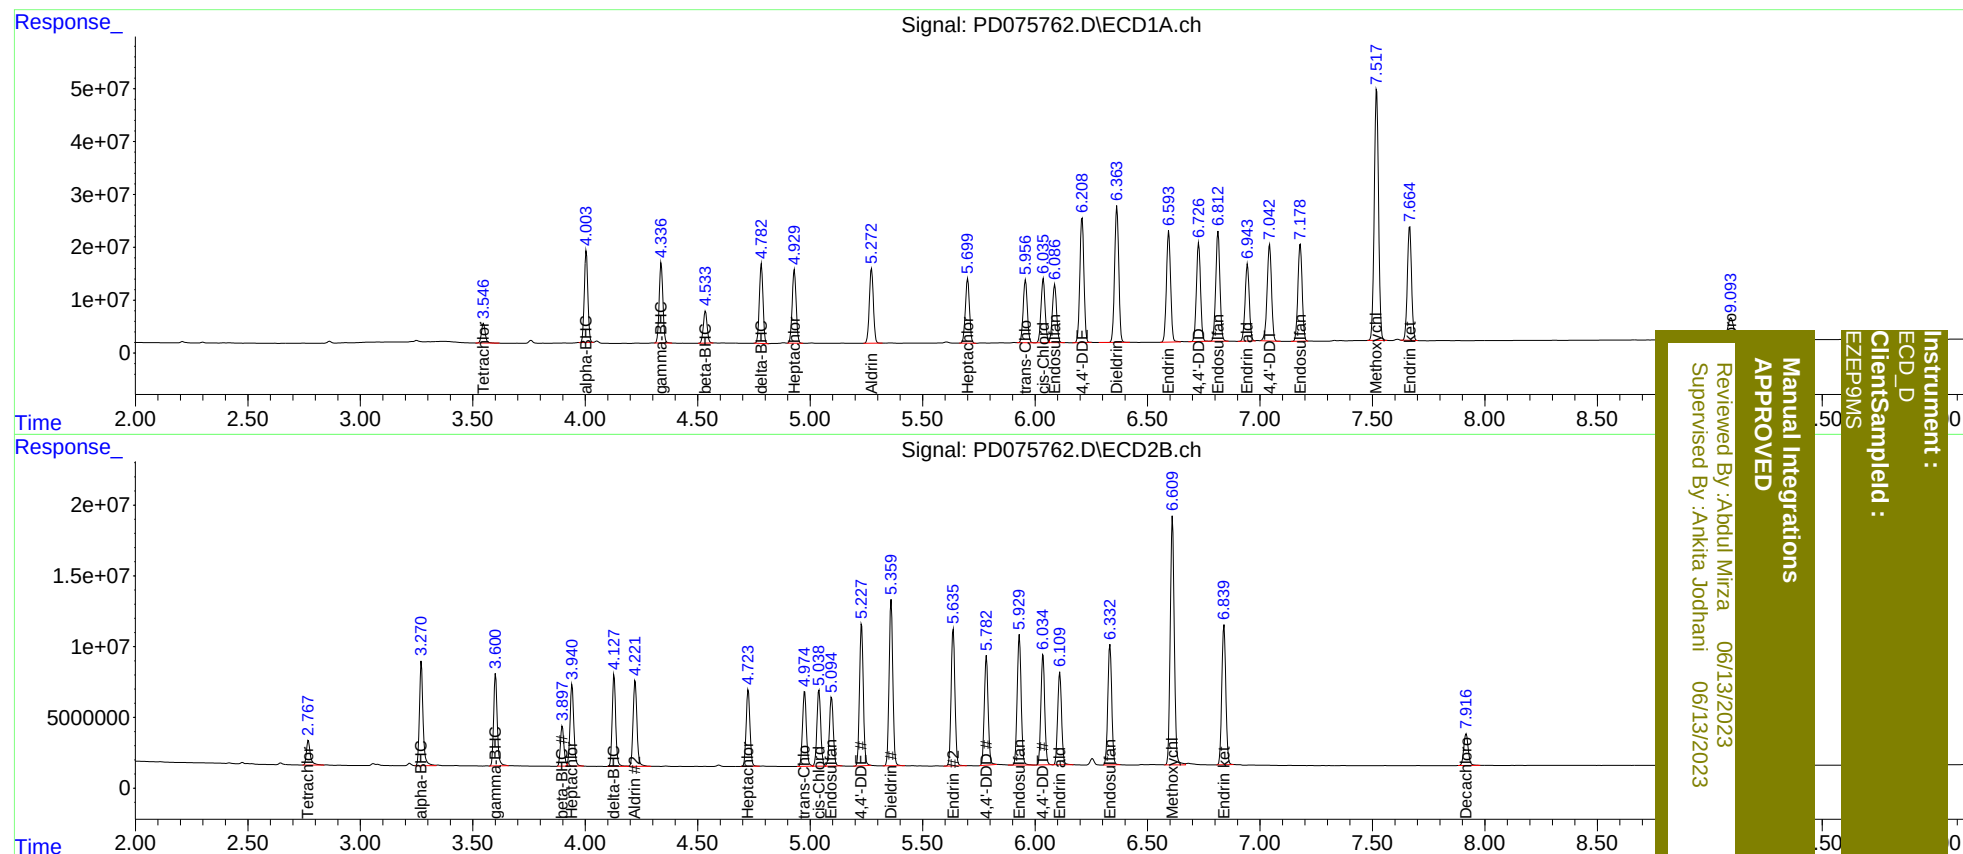

Instrument :
ECD_D
ClientSampled :
EZEP9MS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 06/13/2023
Supervised By: Ankita Jodhani 06/13/2023