

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061223\
 Data File : PD075763.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2023 15:47
 Operator : AR\AJ
 Sample : 03098-03MSD
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZEP9MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/13/2023
 Supervised By : Ankita Jodhani 06/13/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 22:25:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.768	42484627	20415461	21.252	20.136
27)	SA Decachlor...	9.094	7.917	74588299	31248410	32.521	33.275
Target Compounds							
2)	A alpha-BHC	4.004	3.271	187.2E6	80418431	56.208	53.764
3)	MA gamma-BHC...	4.338	3.601	170.2E6	71154357	54.422	51.259
4)	MA Heptachlor	4.929	3.941	167.1E6	66723645	51.534	48.738
5)	MB Aldrin	5.273	4.222	174.8E6	71643462	53.935	50.696
6)	B beta-BHC	4.534	3.896	70008392	30365837	49.540	44.218m
7)	B delta-BHC	4.781	4.128	166.4E6	69627879	52.480m	48.030
8)	B Heptachlo...	5.700	4.724	152.1E6	62833798	49.767	47.756
9)	A Endosulfan I	6.088	5.095	140.1E6	58069842	52.872	50.283
10)	B trans-Chl...	5.957	4.975	149.5E6	62520909	51.148	49.166
11)	B cis-Chlor...	6.036	5.040	151.9E6	63082783	50.456	48.399
12)	B 4,4'-DDE	6.208	5.229	293.6E6	116.0E6	104.859	101.985
13)	MA Dieldrin	6.364	5.360	325.5E6	135.2E6	109.354	103.718
14)	MA Endrin	6.594	5.636	264.3E6	113.8E6	105.213	99.160
15)	B Endosulfa...	6.813	5.931	261.1E6	111.7E6	102.047	99.455
16)	A 4,4'-DDD	6.728	5.784	230.2E6	91526568	108.457	104.161
17)	MA 4,4'-DDT	7.043	6.035	242.9E6	92616521	118.360	113.830
18)	B Endrin al...	6.944	6.110	184.5E6	78219814	89.241	86.548
19)	B Endosulfa...	7.179	6.333	237.9E6	102.9E6	99.578	98.156
20)	A Methoxychlor	7.519	6.611	621.1E6	222.5E6	498.081	460.835
21)	B Endrin ke...	7.666	6.840	273.3E6	123.4E6	103.244	105.486

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061223\
Data File : PD075763.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2023 15:47
Operator : AR\AJ
Sample : 03098-03MSD
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 22:25:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

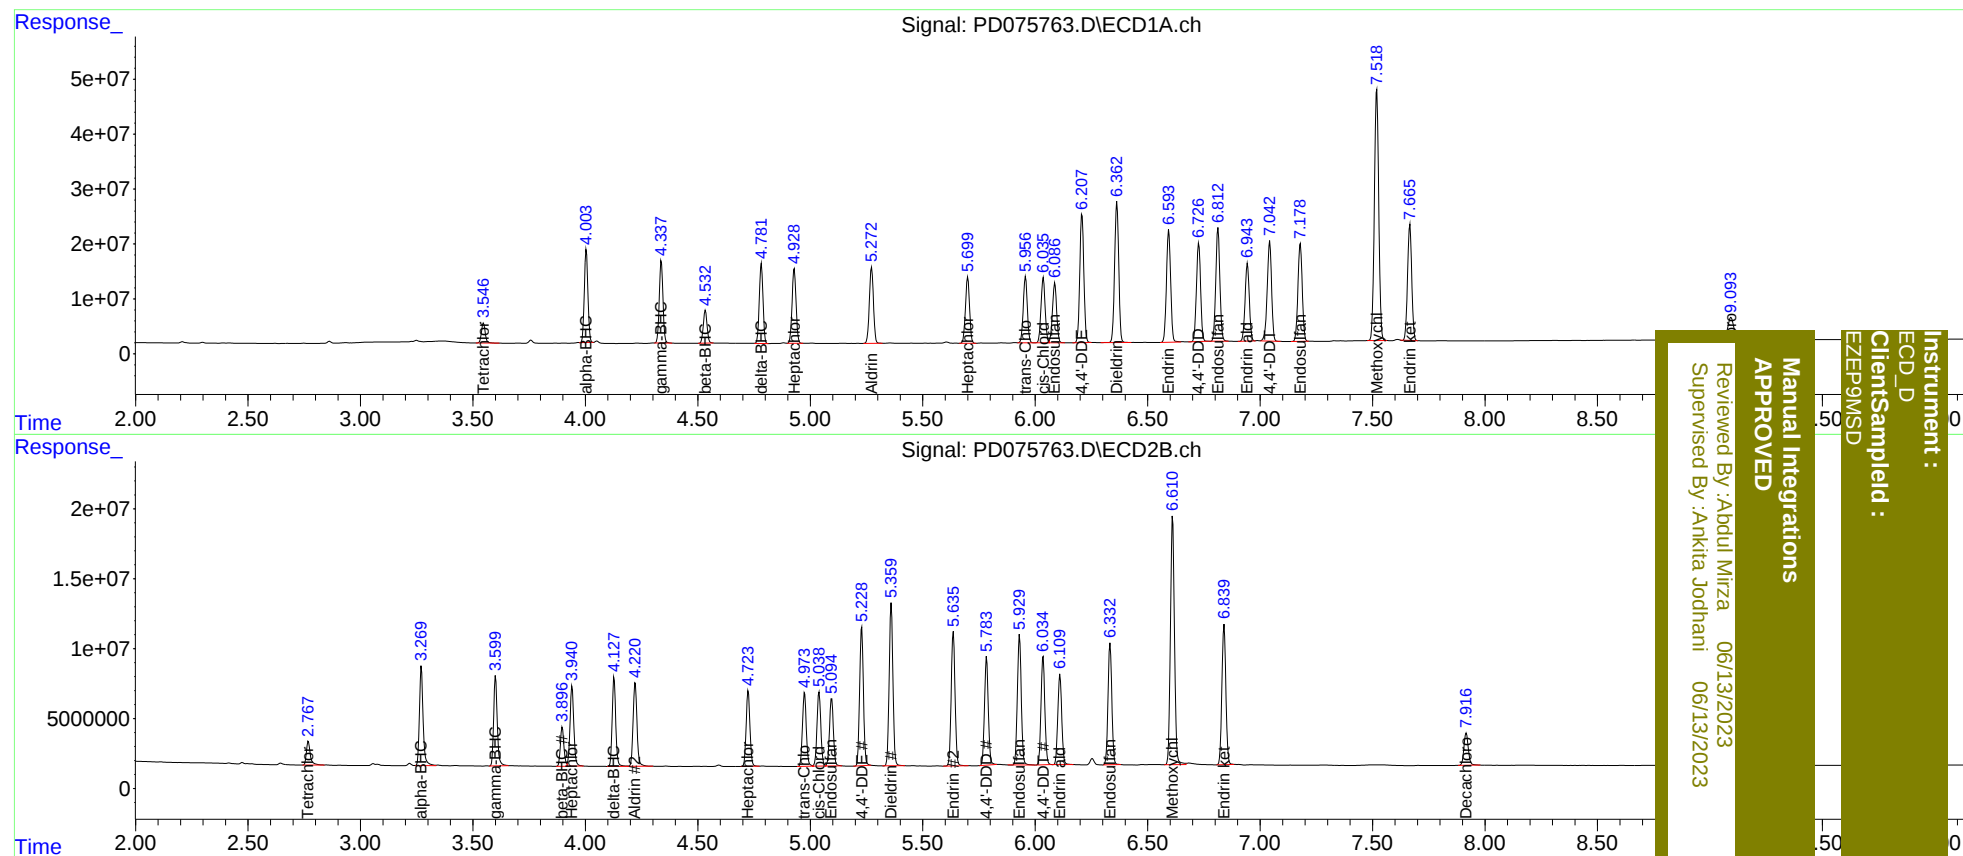

Instrument :
ECD_D
ClientSampled :
EZEP9MSD
Manual Integrations
APPROVED
Reviewed By: Abdul Miza 06/13/2023
Supervised By: Ankita Jodhani 06/13/2023