

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061224\
 Data File : PD083671.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jun 2024 12:07
 Operator : AR\AJ
 Sample : PIBLK184
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 01:25:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.561	2.771	24234561	107.8E6	18.566	19.778
2) SA Decachlor...	9.117	7.898	48293889	140.9E6	24.836	23.209
Target Compounds						
7) B delta-BHC	4.790	0.000	1087325	0	0.414	N.D. #
8) B Heptachlo...	5.711	0.000	2182368	0	1.057	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061224\
Data File : PD083671.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jun 2024 12:07
Operator : AR\AJ
Sample : PIBLK184
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 01:25:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

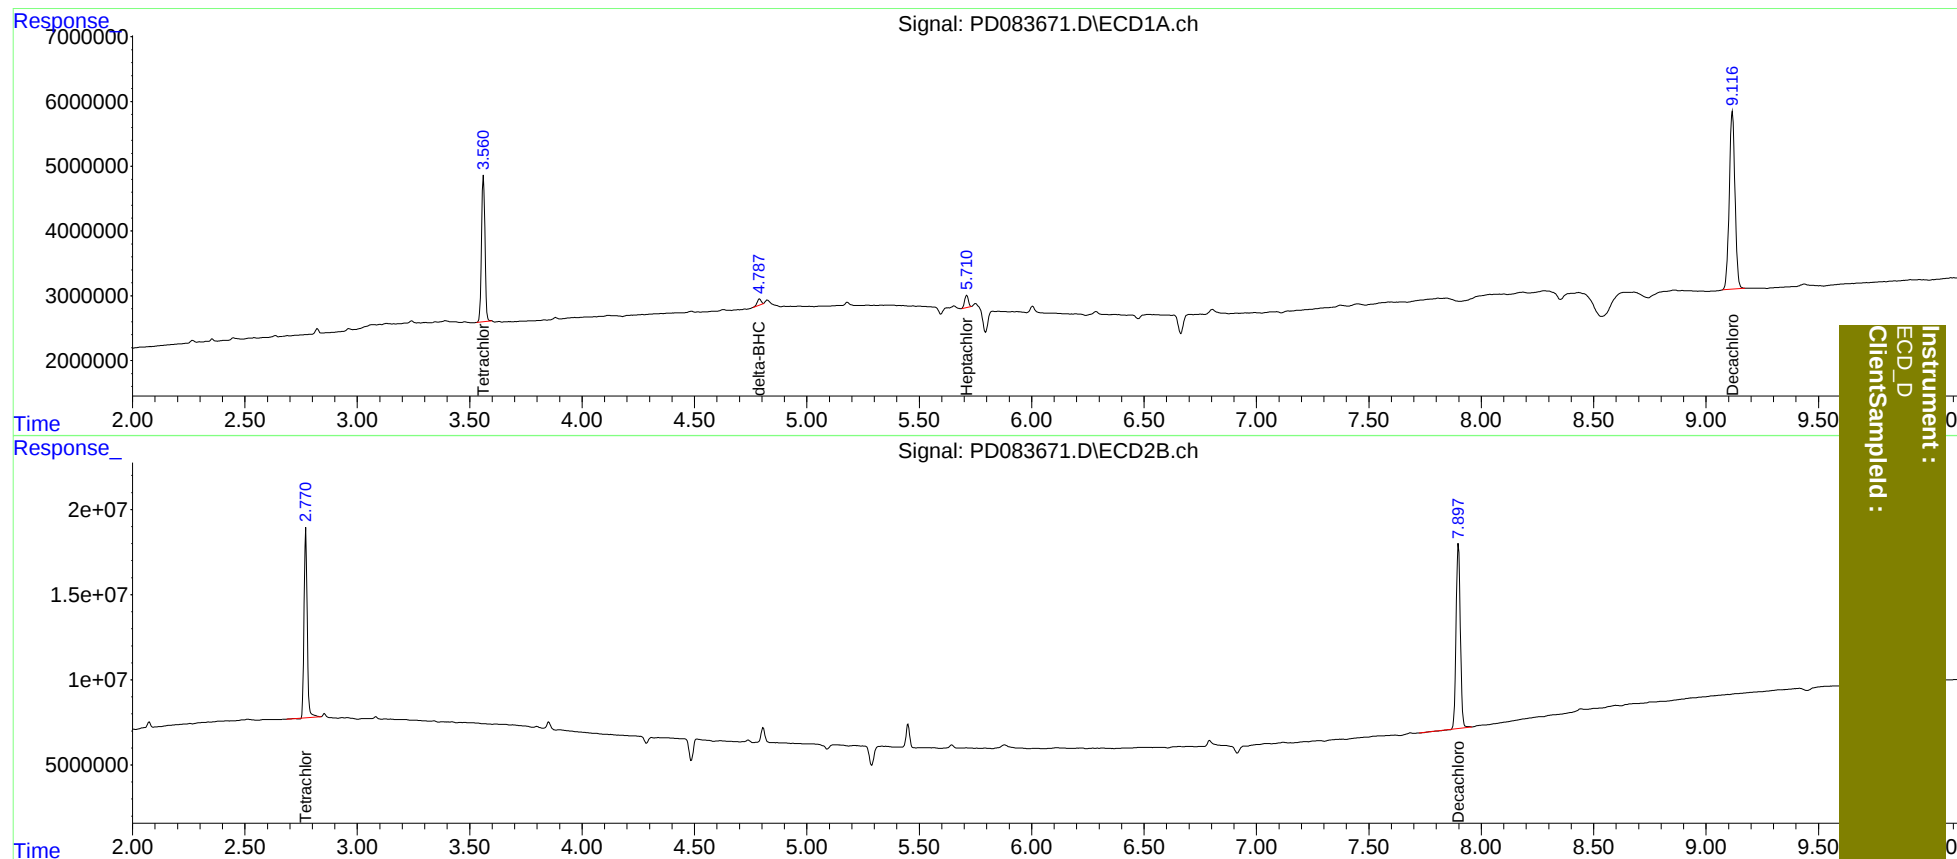


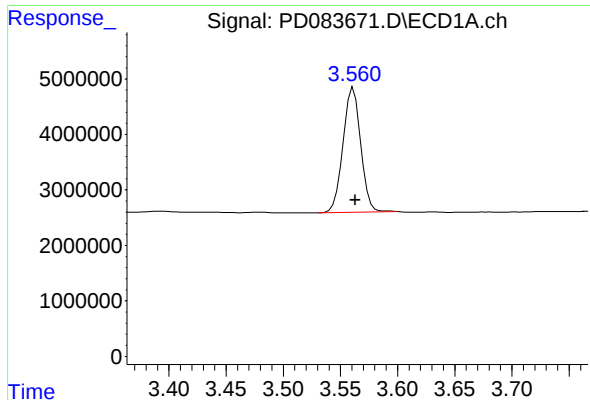

#1 Tetrachloro-m-xylene


R.T.: 3.561 min
Delta R.T.: -0.002 min
Response: 24234561
Conc: 18.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

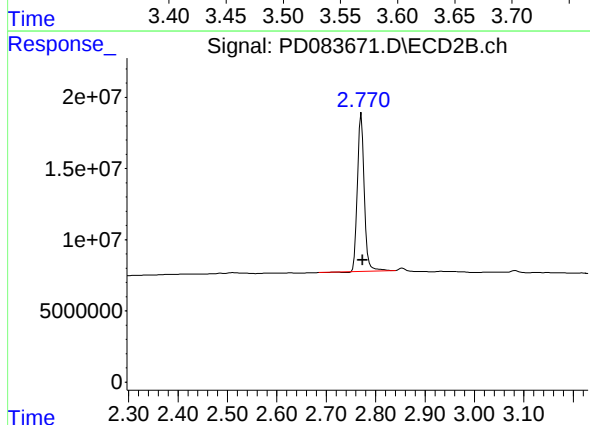


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: -0.003 min
Response: 107809217
Conc: 19.78 ng/ml

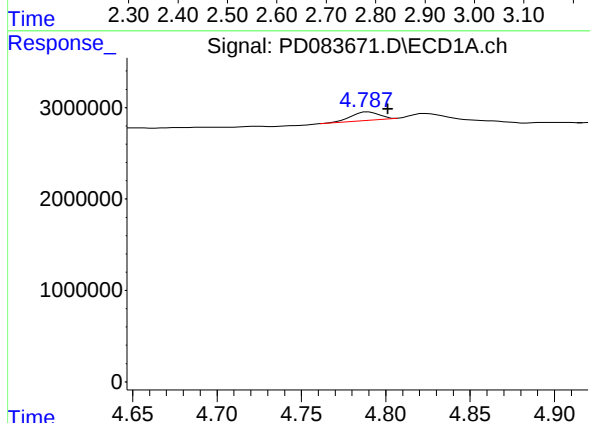


#7 delta-BHC

R.T.: 4.790 min
Delta R.T.: -0.012 min
Response: 1087325
Conc: 0.41 ng/ml

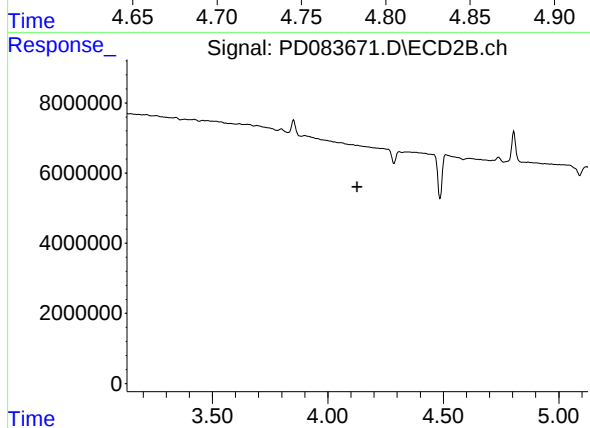

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.128 min
Response: 0
Conc: N.D.

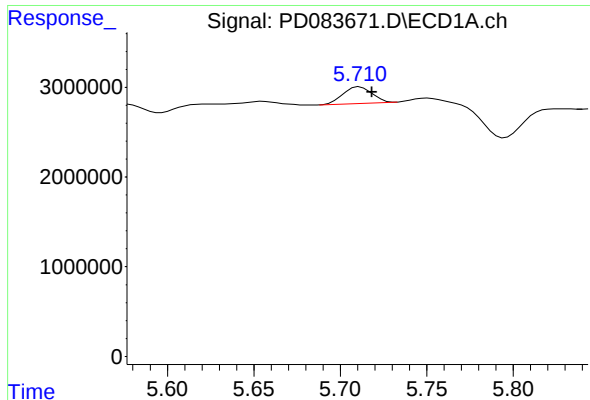

#8 Heptachlor epoxide


R.T.: 5.711 min
Delta R.T.: -0.007 min
Response: 2182368
Conc: 1.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

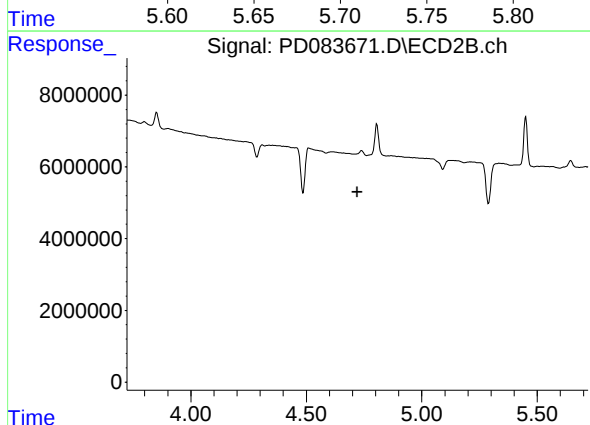


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.721 min
Response: 0
Conc: N.D.

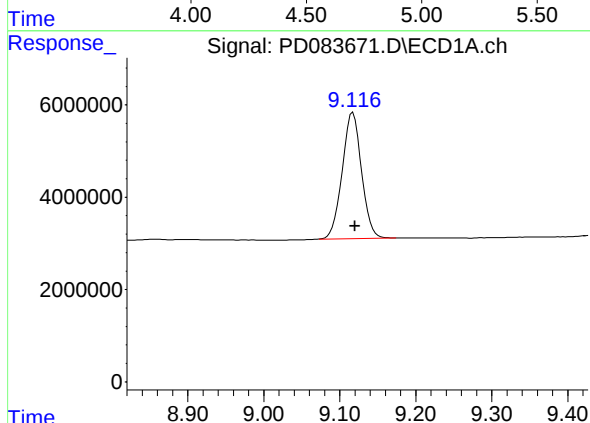

#27 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: -0.003 min
Response: 48293889
Conc: 24.84 ng/ml

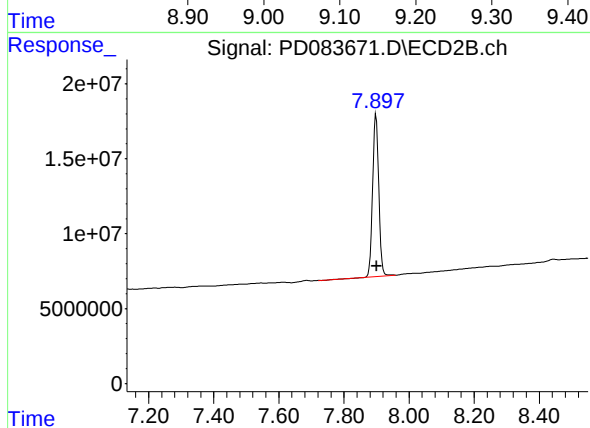

#27 Decachlorobiphenyl

R.T.: 7.898 min
Delta R.T.: -0.002 min
Response: 140928935
Conc: 23.21 ng/ml