

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061321\
 Data File : PD063787.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2021 10:44
 Operator : AR\AJ
 Sample : TOXAPH201
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 02:09:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061321CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 14 02:09:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.970	14890299	156.4E6	10.364	10.819
27)	SA Decachlor...	8.194	9.025	33129986	271.3E6	20.947	21.515
Target Compounds							
22)	Toxaphene-1	5.693	6.353	12245171	95692495	1003.558	1158.034
23)	Toxaphene-2	5.854	6.643	12277363	105.7E6	998.682	1023.352
24)	Toxaphene-3	6.177	7.050	14295232	138.1E6	1028.881	1007.674
25)	Toxaphene-4	6.296	7.127	31150139	435.6E6	976.009	1095.810
26)	Toxaphene-5	7.029	7.626	36305306	225.3E6	1004.835	1396.814 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061321\
Data File : PD063787.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2021 10:44
Operator : AR\AJ
Sample : TOXAPH201
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 02:09:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061321CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 14 02:09:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

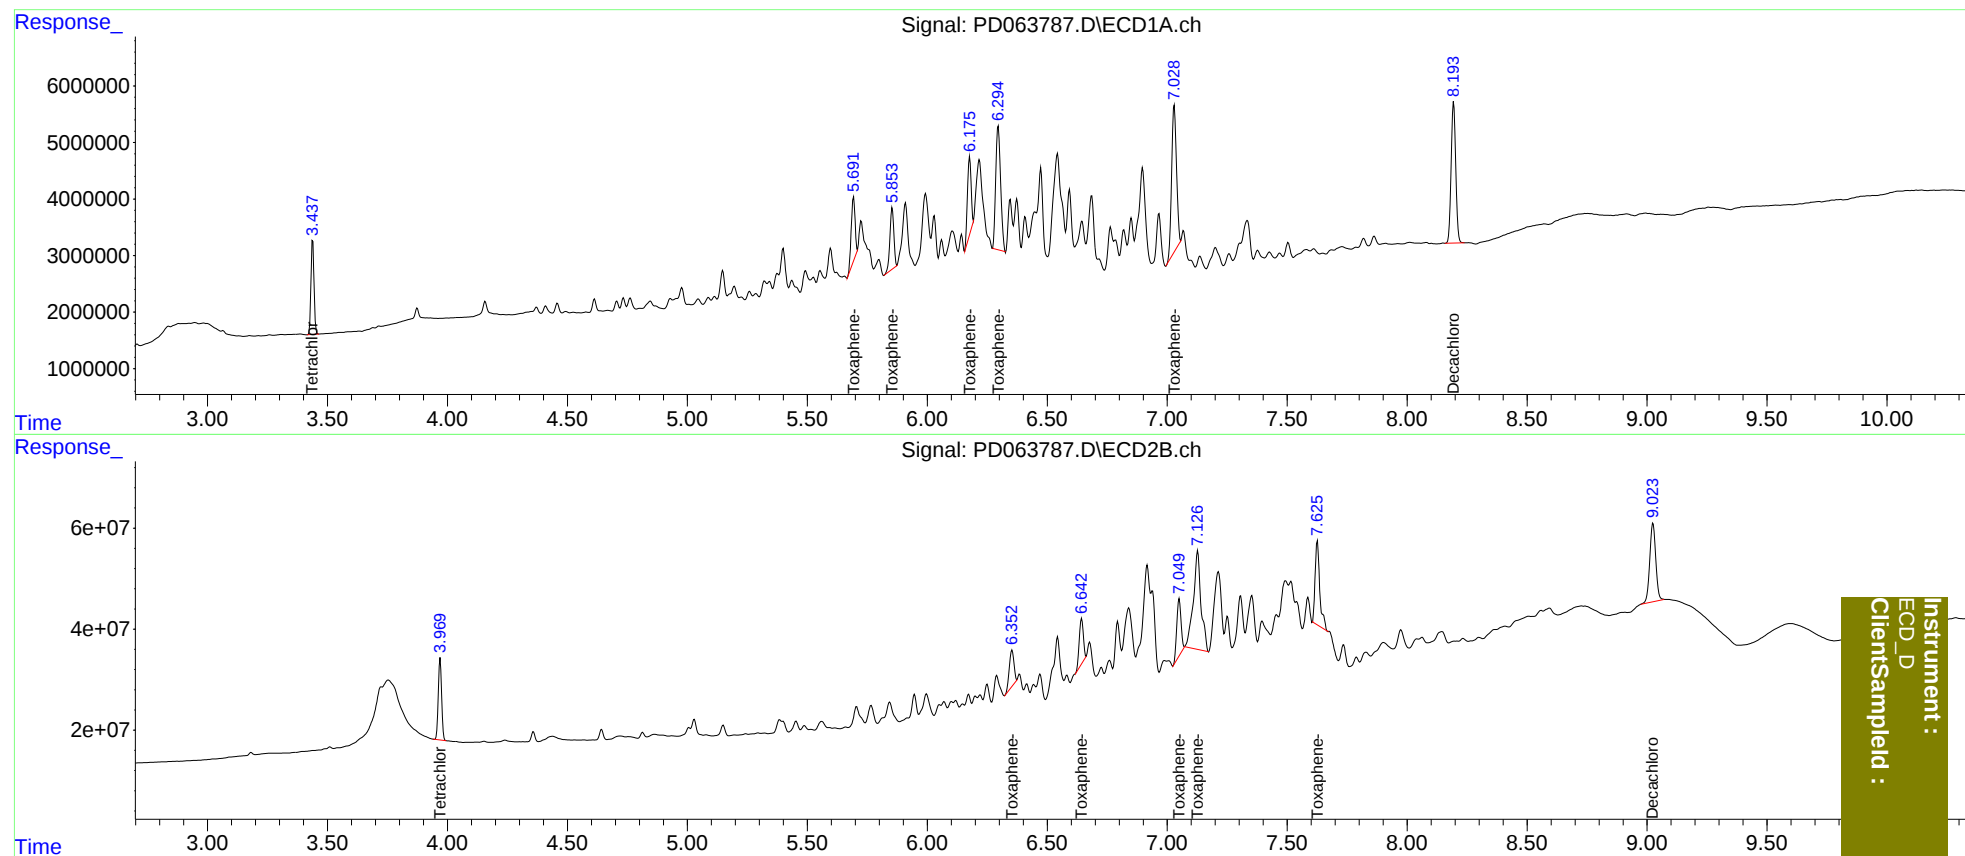

Instrument :
ECD_D
ClientSampled :