

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061321\
 Data File : PD063793.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2021 12:07
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 02:30:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061321CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 14 02:19:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.970	16265374	170.9E6	10.193	10.698
27)	SA Decachlor...	8.194	9.024	35575536	274.1E6	20.732	20.433
Target Compounds							
2)	A alpha-BHC	3.874	4.358	24989738	279.9E6	9.985	10.874
3)	MA gamma-BHC...	4.157	4.643	24998383	262.5E6	10.365	10.979
4)	MA Heptachlor	4.458	5.150	24271938	270.9E6	10.302	11.107
9)	A Endosulfan I	5.488	6.196	20503581	231.3E6	10.423	11.225
13)	MA Dieldrin	5.731	6.452	44070802	467.3E6	19.848	21.762
14)	MA Endrin	5.989	6.671	39172254	394.3E6	20.175	21.792
16)	A 4,4'-DDD	6.115	6.794	34791508	370.7E6	19.743	21.525
17)	MA 4,4'-DDT	6.356	7.092	34256540	344.0E6	18.915	20.612
20)	A Methoxychlor	6.902	7.550	100.4E6	798.9E6	105.464	108.585

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061321\
Data File : PD063793.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2021 12:07
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 02:30:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061321CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 14 02:19:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

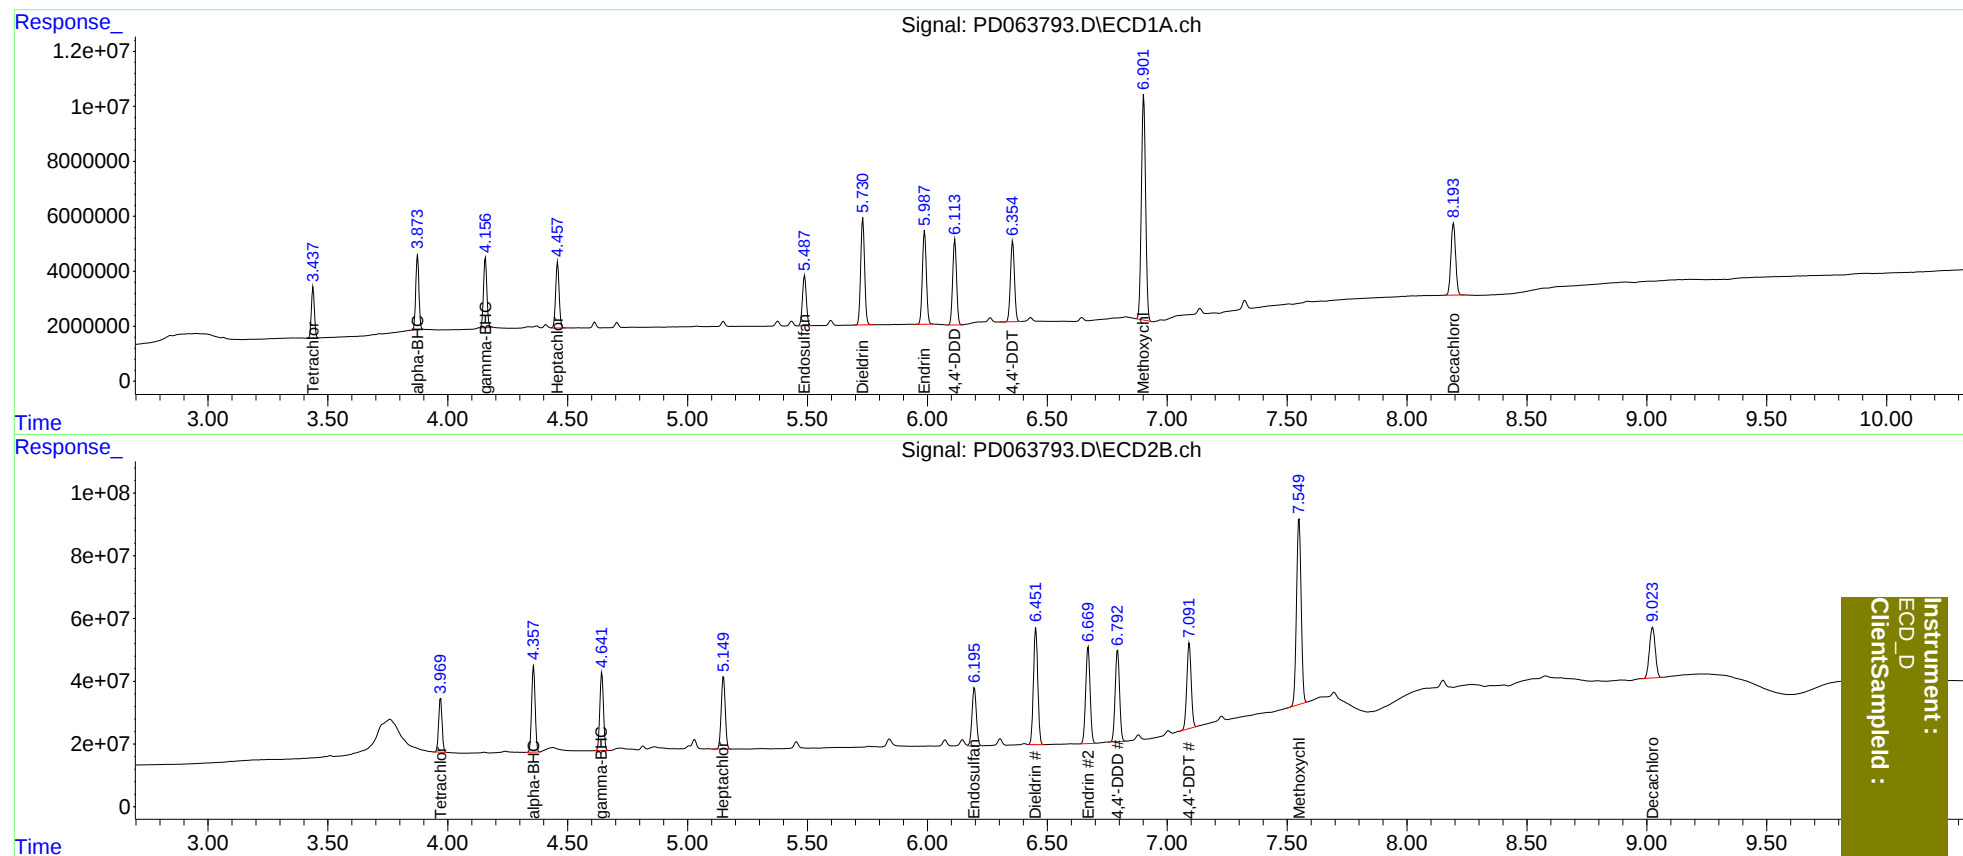


Instrument :
ECD_D
ClientSampled :

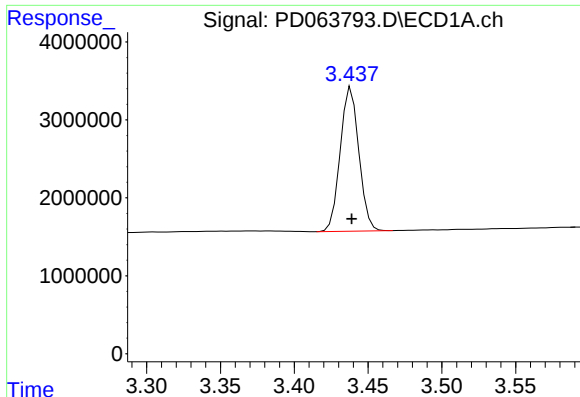

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 16265374
Conc: 10.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

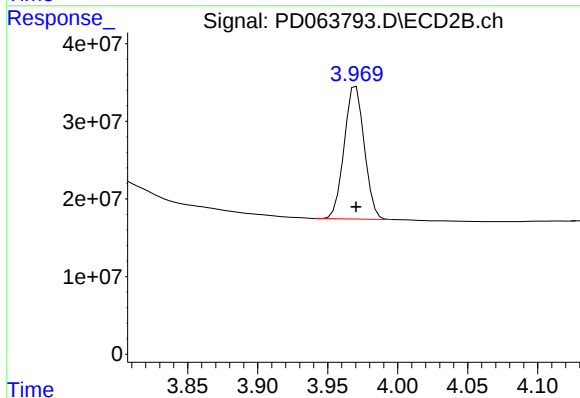


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 170919971
Conc: 10.70 ng/ml

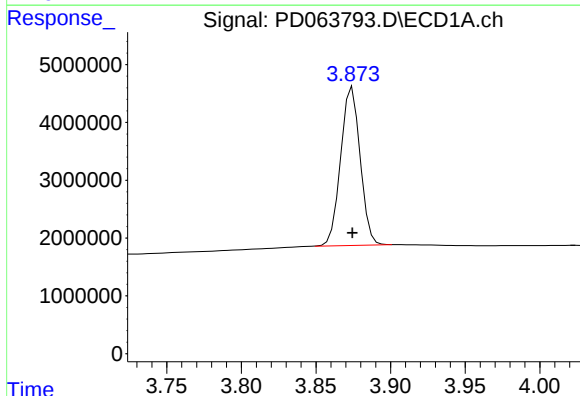


#2 alpha-BHC

R.T.: 3.874 min
Delta R.T.: 0.000 min
Response: 24989738
Conc: 9.99 ng/ml

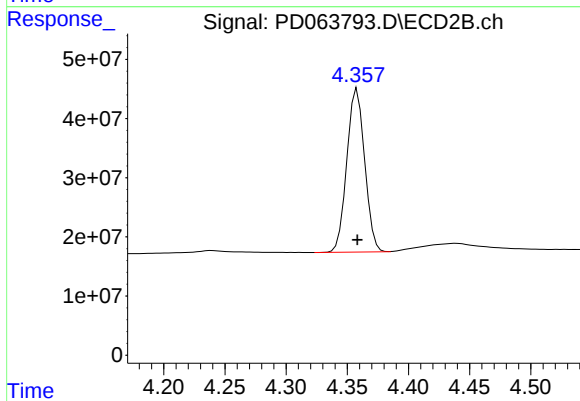

#2 alpha-BHC


R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 279935566
Conc: 10.87 ng/ml

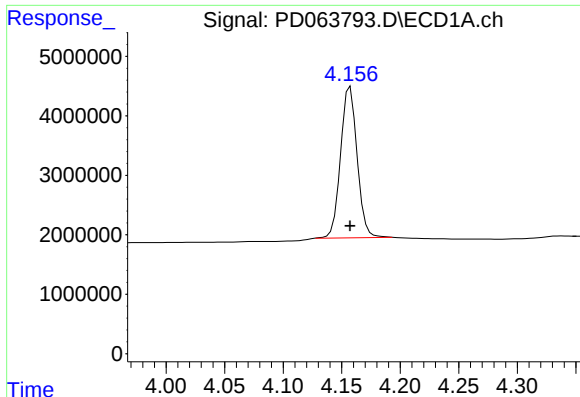

#3 gamma-BHC (Lindane)


R.T.: 4.157 min
Delta R.T.: 0.000 min
Response: 24998383
Conc: 10.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

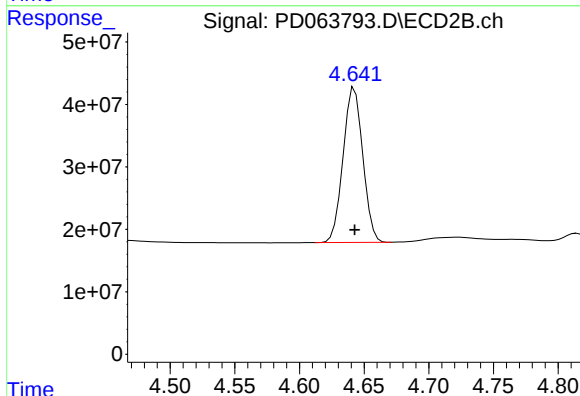


#3 gamma-BHC (Lindane)

R.T.: 4.643 min
Delta R.T.: 0.000 min
Response: 262485963
Conc: 10.98 ng/ml

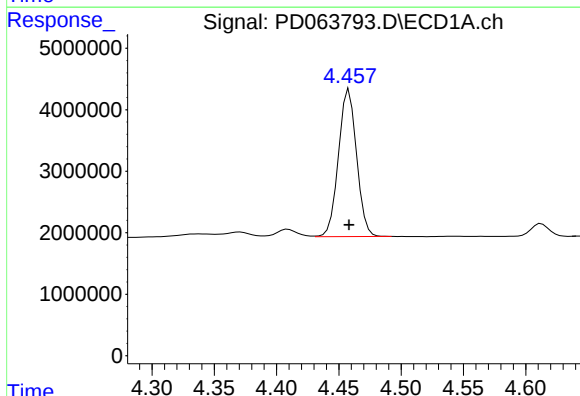


#4 Heptachlor

R.T.: 4.458 min
Delta R.T.: 0.000 min
Response: 24271938
Conc: 10.30 ng/ml

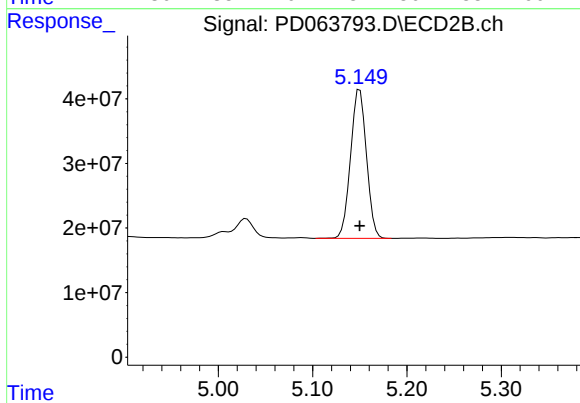

#4 Heptachlor


R.T.: 5.150 min
Delta R.T.: 0.000 min
Response: 270917955
Conc: 11.11 ng/ml

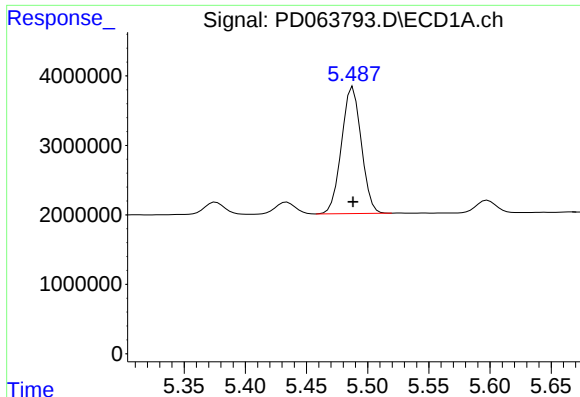

#9 Endosulfan I


R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 20503581
Conc: 10.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

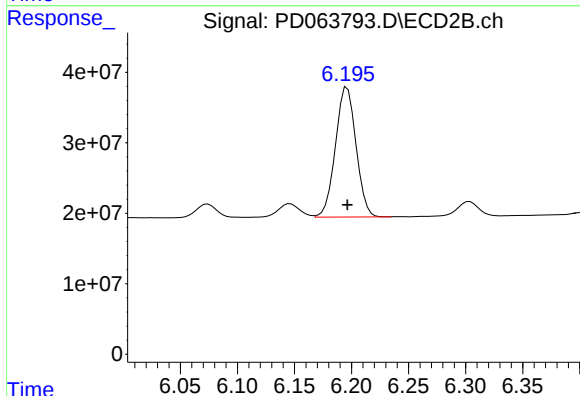


#9 Endosulfan I

R.T.: 6.196 min
Delta R.T.: 0.000 min
Response: 231260082
Conc: 11.22 ng/ml

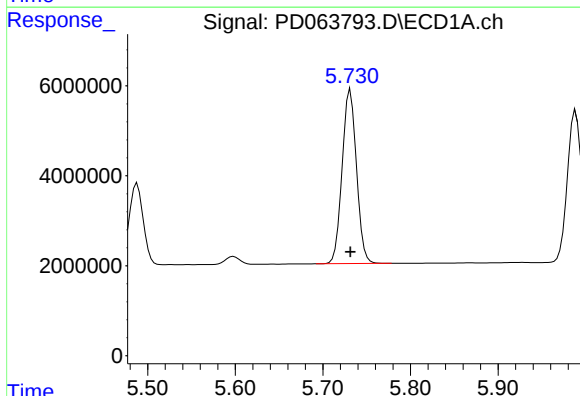


#13 Dieldrin

R.T.: 5.731 min
Delta R.T.: 0.000 min
Response: 44070802
Conc: 19.85 ng/ml

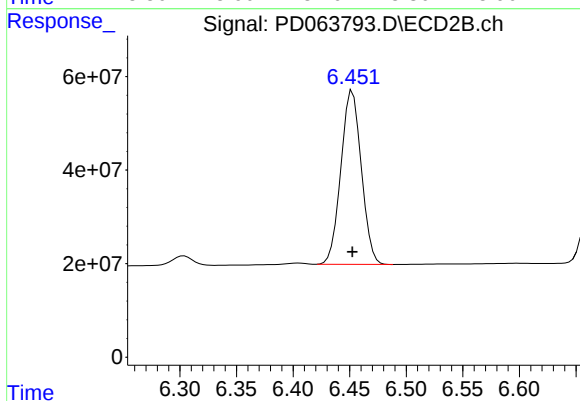

#13 Dieldrin


R.T.: 6.452 min
Delta R.T.: 0.000 min
Response: 467271897
Conc: 21.76 ng/ml

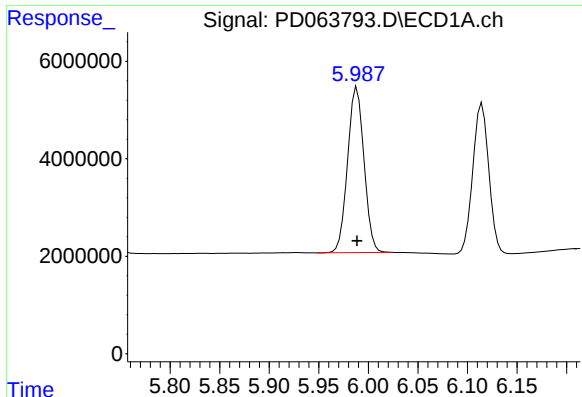

#14 Endrin


R.T.: 5.989 min
Delta R.T.: 0.000 min
Response: 39172254
Conc: 20.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

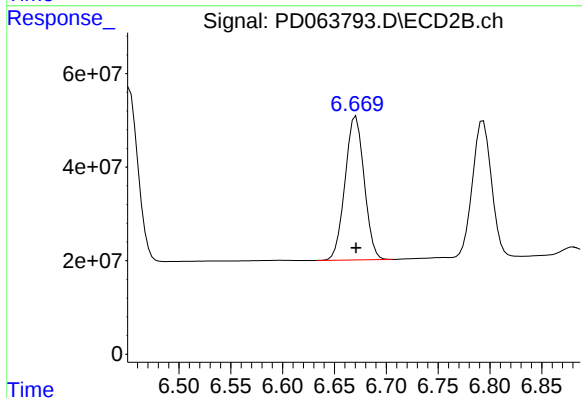


#14 Endrin

R.T.: 6.671 min
Delta R.T.: 0.000 min
Response: 394255799
Conc: 21.79 ng/ml

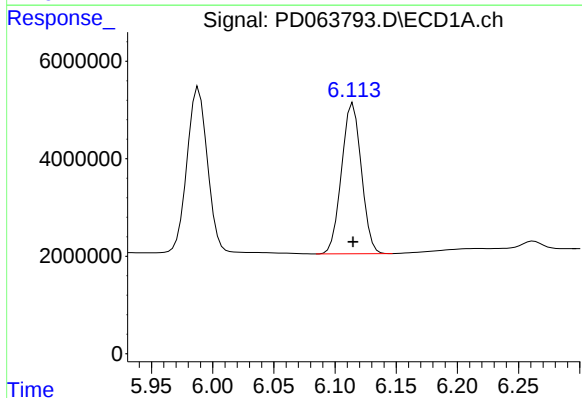


#16 4,4'-DDD

R.T.: 6.115 min
Delta R.T.: 0.000 min
Response: 34791508
Conc: 19.74 ng/ml

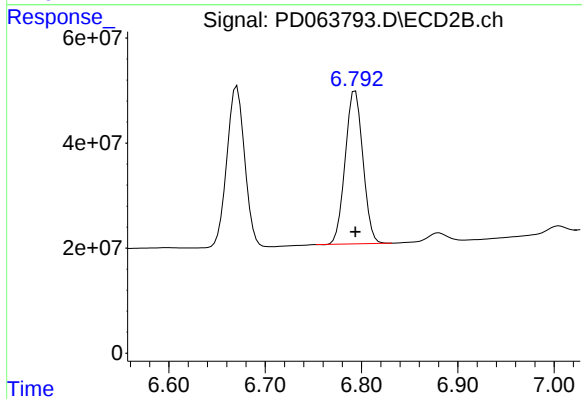

#16 4,4'-DDD


R.T.: 6.794 min
Delta R.T.: 0.000 min
Response: 370728562
Conc: 21.52 ng/ml

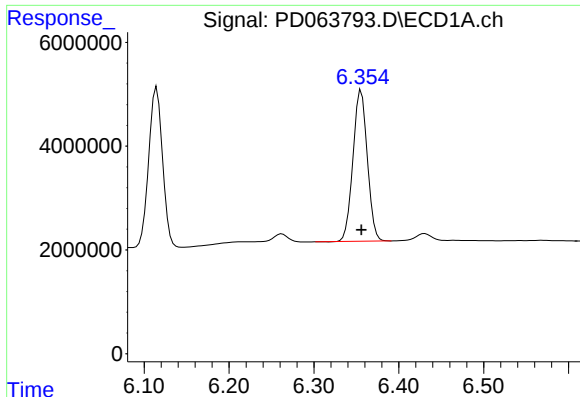

#17 4,4'-DDT


R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 34256540
Conc: 18.91 ng/ml

Instrument :
ECD_D
ClientSampleId :

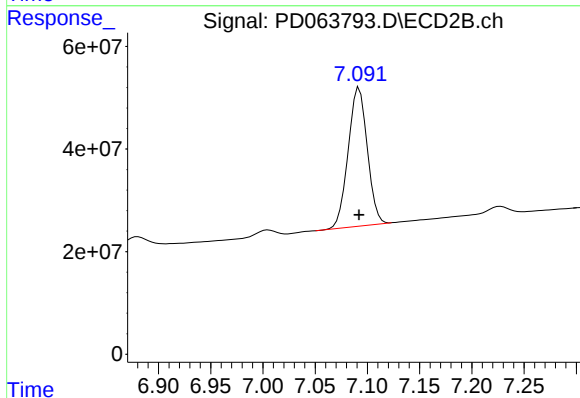


#17 4,4'-DDT

R.T.: 7.092 min
Delta R.T.: 0.000 min
Response: 344003809
Conc: 20.61 ng/ml

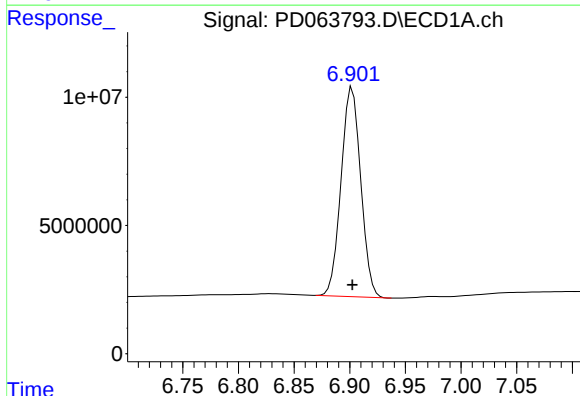


#20 Methoxychlor

R.T.: 6.902 min
Delta R.T.: 0.000 min
Response: 100430034
Conc: 105.46 ng/ml

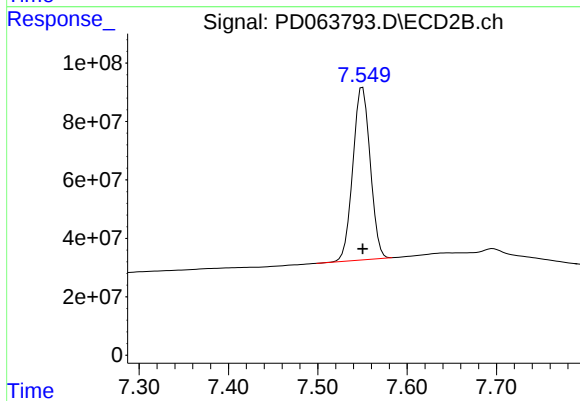

#20 Methoxychlor


R.T.: 7.550 min
Delta R.T.: 0.000 min
Response: 798946464
Conc: 108.58 ng/ml

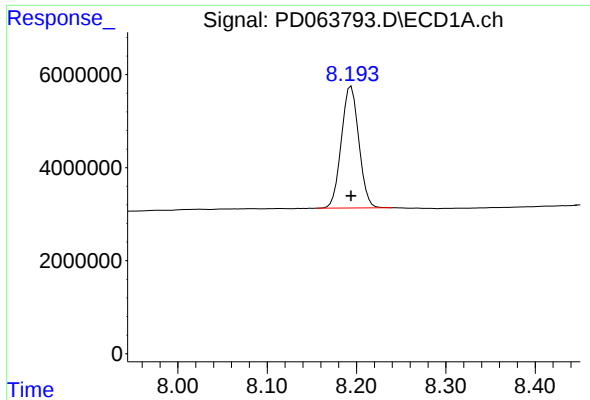

#27 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 35575536
Conc: 20.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

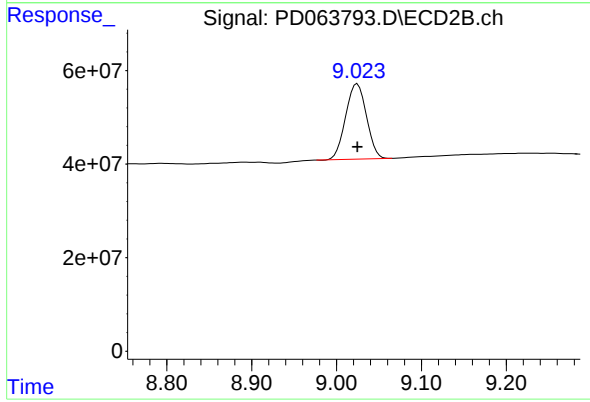

#27 Decachlorobiphenyl

R.T.: 9.024 min
Delta R.T.: 0.000 min
Response: 274073712
Conc: 20.43 ng/ml