

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061322\
 Data File : PD070262.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2022 16:57
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 06:39:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061322.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 14 06:34:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.402	4.124	29793589	270.1E6	22.085	23.499
28)	SA Decachlor...	8.134	9.282	32048478	153.3E6	22.701	22.783
Target Compounds							
9)	A Endosulfan I	5.435	6.387	17321253	139.7E6	10.663	11.710
10)	B gamma-Chl...	5.323	6.263	18472756	151.6E6	10.406	11.599
12)	B 4,4'-DDE	5.547	6.488	35063812	278.9E6	21.143	22.790
13)	MA Dieldrin	5.677	6.645	37916831	289.1E6	21.667	23.253
19)	B Endosulfa...	6.590	7.419	30810270	205.9E6	20.278	21.441
20)	A Methoxychlor	6.853	7.735	83677820	499.4E6	108.238	101.730
21)	B Endrin ke...	7.081	7.892	36302902	225.0E6	21.184	23.047



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061322\
Data File : PD070262.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2022 16:57
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 06:39:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061322.M
Quant Title : GC Extractables
QLast Update : Tue Jun 14 06:34:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

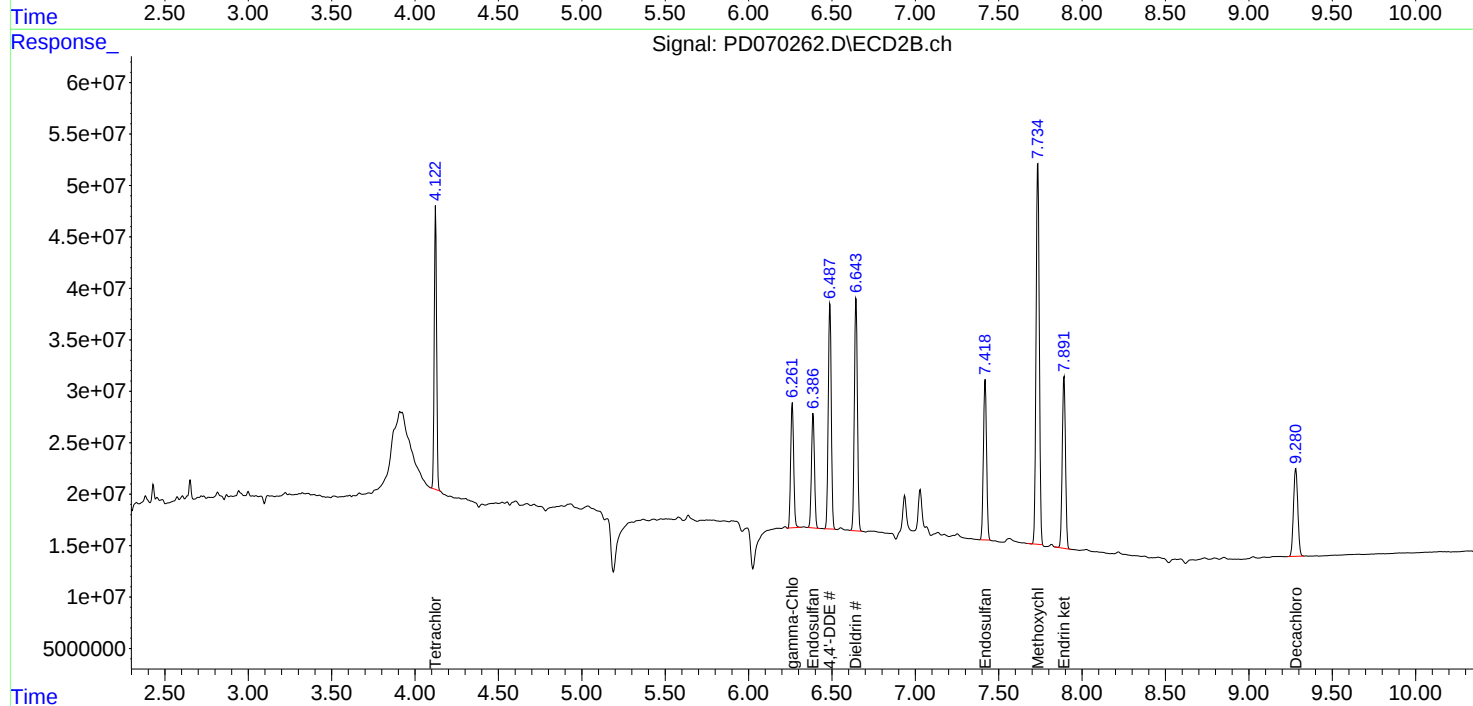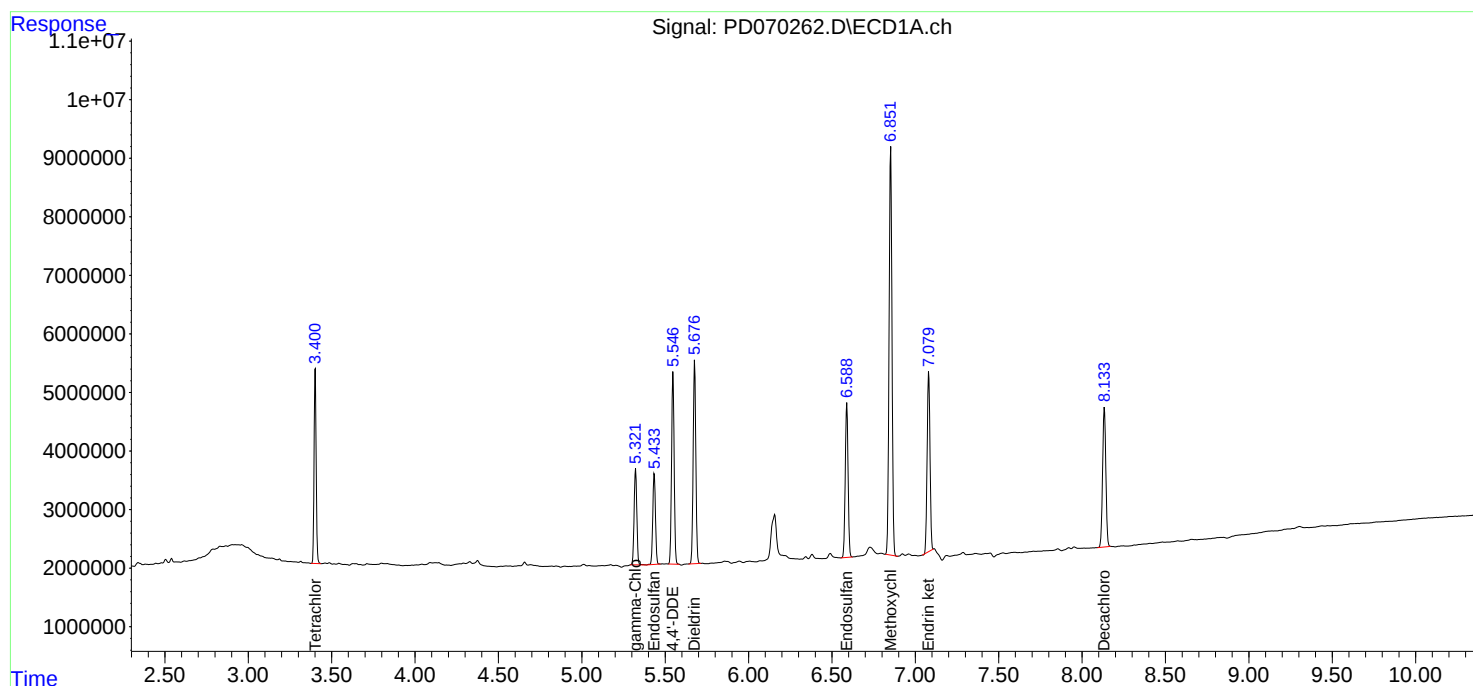


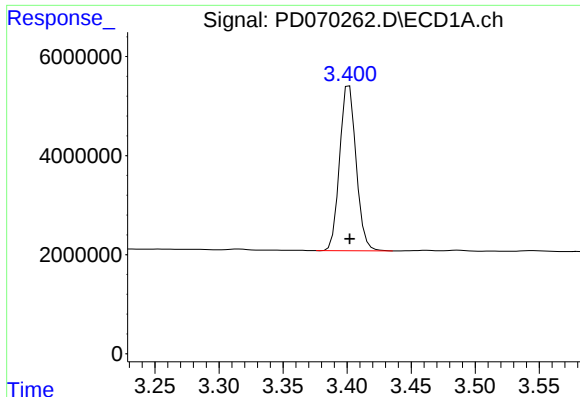

#1 Tetrachloro-m-xylene


R.T.: 3.402 min
Delta R.T.: 0.000 min
Response: 29793589
Conc: 22.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

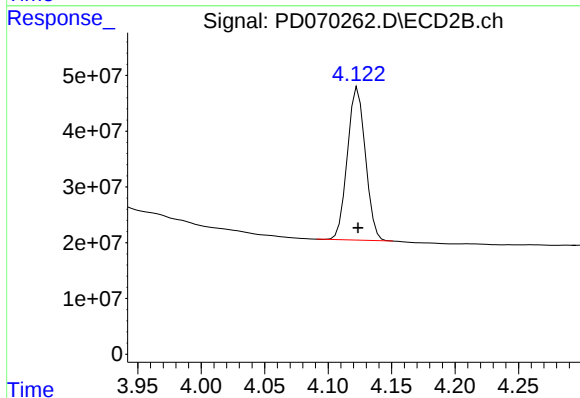


#1 Tetrachloro-m-xylene

R.T.: 4.124 min
Delta R.T.: 0.000 min
Response: 270112499
Conc: 23.50 ng/ml

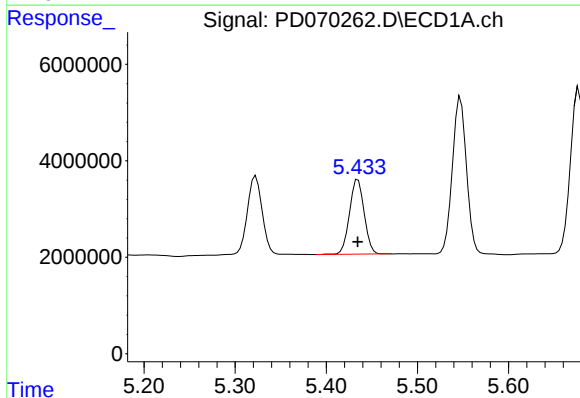


#9 Endosulfan I

R.T.: 5.435 min
Delta R.T.: 0.000 min
Response: 17321253
Conc: 10.66 ng/ml

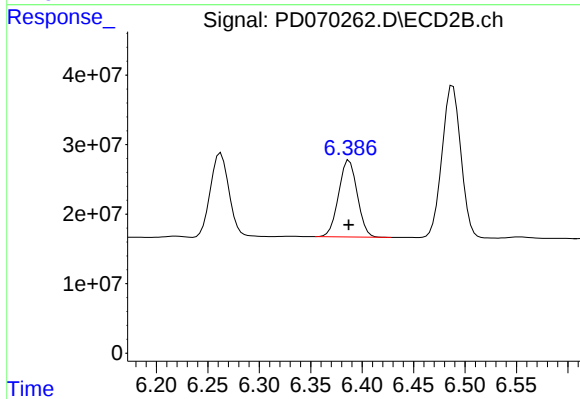

#9 Endosulfan I


R.T.: 6.387 min
Delta R.T.: 0.000 min
Response: 139661594
Conc: 11.71 ng/ml

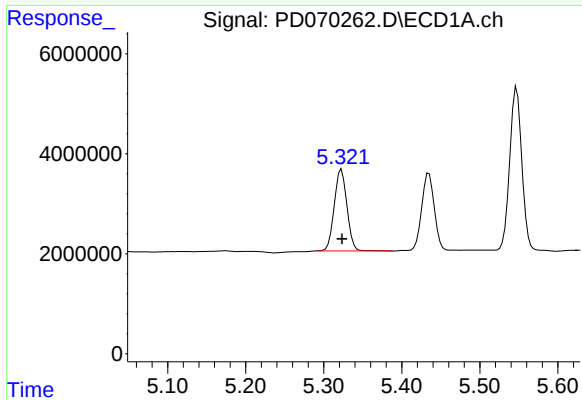

#10 gamma-Chlordane


R.T.: 5.323 min
Delta R.T.: 0.000 min
Response: 18472756
Conc: 10.41 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

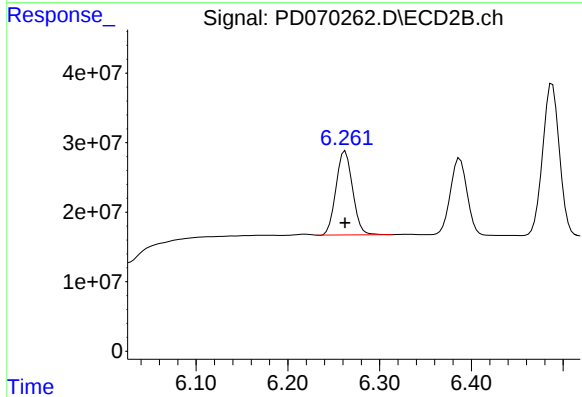


#10 gamma-Chlordane

R.T.: 6.263 min
Delta R.T.: 0.000 min
Response: 151636090
Conc: 11.60 ng/ml

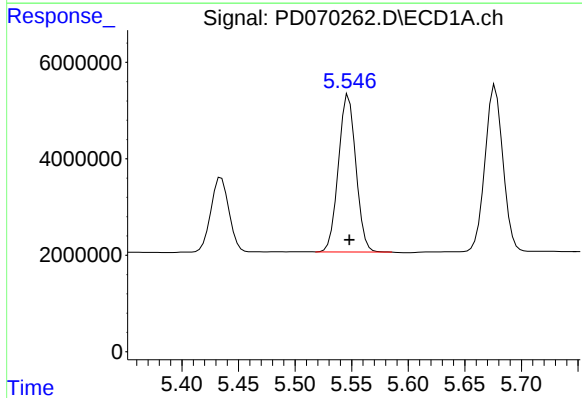


#12 4,4'-DDE

R.T.: 5.547 min
Delta R.T.: 0.000 min
Response: 35063812
Conc: 21.14 ng/ml

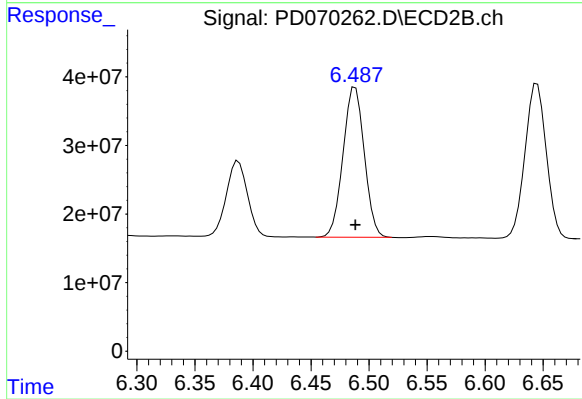

#12 4,4'-DDE


R.T.: 6.488 min
Delta R.T.: 0.000 min
Response: 278913295
Conc: 22.79 ng/ml

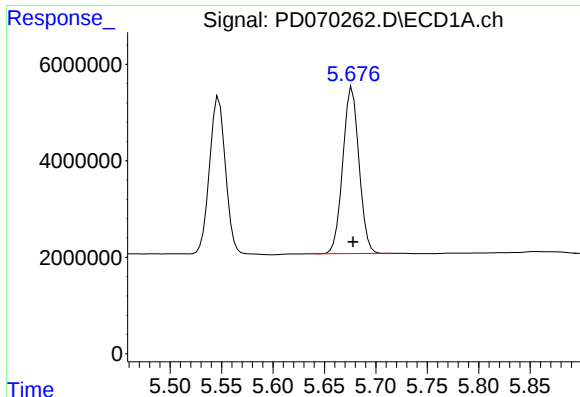

#13 Dieldrin


R.T.: 5.677 min
Delta R.T.: 0.000 min
Response: 37916831
Conc: 21.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

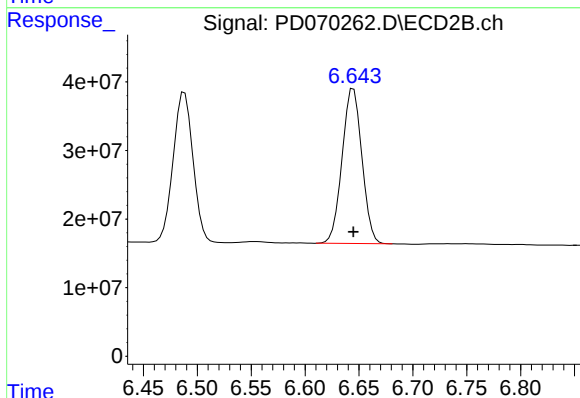


#13 Dieldrin

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 289139767
Conc: 23.25 ng/ml

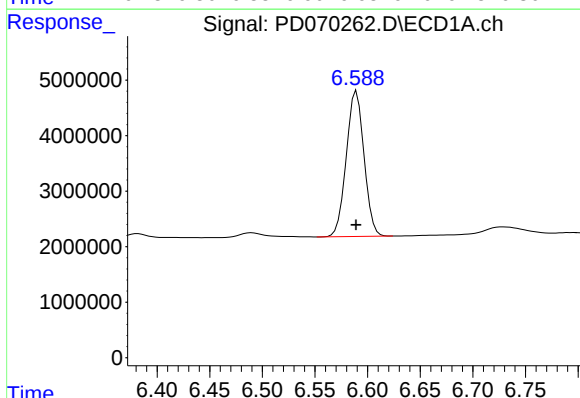


#19 Endosulfan Sulfate

R.T.: 6.590 min
Delta R.T.: 0.000 min
Response: 30810270
Conc: 20.28 ng/ml

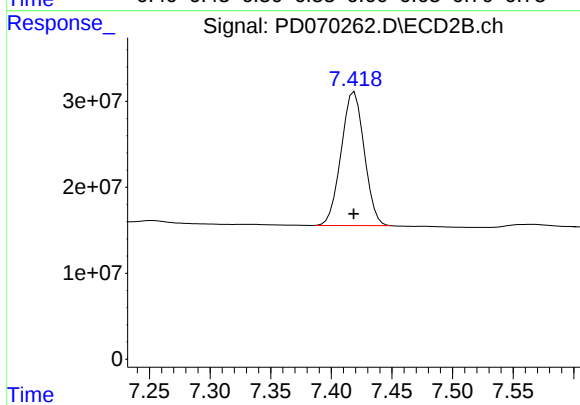

#19 Endosulfan Sulfate


R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 205944084
Conc: 21.44 ng/ml

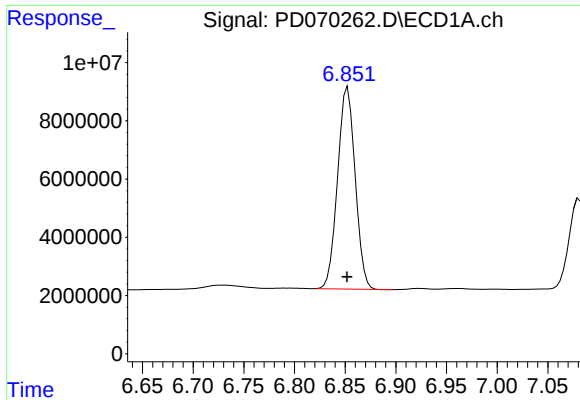

#20 Methoxychlor


R.T.: 6.853 min
Delta R.T.: 0.000 min
Response: 83677820
Conc: 108.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

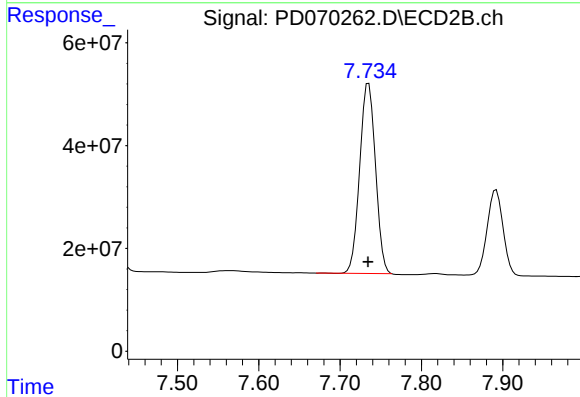


#20 Methoxychlor

R.T.: 7.735 min
Delta R.T.: 0.000 min
Response: 499432109
Conc: 101.73 ng/ml

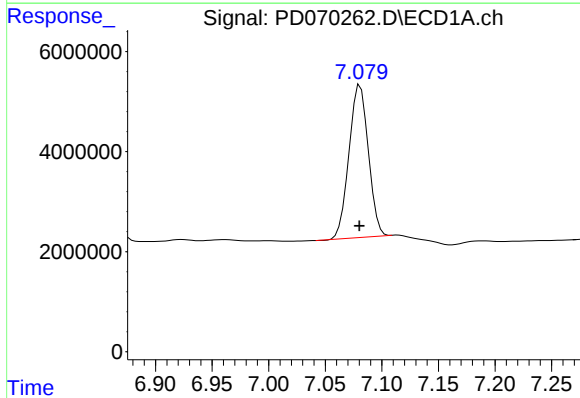


#21 Endrin ketone

R.T.: 7.081 min
Delta R.T.: 0.000 min
Response: 36302902
Conc: 21.18 ng/ml

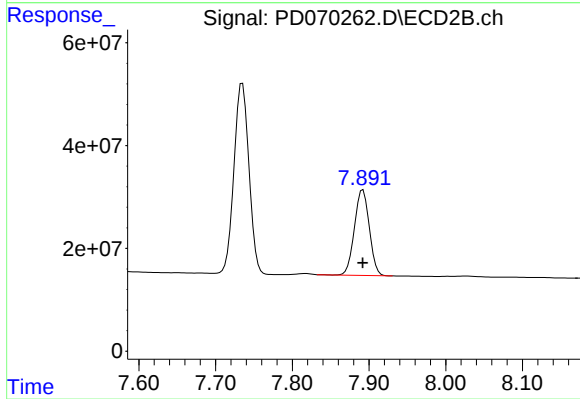

#21 Endrin ketone


R.T.: 7.892 min
Delta R.T.: 0.000 min
Response: 224959360
Conc: 23.05 ng/ml

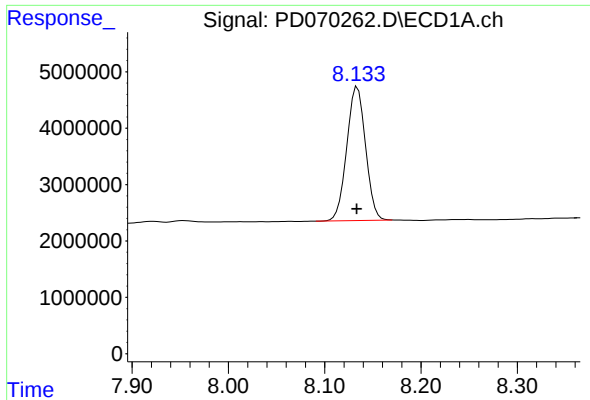

#28 Decachlorobiphenyl

R.T.: 8.134 min
Delta R.T.: 0.000 min
Response: 32048478
Conc: 22.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

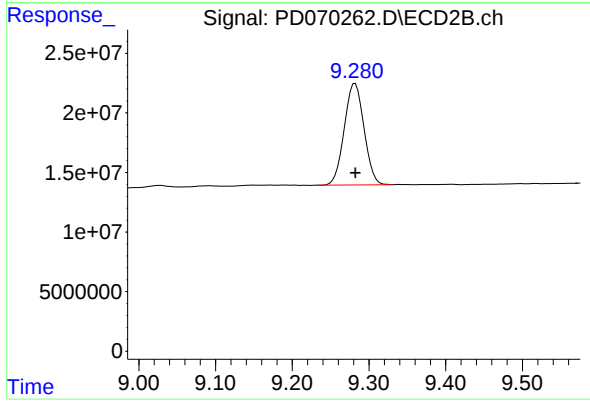

#28 Decachlorobiphenyl

R.T.: 9.282 min
Delta R.T.: 0.000 min
Response: 153316311
Conc: 22.78 ng/ml