

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061322\
 Data File : PD070269.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2022 18:37
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 01:41:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061322.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 14 01:41:01 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.401	4.123	120.4E6	858.2E6	74.587	74.395
28)	SA Decachlor...	8.133	9.282	104.2E6	493.5E6	74.578	74.237
Target Compounds							
23)	Chlordane-1	4.262	5.137	35978574	323.7E6	745.444	743.947
24)	Chlordane-2	4.760	5.609	41047167	359.9E6	744.103	728.242
25)	Chlordane-3	5.323	6.262	129.2E6	1271.9E6	751.285	739.485
26)	Chlordane-4	5.381	6.339	107.8E6	1477.5E6	748.782	740.477
27)	Chlordane-5	6.215	7.147	43798924	265.0E6	749.755	749.059



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061322\
Data File : PD070269.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2022 18:37
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 01:41:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061322.M
Quant Title : GC Extractables
QLast Update : Tue Jun 14 01:41:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

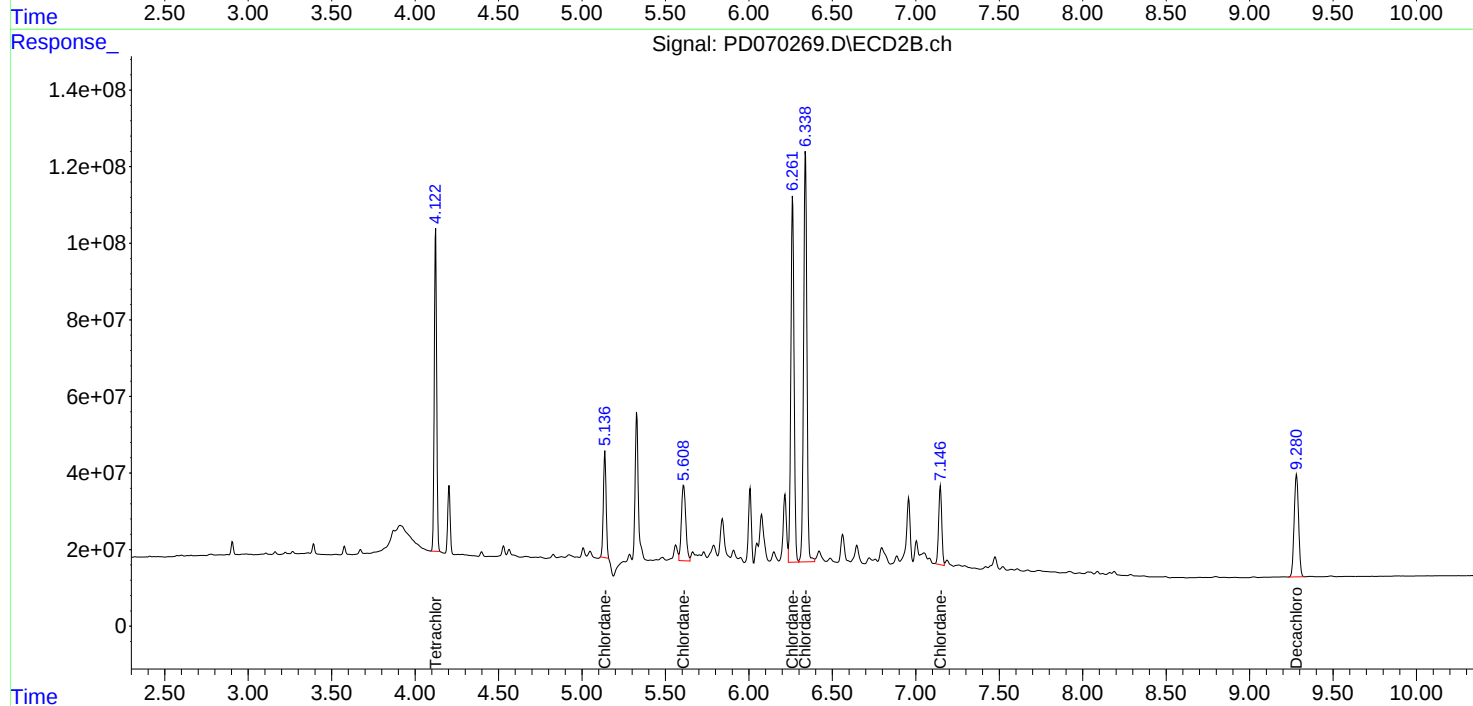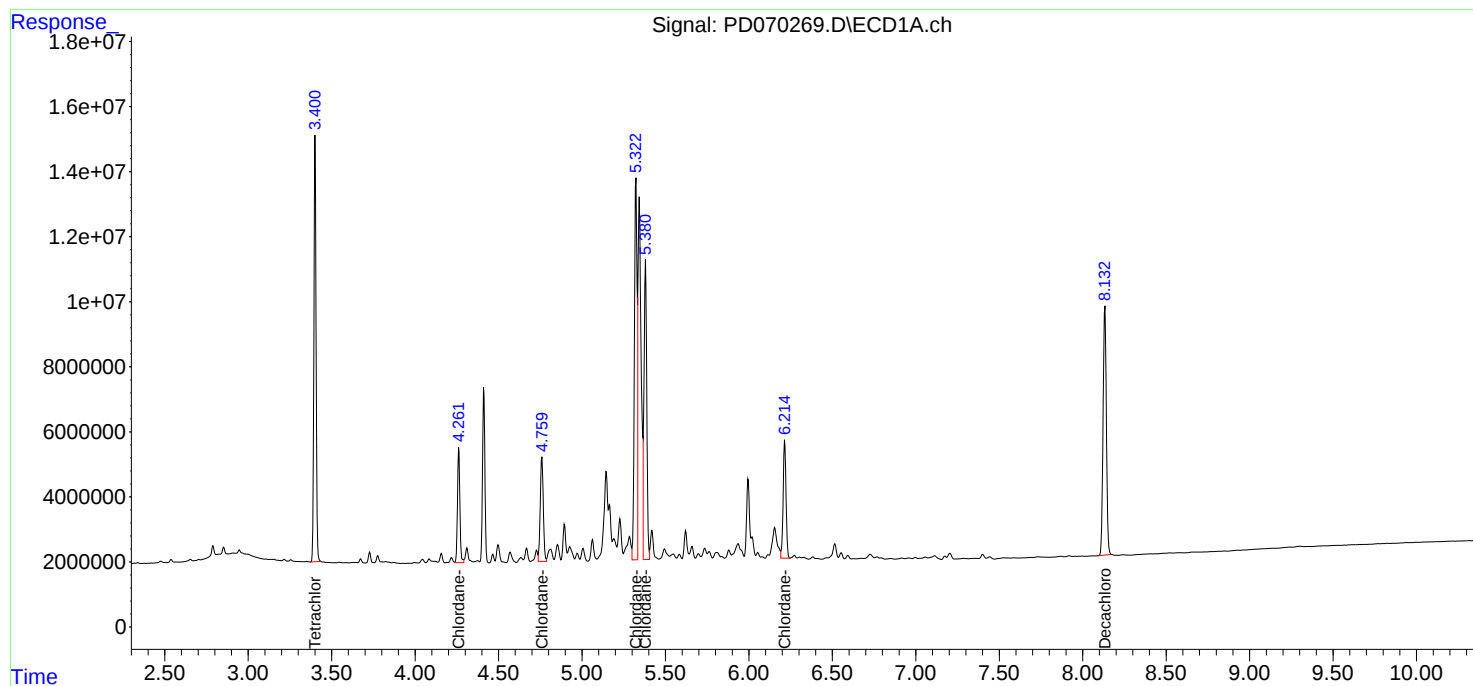


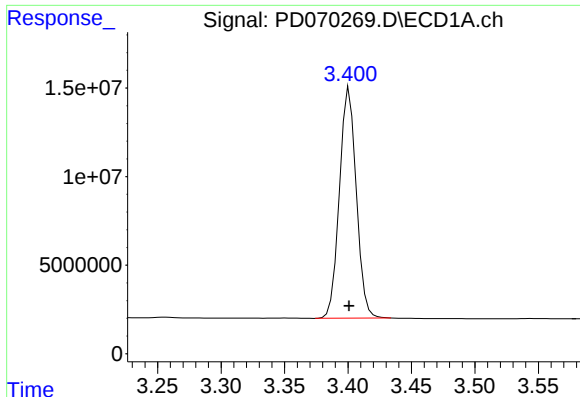

#1 Tetrachloro-m-xylene


R.T.: 3.401 min
Delta R.T.: 0.000 min
Response: 120420632
Conc: 74.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

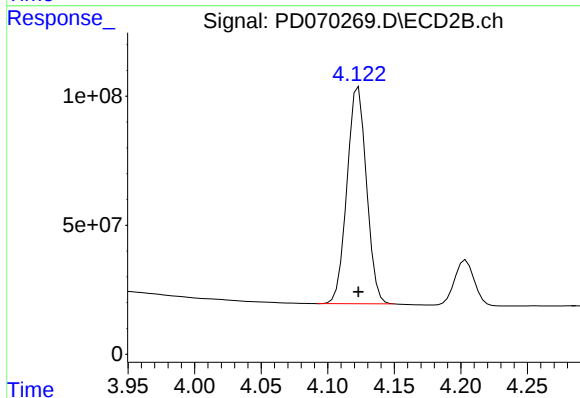


#1 Tetrachloro-m-xylene

R.T.: 4.123 min
Delta R.T.: 0.000 min
Response: 858206560
Conc: 74.39 ng/ml

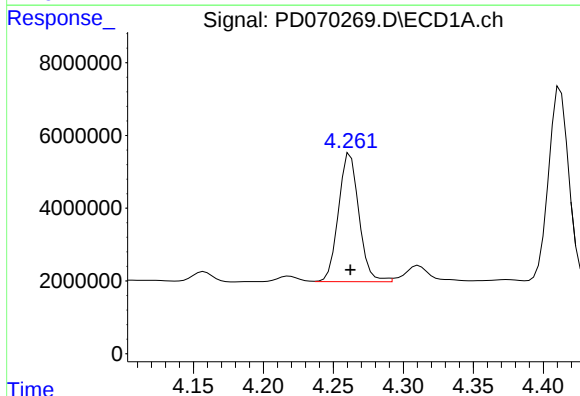


#23 Chlordane-1

R.T.: 4.262 min
Delta R.T.: 0.000 min
Response: 35978574
Conc: 745.44 ng/ml

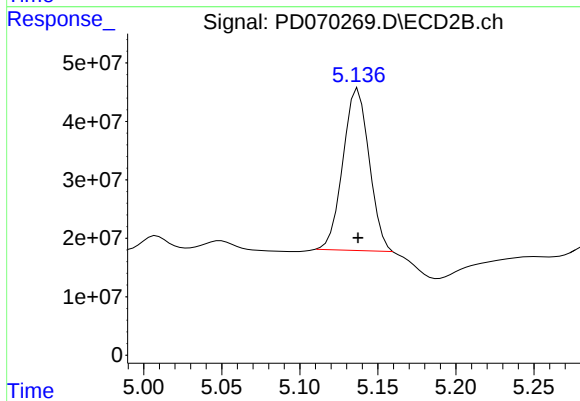

#23 Chlordane-1


R.T.: 5.137 min
Delta R.T.: 0.000 min
Response: 323723870
Conc: 743.95 ng/ml

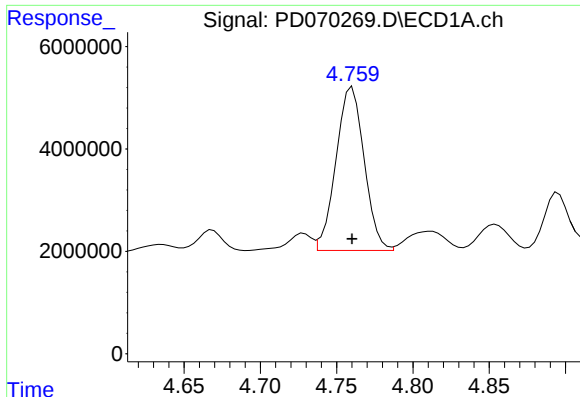

#24 Chlordane-2


R.T.: 4.760 min
Delta R.T.: 0.000 min
Response: 41047167
Conc: 744.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

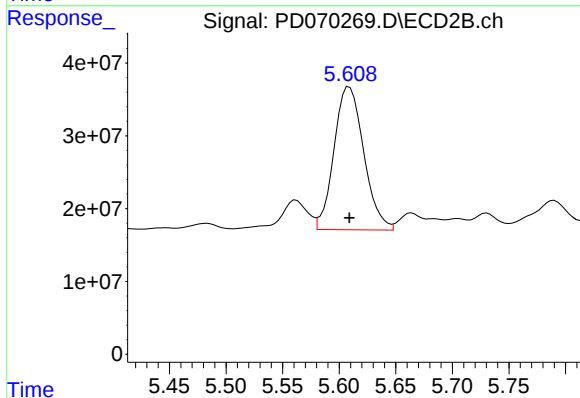


#24 Chlordane-2

R.T.: 5.609 min
Delta R.T.: 0.000 min
Response: 359919267
Conc: 728.24 ng/ml

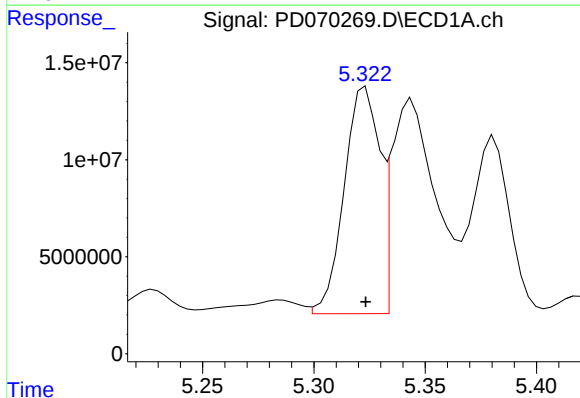


#25 Chlordane-3

R.T.: 5.323 min
Delta R.T.: 0.000 min
Response: 129215743
Conc: 751.29 ng/ml

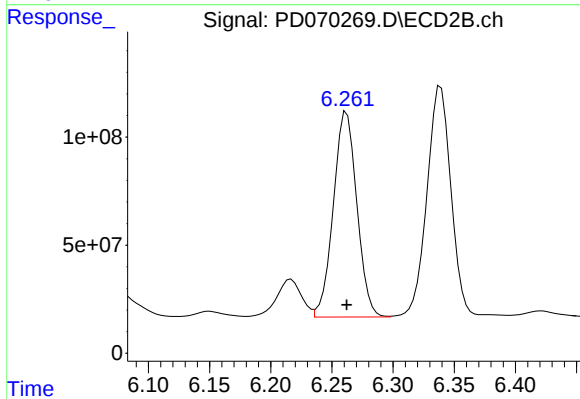

#25 Chlordane-3


R.T.: 6.262 min
Delta R.T.: 0.000 min
Response: 1271865275
Conc: 739.48 ng/ml

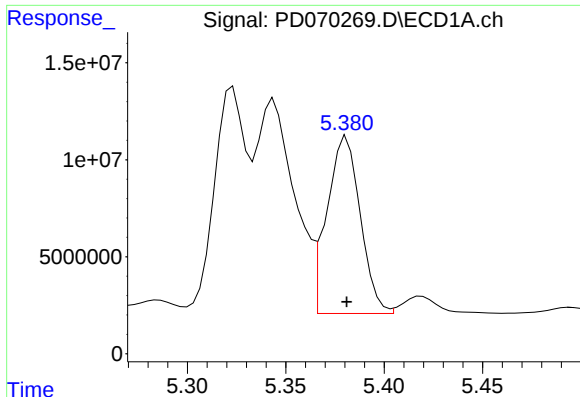

#26 Chlordane-4


R.T.: 5.381 min
Delta R.T.: 0.000 min
Response: 107830648
Conc: 748.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

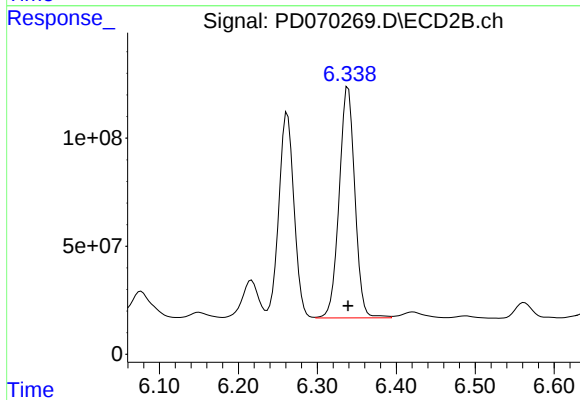


#26 Chlordane-4

R.T.: 6.339 min
Delta R.T.: 0.000 min
Response: 1477544060
Conc: 740.48 ng/ml

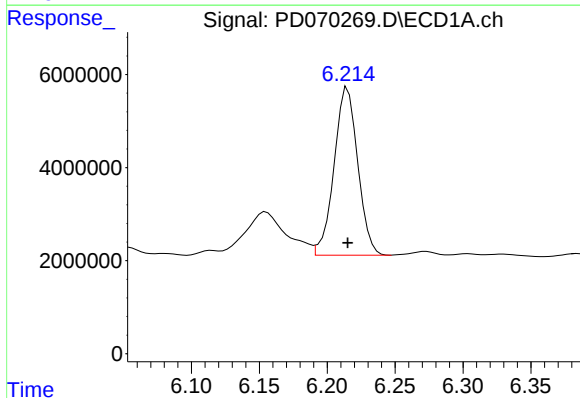


#27 Chlordane-5

R.T.: 6.215 min
Delta R.T.: 0.000 min
Response: 43798924
Conc: 749.76 ng/ml

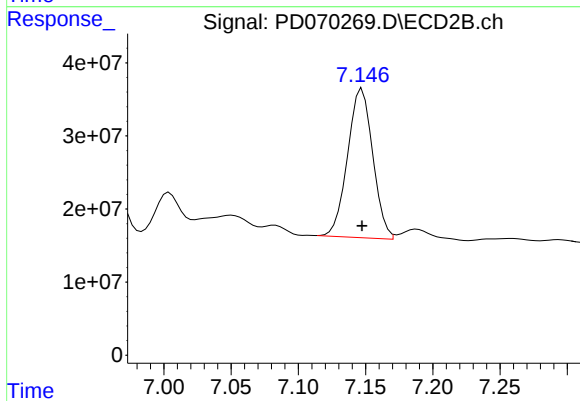

#27 Chlordane-5

R.T.: 7.147 min
Delta R.T.: 0.000 min
Response: 264973955
Conc: 749.06 ng/ml

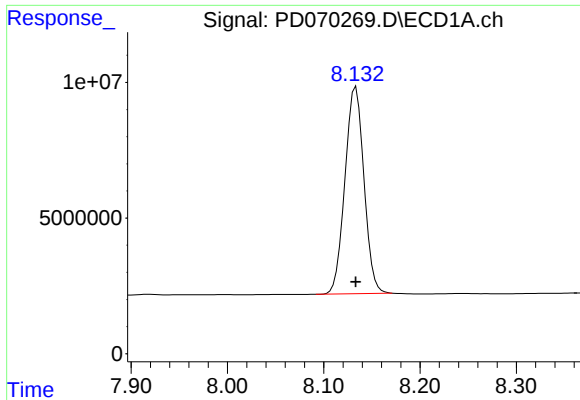

#28 Decachlorobiphenyl


R.T.: 8.133 min

Delta R.T.: 0.000 min

Response: 104233795

Conc: 74.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

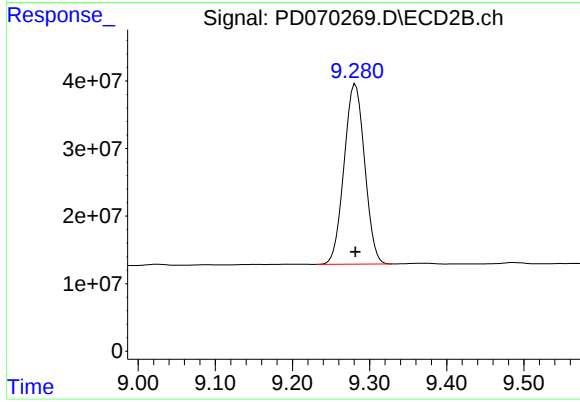

#28 Decachlorobiphenyl

R.T.: 9.282 min

Delta R.T.: 0.000 min

Response: 493479427

Conc: 74.24 ng/ml