

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061322\
 Data File : PD070279.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2022 20:58
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD061322

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 01:53:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061322.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 14 01:47:50 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.402	4.123	81170320	577.4E6	52.453	49.383
28)	SA Decachlor...	8.133	9.281	73870439	341.3E6	51.624	49.434
Target Compounds							
23)	Chlordane-1	4.262	5.137	24486723	217.7E6	508.265	493.777
24)	Chlordane-2	4.760	5.609	28752700	259.0E6	525.898	521.171
25)	Chlordane-3	5.323	6.263	88030235	865.3E6	533.393	492.056
26)	Chlordane-4	5.381	6.339	73332385	1006.9E6	530.830	491.277
27)	Chlordane-5	6.215	7.147	29783397	171.9E6	510.645	475.565



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061322\
Data File : PD070279.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2022 20:58
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD061322

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 01:53:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061322.M
Quant Title : GC Extractables
QLast Update : Tue Jun 14 01:47:50 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

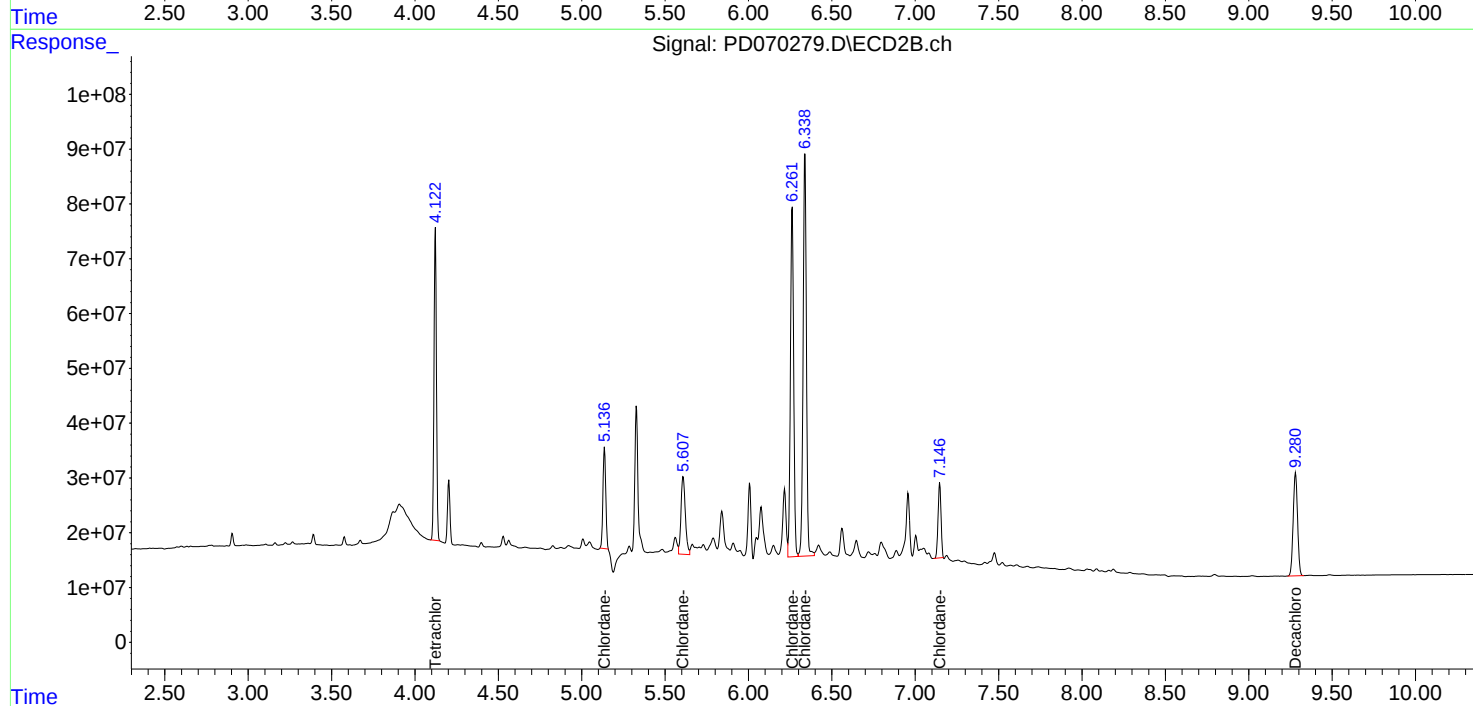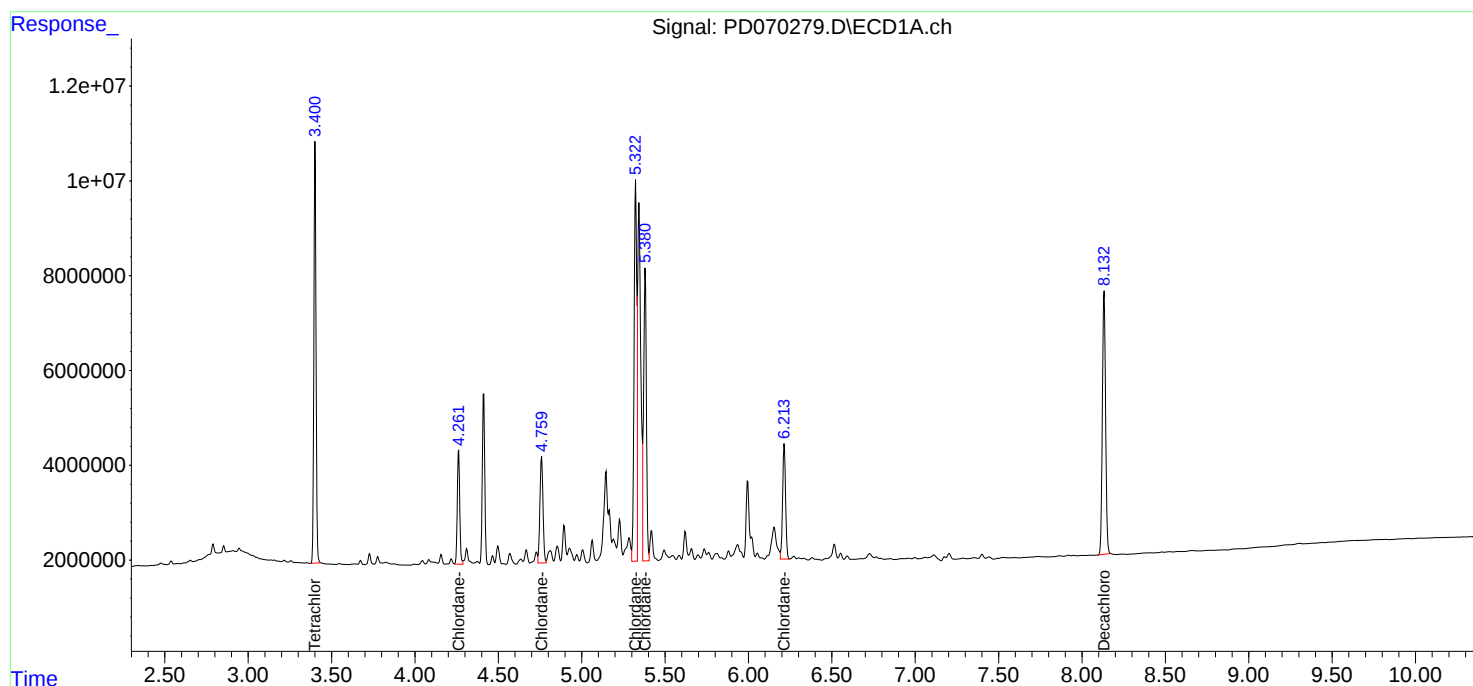


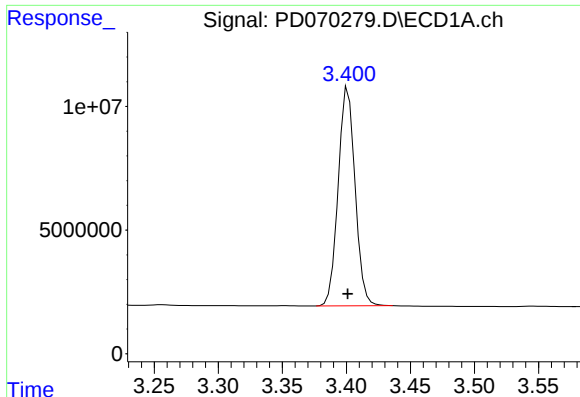

#1 Tetrachloro-m-xylene


R.T.: 3.402 min
Delta R.T.: 0.000 min
Response: 81170320
Conc: 52.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD061322

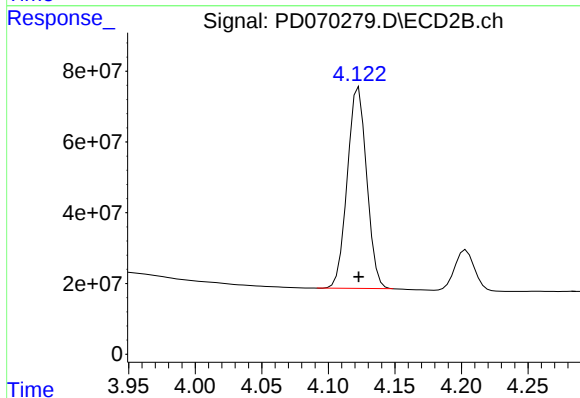


#1 Tetrachloro-m-xylene

R.T.: 4.123 min
Delta R.T.: 0.000 min
Response: 577430177
Conc: 49.38 ng/ml

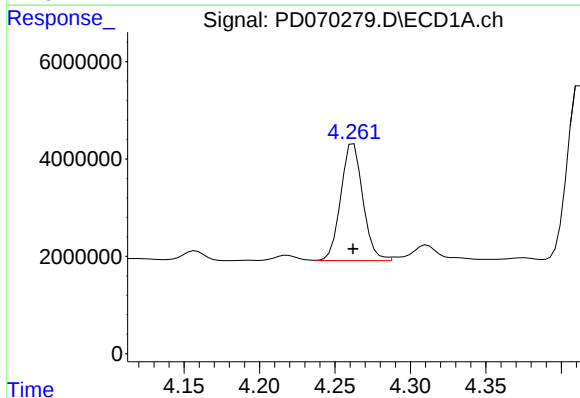


#23 Chlordane-1

R.T.: 4.262 min
Delta R.T.: 0.000 min
Response: 24486723
Conc: 508.26 ng/ml

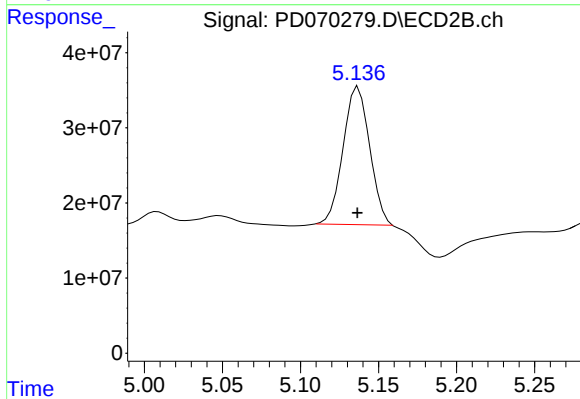

#23 Chlordane-1


R.T.: 5.137 min
Delta R.T.: 0.000 min
Response: 217726972
Conc: 493.78 ng/ml

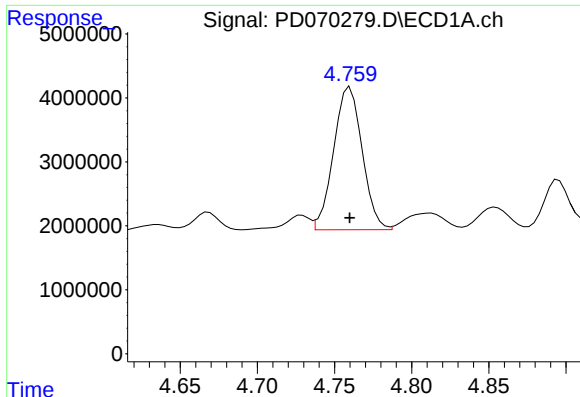

#24 Chlordane-2


R.T.: 4.760 min
Delta R.T.: 0.000 min
Response: 28752700
Conc: 525.90 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD061322

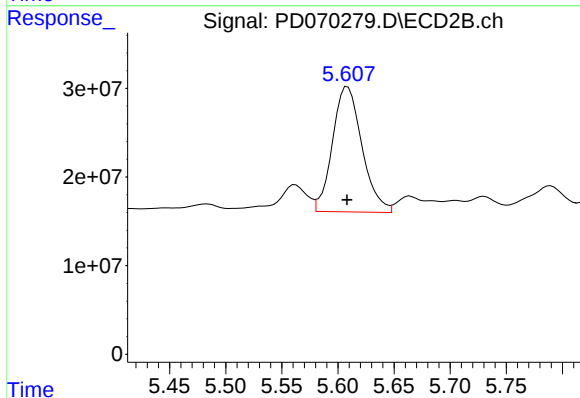


#24 Chlordane-2

R.T.: 5.609 min
Delta R.T.: 0.000 min
Response: 258955468
Conc: 521.17 ng/ml

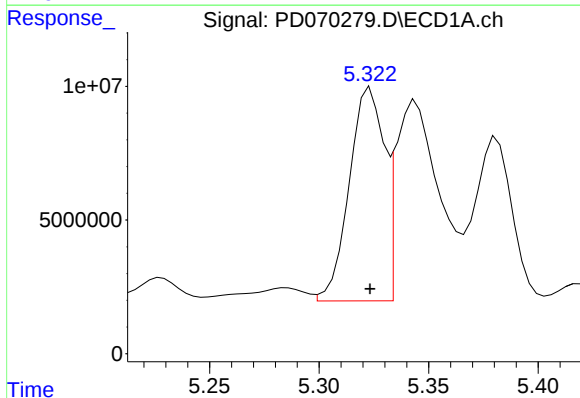


#25 Chlordane-3

R.T.: 5.323 min
Delta R.T.: 0.000 min
Response: 88030235
Conc: 533.39 ng/ml

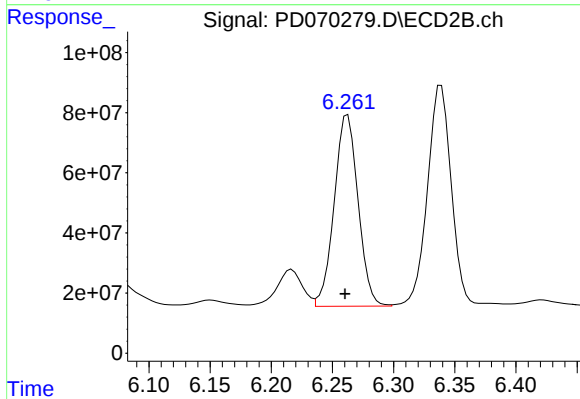

#25 Chlordane-3


R.T.: 6.263 min
Delta R.T.: 0.002 min
Response: 865348013
Conc: 492.06 ng/ml

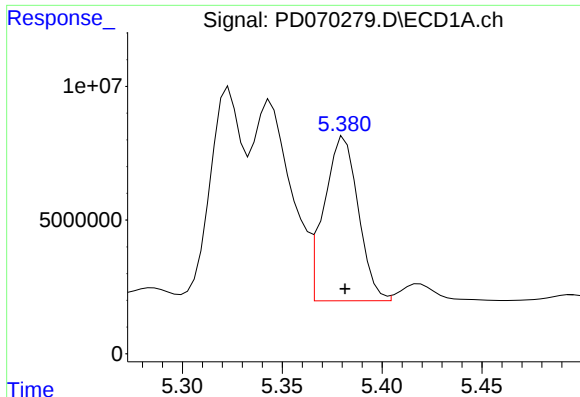

#26 Chlordane-4


R.T.: 5.381 min
Delta R.T.: 0.000 min
Response: 73332385
Conc: 530.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD061322

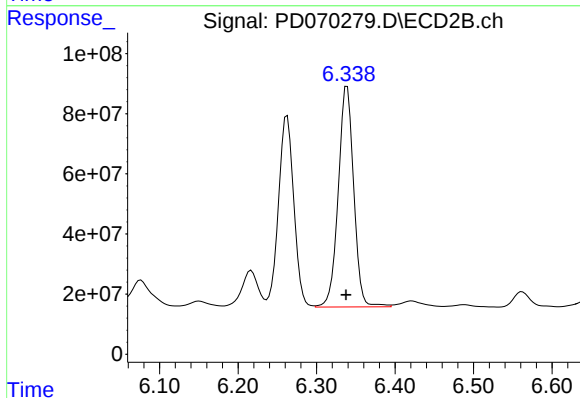


#26 Chlordane-4

R.T.: 6.339 min
Delta R.T.: 0.001 min
Response: 1006868586
Conc: 491.28 ng/ml

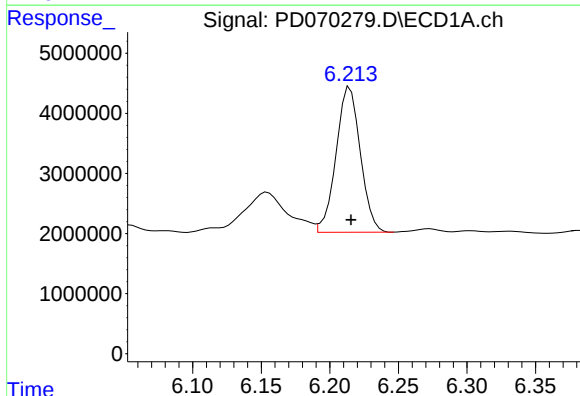


#27 Chlordane-5

R.T.: 6.215 min
Delta R.T.: 0.000 min
Response: 29783397
Conc: 510.64 ng/ml

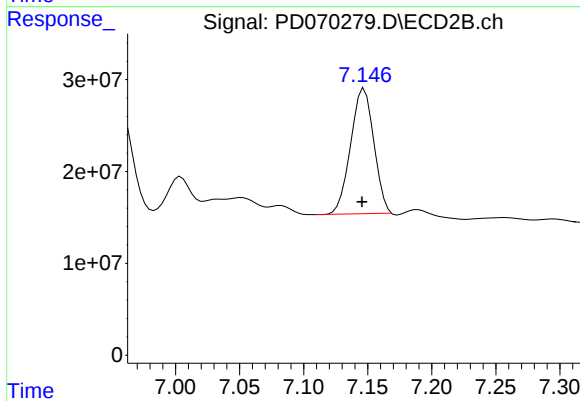

#27 Chlordane-5


R.T.: 7.147 min
Delta R.T.: 0.002 min
Response: 171908329
Conc: 475.57 ng/ml

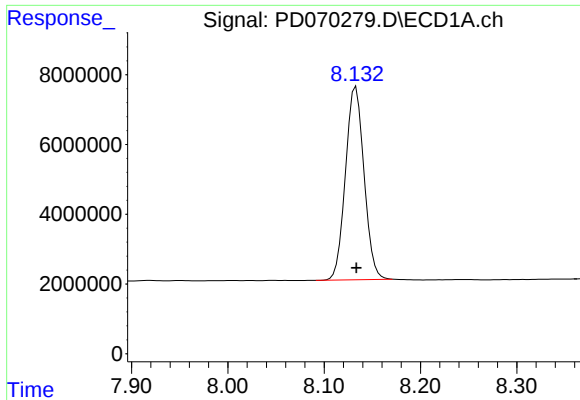

#28 Decachlorobiphenyl

R.T.: 8.133 min
Delta R.T.: 0.000 min
Response: 73870439
Conc: 51.62 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD061322

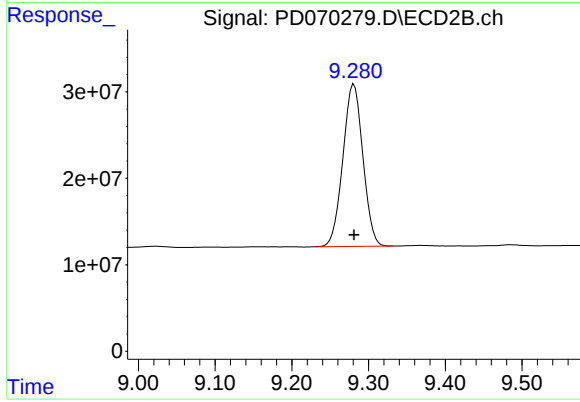

#28 Decachlorobiphenyl

R.T.: 9.281 min
Delta R.T.: 0.000 min
Response: 341261501
Conc: 49.43 ng/ml