

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061325\
 Data File : PD088954.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jun 2025 18:15
 Operator : AR\AJ
 Sample : Q2301-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 WC-URBAN-FILL-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 13 22:36:04 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051925.M
 Quant Title : GC Extractables
 QLast Update : Mon May 19 15:27:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.549	2.880	49396598	319.3E6	22.829	21.107
28)	SA Decachlor...	9.070	8.071	77257793	419.6E6	22.575	22.984

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061325\
Data File : PD088954.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jun 2025 18:15
Operator : AR\AJ
Sample : Q2301-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
WC-URBAN-FILL-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 13 22:36:04 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051925.M
Quant Title : GC Extractables
QLast Update : Mon May 19 15:27:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

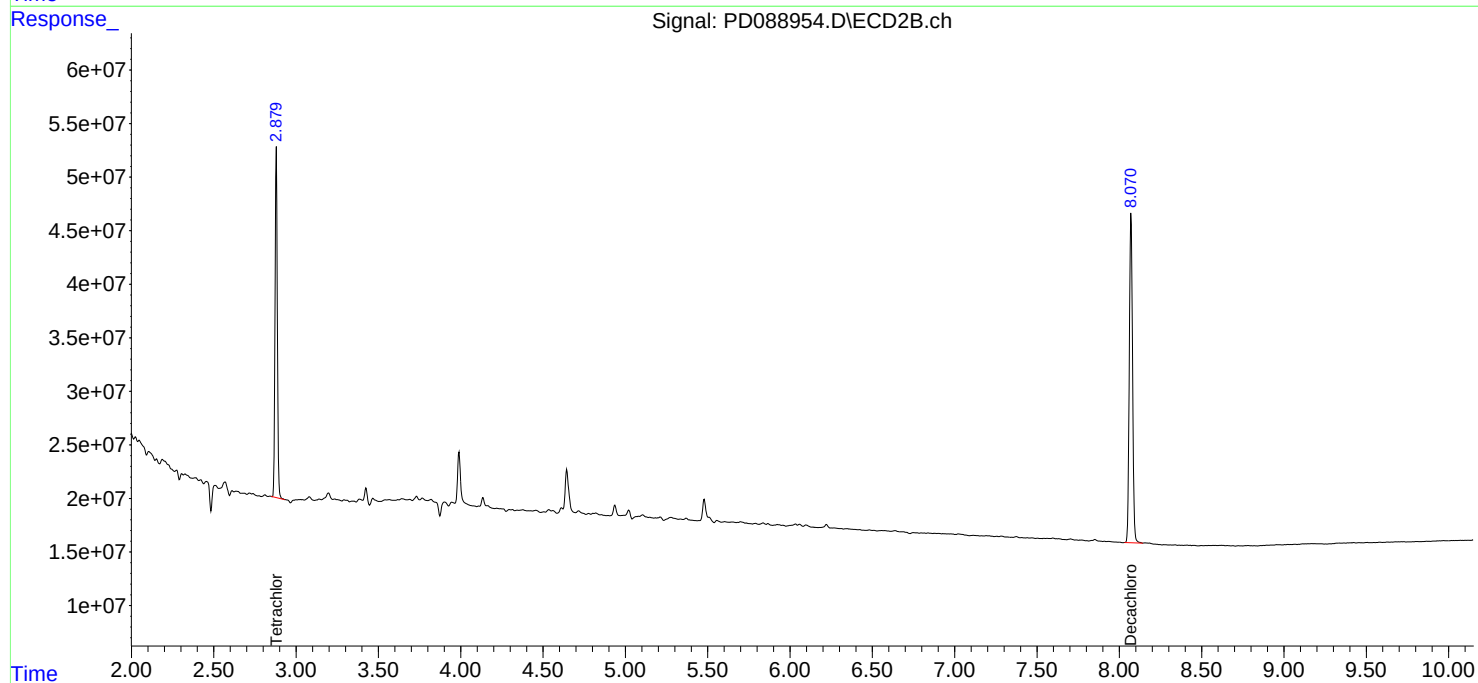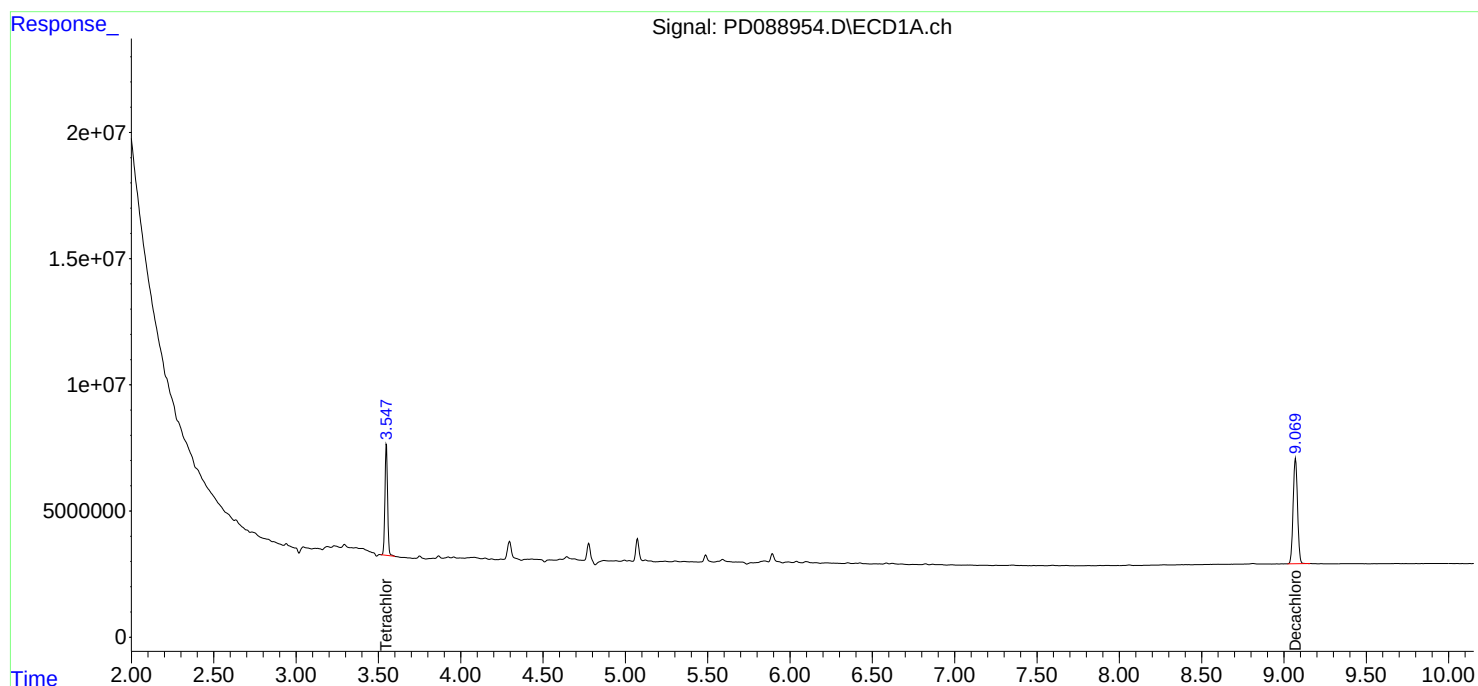


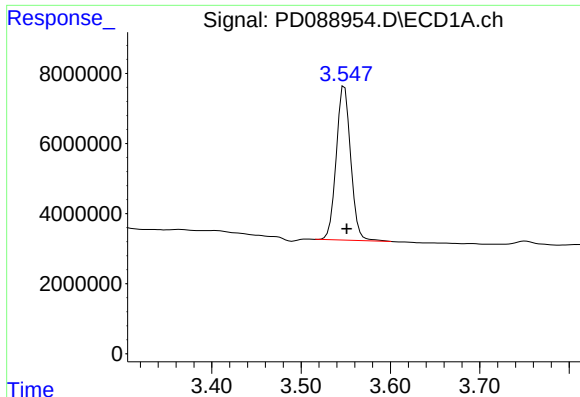

#1 Tetrachloro-m-xylene


R.T.: 3.549 min
Delta R.T.: -0.002 min
Response: 49396598
Conc: 22.83 ng/ml

Instrument :
ECD_D
ClientSampleId :
WC-URBAN-FILL-C

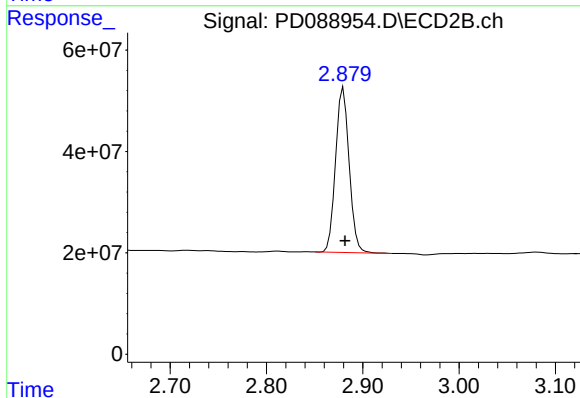


#1 Tetrachloro-m-xylene

R.T.: 2.880 min
Delta R.T.: -0.002 min
Response: 319282395
Conc: 21.11 ng/ml

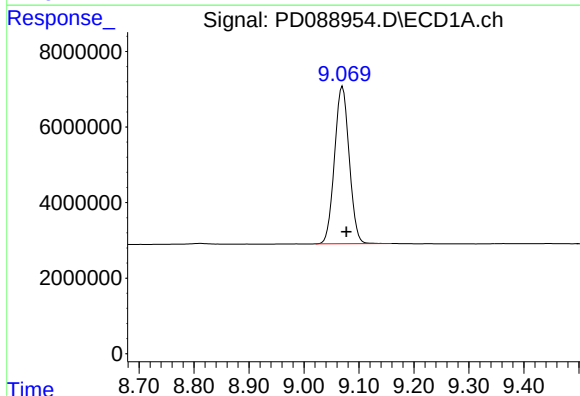

#28 Decachlorobiphenyl

R.T.: 9.070 min
Delta R.T.: -0.007 min
Response: 77257793
Conc: 22.57 ng/ml

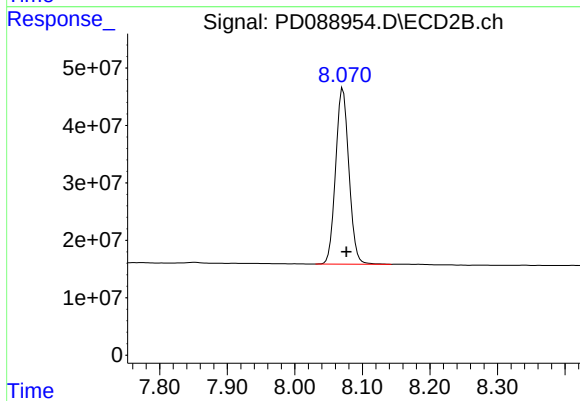

#28 Decachlorobiphenyl

R.T.: 8.071 min
Delta R.T.: -0.005 min
Response: 419599202
Conc: 22.98 ng/ml