

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061421\
 Data File : PD063817.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2021 11:35
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 12:56:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 14 12:55:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.971	7847393	84278711	5.047	5.278
27)	SA Decachlor...	8.194	9.026	18063174	144.3E6	10.431	10.275
Target Compounds							
2)	A alpha-BHC	3.874	4.359	11043423	130.8E6	4.749	5.245
3)	MA gamma-BHC...	4.158	4.644	11229879	119.3E6	4.978	5.206
4)	MA Heptachlor	4.459	5.151	10547691	124.5E6	4.862	5.330
9)	A Endosulfan I	5.488	6.197	8941484	104.5E6	4.911	5.257
13)	MA Dieldrin	5.731	6.454	19720893	220.2E6	9.414	10.459
14)	MA Endrin	5.989	6.672	17379740	185.1E6	9.603	10.519
16)	A 4,4'-DDD	6.115	6.795	15213400	174.8E6	9.146	10.284
17)	MA 4,4'-DDT	6.357	7.093	14605487	162.7E6	8.609	9.778
20)	A Methoxychlor	6.904	7.551	47064598	424.2E6	49.978	53.767


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061421\
Data File : PD063817.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2021 11:35
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 12:56:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 14 12:55:47 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

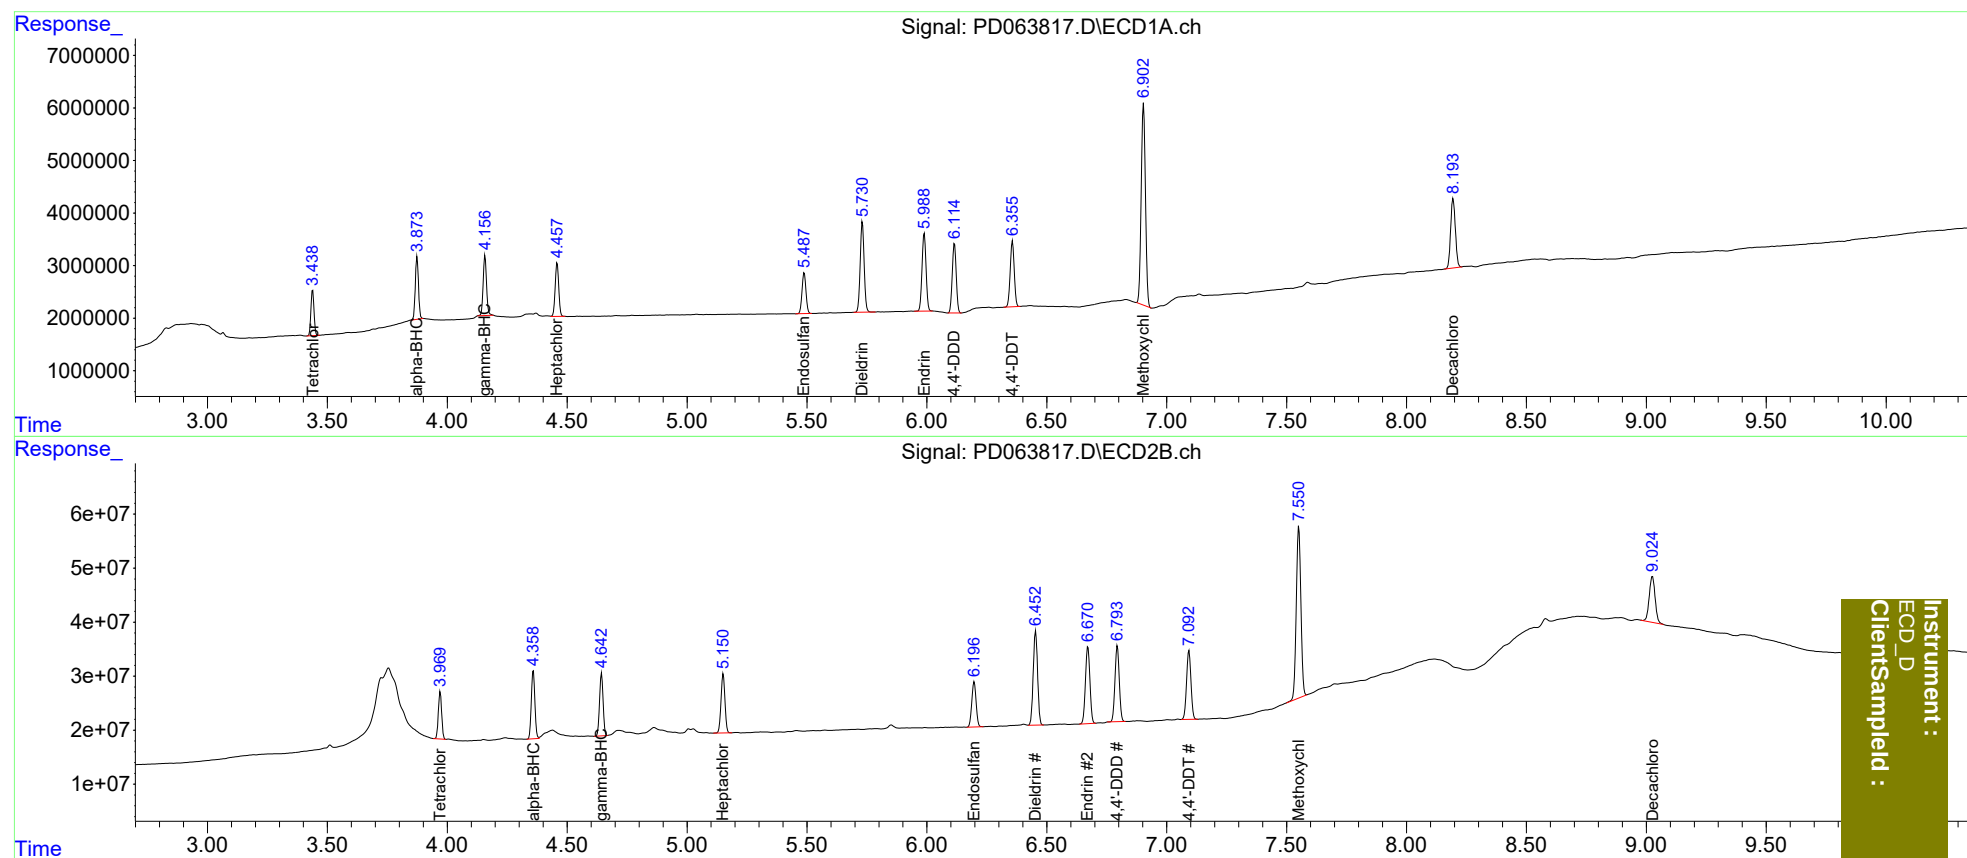


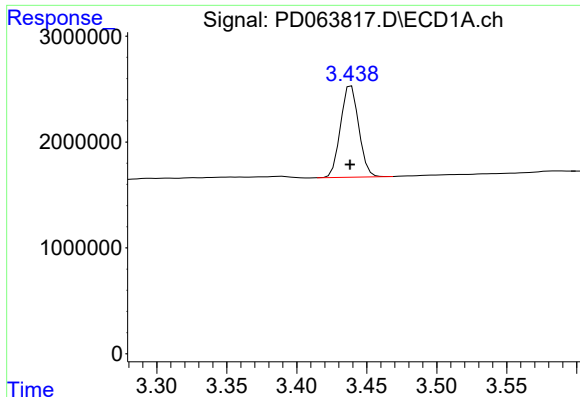

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.000 min
Response: 7847393
Conc: 5.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

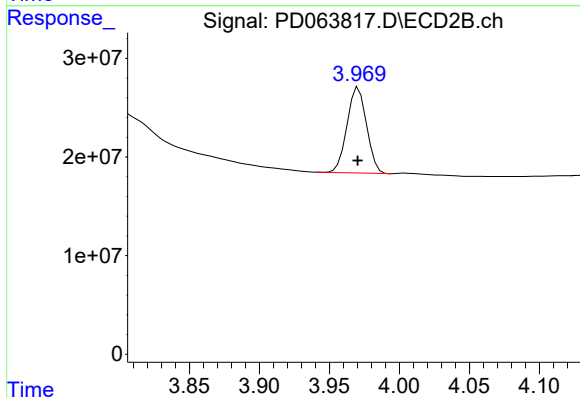


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 84278711
Conc: 5.28 ng/ml

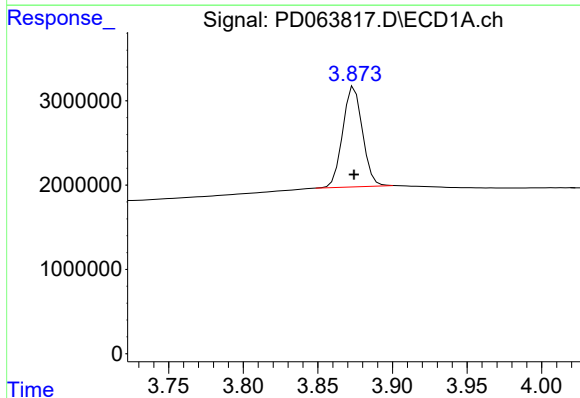


#2 alpha-BHC

R.T.: 3.874 min
Delta R.T.: 0.000 min
Response: 11043423
Conc: 4.75 ng/ml

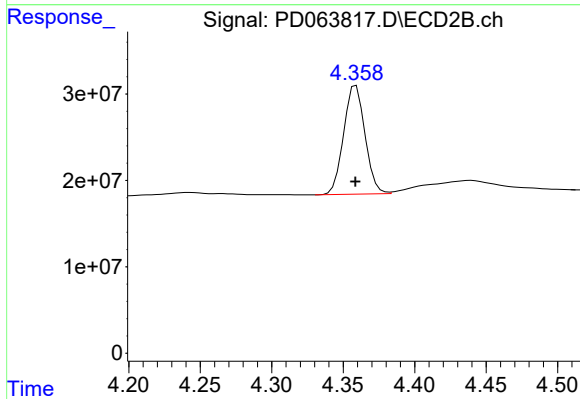

#2 alpha-BHC


R.T.: 4.359 min
Delta R.T.: 0.000 min
Response: 130800358
Conc: 5.25 ng/ml

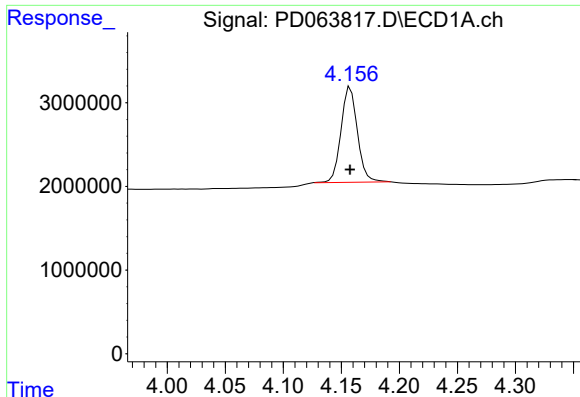

#3 gamma-BHC (Lindane)


R.T.: 4.158 min
Delta R.T.: 0.000 min
Response: 11229879
Conc: 4.98 ng/ml

Instrument :
ECD_D
ClientSampleId :

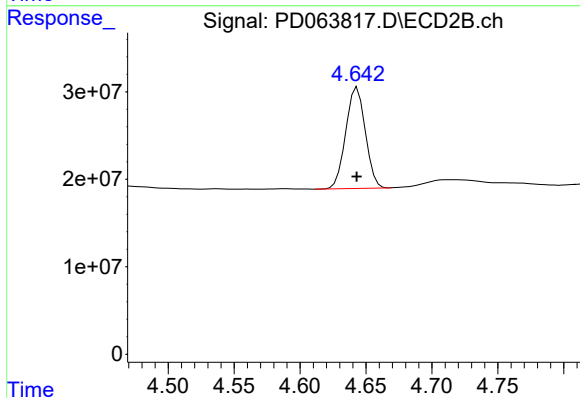


#3 gamma-BHC (Lindane)

R.T.: 4.644 min
Delta R.T.: 0.000 min
Response: 119334395
Conc: 5.21 ng/ml

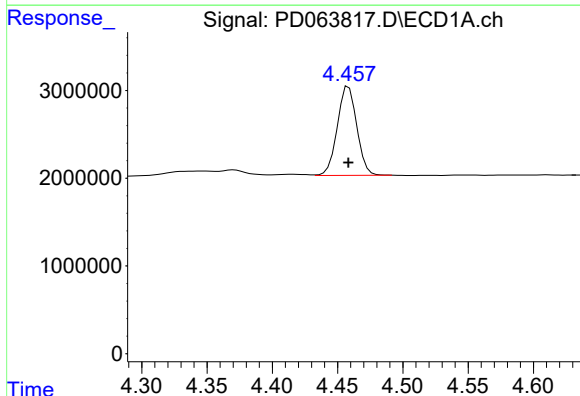


#4 Heptachlor

R.T.: 4.459 min
Delta R.T.: 0.000 min
Response: 10547691
Conc: 4.86 ng/ml

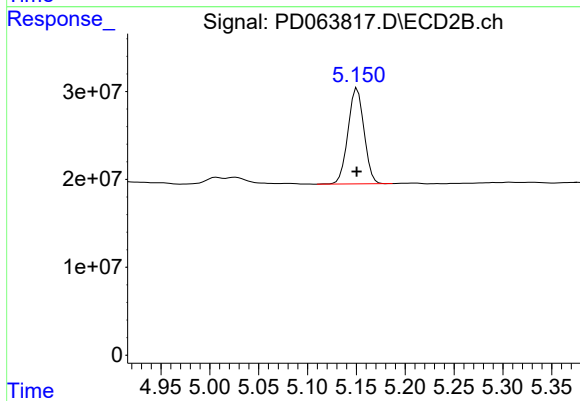

#4 Heptachlor


R.T.: 5.151 min
Delta R.T.: 0.000 min
Response: 124517417
Conc: 5.33 ng/ml

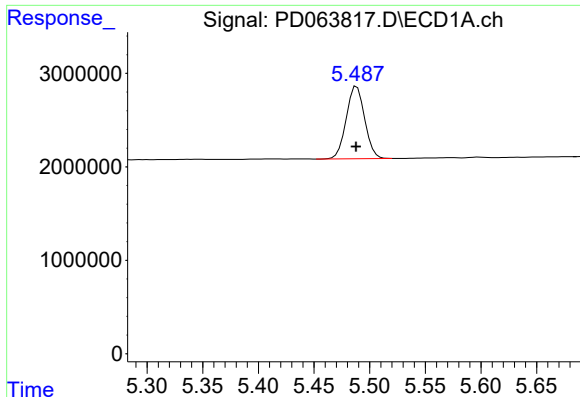

#9 Endosulfan I


R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 8941484
Conc: 4.91 ng/ml

Instrument :
ECD_D
ClientSampleId :

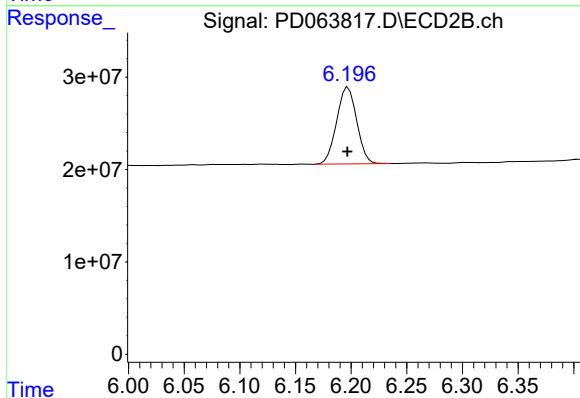


#9 Endosulfan I

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 104523167
Conc: 5.26 ng/ml

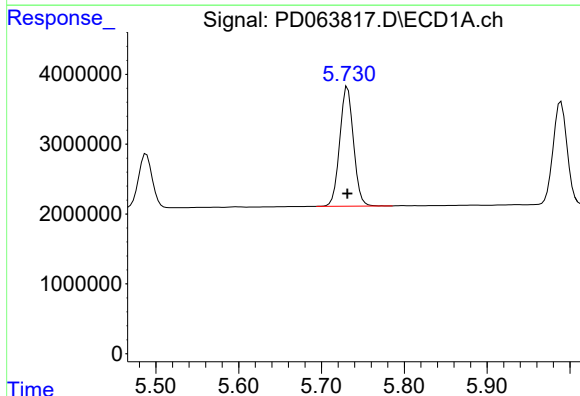


#13 Dieldrin

R.T.: 5.731 min
Delta R.T.: 0.000 min
Response: 19720893
Conc: 9.41 ng/ml

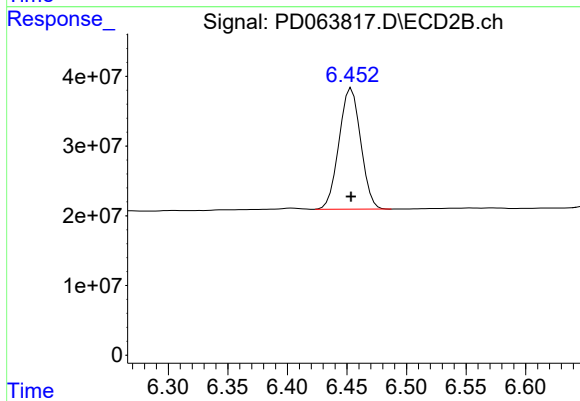

#13 Dieldrin


R.T.: 6.454 min
Delta R.T.: 0.000 min
Response: 220205496
Conc: 10.46 ng/ml

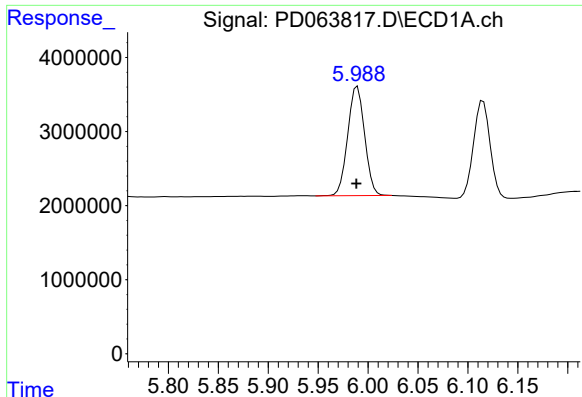

#14 Endrin


R.T.: 5.989 min
Delta R.T.: 0.000 min
Response: 17379740
Conc: 9.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

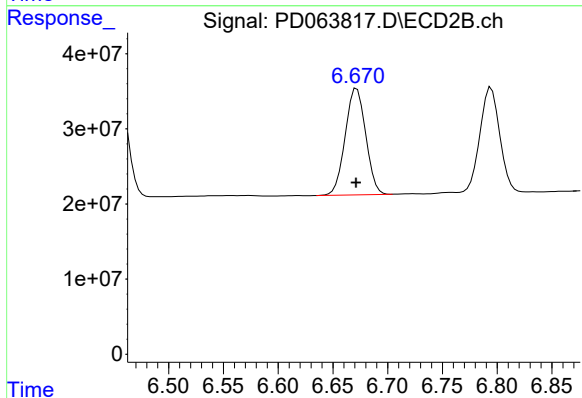


#14 Endrin

R.T.: 6.672 min
Delta R.T.: 0.000 min
Response: 185136674
Conc: 10.52 ng/ml

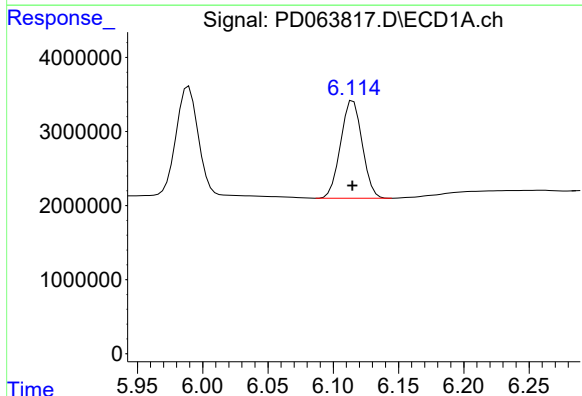


#16 4,4'-DDD

R.T.: 6.115 min
Delta R.T.: 0.000 min
Response: 15213400
Conc: 9.15 ng/ml

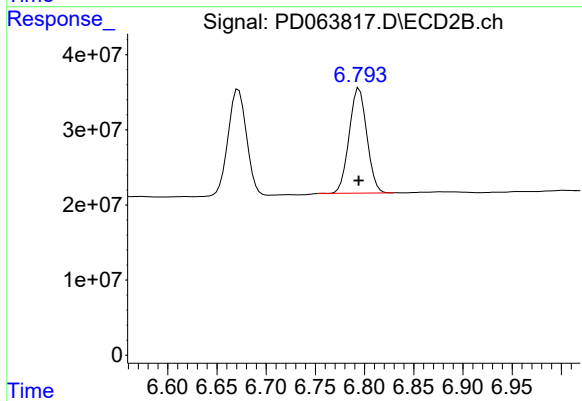

#16 4,4'-DDD


R.T.: 6.795 min
Delta R.T.: 0.000 min
Response: 174820813
Conc: 10.28 ng/ml

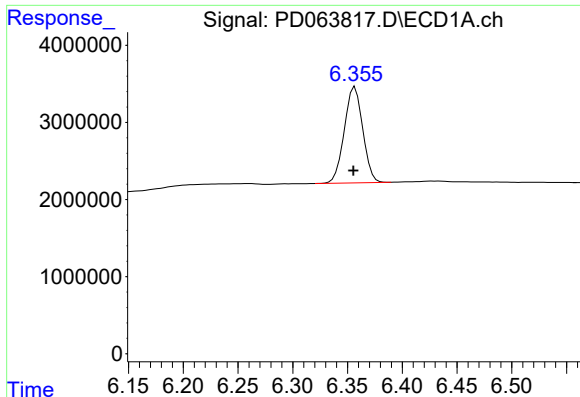

#17 4,4'-DDT


R.T.: 6.357 min
Delta R.T.: 0.001 min
Response: 14605487
Conc: 8.61 ng/ml

Instrument :
ECD_D
ClientSampleId :

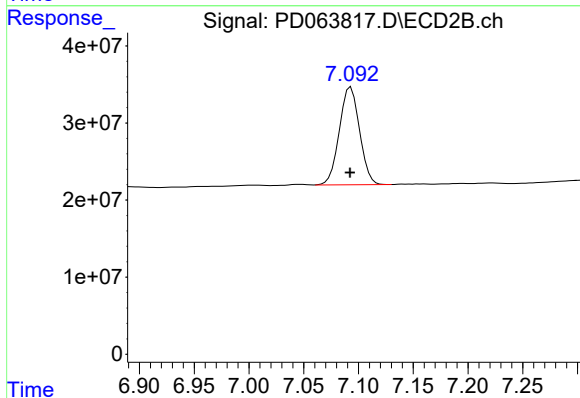


#17 4,4'-DDT

R.T.: 7.093 min
Delta R.T.: 0.000 min
Response: 162727379
Conc: 9.78 ng/ml

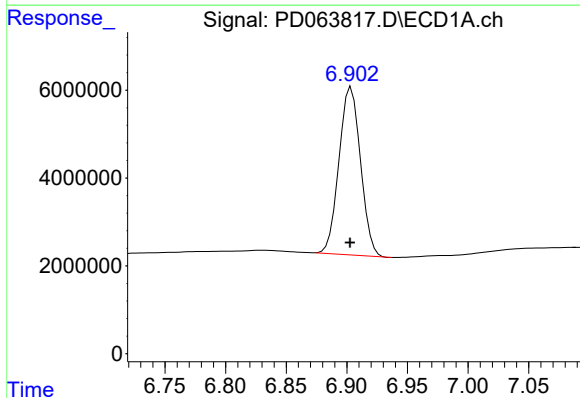


#20 Methoxychlor

R.T.: 6.904 min
Delta R.T.: 0.001 min
Response: 47064598
Conc: 49.98 ng/ml

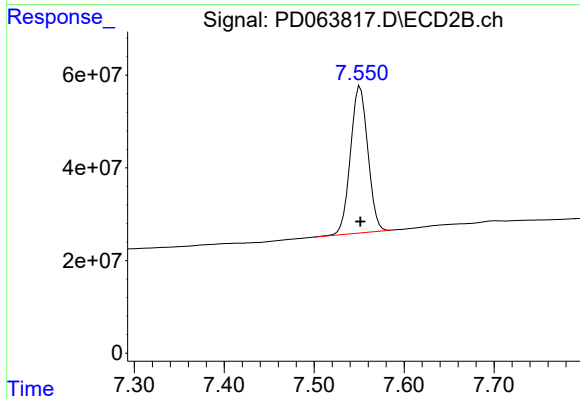

#20 Methoxychlor


R.T.: 7.551 min
Delta R.T.: 0.000 min
Response: 424226681
Conc: 53.77 ng/ml

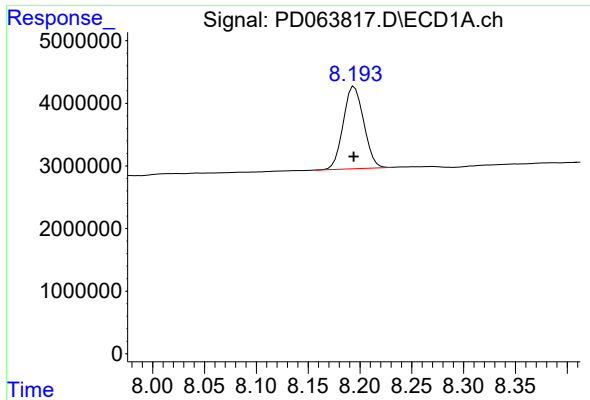

#27 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 18063174
Conc: 10.43 ng/ml

Instrument :
ECD_D
ClientSampleId :

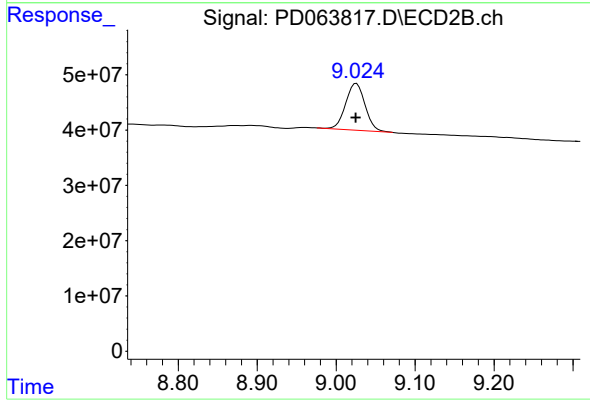

#27 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: 0.000 min
Response: 144312998
Conc: 10.27 ng/ml