

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061421\
 Data File : PD063819.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2021 12:03
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 12:56:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 14 12:55:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.970	15751085	166.5E6	10.130	10.426
27)	SA Decachlor...	8.194	9.025	35444059	274.5E6	20.468	19.542
Target Compounds							
2)	A alpha-BHC	3.874	4.358	22654642	257.1E6	9.741	10.309
3)	MA gamma-BHC...	4.157	4.642	22689591	237.5E6	10.059	10.362
4)	MA Heptachlor	4.457	5.150	21524544	243.1E6	9.921	10.404
9)	A Endosulfan I	5.487	6.197	18181445	210.9E6	9.986	10.606
13)	MA Dieldrin	5.730	6.453	40898963	437.9E6	19.523	20.797
14)	MA Endrin	5.988	6.671	35659250	367.3E6	19.704	20.869
16)	A 4,4'-DDD	6.114	6.794	32147322	354.2E6	19.327	20.836
17)	MA 4,4'-DDT	6.355	7.092	32048829	344.2E6	18.891	20.681
20)	A Methoxychlor	6.902	7.551	95760088	832.6E6	101.687	105.519

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061421\
Data File : PD063819.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2021 12:03
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 12:56:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 14 12:55:47 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

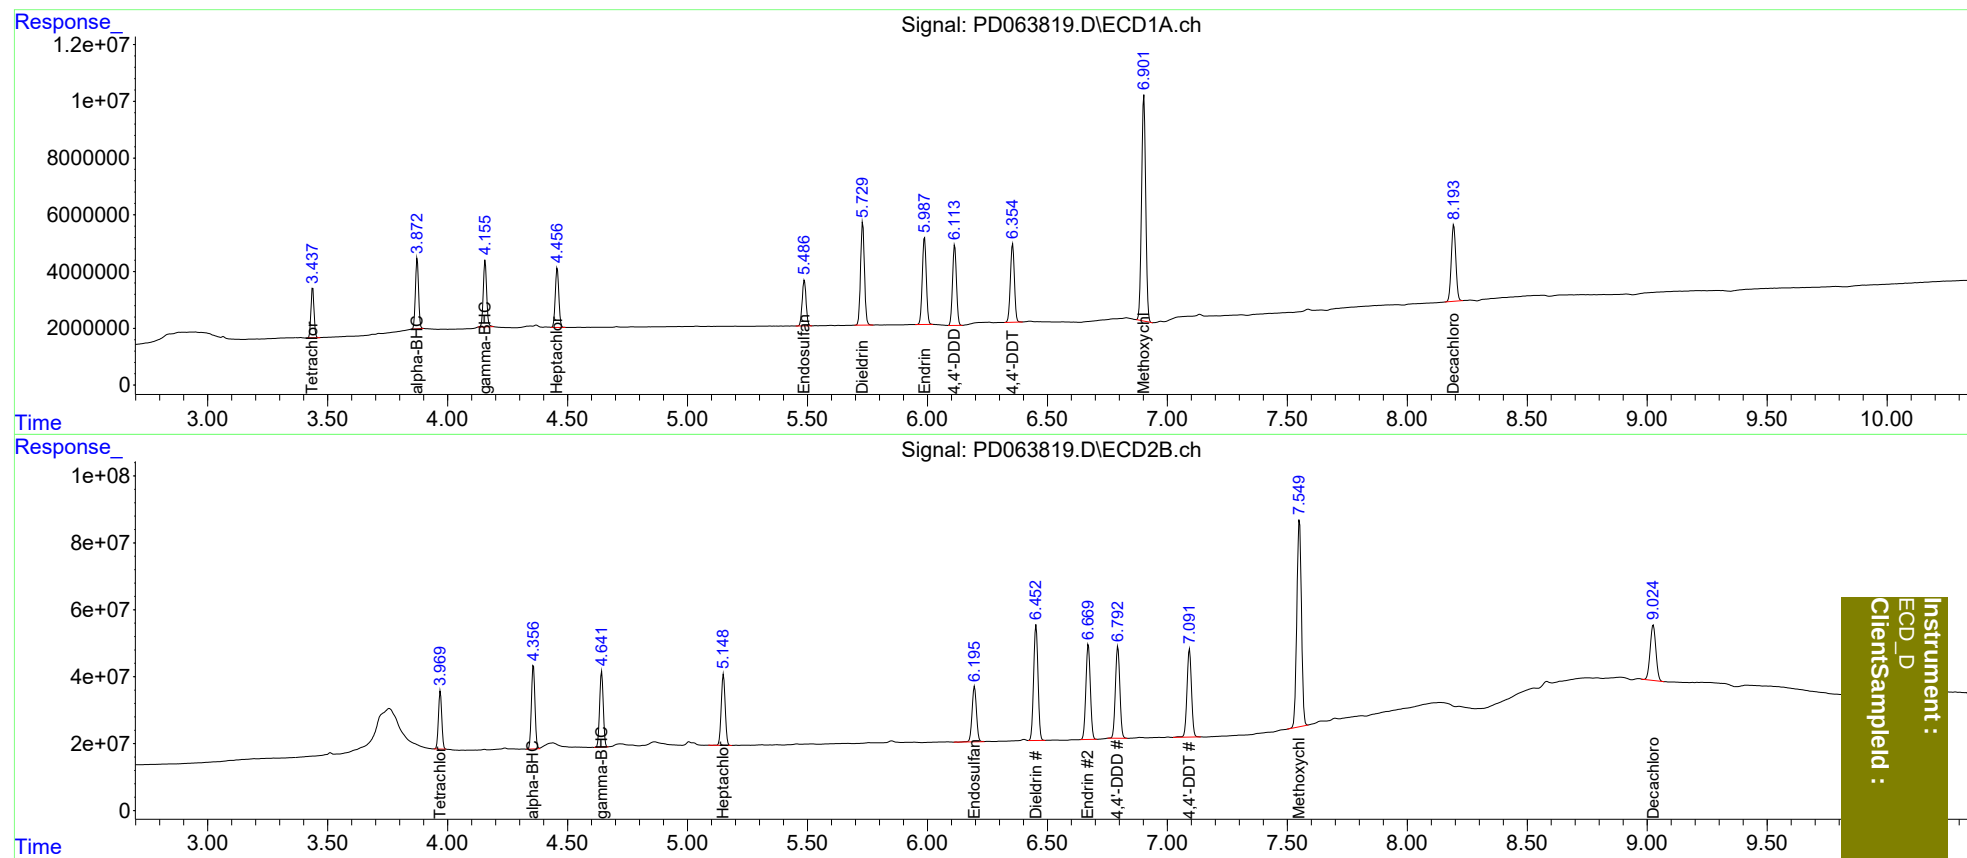


Instrument :
ECD_D
ClientSampled :

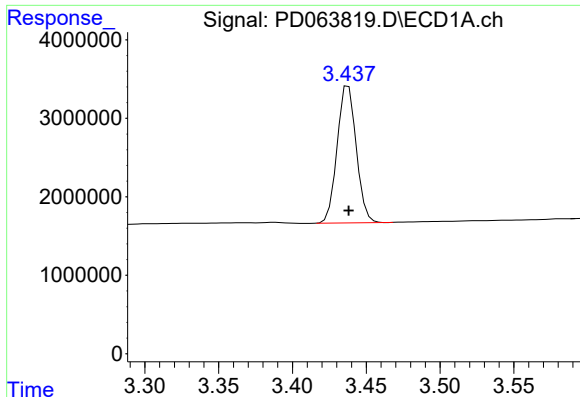

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: 0.000 min
Response: 15751085
Conc: 10.13 ng/ml

Instrument :
ECD_D
ClientSampleId :

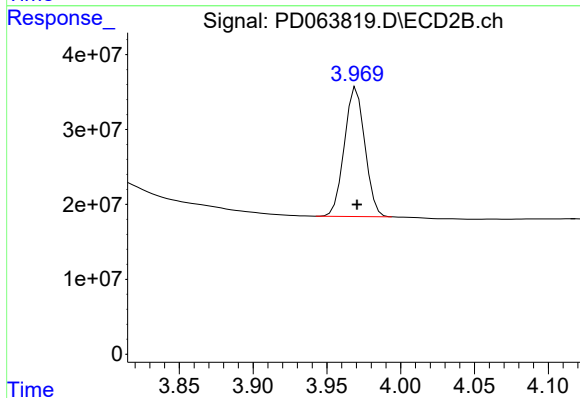


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 166469770
Conc: 10.43 ng/ml

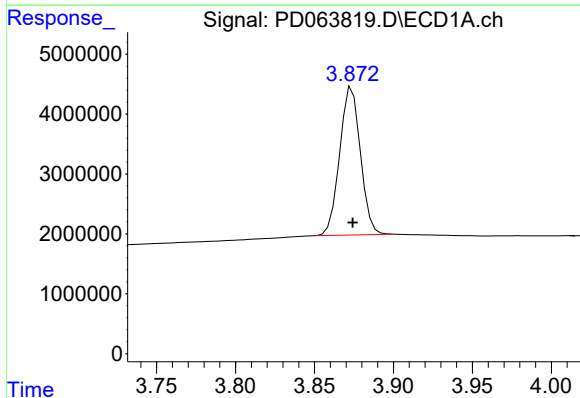


#2 alpha-BHC

R.T.: 3.874 min
Delta R.T.: 0.000 min
Response: 22654642
Conc: 9.74 ng/ml

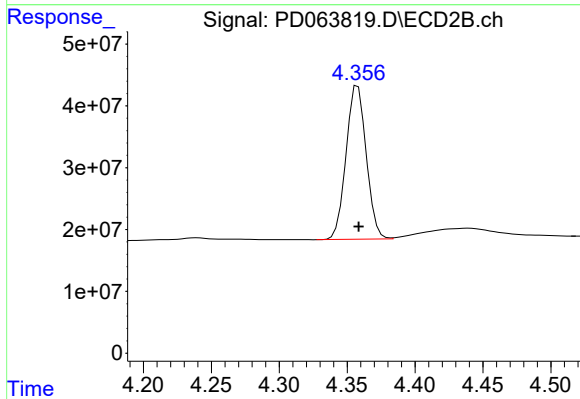

#2 alpha-BHC


R.T.: 4.358 min
Delta R.T.: 0.000 min
Response: 257070925
Conc: 10.31 ng/ml

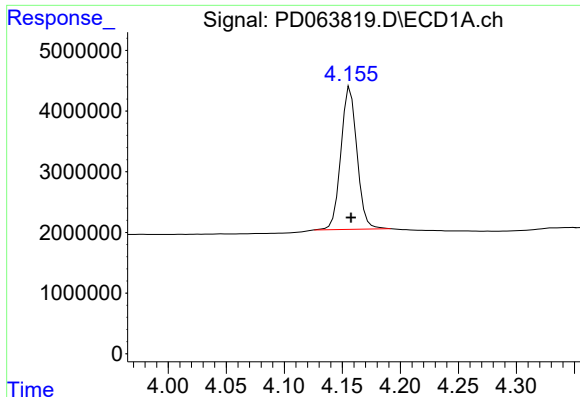

#3 gamma-BHC (Lindane)


R.T.: 4.157 min
Delta R.T.: 0.000 min
Response: 22689591
Conc: 10.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

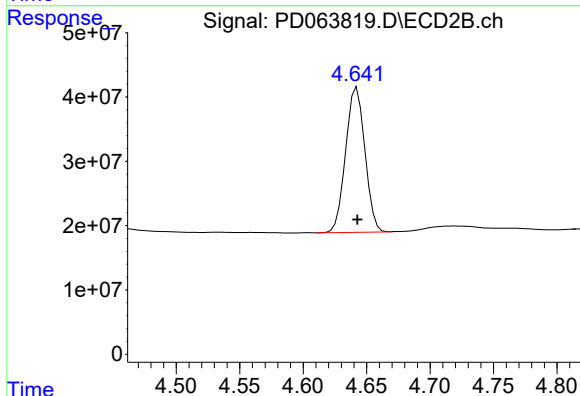


#3 gamma-BHC (Lindane)

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 237513953
Conc: 10.36 ng/ml

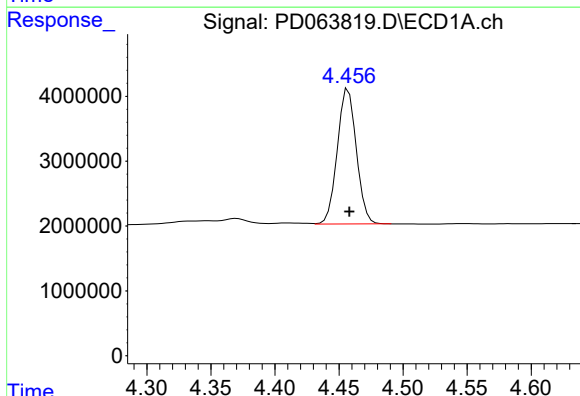


#4 Heptachlor

R.T.: 4.457 min
Delta R.T.: 0.000 min
Response: 21524544
Conc: 9.92 ng/ml

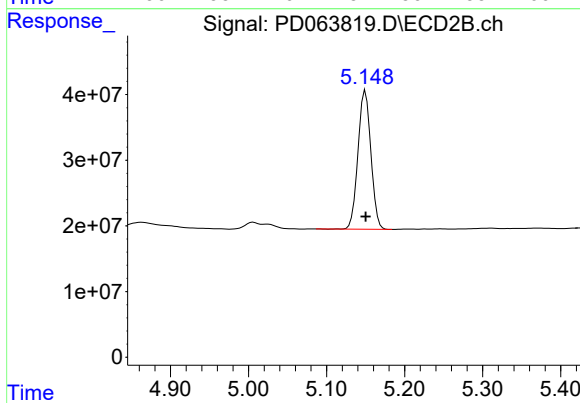

#4 Heptachlor


R.T.: 5.150 min
Delta R.T.: 0.000 min
Response: 243050407
Conc: 10.40 ng/ml

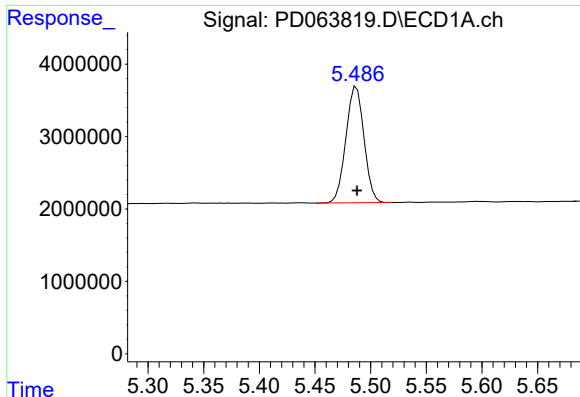

#9 Endosulfan I


R.T.: 5.487 min
Delta R.T.: 0.000 min
Response: 18181445
Conc: 9.99 ng/ml

Instrument :
ECD_D
ClientSampleId :

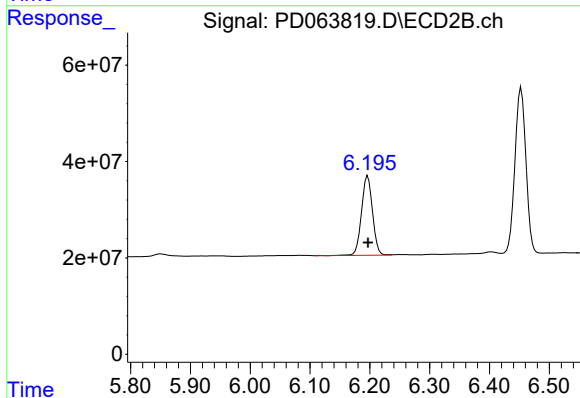


#9 Endosulfan I

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 210901437
Conc: 10.61 ng/ml

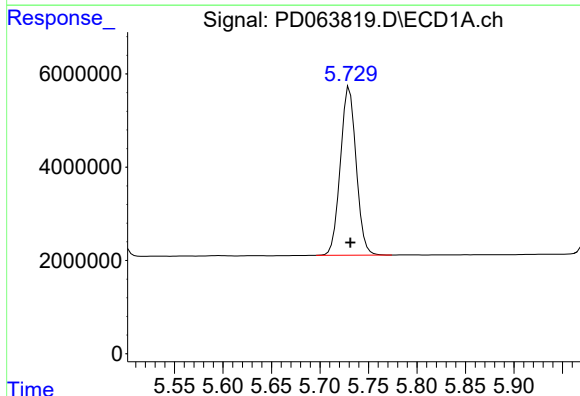


#13 Dieldrin

R.T.: 5.730 min
Delta R.T.: -0.001 min
Response: 40898963
Conc: 19.52 ng/ml

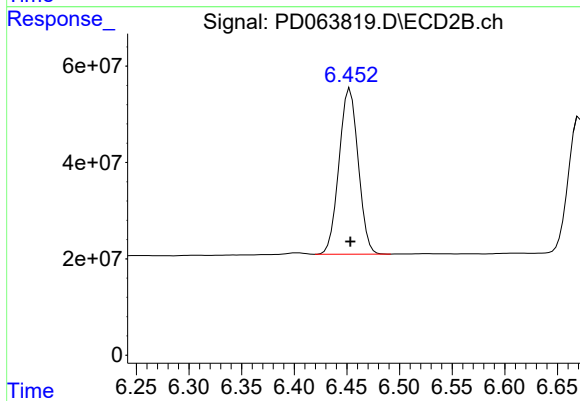

#13 Dieldrin


R.T.: 6.453 min
Delta R.T.: 0.000 min
Response: 437863527
Conc: 20.80 ng/ml

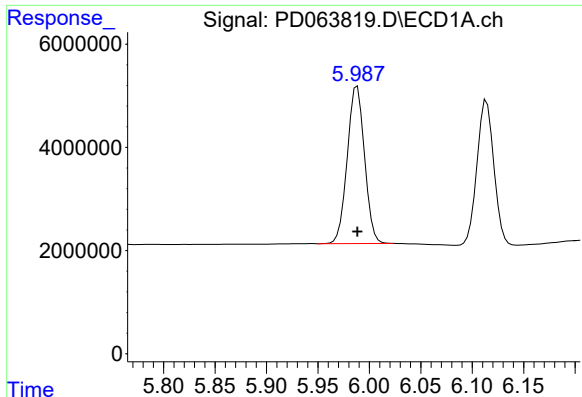

#14 Endrin


R.T.: 5.988 min
Delta R.T.: 0.000 min
Response: 35659250
Conc: 19.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

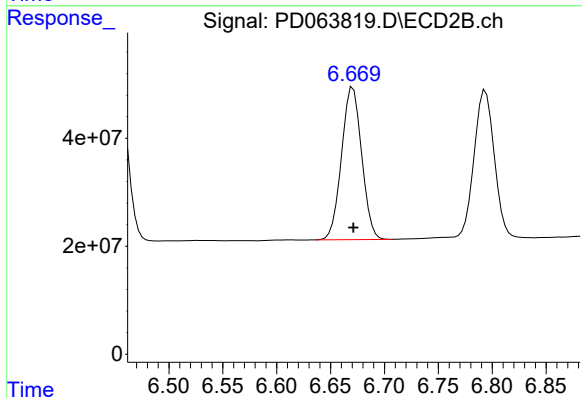


#14 Endrin

R.T.: 6.671 min
Delta R.T.: 0.000 min
Response: 367323099
Conc: 20.87 ng/ml

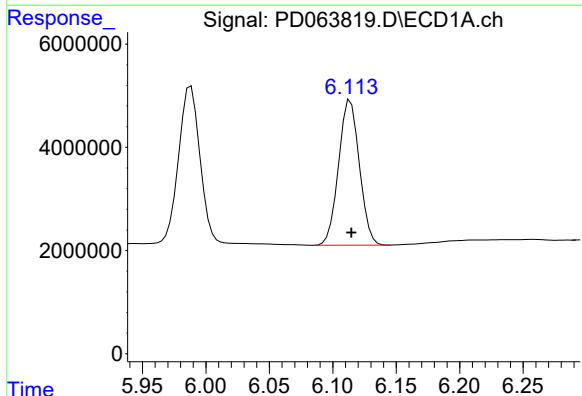


#16 4,4'-DDD

R.T.: 6.114 min
Delta R.T.: 0.000 min
Response: 32147322
Conc: 19.33 ng/ml

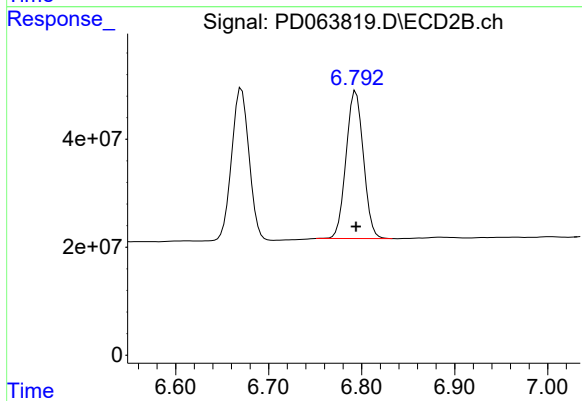

#16 4,4'-DDD


R.T.: 6.794 min
Delta R.T.: 0.000 min
Response: 354207478
Conc: 20.84 ng/ml

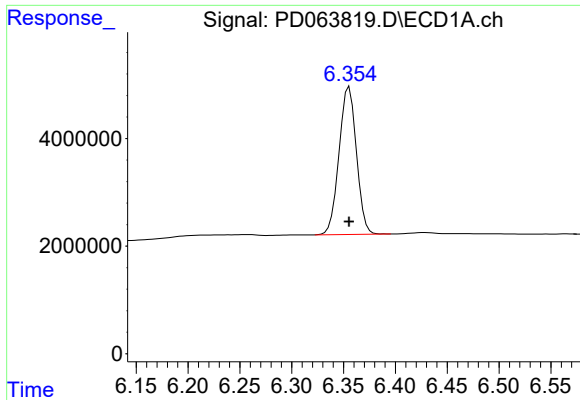

#17 4,4'-DDT


R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 32048829
Conc: 18.89 ng/ml

Instrument :
ECD_D
ClientSampleId :

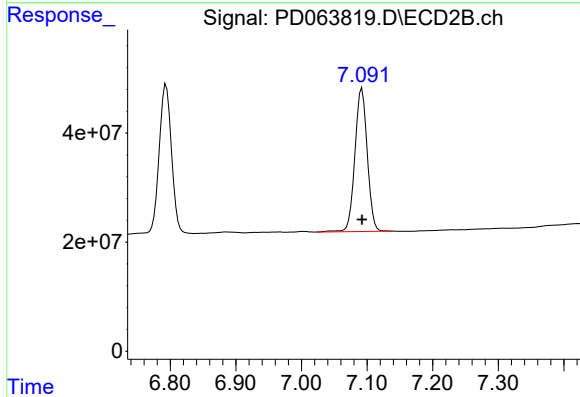


#17 4,4'-DDT

R.T.: 7.092 min
Delta R.T.: 0.000 min
Response: 344170688
Conc: 20.68 ng/ml

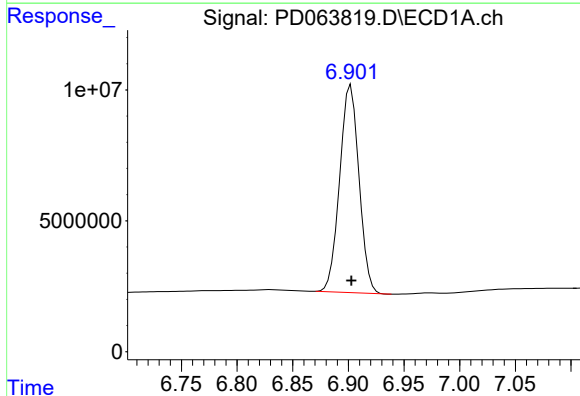


#20 Methoxychlor

R.T.: 6.902 min
Delta R.T.: 0.000 min
Response: 95760088
Conc: 101.69 ng/ml

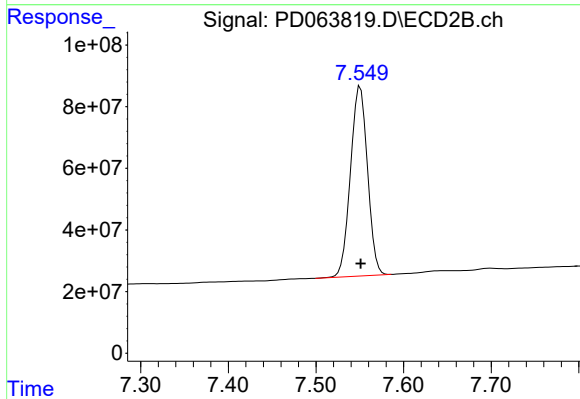

#20 Methoxychlor

R.T.: 7.551 min
Delta R.T.: 0.000 min
Response: 832555403
Conc: 105.52 ng/ml

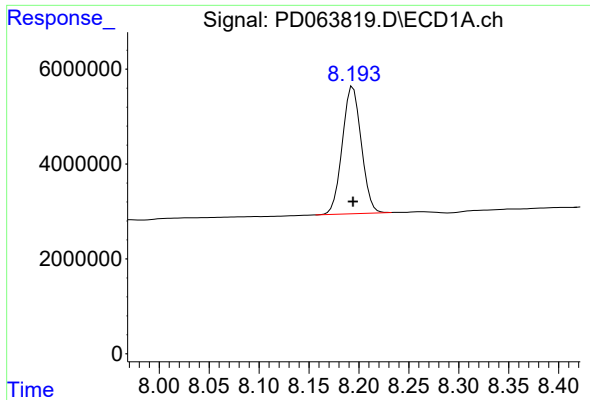

#27 Decachlorobiphenyl


R.T.: 8.194 min

Delta R.T.: 0.000 min

Response: 35444059

Conc: 20.47 ng/ml

Instrument :
ECD_D
ClientSampleId :

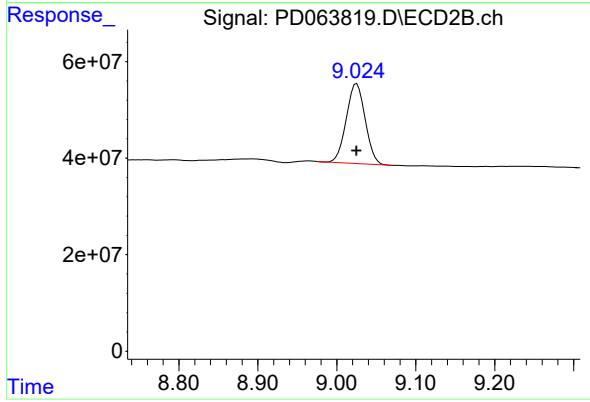

#27 Decachlorobiphenyl

R.T.: 9.025 min

Delta R.T.: 0.000 min

Response: 274478502

Conc: 19.54 ng/ml