

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061421\
 Data File : PD063821.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2021 12:30
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 12:56:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 14 12:55:47 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.970	31099038	319.3E6	20.000	20.000
27)	SA Decachlor...	8.194	9.025	69268533	561.8E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.874	4.359	46511611	498.8E6	20.000	20.000
3)	MA gamma-BHC...	4.157	4.643	45115018	458.4E6	20.000	20.000
4)	MA Heptachlor	4.458	5.150	43391096	467.2E6	20.000	20.000
9)	A Endosulfan I	5.488	6.197	36412389	397.7E6	20.000	20.000
13)	MA Dieldrin	5.731	6.453	83796879	842.2E6	40.000	40.000
14)	MA Endrin	5.988	6.671	72391427	704.0E6	40.000	40.000
16)	A 4,4'-DDD	6.115	6.794	66533882	680.0E6	40.000	40.000
17)	MA 4,4'-DDT	6.355	7.092	67861801	665.7E6	40.000	40.000
20)	A Methoxychlor	6.903	7.551	188.3E6	1578.0E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061421\
Data File : PD063821.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2021 12:30
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 12:56:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 14 12:55:47 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

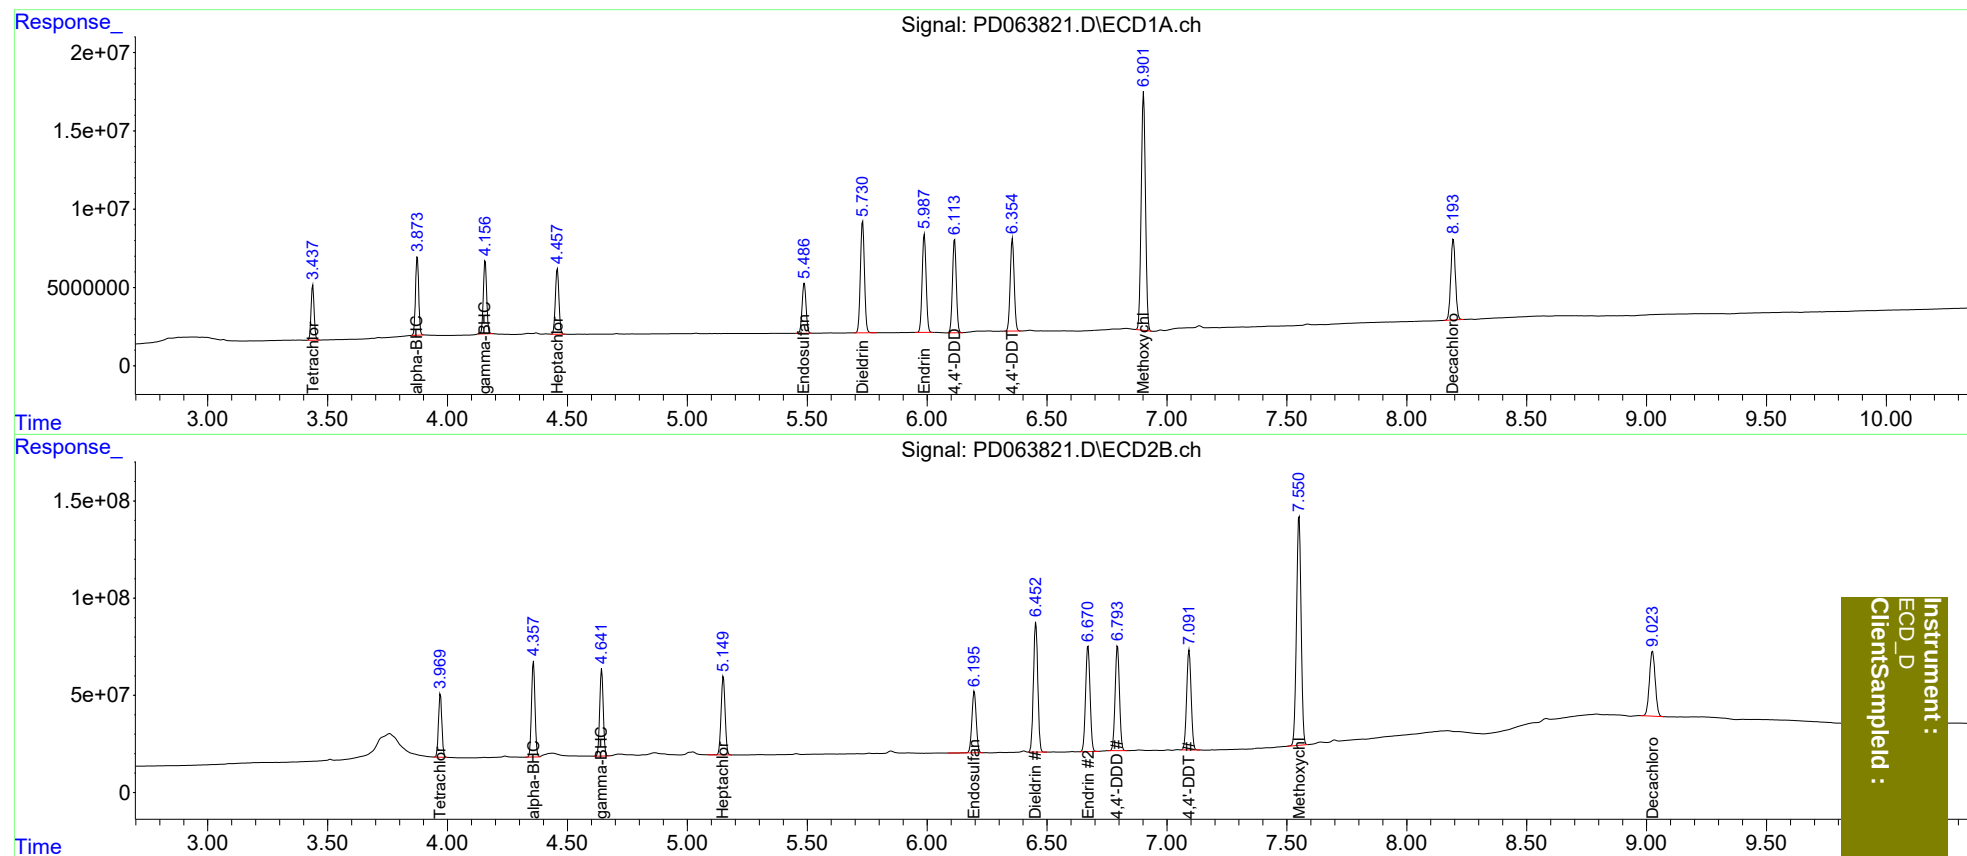


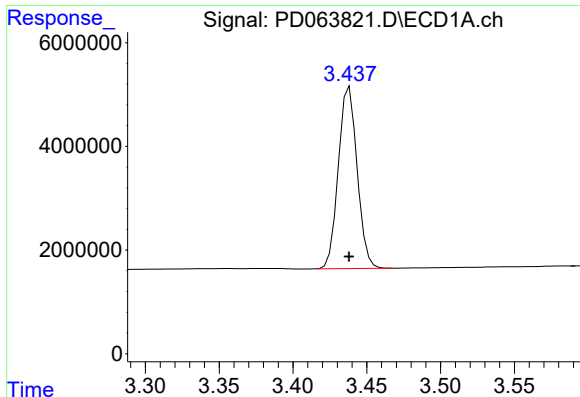

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: 0.000 min
Response: 31099038
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

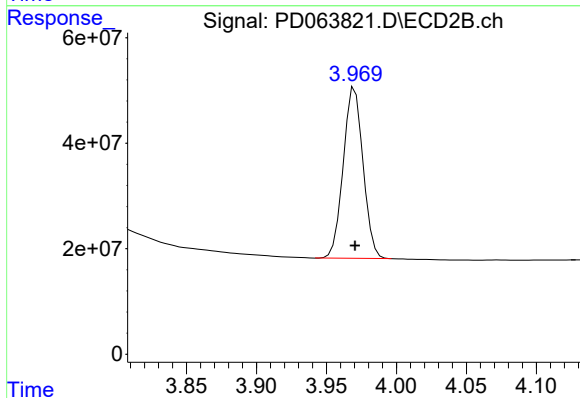


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 319336100
Conc: 20.00 ng/ml

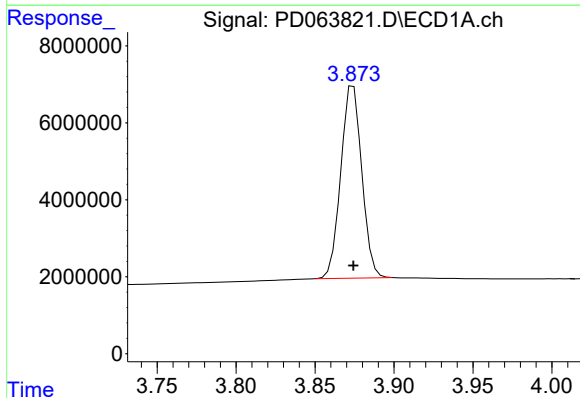


#2 alpha-BHC

R.T.: 3.874 min
Delta R.T.: 0.000 min
Response: 46511611
Conc: 20.00 ng/ml

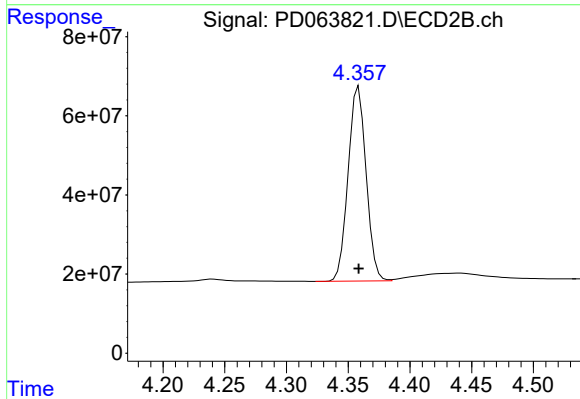

#2 alpha-BHC


R.T.: 4.359 min
Delta R.T.: 0.000 min
Response: 498751551
Conc: 20.00 ng/ml

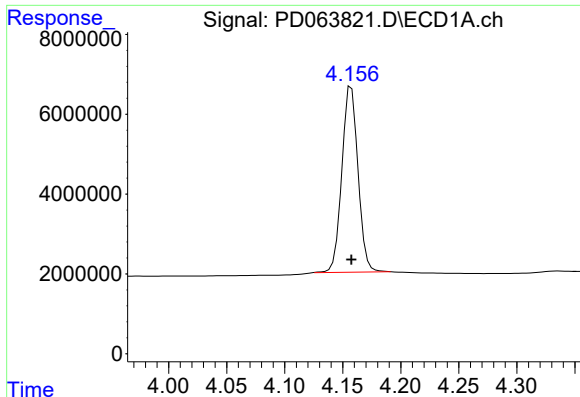

#3 gamma-BHC (Lindane)


R.T.: 4.157 min
Delta R.T.: 0.000 min
Response: 45115018
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

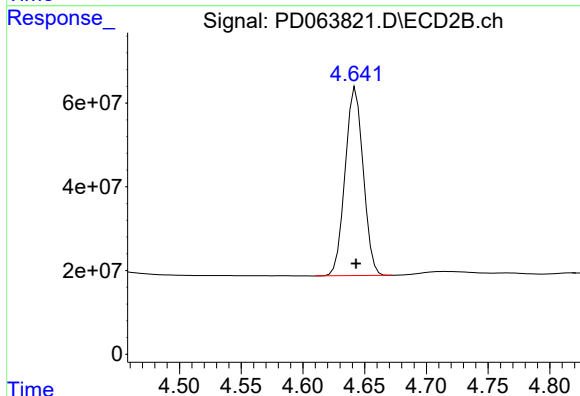


#3 gamma-BHC (Lindane)

R.T.: 4.643 min
Delta R.T.: 0.000 min
Response: 458447539
Conc: 20.00 ng/ml

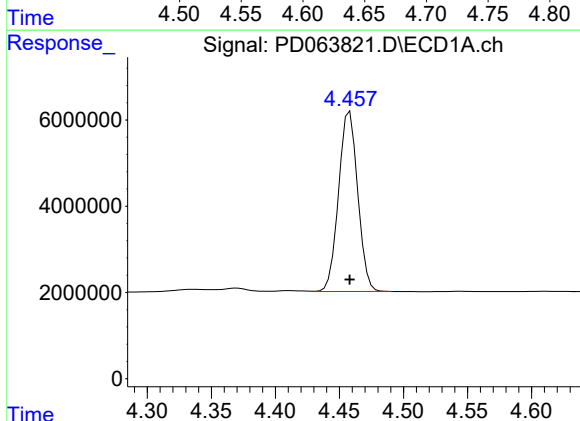


#4 Heptachlor

R.T.: 4.458 min
Delta R.T.: 0.000 min
Response: 43391096
Conc: 20.00 ng/ml

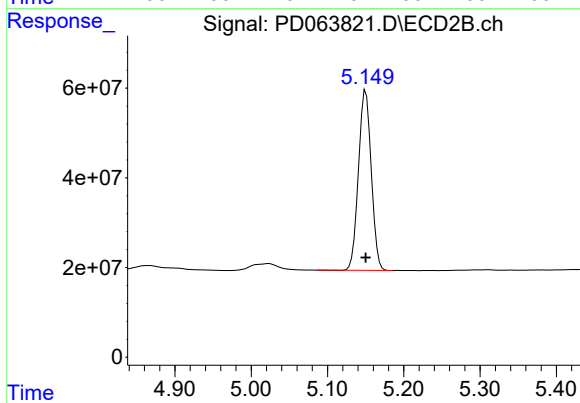

#4 Heptachlor


R.T.: 5.150 min
Delta R.T.: 0.000 min
Response: 467233232
Conc: 20.00 ng/ml

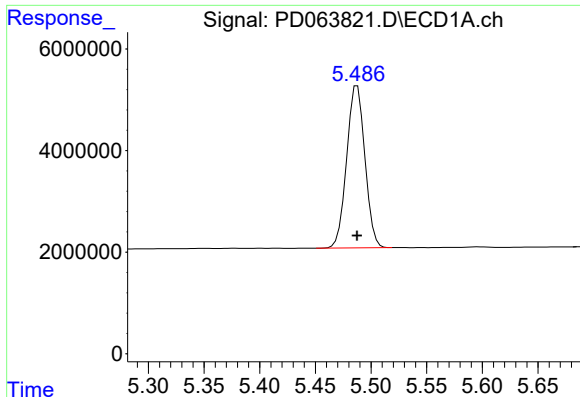

#9 Endosulfan I


R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 36412389
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

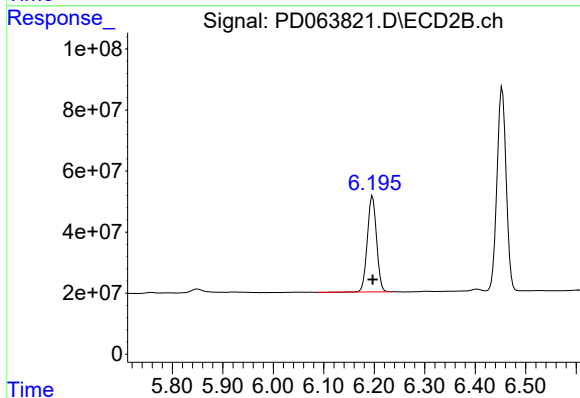


#9 Endosulfan I

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 397684848
Conc: 20.00 ng/ml

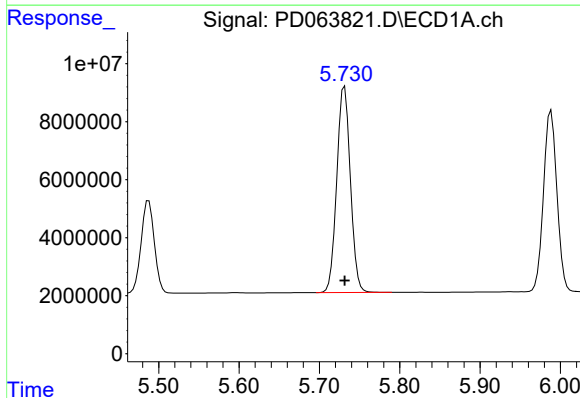


#13 Dieldrin

R.T.: 5.731 min
Delta R.T.: 0.000 min
Response: 83796879
Conc: 40.00 ng/ml

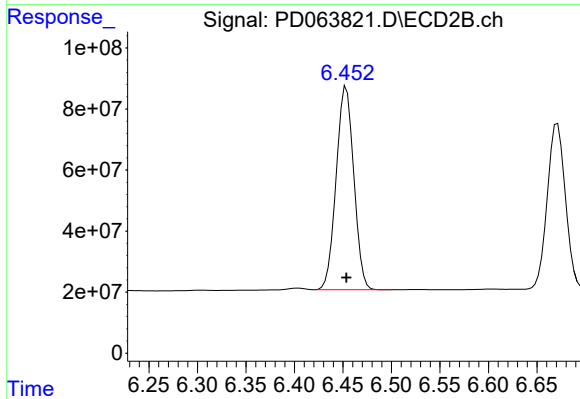

#13 Dieldrin


R.T.: 6.453 min
Delta R.T.: 0.000 min
Response: 842180215
Conc: 40.00 ng/ml

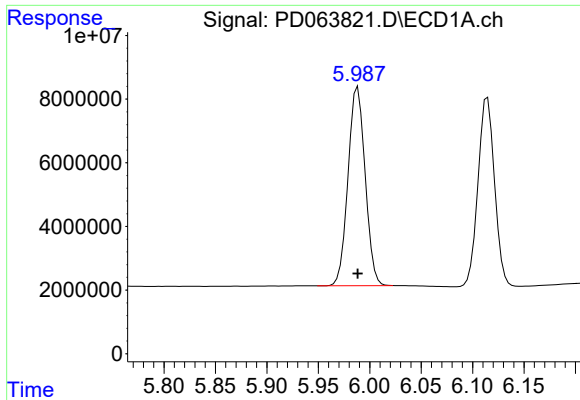

#14 Endrin


R.T.: 5.988 min
Delta R.T.: 0.000 min
Response: 72391427
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

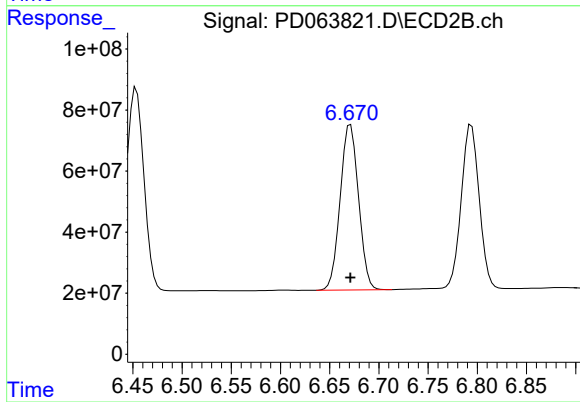


#14 Endrin

R.T.: 6.671 min
Delta R.T.: 0.000 min
Response: 704039696
Conc: 40.00 ng/ml

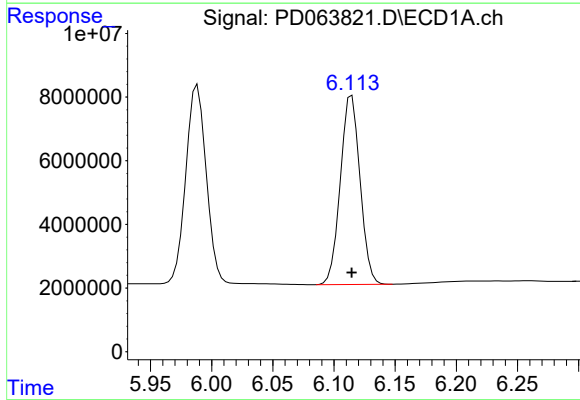


#16 4,4'-DDD

R.T.: 6.115 min
Delta R.T.: 0.000 min
Response: 66533882
Conc: 40.00 ng/ml

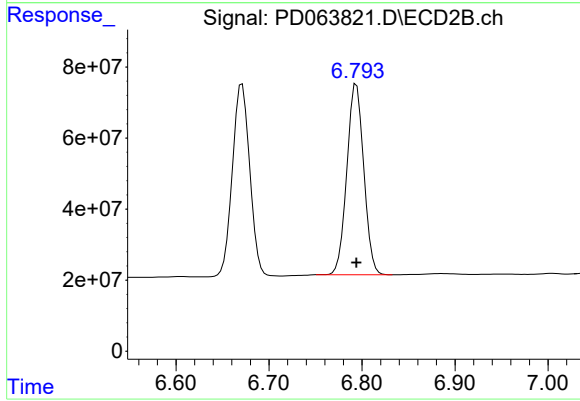

#16 4,4'-DDD


R.T.: 6.794 min
Delta R.T.: 0.000 min
Response: 679976182
Conc: 40.00 ng/ml

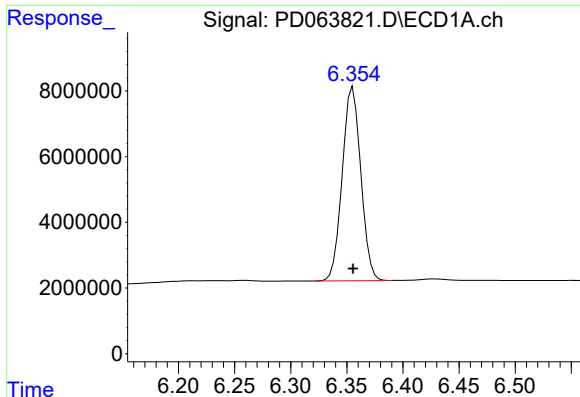

#17 4,4'-DDT


R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 67861801
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

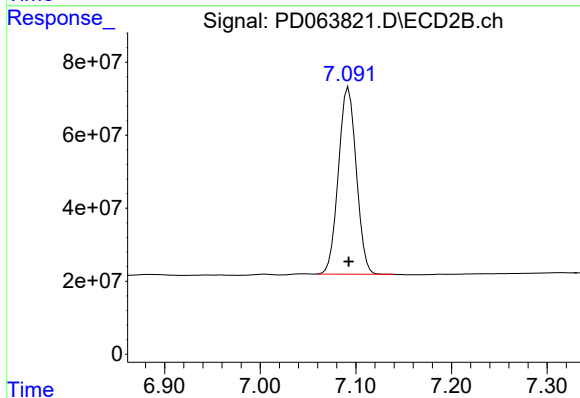


#17 4,4'-DDT

R.T.: 7.092 min
Delta R.T.: 0.000 min
Response: 665676761
Conc: 40.00 ng/ml

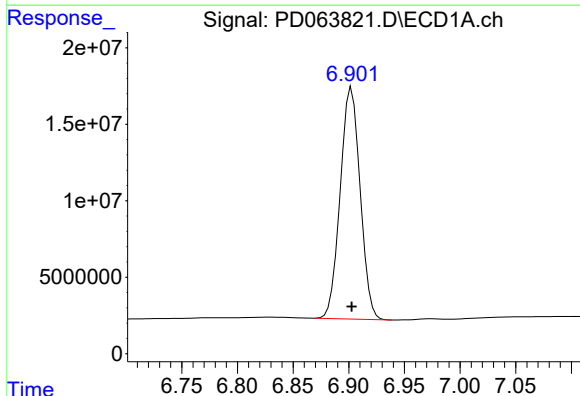


#20 Methoxychlor

R.T.: 6.903 min
Delta R.T.: 0.000 min
Response: 188342669
Conc: 200.00 ng/ml

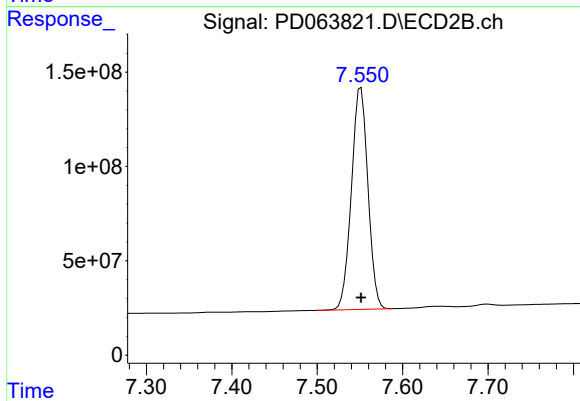

#20 Methoxychlor


R.T.: 7.551 min
Delta R.T.: 0.000 min
Response: 1578019284
Conc: 200.00 ng/ml

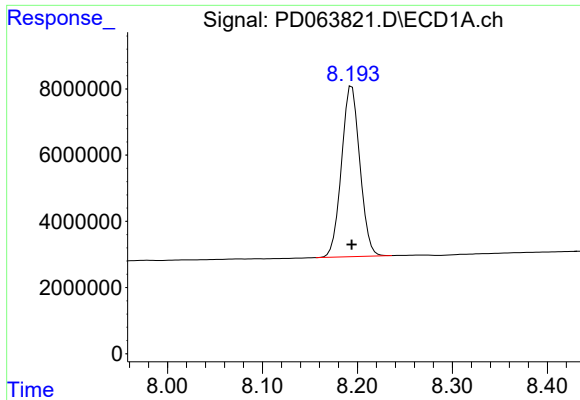

#27 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 69268533
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

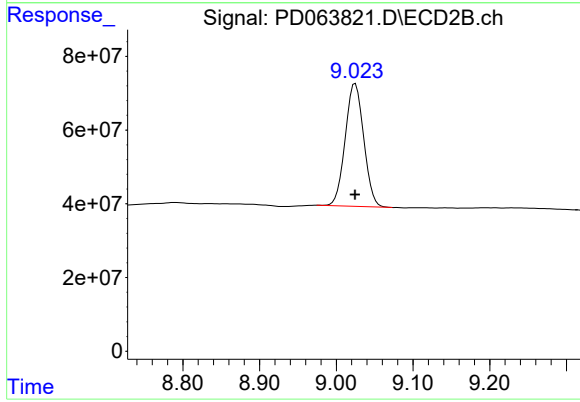

#27 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.000 min
Response: 561828563
Conc: 40.00 ng/ml