

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061421\
 Data File : PD063823.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2021 12:58
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 13:22:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 14 12:59:06 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.971	61803901	609.5E6	39.453	36.960
27)	SA Decachlor...	8.194	9.026	136.4E6	1106.9E6	77.058	78.689
Target Compounds							
2)	A alpha-BHC	3.874	4.359	96900158	967.1E6	42.752	37.777
3)	MA gamma-BHC...	4.158	4.643	91935560	887.4E6	40.735	37.741
4)	MA Heptachlor	4.458	5.150	89321241	899.0E6	41.664	37.166
9)	A Endosulfan I	5.488	6.197	74446004	766.5E6	41.153	37.162
13)	MA Dieldrin	5.732	6.453	173.7E6	1627.9E6	85.282	75.171
14)	MA Endrin	5.989	6.671	148.8E6	1351.6E6	83.758	74.424
16)	A 4,4'-DDD	6.115	6.794	138.2E6	1306.6E6	86.521	75.105
17)	MA 4,4'-DDT	6.356	7.093	144.7E6	1297.0E6	91.189	77.626
20)	A Methoxychlor	6.903	7.551	368.2E6	2916.5E6	388.820	354.233


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061421\
Data File : PD063823.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2021 12:58
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 13:22:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 14 12:59:06 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

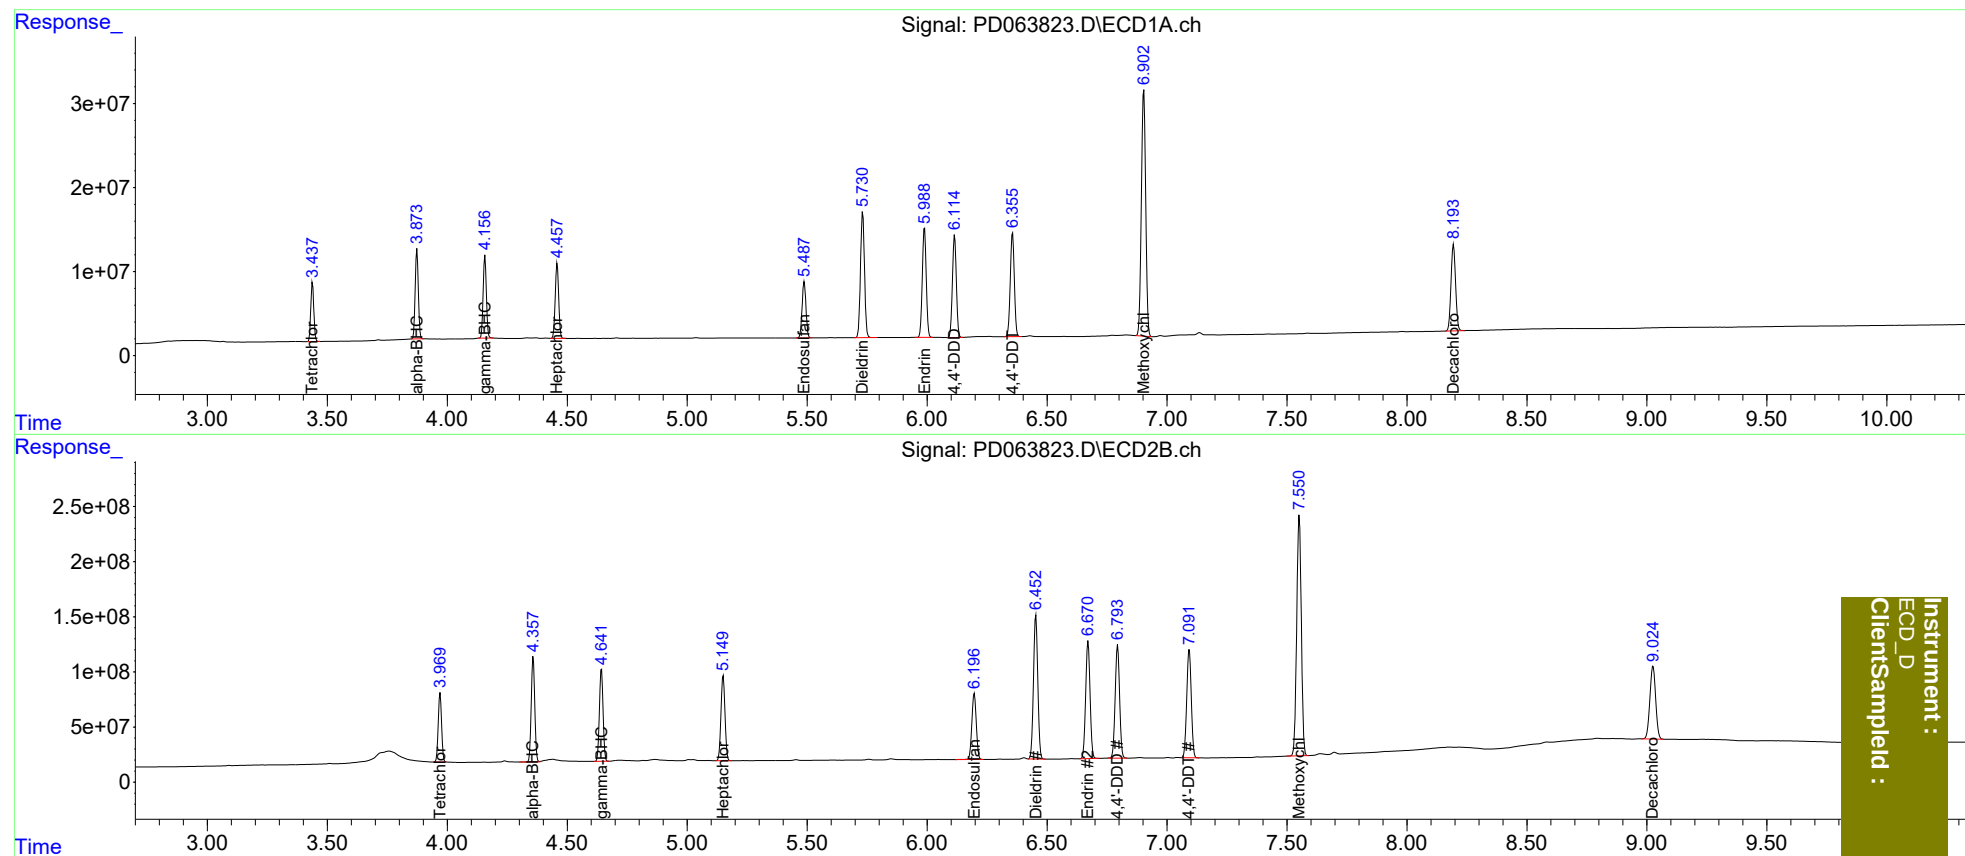


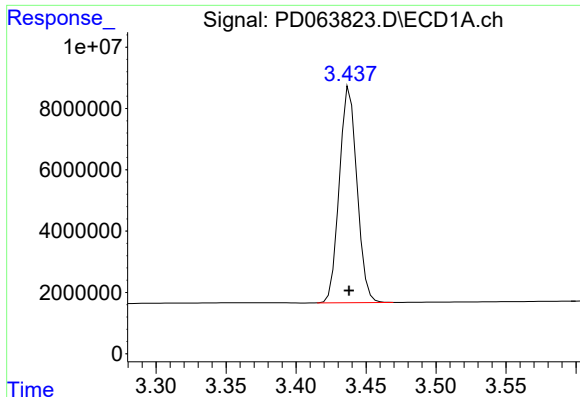

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: 0.000 min
Response: 61803901
Conc: 39.45 ng/ml

Instrument :
ECD_D
ClientSampleId :

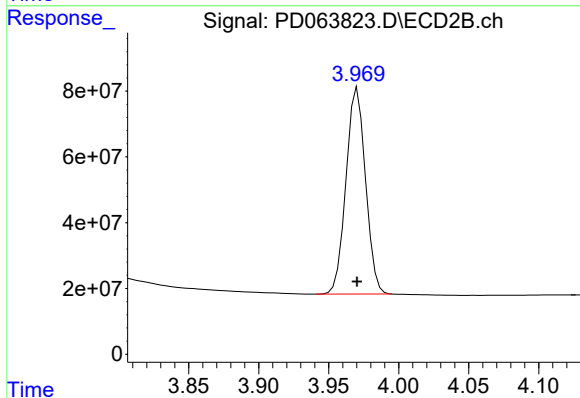


#1 Tetrachloro-m-xylene

R.T.: 3.971 min
Delta R.T.: 0.000 min
Response: 609470749
Conc: 36.96 ng/ml

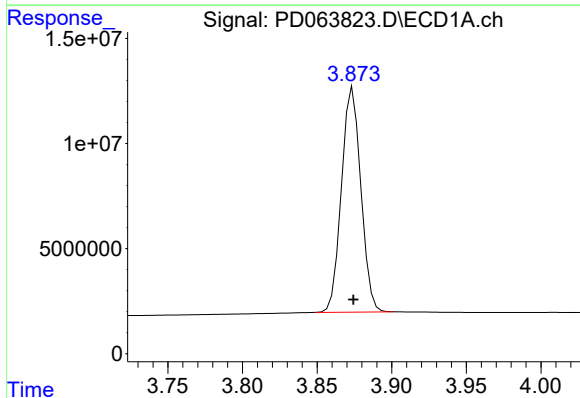


#2 alpha-BHC

R.T.: 3.874 min
Delta R.T.: 0.000 min
Response: 96900158
Conc: 42.75 ng/ml

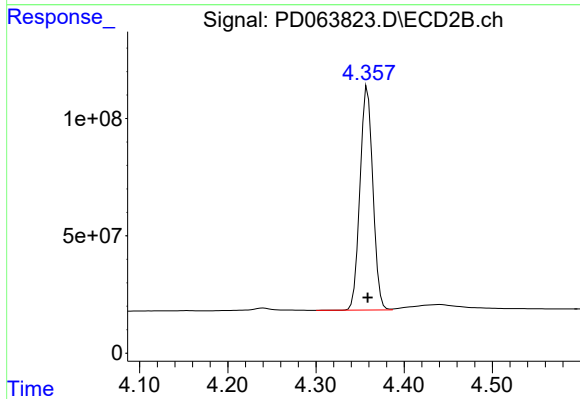

#2 alpha-BHC


R.T.: 4.359 min
Delta R.T.: 0.000 min
Response: 967139544
Conc: 37.78 ng/ml

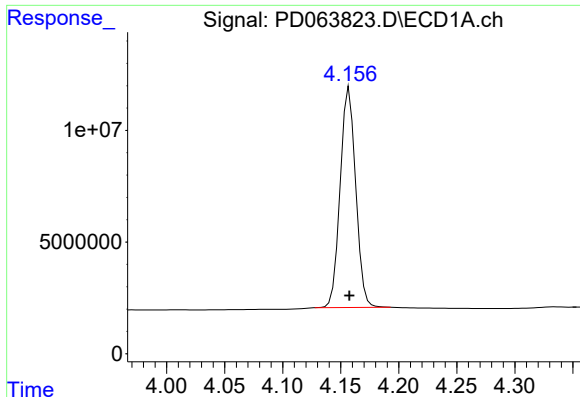

#3 gamma-BHC (Lindane)


R.T.: 4.158 min
Delta R.T.: 0.000 min
Response: 91935560
Conc: 40.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

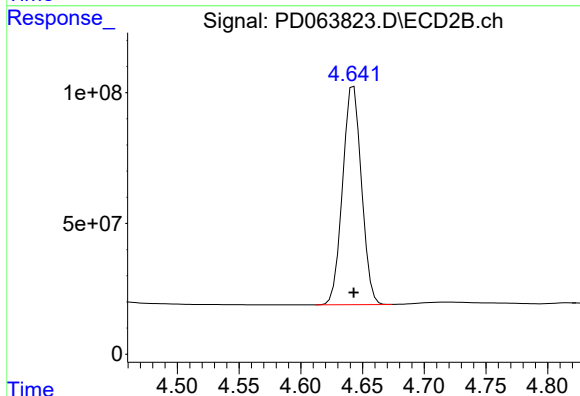


#3 gamma-BHC (Lindane)

R.T.: 4.643 min
Delta R.T.: 0.000 min
Response: 887436597
Conc: 37.74 ng/ml

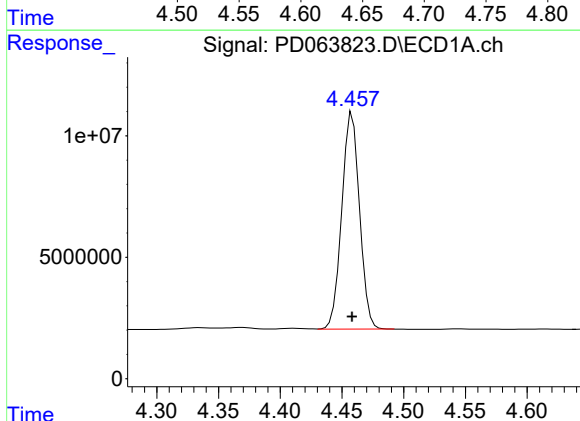


#4 Heptachlor

R.T.: 4.458 min
Delta R.T.: 0.000 min
Response: 89321241
Conc: 41.66 ng/ml

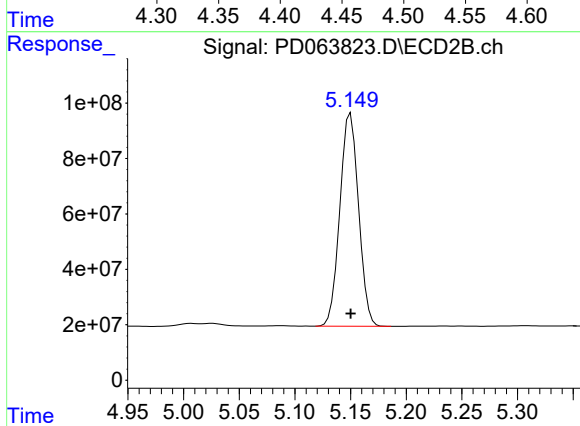

#4 Heptachlor


R.T.: 5.150 min
Delta R.T.: 0.000 min
Response: 899042103
Conc: 37.17 ng/ml

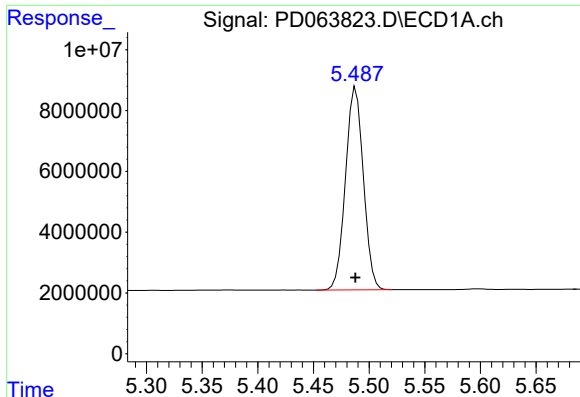

#9 Endosulfan I


R.T.: 5.488 min
Delta R.T.: 0.000 min
Response: 74446004
Conc: 41.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

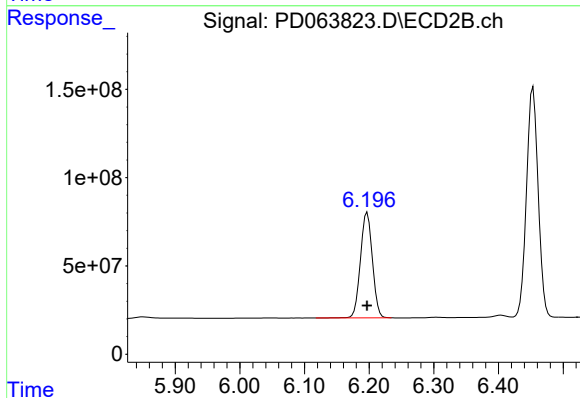


#9 Endosulfan I

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 766517333
Conc: 37.16 ng/ml

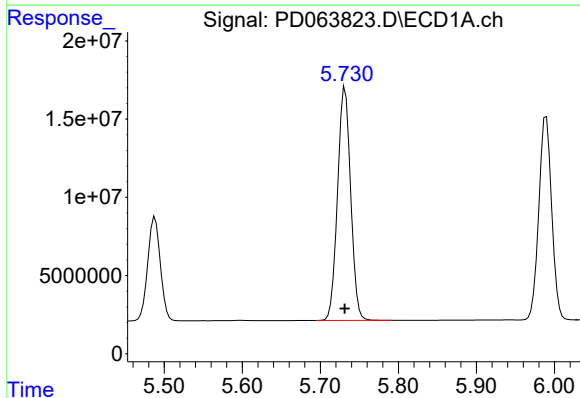


#13 Dieldrin

R.T.: 5.732 min
Delta R.T.: 0.000 min
Response: 173745714
Conc: 85.28 ng/ml

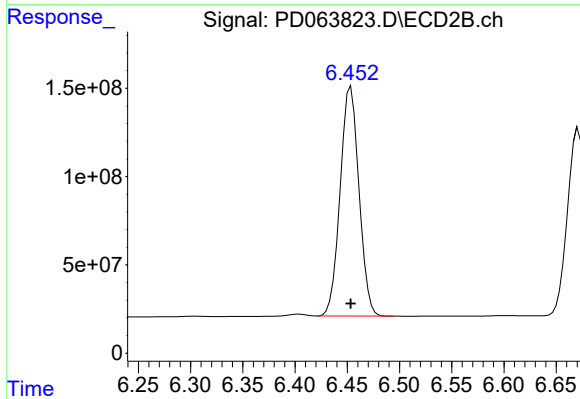

#13 Dieldrin


R.T.: 6.453 min
Delta R.T.: 0.000 min
Response: 1627910017
Conc: 75.17 ng/ml

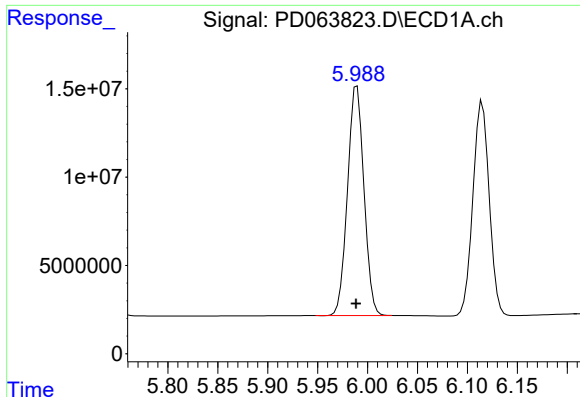

#14 Endrin


R.T.: 5.989 min
Delta R.T.: 0.001 min
Response: 148830043
Conc: 83.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

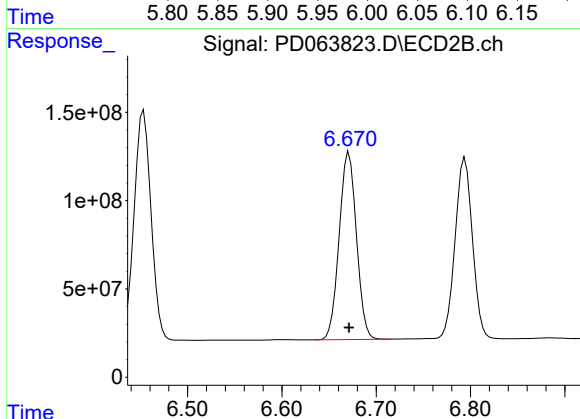


#14 Endrin

R.T.: 6.671 min
Delta R.T.: 0.000 min
Response: 1351567901
Conc: 74.42 ng/ml

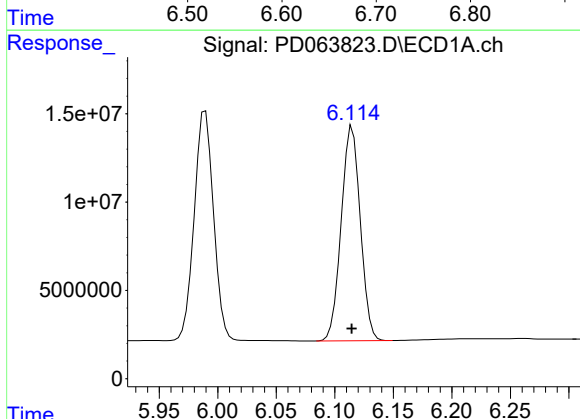


#16 4,4'-DDD

R.T.: 6.115 min
Delta R.T.: 0.000 min
Response: 138203721
Conc: 86.52 ng/ml

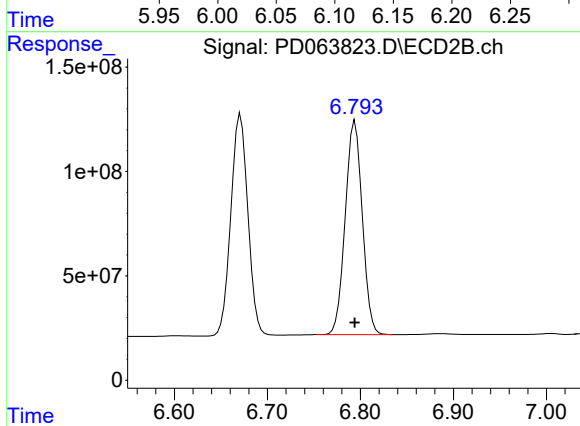

#16 4,4'-DDD


R.T.: 6.794 min
Delta R.T.: 0.000 min
Response: 1306622363
Conc: 75.10 ng/ml

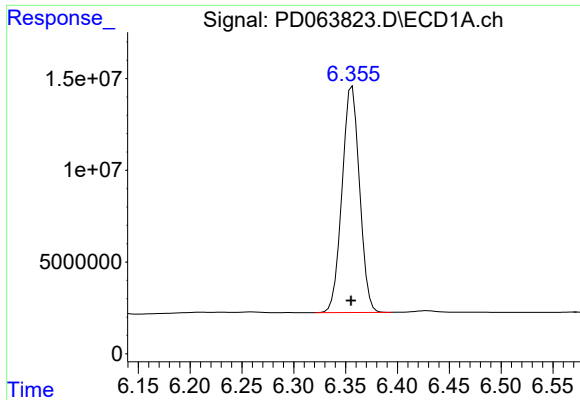

#17 4,4'-DDT


R.T.: 6.356 min
Delta R.T.: 0.000 min
Response: 144672812
Conc: 91.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

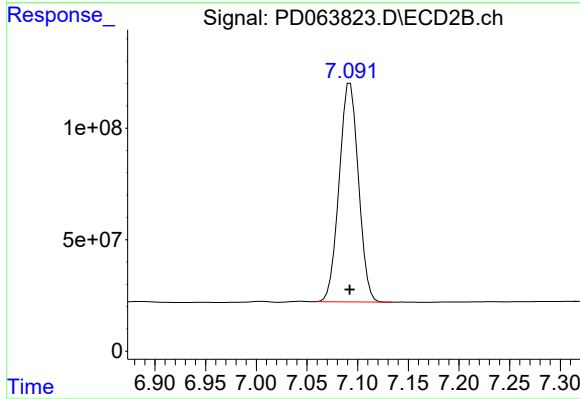


#17 4,4'-DDT

R.T.: 7.093 min
Delta R.T.: 0.000 min
Response: 1296961309
Conc: 77.63 ng/ml

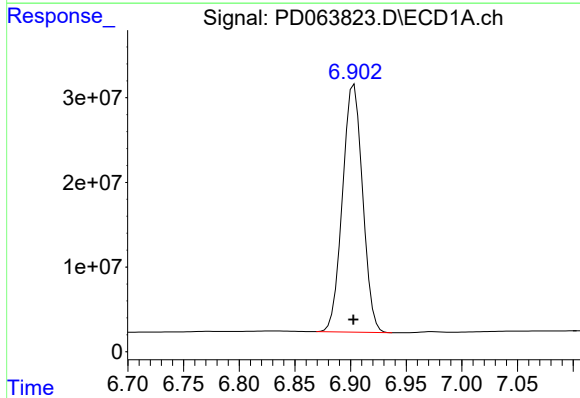


#20 Methoxychlor

R.T.: 6.903 min
Delta R.T.: 0.000 min
Response: 368161047
Conc: 388.82 ng/ml

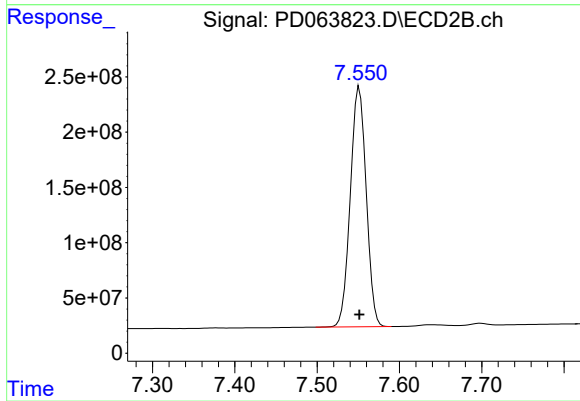

#20 Methoxychlor


R.T.: 7.551 min
Delta R.T.: 0.000 min
Response: 2916536349
Conc: 354.23 ng/ml

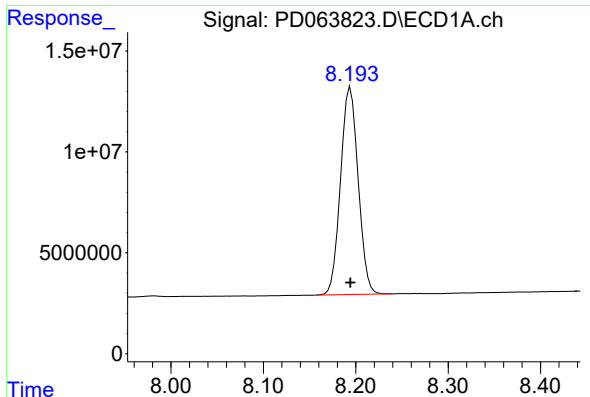

#27 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 136398848
Conc: 77.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

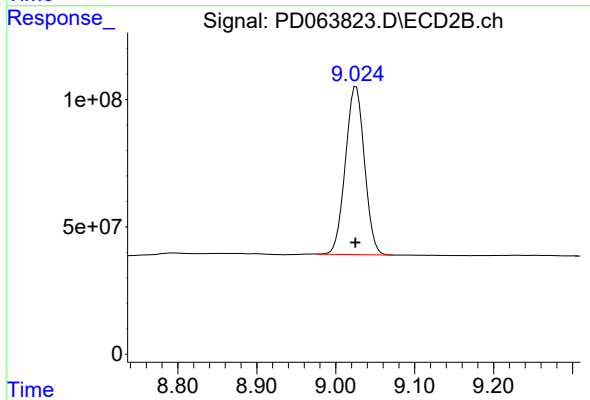

#27 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: 0.001 min
Response: 1106919319
Conc: 78.69 ng/ml