

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061421\
 Data File : PD063824.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2021 13:12
 Operator : AR\AJ
 Sample : INDB401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 13:51:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 14 13:50:13 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	3.970	58670839	582.4E6	40.057	38.392
27)	SA Decachlor...	8.194	9.025	133.8E6	1094.5E6	78.696	79.698
Target Compounds							
5)	MB Aldrin	4.706	5.454	83635521	862.0E6	41.543	38.951
6)	B beta-BHC	4.409	4.813	37845385	370.2E6	39.310	37.678
7)	B delta-BHC	4.613	5.029	89120741	869.6E6	41.861	38.741
8)	B Heptachlo...	5.149	5.840	77172829	777.6E6	40.929	38.225
10)	B trans-Chl...	5.375	6.074	79423100	822.7E6	41.132	38.689
11)	B cis-Chlor...	5.434	6.146	77227060	776.6E6	40.816	38.480
12)	B 4,4'-DDE	5.597	6.303	164.1E6	1572.4E6	83.281	77.671
15)	B Endosulfa...	6.262	6.880	133.8E6	1253.0E6	82.123	77.006
18)	B Endrin al...	6.431	7.004	114.8E6	1089.1E6	80.883	76.414
19)	B Endosulfa...	6.644	7.227	127.4E6	1273.4E6	81.905	76.995
21)	B Endrin ke...	7.136	7.698	156.5E6	1250.5E6	82.064	77.999

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061421\
Data File : PD063824.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2021 13:12
Operator : AR\AJ
Sample : INDB401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 13:51:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Mon Jun 14 13:50:13 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

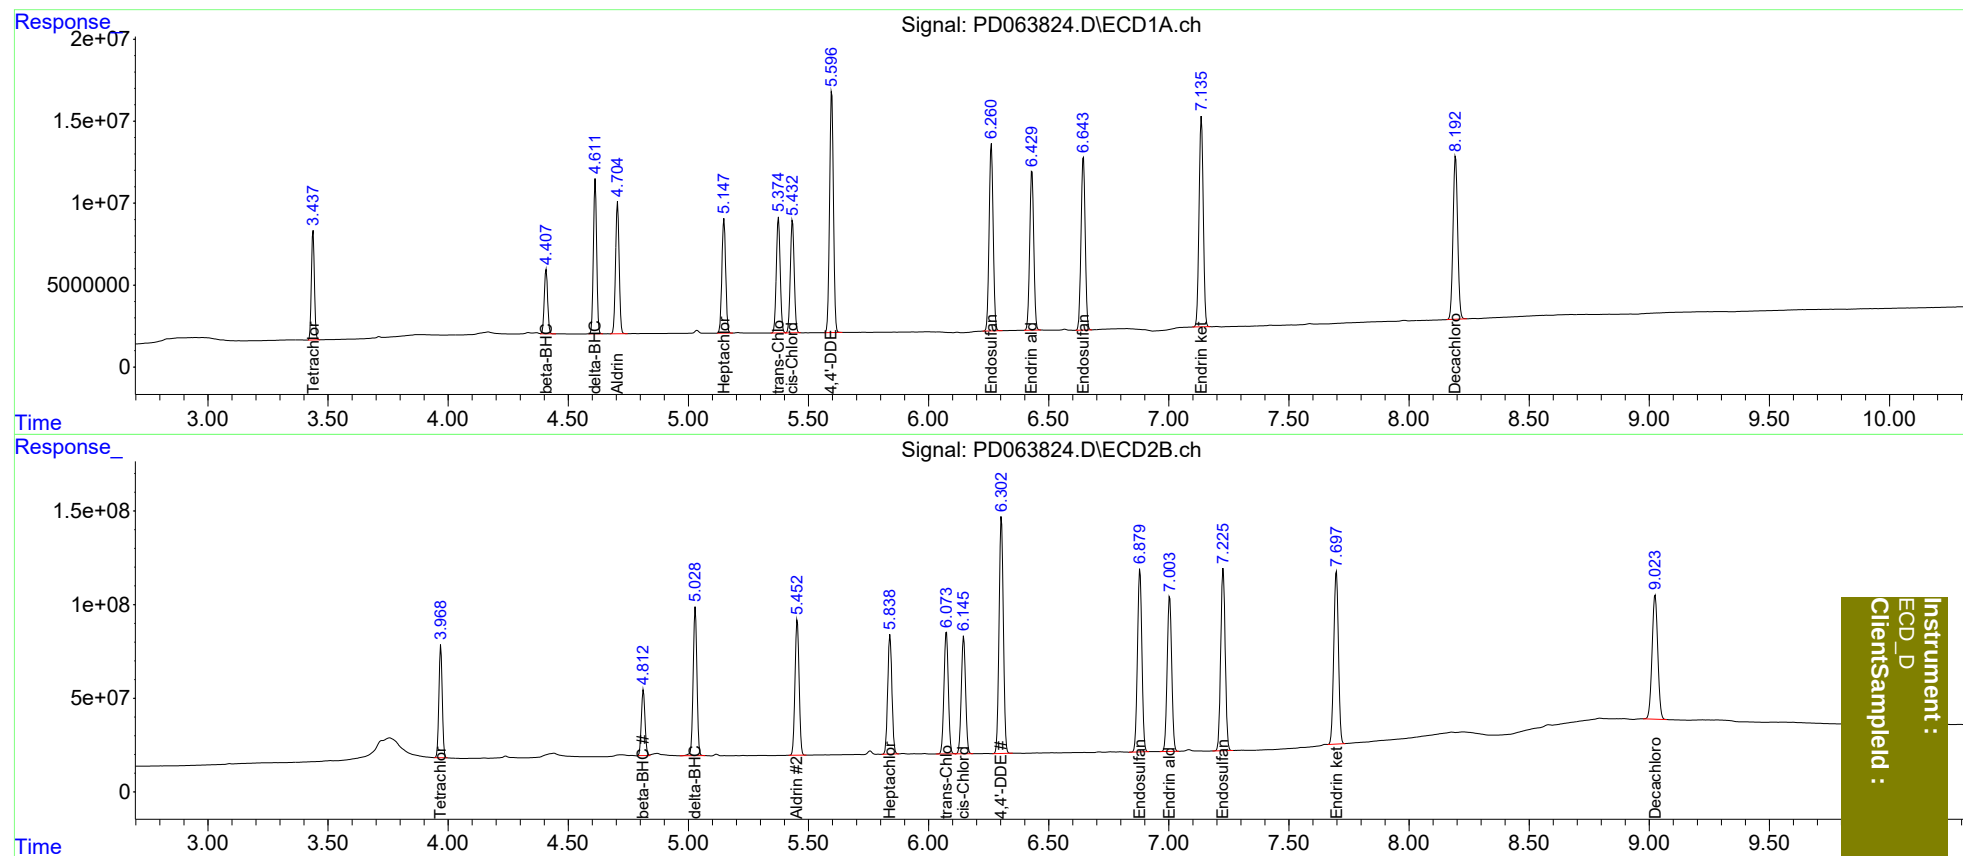


Instrument :
ECD_D
ClientSampled :

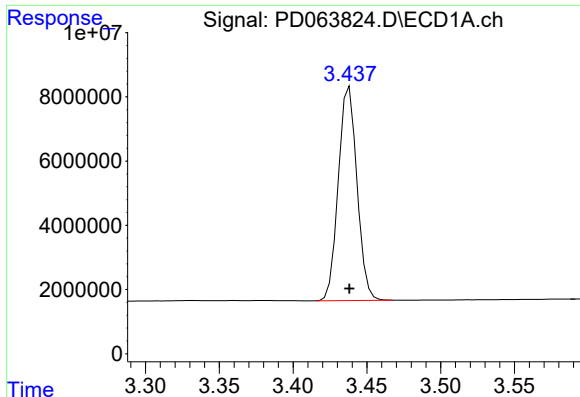

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: 0.000 min
Response: 58670839
Conc: 40.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

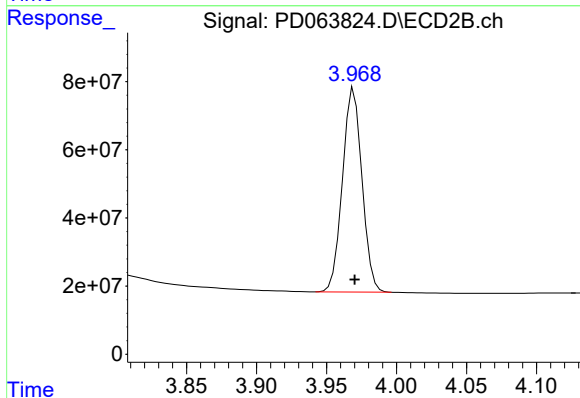


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: 0.000 min
Response: 582428813
Conc: 38.39 ng/ml

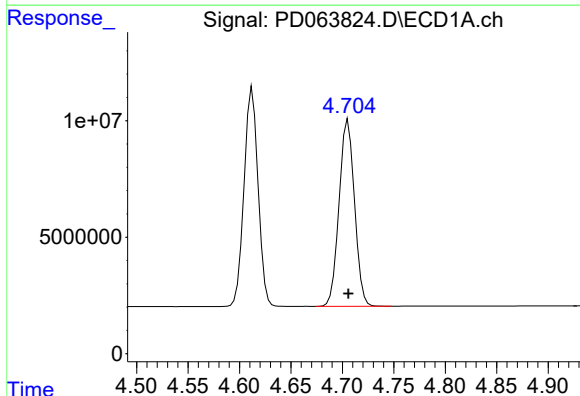


#5 Aldrin

R.T.: 4.706 min
Delta R.T.: 0.000 min
Response: 83635521
Conc: 41.54 ng/ml

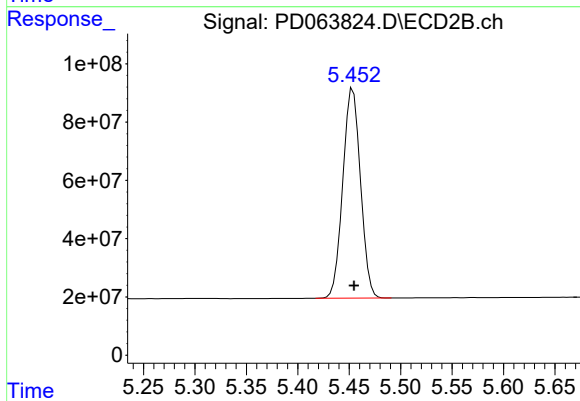

#5 Aldrin


R.T.: 5.454 min
Delta R.T.: -0.001 min
Response: 862033115
Conc: 38.95 ng/ml

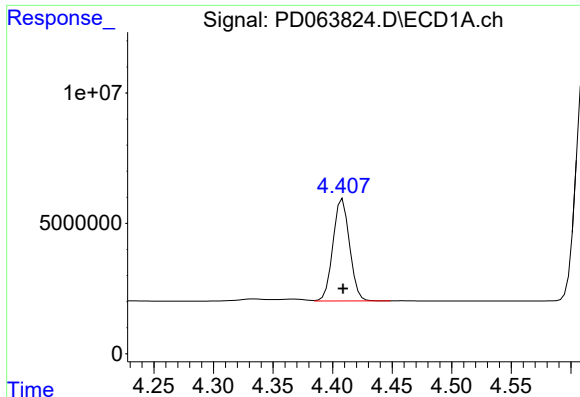

#6 beta-BHC


R.T.: 4.409 min
Delta R.T.: 0.000 min
Response: 37845385
Conc: 39.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

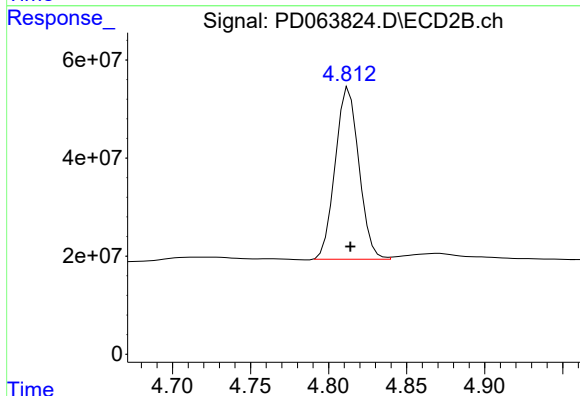


#6 beta-BHC

R.T.: 4.813 min
Delta R.T.: 0.000 min
Response: 370160115
Conc: 37.68 ng/ml

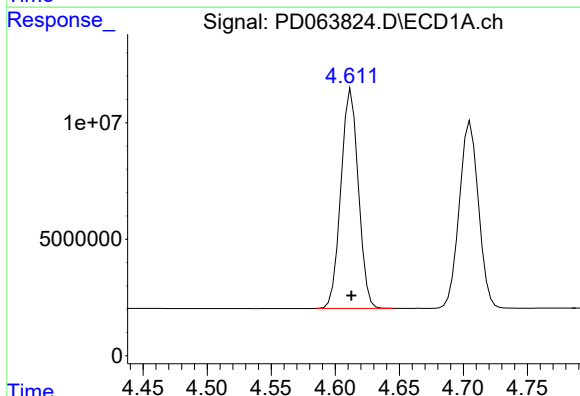


#7 delta-BHC

R.T.: 4.613 min
Delta R.T.: 0.000 min
Response: 89120741
Conc: 41.86 ng/ml

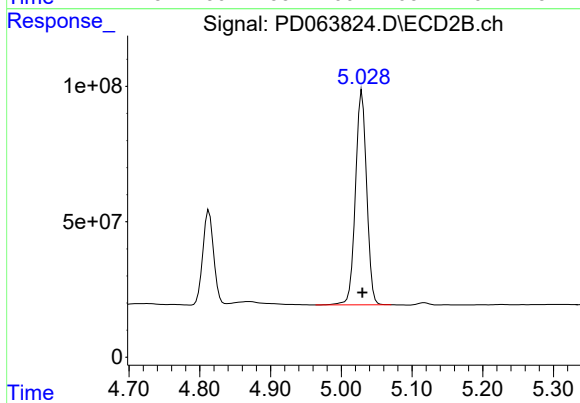

#7 delta-BHC


R.T.: 5.029 min
Delta R.T.: 0.000 min
Response: 869579529
Conc: 38.74 ng/ml

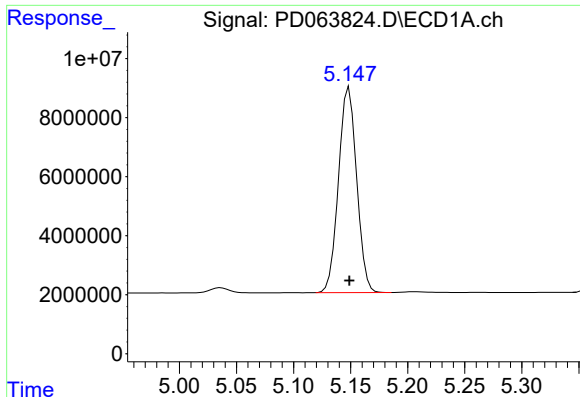

#8 Heptachlor epoxide


R.T.: 5.149 min
Delta R.T.: 0.000 min
Response: 77172829
Conc: 40.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

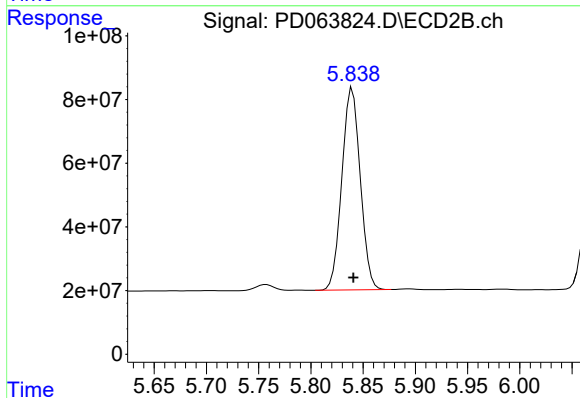


#8 Heptachlor epoxide

R.T.: 5.840 min
Delta R.T.: -0.001 min
Response: 777622681
Conc: 38.23 ng/ml

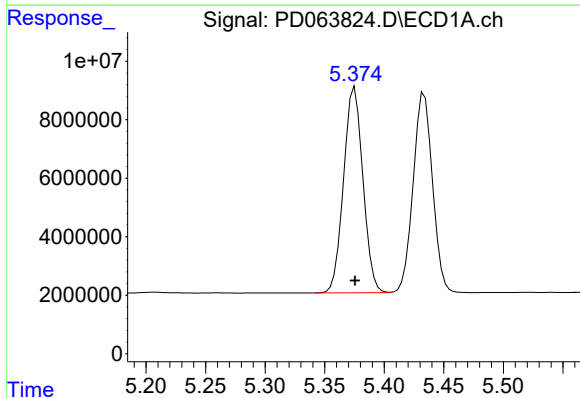


#10 trans-Chlordane

R.T.: 5.375 min
Delta R.T.: 0.000 min
Response: 79423100
Conc: 41.13 ng/ml

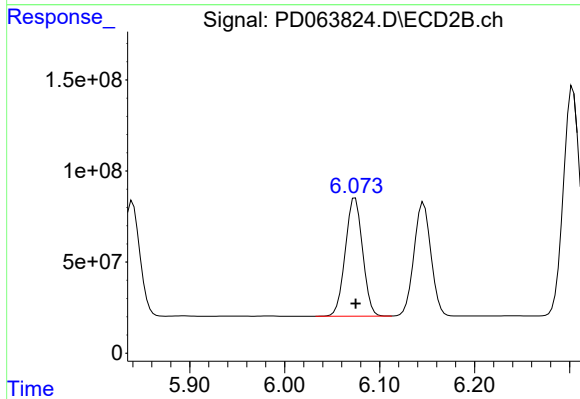

#10 trans-Chlordane


R.T.: 6.074 min
Delta R.T.: 0.000 min
Response: 822735294
Conc: 38.69 ng/ml

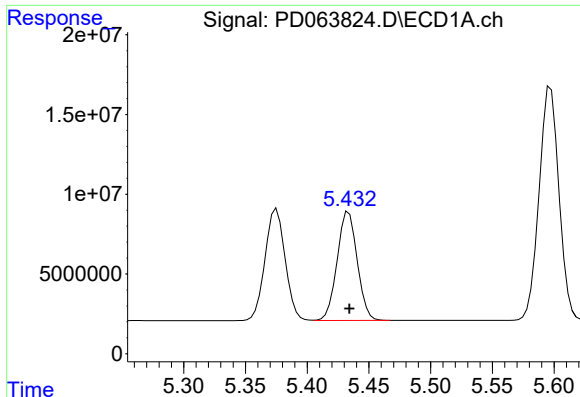

#11 cis-Chlordane


R.T.: 5.434 min
Delta R.T.: 0.000 min
Response: 77227060
Conc: 40.82 ng/ml

Instrument :
ECD_D
ClientSampleId :

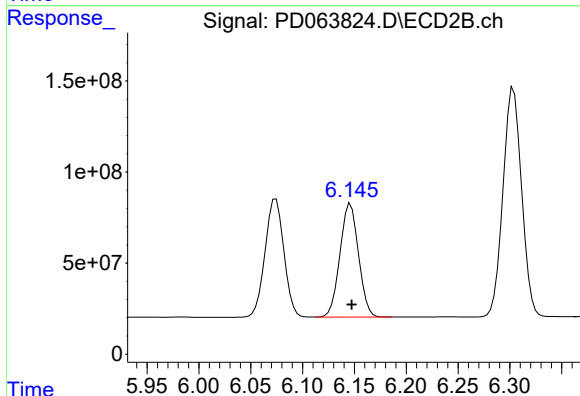


#11 cis-Chlordane

R.T.: 6.146 min
Delta R.T.: 0.000 min
Response: 776633368
Conc: 38.48 ng/ml

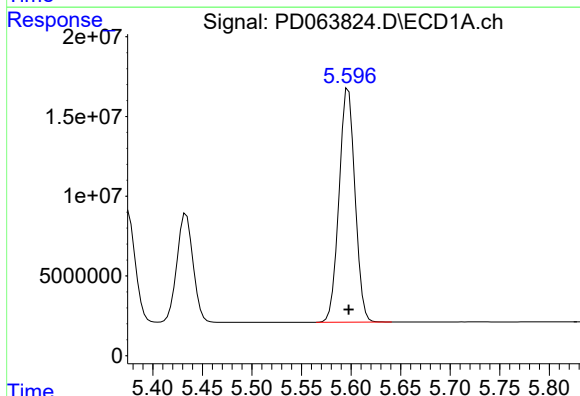


#12 4,4'-DDE

R.T.: 5.597 min
Delta R.T.: 0.000 min
Response: 164078454
Conc: 83.28 ng/ml

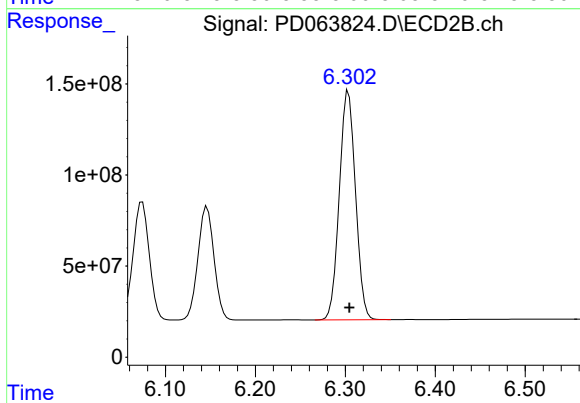

#12 4,4'-DDE


R.T.: 6.303 min
Delta R.T.: -0.001 min
Response: 1572383233
Conc: 77.67 ng/ml

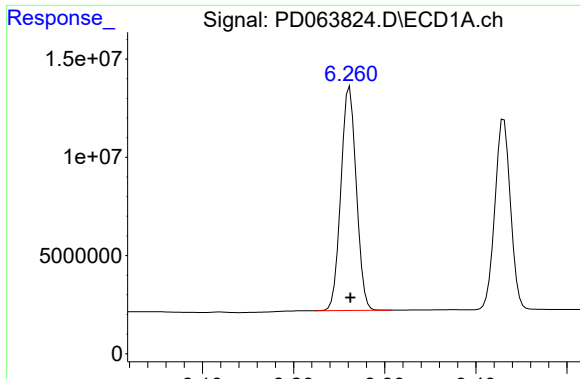

#15 Endosulfan II


R.T.: 6.262 min
Delta R.T.: 0.000 min
Response: 133832465
Conc: 82.12 ng/ml

Instrument :
ECD_D
ClientSampleId :

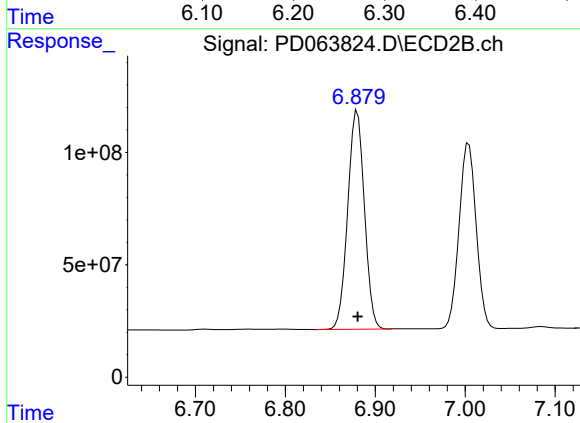


#15 Endosulfan II

R.T.: 6.880 min
Delta R.T.: 0.000 min
Response: 1252986709
Conc: 77.01 ng/ml

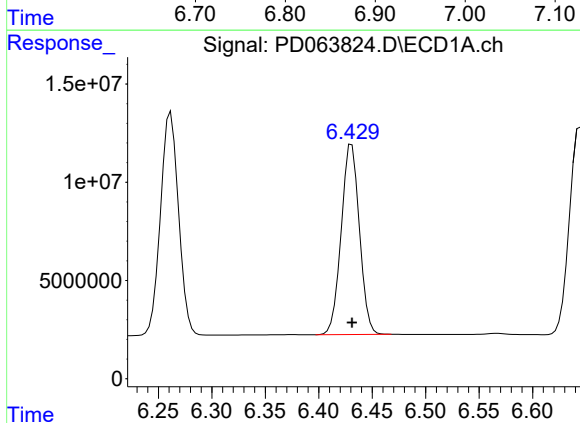


#18 Endrin aldehyde

R.T.: 6.431 min
Delta R.T.: 0.000 min
Response: 114841754
Conc: 80.88 ng/ml

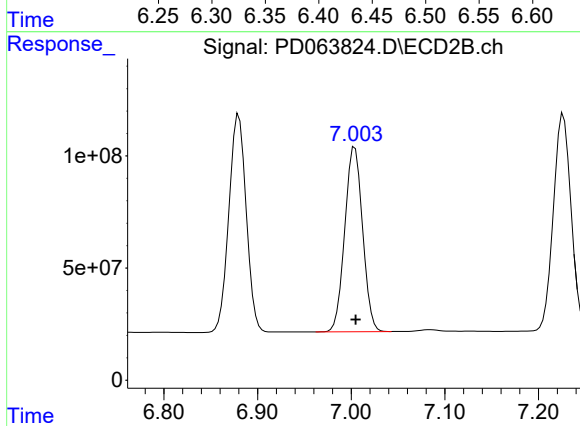

#18 Endrin aldehyde


R.T.: 7.004 min
Delta R.T.: 0.000 min
Response: 1089086014
Conc: 76.41 ng/ml

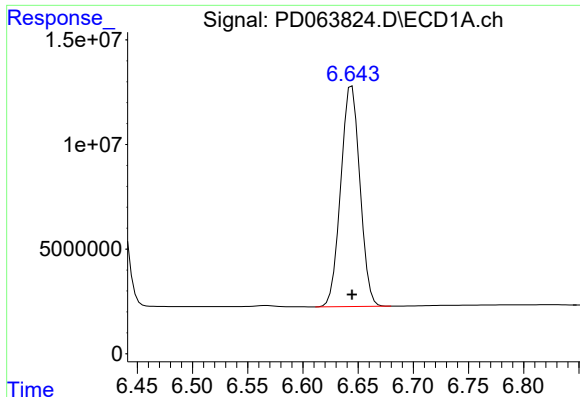

#19 Endosulfan Sulfate


R.T.: 6.644 min
Delta R.T.: 0.000 min
Response: 127409976
Conc: 81.91 ng/ml

Instrument :
ECD_D
ClientSampleId :

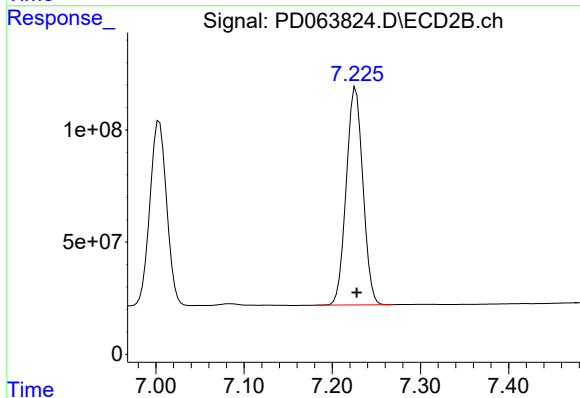


#19 Endosulfan Sulfate

R.T.: 7.227 min
Delta R.T.: -0.001 min
Response: 1273441921
Conc: 77.00 ng/ml

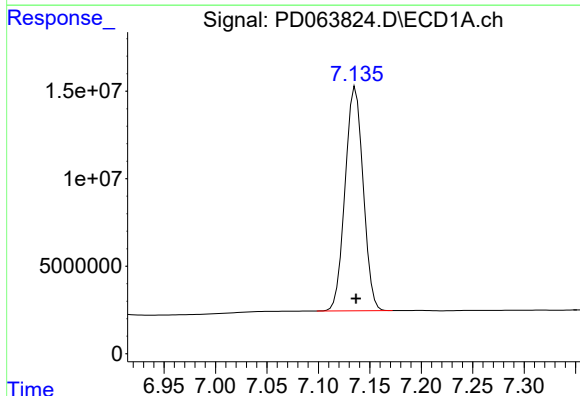


#21 Endrin ketone

R.T.: 7.136 min
Delta R.T.: 0.000 min
Response: 156477921
Conc: 82.06 ng/ml

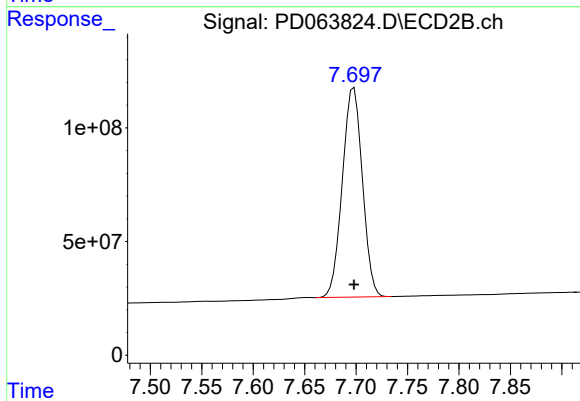

#21 Endrin ketone


R.T.: 7.698 min
Delta R.T.: 0.000 min
Response: 1250518799
Conc: 78.00 ng/ml

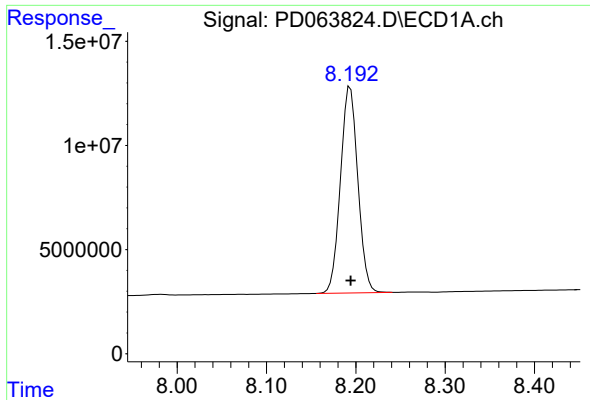

#27 Decachlorobiphenyl

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 133843936
Conc: 78.70 ng/ml

Instrument :
ECD_D
ClientSampleId :

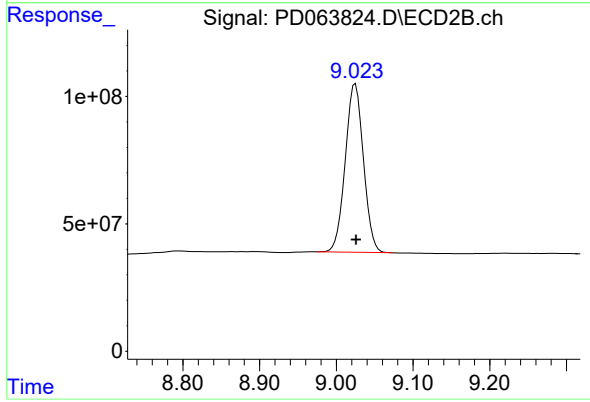

#27 Decachlorobiphenyl

R.T.: 9.025 min
Delta R.T.: 0.000 min
Response: 1094524633
Conc: 79.70 ng/ml