

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061421\
 Data File : PD063810.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2021 09:59
 Operator : AR\AJ
 Sample : RESC02
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC002

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 03:14:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 15 03:10:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.971	30690105	315.4E6	19.743	19.913
27)	SA Decachlor...	8.195	9.026	67651830	549.3E6	39.083	39.605
Target Compounds							
2)	A alpha-BHC	3.875	4.359	22330022	252.4E6	9.547	10.160
3)	MA gamma-BHC...	4.158	4.643	22298319	233.6E6	9.798	10.236
4)	MA Heptachlor	4.459	5.150	21188256	240.0E6	9.705	10.301
5)	MB Aldrin	4.707	5.454	19926783	230.4E6	9.832	10.458
6)	B beta-BHC	4.409	4.814	10249479	103.3E6	10.556	10.589
7)	B delta-BHC	4.613	5.030	21598673	254.2E6	10.006	10.850
8)	B Heptachlo...	5.149	5.841	18781243	212.2E6	9.904	10.313
9)	A Endosulfan I	5.488	6.197	17896711	199.0E6	9.780	10.043
10)	B trans-Chl...	5.376	6.075	19099695	215.0E6	9.822	10.222
11)	B cis-Chlor...	5.435	6.147	18801331	206.2E6	9.896	10.238
12)	B 4,4'-DDE	5.599	6.305	38629209	412.4E6	19.565	20.410
13)	MA Dieldrin	5.732	6.454	40473854	425.1E6	19.340	20.323
14)	MA Endrin	5.990	6.672	35351833	354.8E6	19.547	20.278
15)	B Endosulfa...	6.263	6.881	32263182	333.1E6	19.744	20.584
16)	A 4,4'-DDD	6.116	6.794	31802574	331.8E6	19.262	19.711
17)	MA 4,4'-DDT	6.357	7.093	31568906	326.0E6	18.757	19.800
18)	B Endrin al...	6.432	7.005	28912833	288.1E6	20.252	20.476
19)	B Endosulfa...	6.646	7.228	30783492	341.4E6	19.830	20.743
20)	A Methoxychlor	6.904	7.551	92693782	808.5E6	100.542	104.509
21)	B Endrin ke...	7.138	7.699	39251772	328.4E6	20.690	20.692

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061421\
Data File : PD063810.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2021 09:59
Operator : AR\AJ
Sample : RESC02
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 03:14:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 15 03:10:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

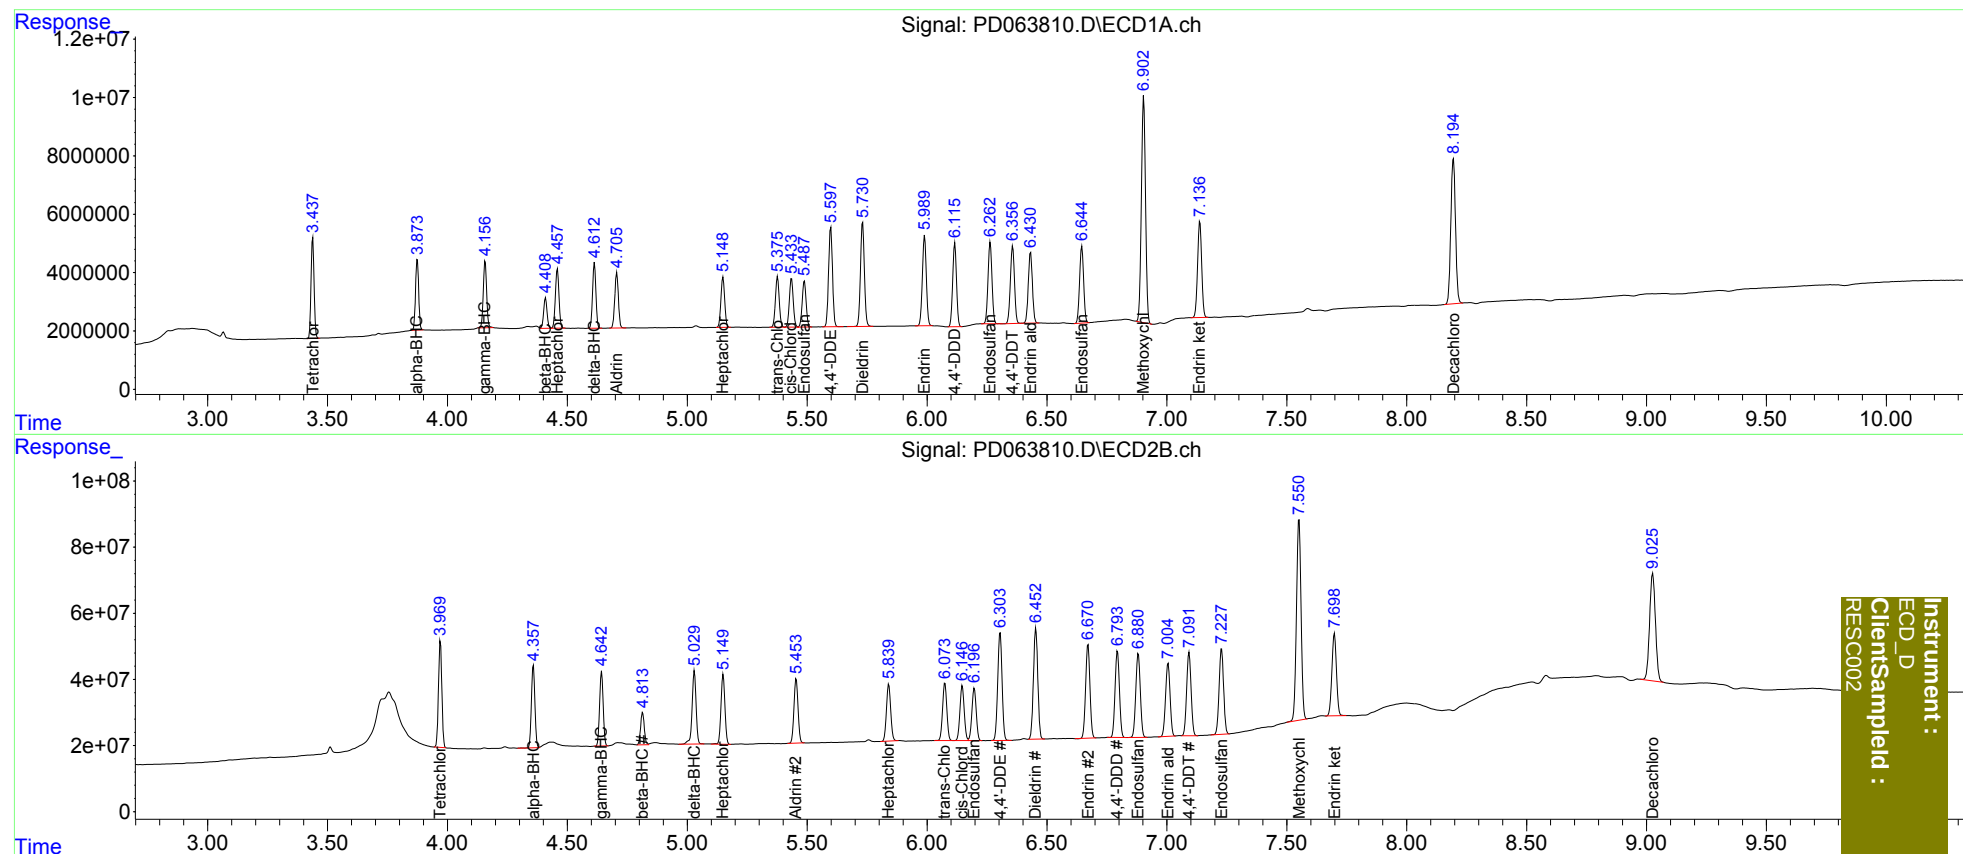

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061421\
Data File : PD063810.D
Acq On : 14 Jun 2021 09:59
Operator : AR\AJ
Sample : RESC02
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC002

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Title : GC Extractables
Last Update : Tue Jun 15 03:10:50 2021
Integrator: ChemStation

RT#1	RT#2	Resolution
3.439	3.714	100.00%
3.714	3.875	100.00%
3.875	4.158	100.00%
4.158	4.409	100.00%
4.409	4.459	100.00%
4.459	4.613	100.00%
4.613	4.707	100.00%
4.707	5.037	100.00%
5.037	5.149	100.00%
5.149	5.376	100.00%
5.376	5.435	99.26%
5.435	5.488	99.73%
5.488	5.599	100.00%
5.599	5.732	100.00%
5.732	5.990	100.00%
5.990	6.116	100.00%
6.116	6.263	100.00%
6.263	6.357	100.00%
6.357	6.432	100.00%
6.432	6.646	100.00%
6.646	6.904	100.00%
6.904	7.138	100.00%
7.138	8.195	100.00%

Signal #2


3.971	4.359	100.00%
4.359	4.643	100.00%
4.643	4.814	100.00%
4.814	5.030	100.00%
5.030	5.150	100.00%
5.150	5.454	100.00%
5.454	5.841	100.00%
5.841	6.075	100.00%
6.075	6.147	100.00%
6.147	6.197	98.12%
6.197	6.305	100.00%
6.305	6.454	100.00%
6.454	6.672	100.00%
6.672	6.794	100.00%
6.794	6.881	100.00%
6.881	7.005	100.00%
7.005	7.093	100.00%
7.093	7.228	100.00%
7.228	7.551	100.00%
7.551	7.699	100.00%
7.699	9.026	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061421\
Data File : PD063810.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2021 09:59
Operator : AR\AJ
Sample : RESC02
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC002

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 03:14:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 15 03:10:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

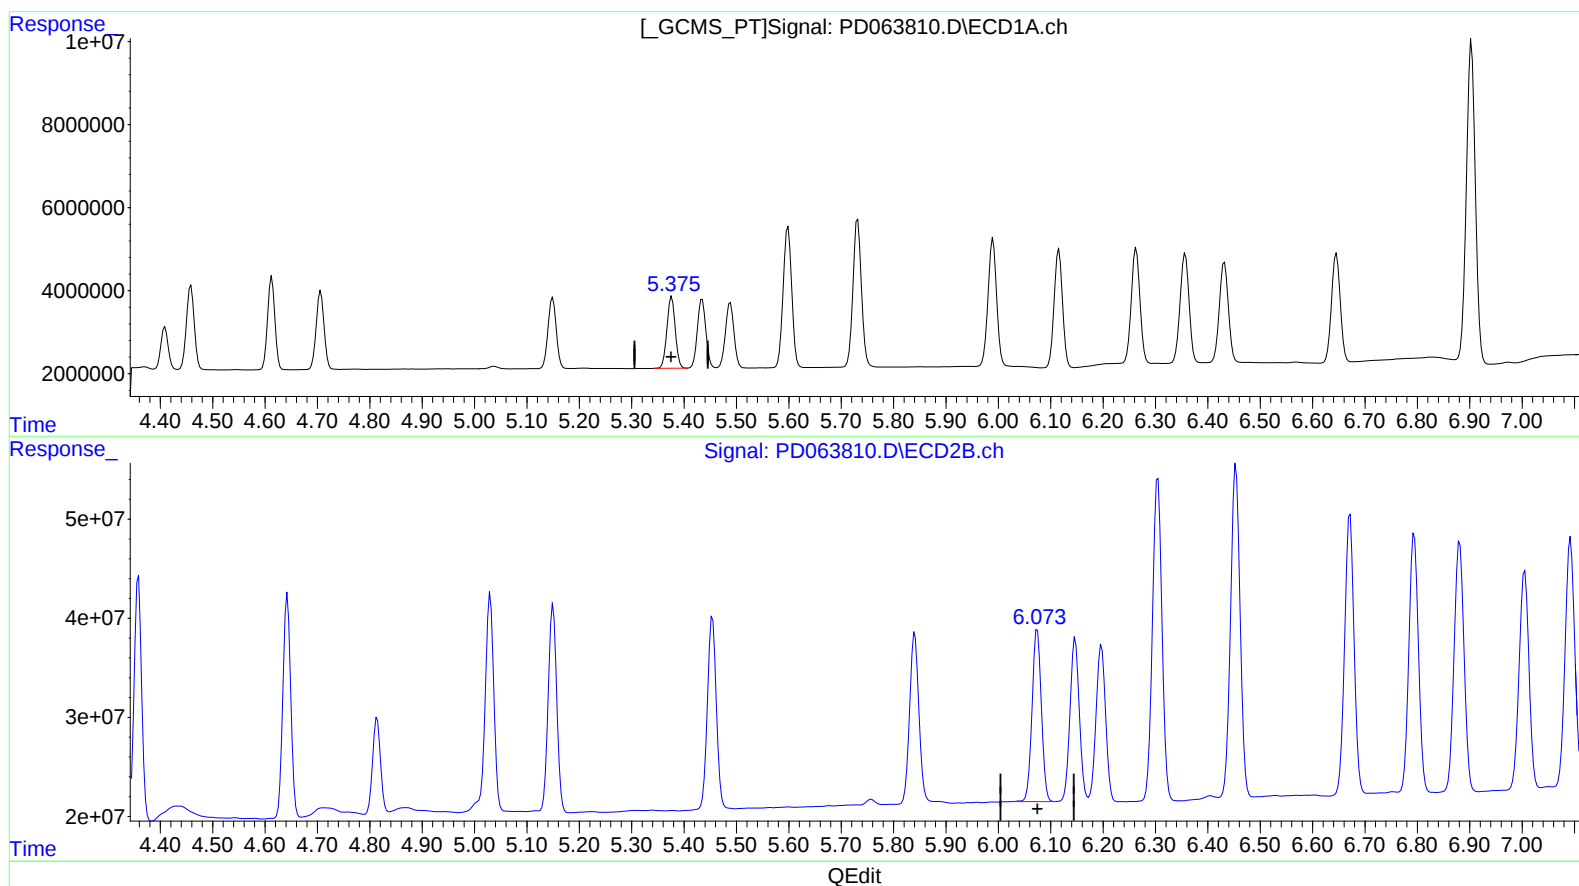

(10) trans-Chlordane (B)

5.376min 9.822 ng/ml

response 19099695

(10) trans-Chlordane #2 (B)

6.075min 10.222 ng/ml


response 215027535

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061421\
Data File : PD063810.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2021 09:59
Operator : AR\AJ
Sample : RESC02
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC002

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 03:14:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 15 03:10:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

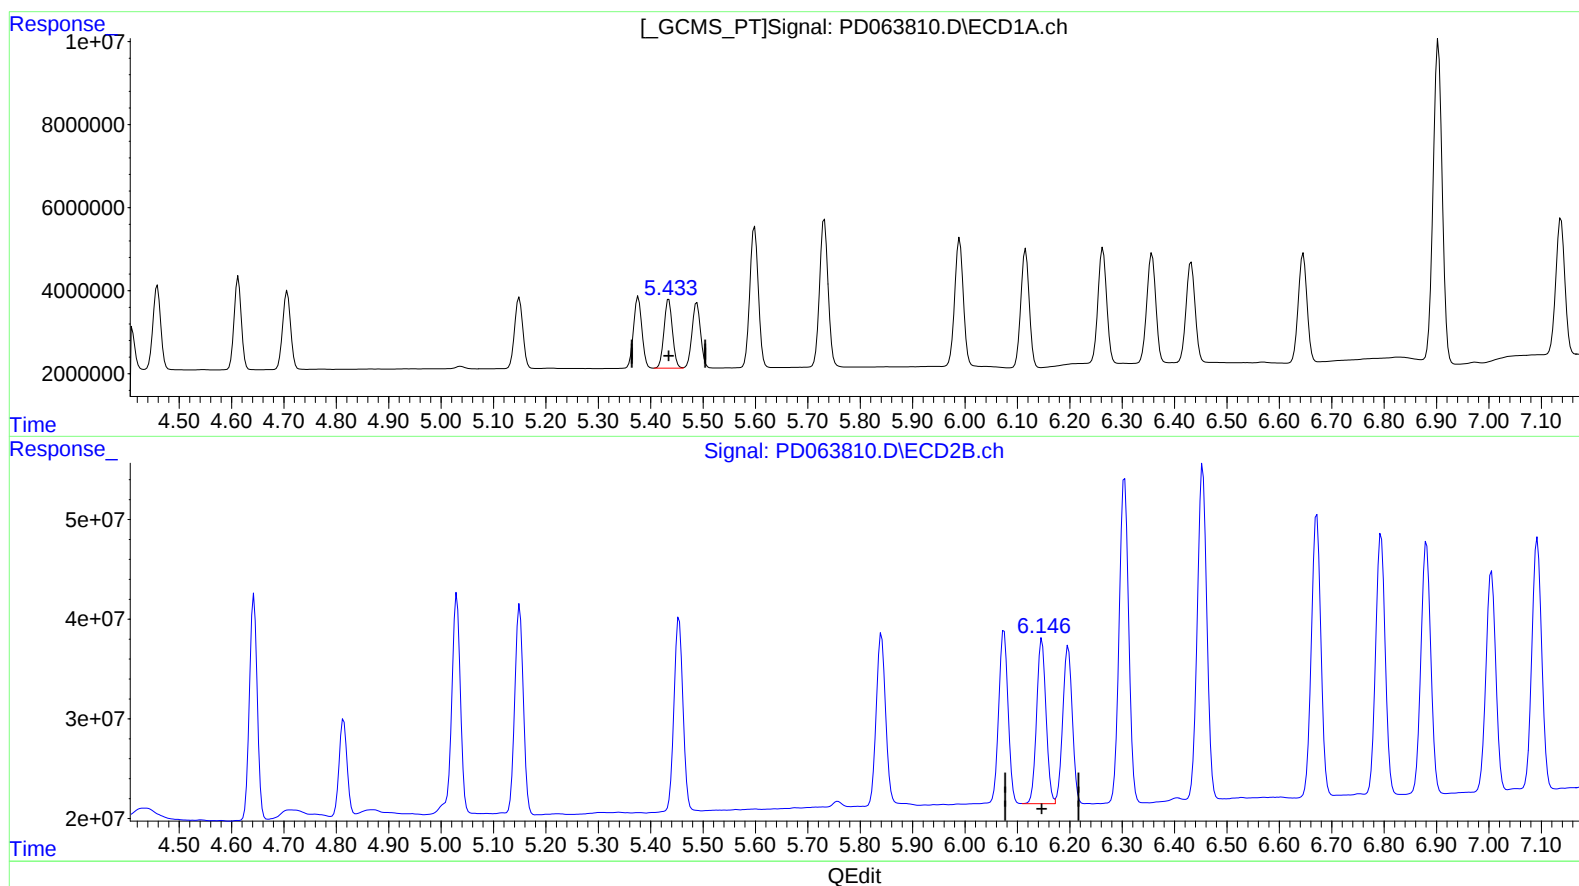

(11) cis-Chlordane (B)

5.435min 9.896 ng/ml

response 18801331

(11) cis-Chlordane #2 (B)

6.147min 10.238 ng/ml

response 206195015