

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061421\
 Data File : PD063838.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2021 16:25
 Operator : AR\AJ
 Sample : INDA350
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 03:46:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 15 03:10:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.971	28601971	283.1E6	18.399	17.877
27)	SA Decachlor...	8.194	9.026	65707415	548.1E6	37.960	39.521
Target Compounds							
2)	A alpha-BHC	3.875	4.359	42182806	446.7E6	18.034	17.981
3)	MA gamma-BHC...	4.158	4.643	41122224	409.0E6	18.069	17.924
4)	MA Heptachlor	4.458	5.150	39541209	417.9E6	18.111	17.937
9)	A Endosulfan I	5.488	6.197	34195328	359.1E6	18.687	18.126
13)	MA Dieldrin	5.732	6.454	76357930	772.5E6	36.487	36.925
14)	MA Endrin	5.989	6.671	66970517	647.6E6	37.031	37.014
16)	A 4,4'-DDD	6.115	6.794	60501575	619.4E6	36.645	36.797
17)	MA 4,4'-DDT	6.356	7.093	65898544	651.3E6	39.155	39.564
20)	A Methoxychlor	6.903	7.551	174.7E6	1474.0E6	189.487	190.521

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061421\
Data File : PD063838.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2021 16:25
Operator : AR\AJ
Sample : INDA350
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 03:46:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 15 03:10:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

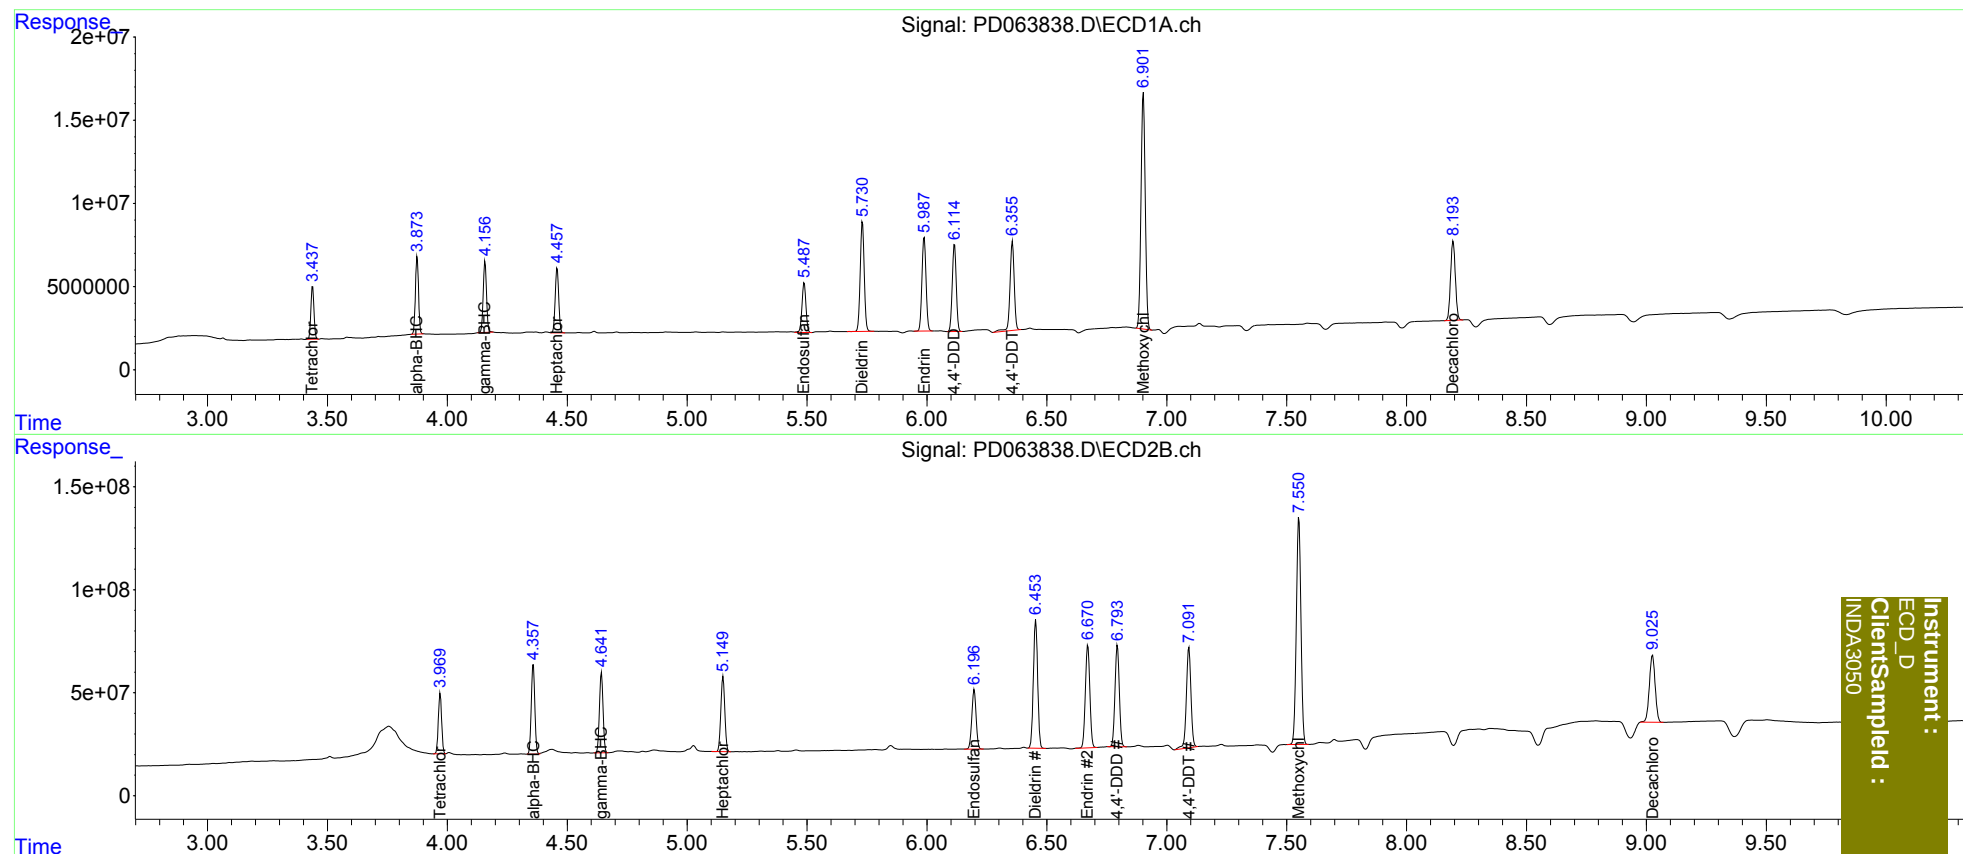

Instrument :
ECD_D
ClientSampled :
INDA3050