

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061422\
 Data File : PD070289.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2022 12:34
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 15:26:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 14 15:17:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.400	4.122	7607089	72458872	5.408	5.459
27)	SA Decachlor...	8.130	9.280	16844329	80094049	10.929	11.372
Target Compounds							
2)	A alpha-BHC	3.835	4.515	10261430	101.9E6	5.044	5.308
3)	MA gamma-BHC...	4.116	4.803	9898624	97541327	5.091	5.475
4)	MA Heptachlor	4.410	5.327	9960213	96626006	5.168	5.381
9)	A Endosulfan I	5.432	6.386	8714932	74637505	5.326	5.653
13)	MA Dieldrin	5.675	6.643	18678830	148.4E6	10.096	11.070
14)	MA Endrin	5.932	6.863	16889831	129.8E6	10.167	11.672
16)	A 4,4'-DDD	6.060	6.976	14820139	120.9E6	10.024	11.315
17)	MA 4,4'-DDT	6.300	7.279	13323762	114.1E6	9.327	11.514
20)	A Methoxychlor	6.849	7.733	44631015	265.6E6	53.496	57.864


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061422\
Data File : PD070289.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2022 12:34
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 15:26:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 14 15:17:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

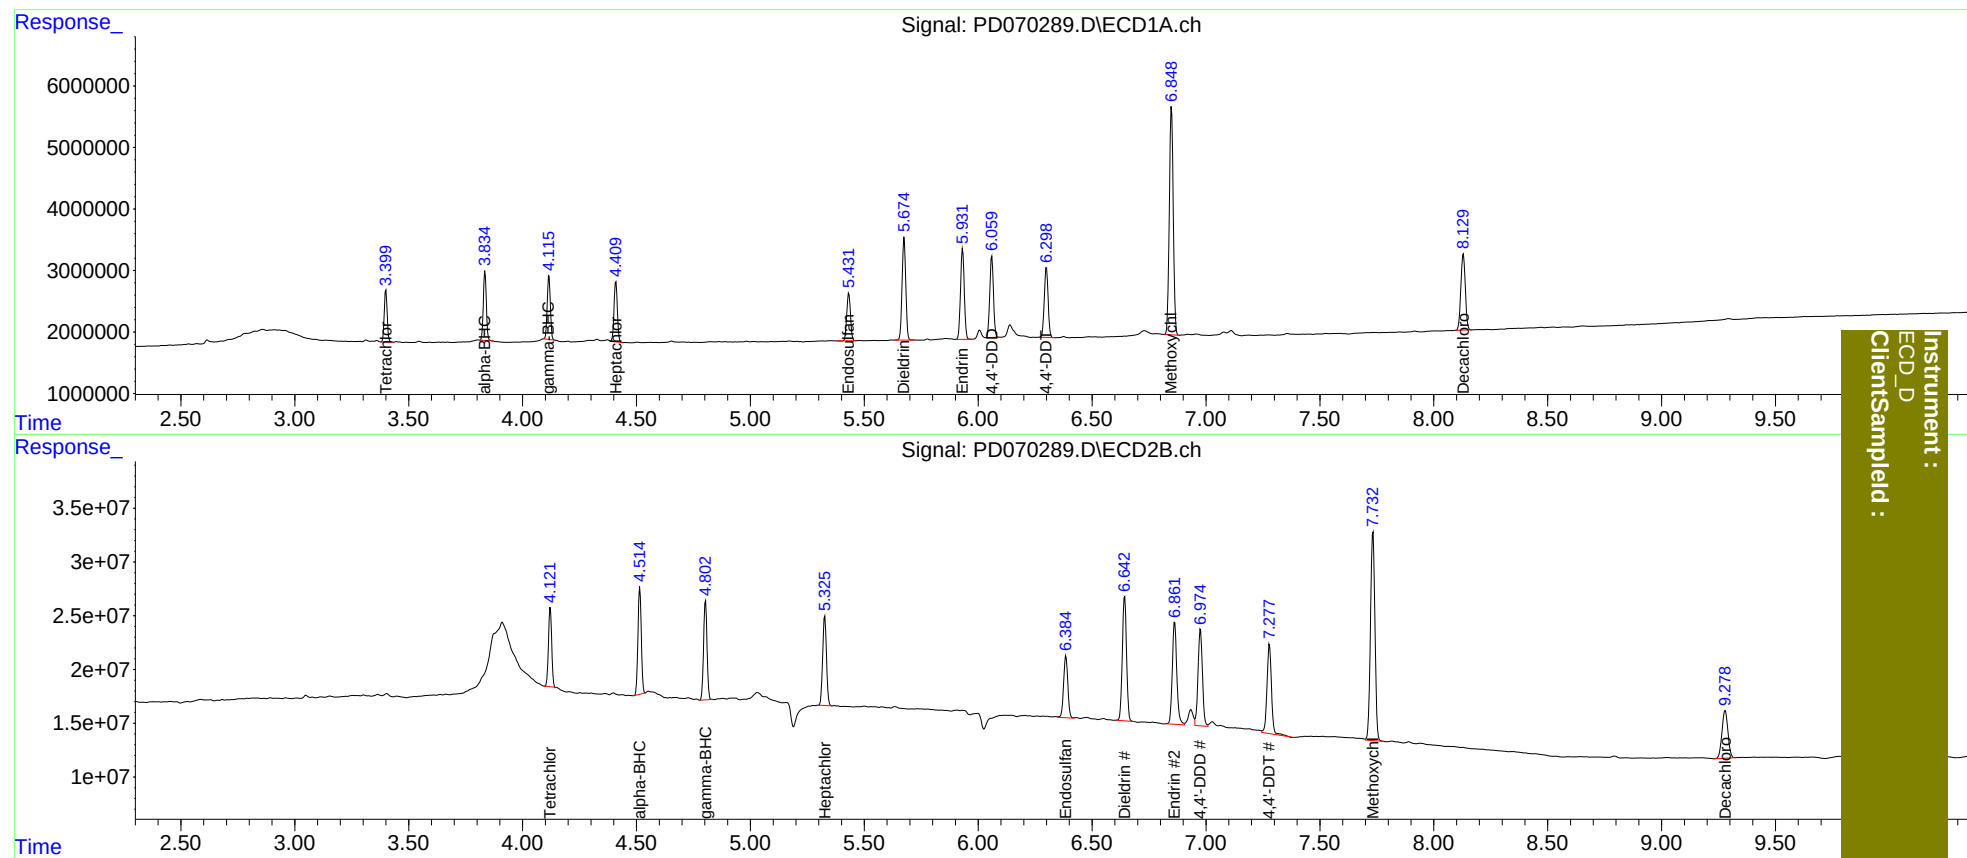


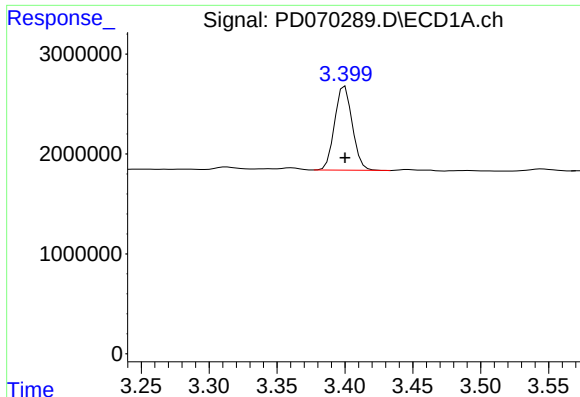

#1 Tetrachloro-m-xylene


R.T.: 3.400 min
Delta R.T.: 0.000 min
Response: 7607089
Conc: 5.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

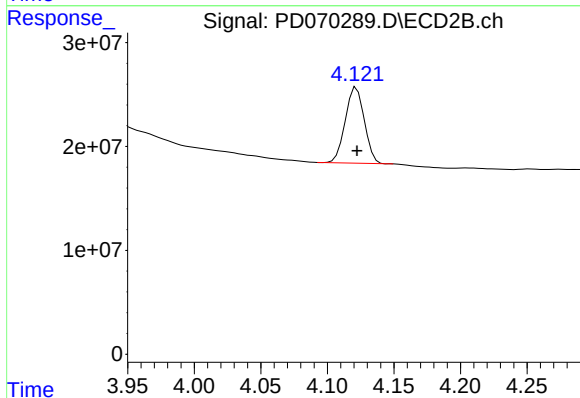


#1 Tetrachloro-m-xylene

R.T.: 4.122 min
Delta R.T.: 0.000 min
Response: 72458872
Conc: 5.46 ng/ml

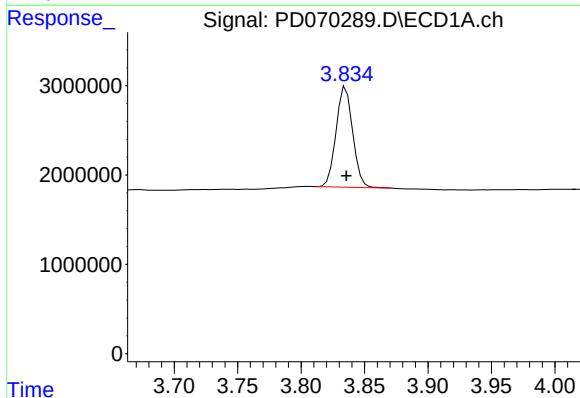


#2 alpha-BHC

R.T.: 3.835 min
Delta R.T.: 0.000 min
Response: 10261430
Conc: 5.04 ng/ml

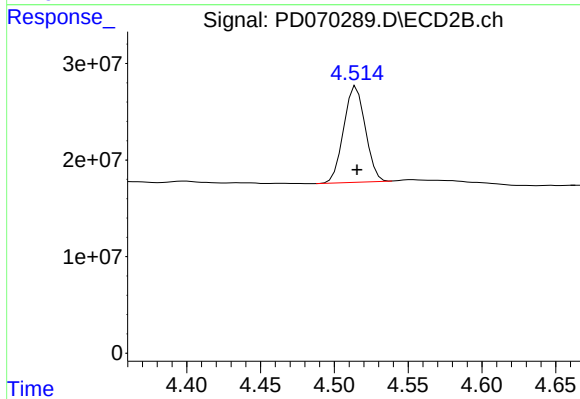

#2 alpha-BHC


R.T.: 4.515 min
Delta R.T.: 0.000 min
Response: 101852638
Conc: 5.31 ng/ml

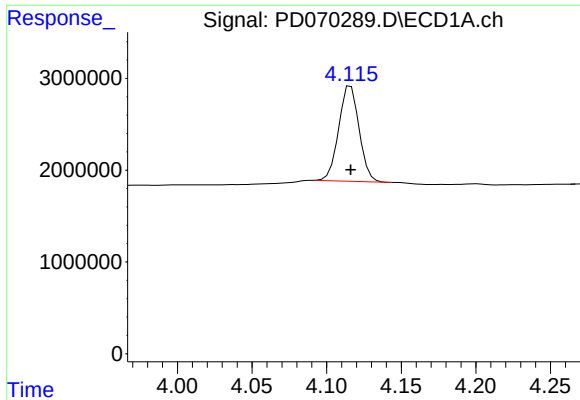

#3 gamma-BHC (Lindane)


R.T.: 4.116 min
Delta R.T.: 0.000 min
Response: 9898624
Conc: 5.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

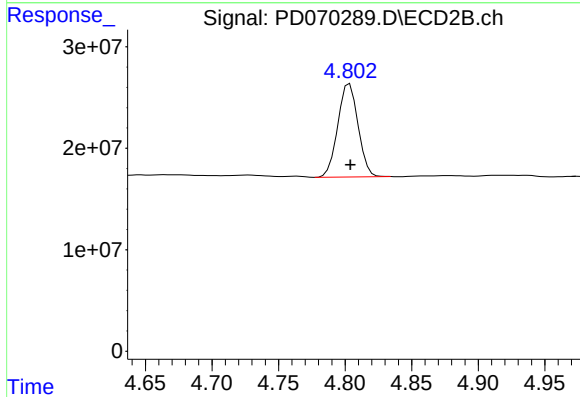


#3 gamma-BHC (Lindane)

R.T.: 4.803 min
Delta R.T.: 0.000 min
Response: 97541327
Conc: 5.47 ng/ml

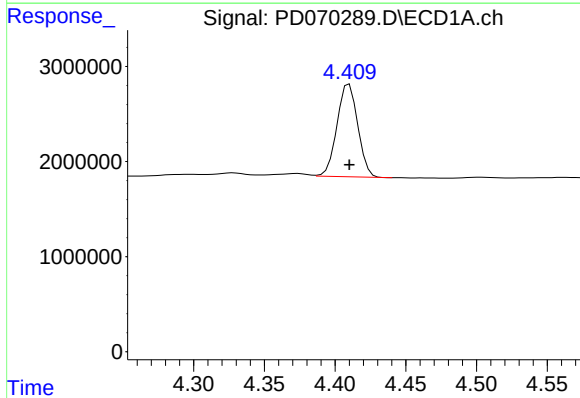


#4 Heptachlor

R.T.: 4.410 min
Delta R.T.: 0.000 min
Response: 9960213
Conc: 5.17 ng/ml

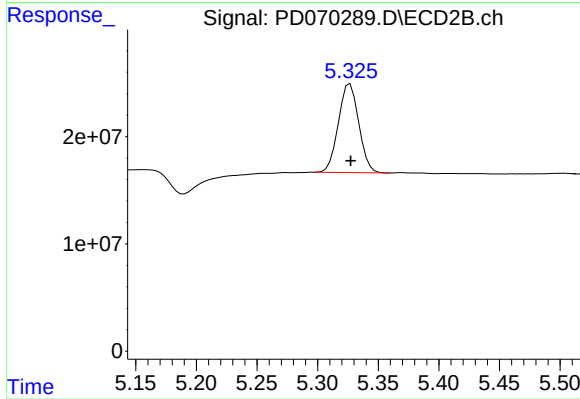

#4 Heptachlor


R.T.: 5.327 min
Delta R.T.: 0.000 min
Response: 96626006
Conc: 5.38 ng/ml

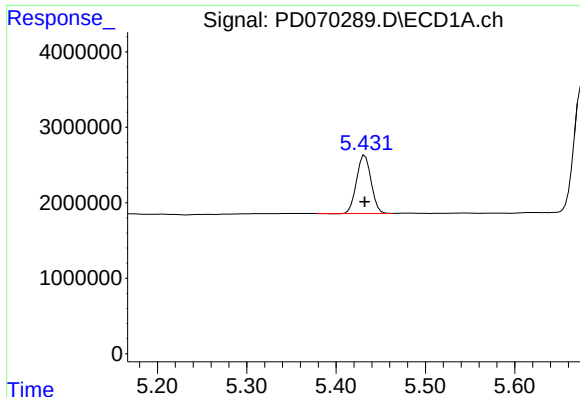

#9 Endosulfan I


R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 8714932
Conc: 5.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

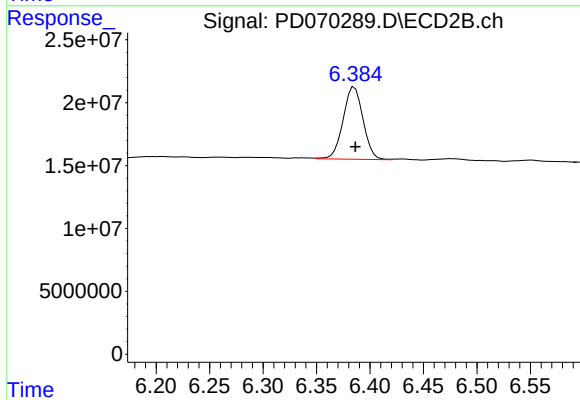


#9 Endosulfan I

R.T.: 6.386 min
Delta R.T.: 0.000 min
Response: 74637505
Conc: 5.65 ng/ml

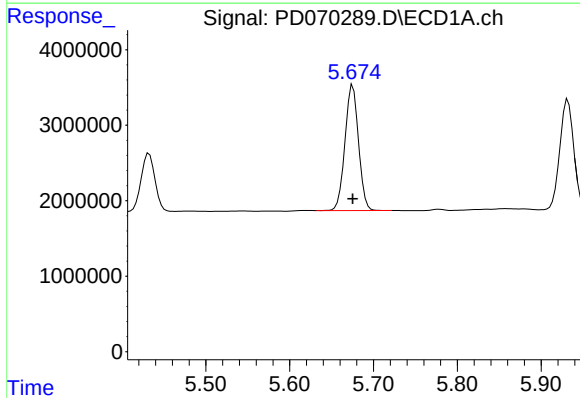


#13 Dieldrin

R.T.: 5.675 min
Delta R.T.: 0.000 min
Response: 18678830
Conc: 10.10 ng/ml

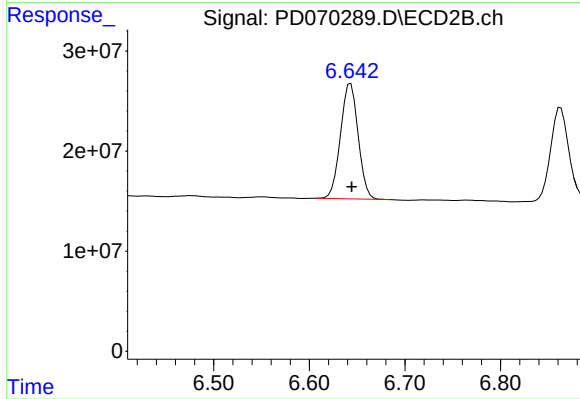

#13 Dieldrin


R.T.: 6.643 min
Delta R.T.: -0.001 min
Response: 148425431
Conc: 11.07 ng/ml

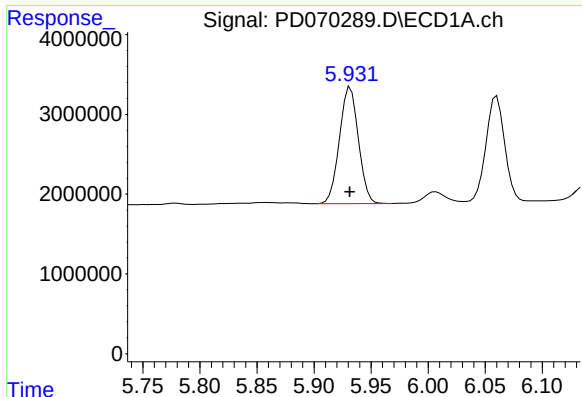

#14 Endrin


R.T.: 5.932 min
Delta R.T.: 0.000 min
Response: 16889831
Conc: 10.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

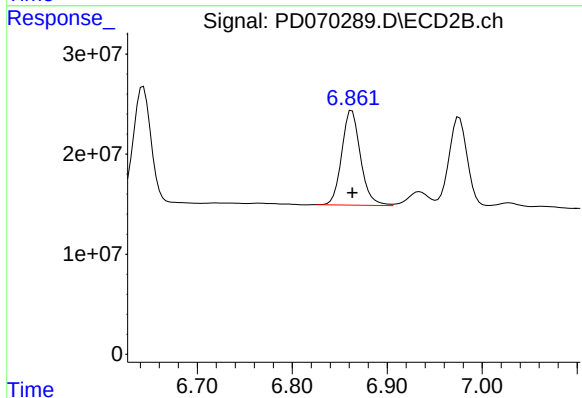


#14 Endrin

R.T.: 6.863 min
Delta R.T.: 0.000 min
Response: 129808454
Conc: 11.67 ng/ml

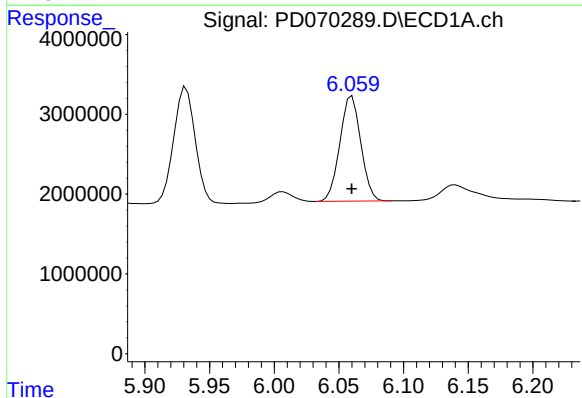


#16 4,4'-DDD

R.T.: 6.060 min
Delta R.T.: 0.000 min
Response: 14820139
Conc: 10.02 ng/ml

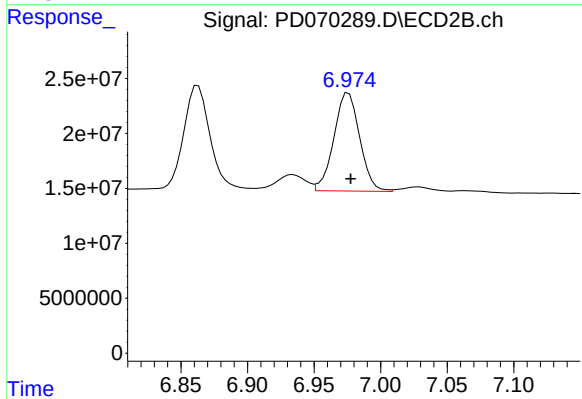

#16 4,4'-DDD


R.T.: 6.976 min
Delta R.T.: -0.002 min
Response: 120880009
Conc: 11.31 ng/ml

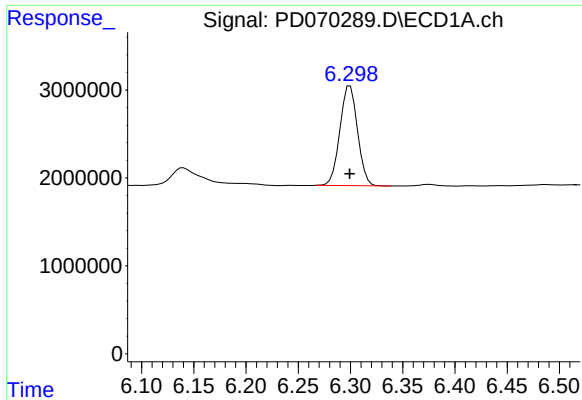

#17 4,4'-DDT


R.T.: 6.300 min
Delta R.T.: 0.000 min
Response: 13323762
Conc: 9.33 ng/ml

Instrument :
ECD_D
ClientSampleId :

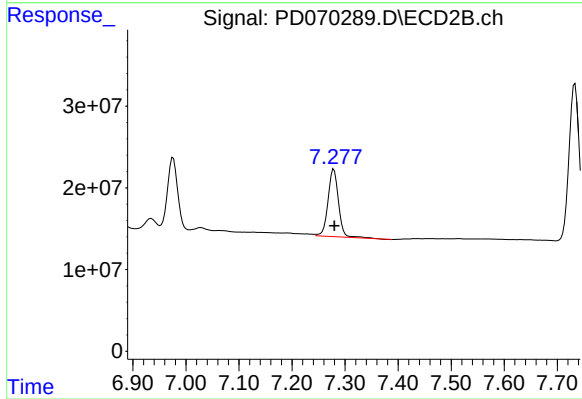


#17 4,4'-DDT

R.T.: 7.279 min
Delta R.T.: 0.000 min
Response: 114063769
Conc: 11.51 ng/ml

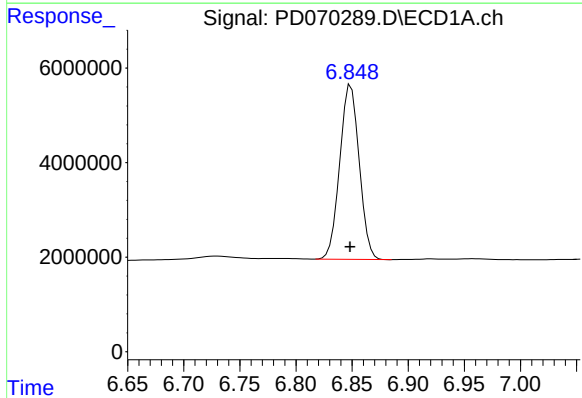


#20 Methoxychlor

R.T.: 6.849 min
Delta R.T.: 0.000 min
Response: 44631015
Conc: 53.50 ng/ml

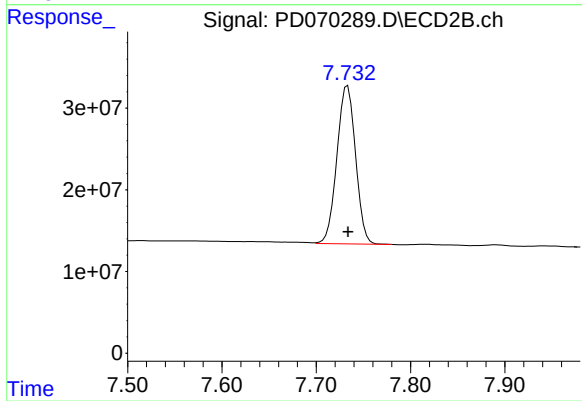

#20 Methoxychlor


R.T.: 7.733 min
Delta R.T.: 0.000 min
Response: 265565206
Conc: 57.86 ng/ml

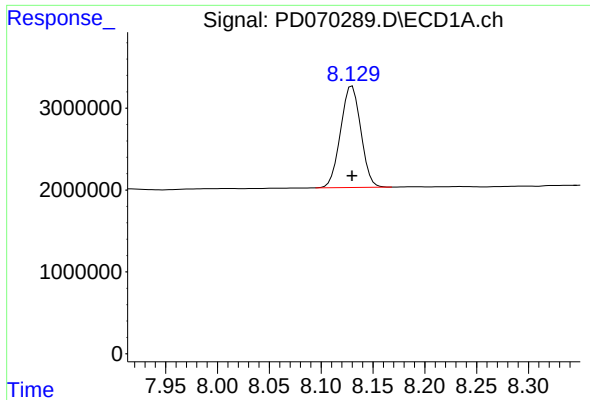

#27 Decachlorobiphenyl

R.T.: 8.130 min
Delta R.T.: 0.000 min
Response: 16844329
Conc: 10.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

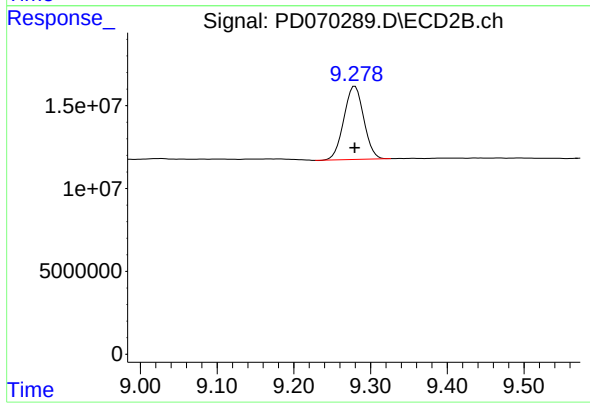

#27 Decachlorobiphenyl

R.T.: 9.280 min
Delta R.T.: 0.000 min
Response: 80094049
Conc: 11.37 ng/ml