

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061422\
 Data File : PD070291.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2022 13:02
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 15:28:56 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 14 15:17:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.400	4.122	14578703	143.4E6	9.958	10.331
27)	SA Decachlor...	8.129	9.280	35369396	162.1E6	21.930	21.534
Target Compounds							
2)	A alpha-BHC	3.835	4.516	20433770	203.2E6	10.000	10.271
3)	MA gamma-BHC...	4.117	4.804	19558214	191.2E6	9.968	10.244
4)	MA Heptachlor	4.410	5.327	19096770	186.3E6	9.745	9.992
9)	A Endosulfan I	5.433	6.386	16488603	143.6E6	9.759	10.207
13)	MA Dieldrin	5.676	6.643	36753821	286.2E6	19.770	20.261
14)	MA Endrin	5.932	6.864	33128024	238.0E6	19.776	19.749
16)	A 4,4'-DDD	6.060	6.977	29514460	232.5E6	19.939	20.422
17)	MA 4,4'-DDT	6.300	7.279	27289505	213.1E6	19.769	20.001
20)	A Methoxychlor	6.849	7.734	86071433	503.5E6	99.683	101.706


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061422\
Data File : PD070291.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2022 13:02
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 15:28:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 14 15:17:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

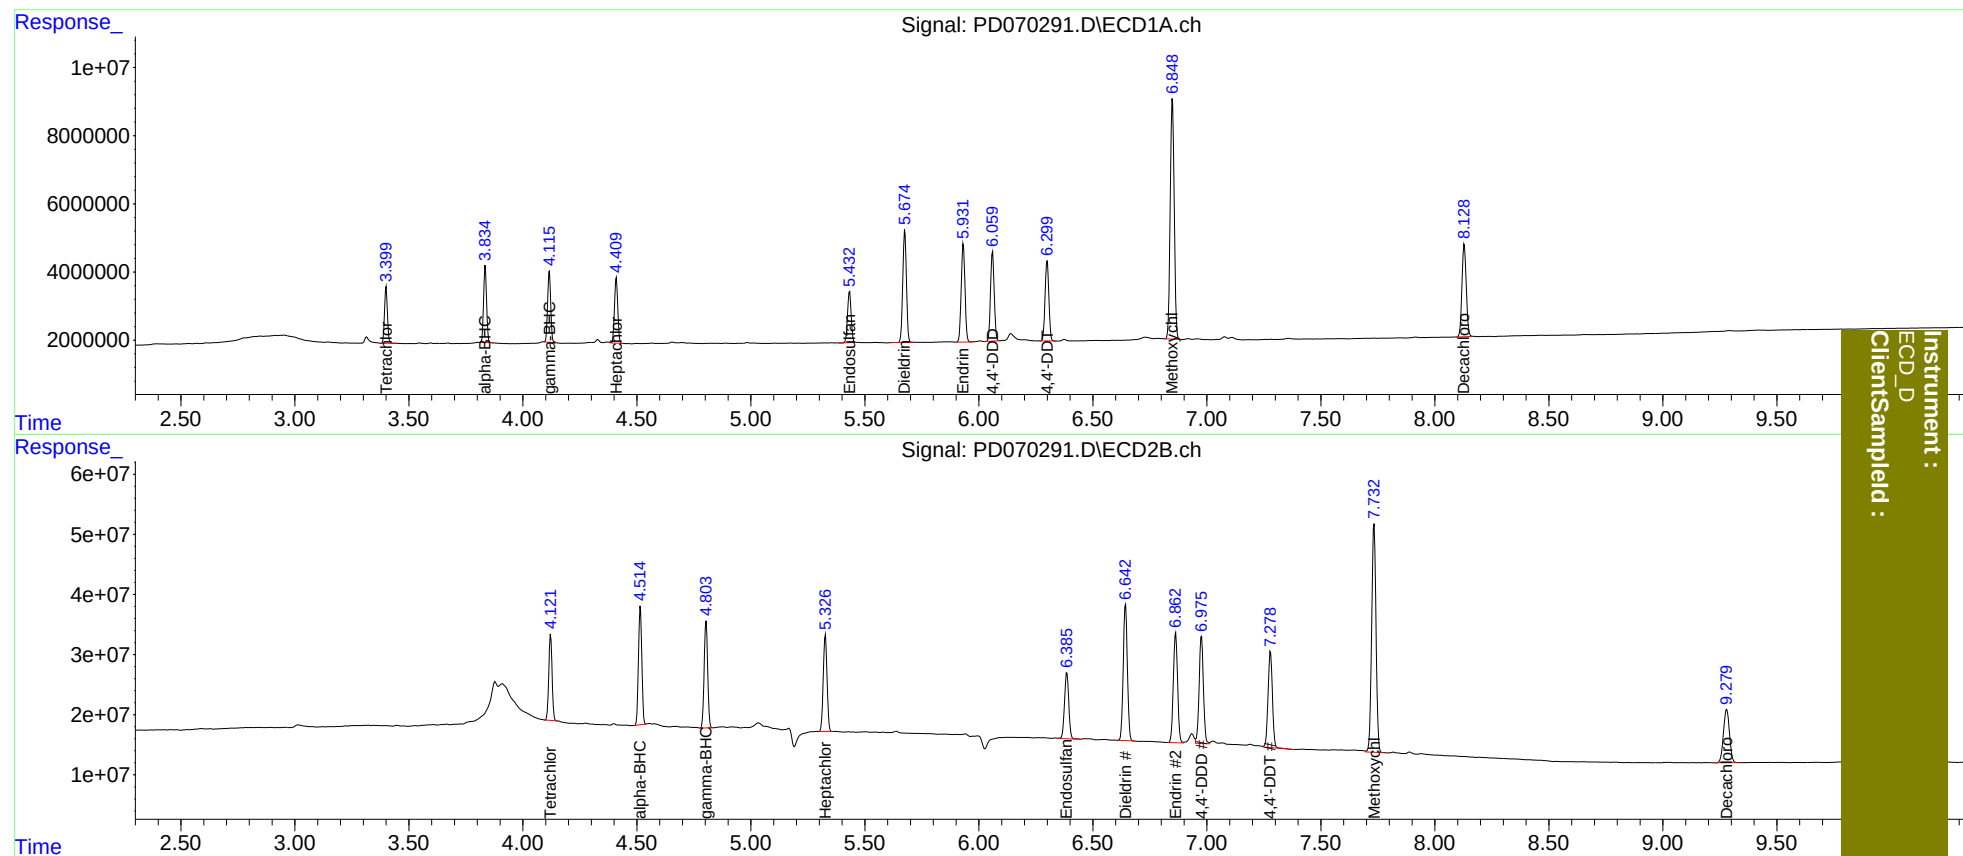


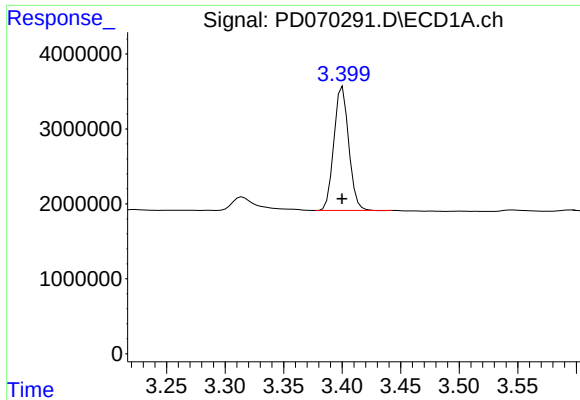

#1 Tetrachloro-m-xylene


R.T.: 3.400 min
Delta R.T.: 0.000 min
Response: 14578703
Conc: 9.96 ng/ml

Instrument :
ECD_D
ClientSampleId :

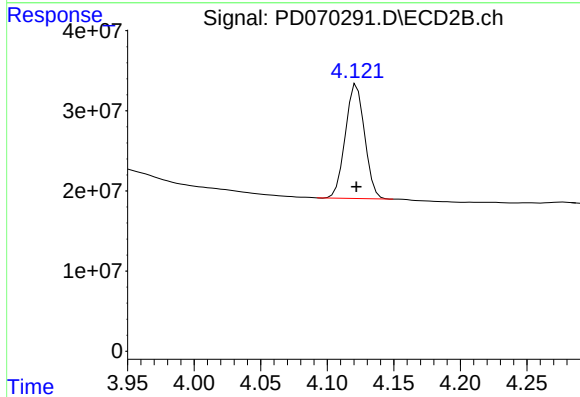


#1 Tetrachloro-m-xylene

R.T.: 4.122 min
Delta R.T.: 0.000 min
Response: 143420510
Conc: 10.33 ng/ml

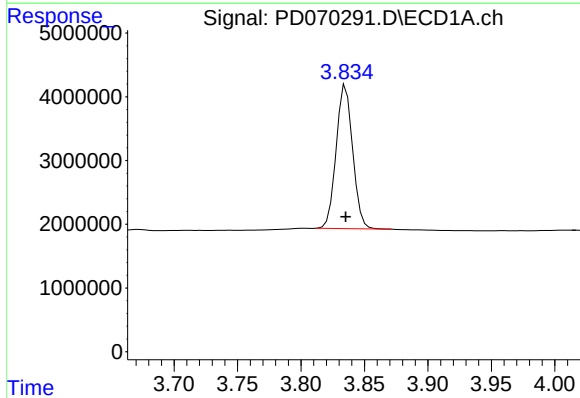


#2 alpha-BHC

R.T.: 3.835 min
Delta R.T.: 0.000 min
Response: 20433770
Conc: 10.00 ng/ml

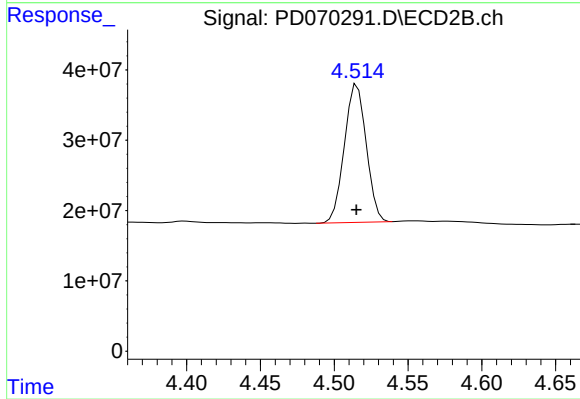

#2 alpha-BHC


R.T.: 4.516 min
Delta R.T.: 0.000 min
Response: 203154126
Conc: 10.27 ng/ml

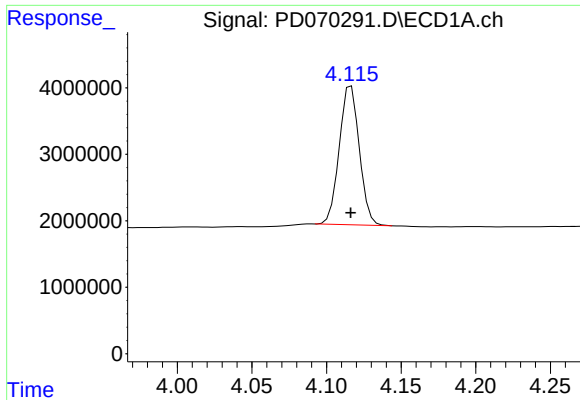

#3 gamma-BHC (Lindane)


R.T.: 4.117 min
Delta R.T.: 0.000 min
Response: 19558214
Conc: 9.97 ng/ml

Instrument :
ECD_D
ClientSampleId :

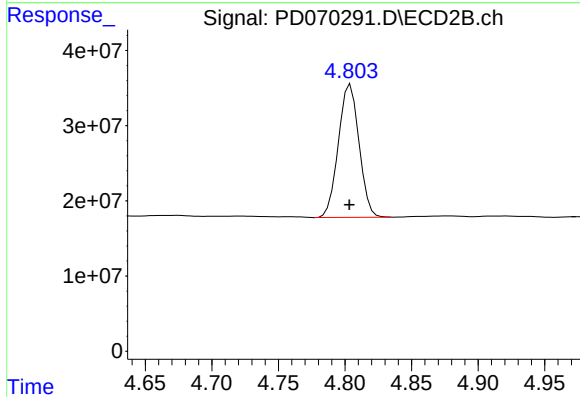


#3 gamma-BHC (Lindane)

R.T.: 4.804 min
Delta R.T.: 0.000 min
Response: 191171106
Conc: 10.24 ng/ml

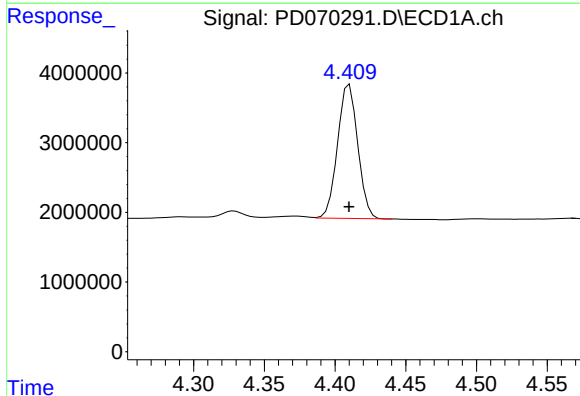


#4 Heptachlor

R.T.: 4.410 min
Delta R.T.: 0.000 min
Response: 19096770
Conc: 9.74 ng/ml

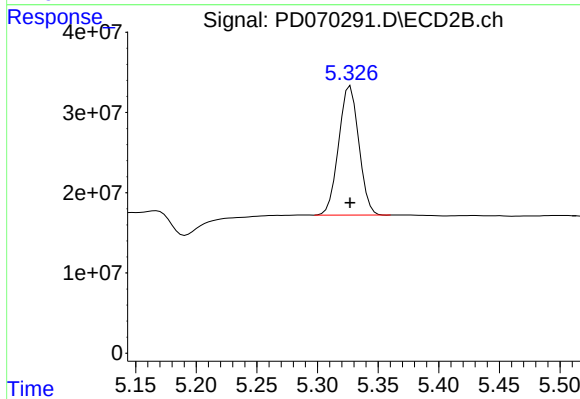

#4 Heptachlor


R.T.: 5.327 min
Delta R.T.: 0.000 min
Response: 186267290
Conc: 9.99 ng/ml

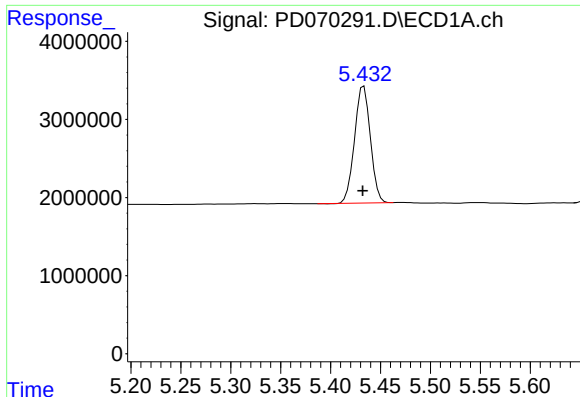

#9 Endosulfan I


R.T.: 5.433 min
Delta R.T.: 0.001 min
Response: 16488603
Conc: 9.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

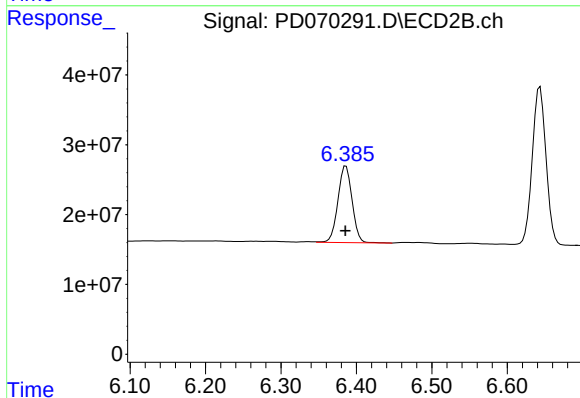


#9 Endosulfan I

R.T.: 6.386 min
Delta R.T.: 0.000 min
Response: 143563654
Conc: 10.21 ng/ml

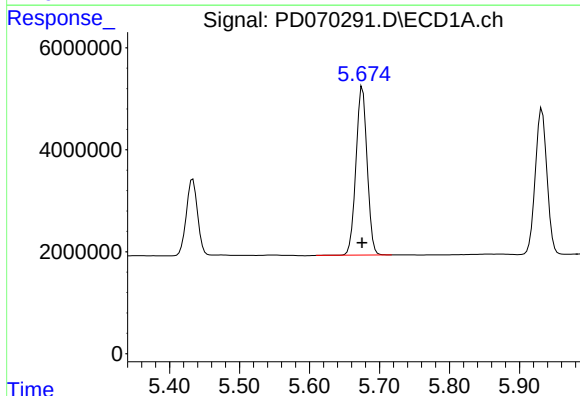


#13 Dieldrin

R.T.: 5.676 min
Delta R.T.: 0.000 min
Response: 36753821
Conc: 19.77 ng/ml

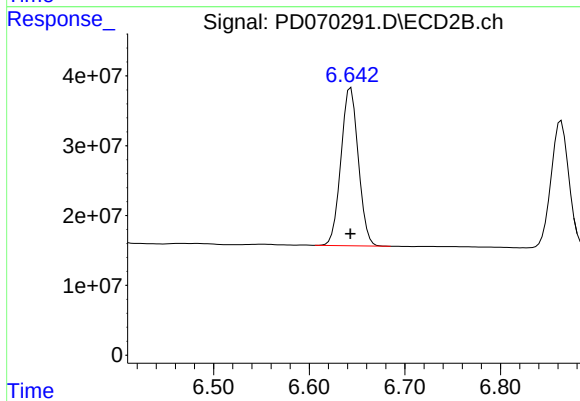

#13 Dieldrin


R.T.: 6.643 min
Delta R.T.: 0.000 min
Response: 286187097
Conc: 20.26 ng/ml

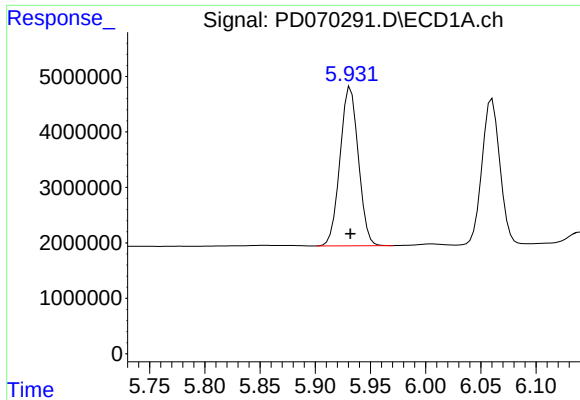

#14 Endrin


R.T.: 5.932 min
Delta R.T.: 0.000 min
Response: 33128024
Conc: 19.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

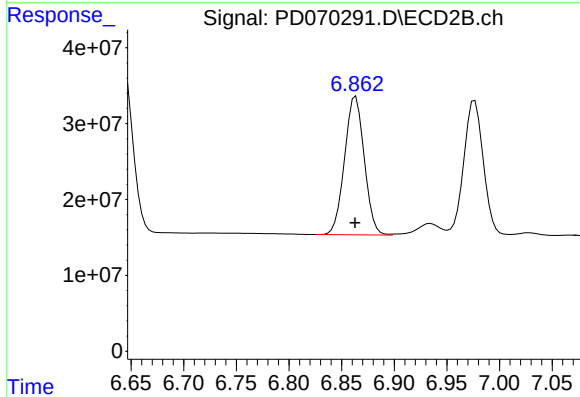


#14 Endrin

R.T.: 6.864 min
Delta R.T.: 0.000 min
Response: 237999943
Conc: 19.75 ng/ml

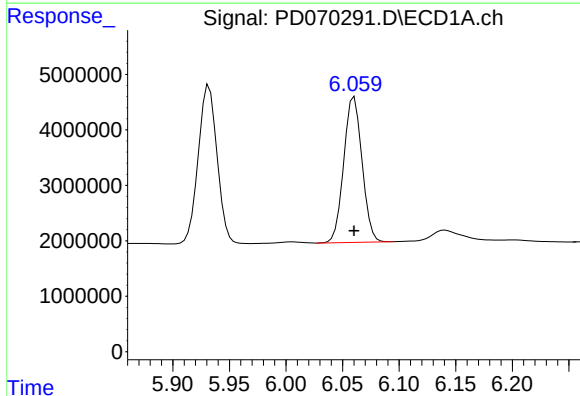


#16 4,4'-DDD

R.T.: 6.060 min
Delta R.T.: 0.000 min
Response: 29514460
Conc: 19.94 ng/ml

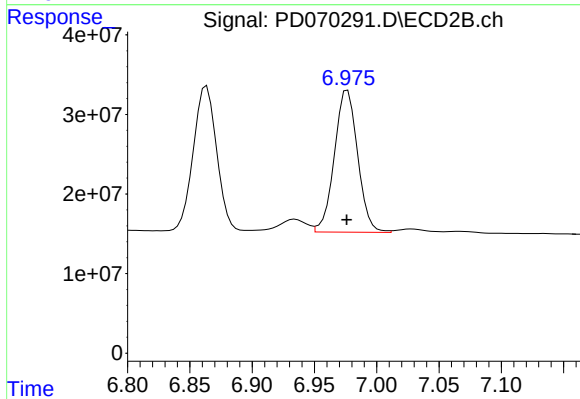

#16 4,4'-DDD


R.T.: 6.977 min
Delta R.T.: 0.000 min
Response: 232511531
Conc: 20.42 ng/ml

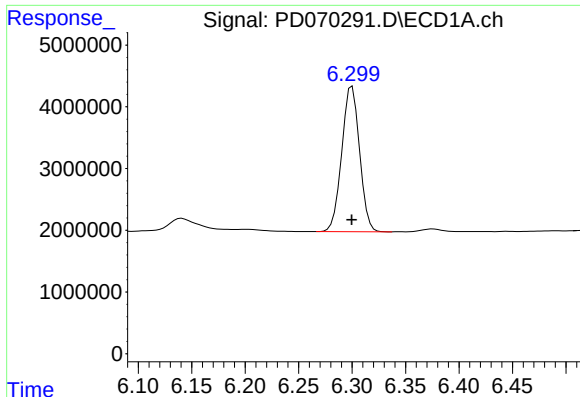

#17 4,4'-DDT


R.T.: 6.300 min
Delta R.T.: 0.000 min
Response: 27289505
Conc: 19.77 ng/ml

Instrument :
ECD_D
ClientSampleId :

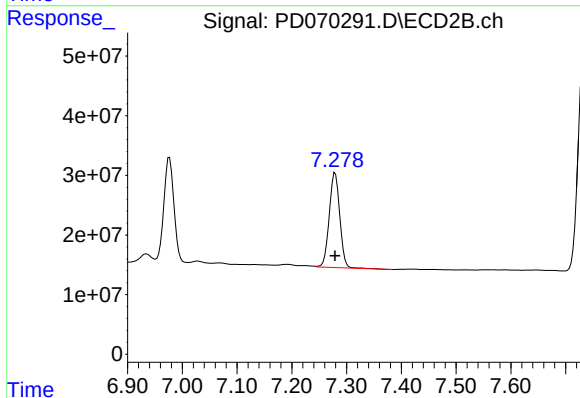


#17 4,4'-DDT

R.T.: 7.279 min
Delta R.T.: 0.000 min
Response: 213136343
Conc: 20.00 ng/ml

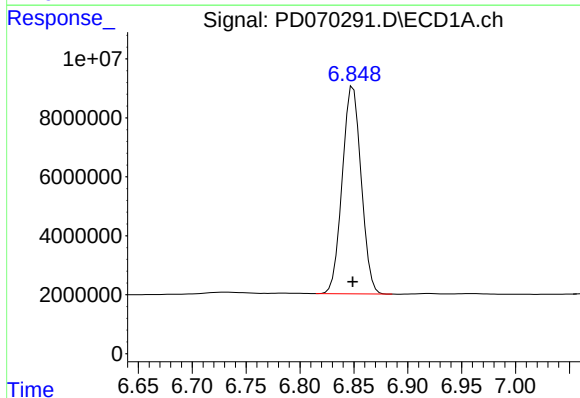


#20 Methoxychlor

R.T.: 6.849 min
Delta R.T.: 0.000 min
Response: 86071433
Conc: 99.68 ng/ml

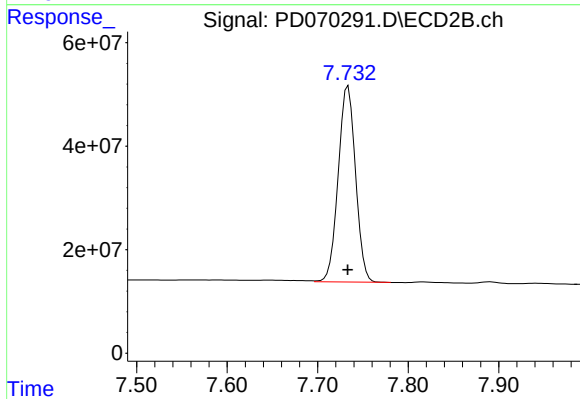

#20 Methoxychlor


R.T.: 7.734 min
Delta R.T.: 0.000 min
Response: 503482215
Conc: 101.71 ng/ml

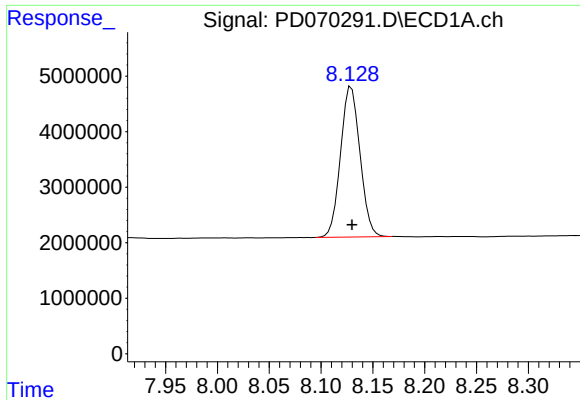

#27 Decachlorobiphenyl

R.T.: 8.129 min
Delta R.T.: 0.000 min
Response: 35369396
Conc: 21.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

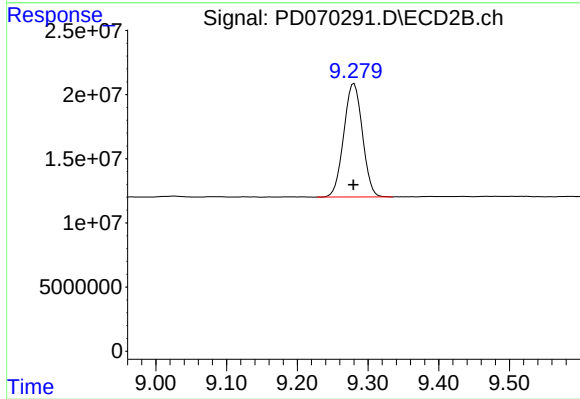

#27 Decachlorobiphenyl

R.T.: 9.280 min
Delta R.T.: 0.000 min
Response: 162074575
Conc: 21.53 ng/ml