

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061422\
 Data File : PD070293.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2022 13:31
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 15:20:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 14 15:17:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.400	4.122	28134939	265.5E6	20.000	20.000
27)	SA Decachlor...	8.130	9.280	61649166	281.7E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.836	4.515	40688959	383.8E6	20.000	20.000
3)	MA gamma-BHC...	4.116	4.804	38887343	356.3E6	20.000	20.000
4)	MA Heptachlor	4.410	5.327	38548097	359.2E6	20.000	20.000
9)	A Endosulfan I	5.432	6.386	32723343	264.1E6	20.000	20.000
13)	MA Dieldrin	5.675	6.644	74007251	536.3E6	40.000	40.000
14)	MA Endrin	5.931	6.863	66450642	444.9E6	40.000	40.000
16)	A 4,4'-DDD	6.060	6.978	59140870	427.3E6	40.000	40.000
17)	MA 4,4'-DDT	6.299	7.280	57138759	396.3E6	40.000	40.000
20)	A Methoxychlor	6.848	7.734	166.9E6	917.9E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061422\
Data File : PD070293.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2022 13:31
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 15:20:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 14 15:17:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

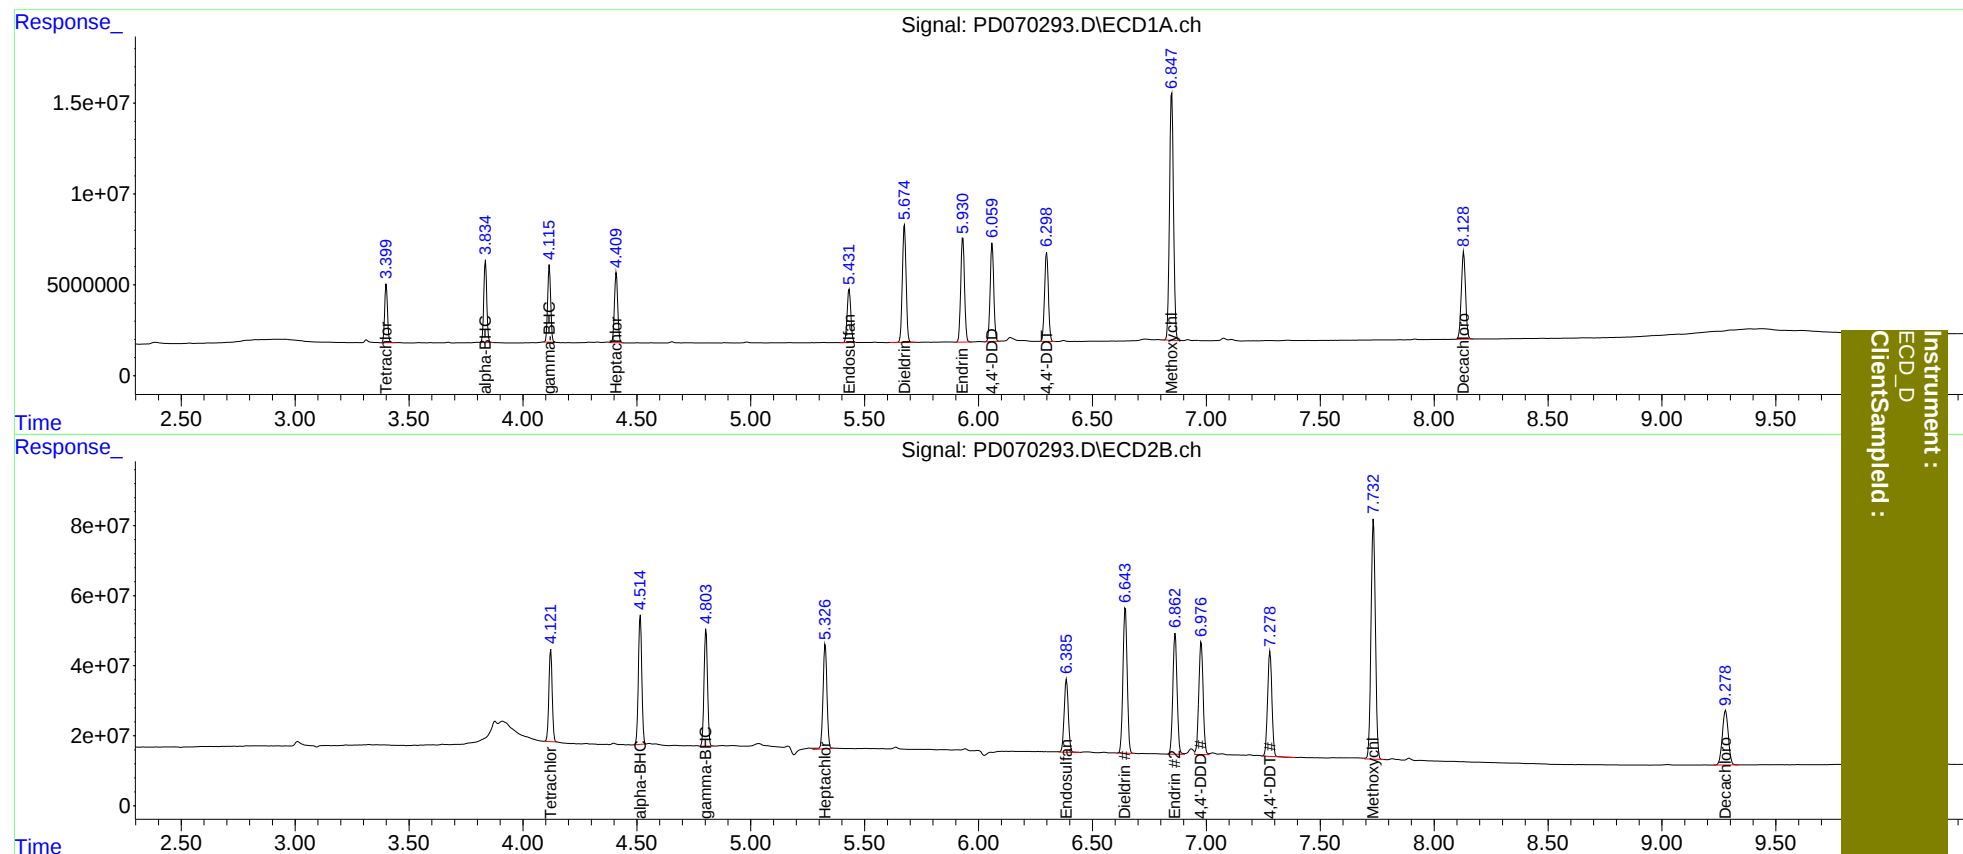


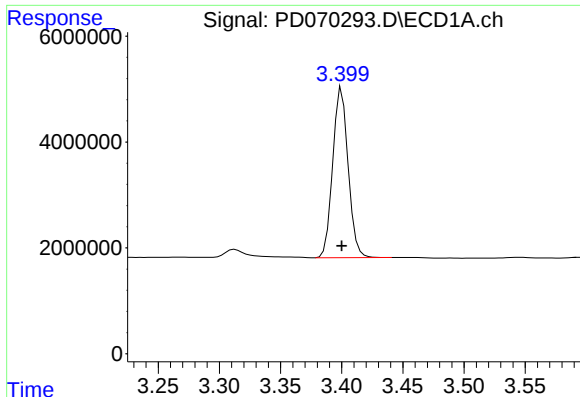

#1 Tetrachloro-m-xylene


R.T.: 3.400 min
Delta R.T.: 0.000 min
Response: 28134939
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

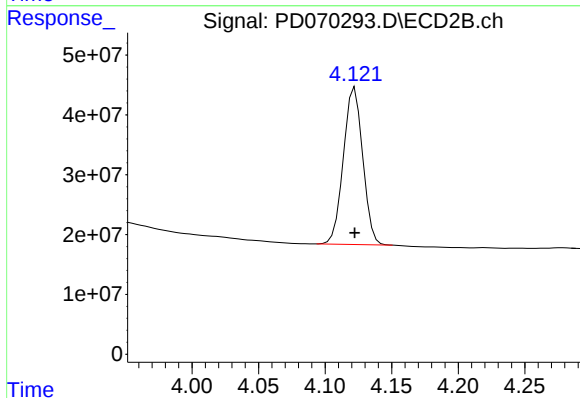


#1 Tetrachloro-m-xylene

R.T.: 4.122 min
Delta R.T.: 0.000 min
Response: 265452741
Conc: 20.00 ng/ml

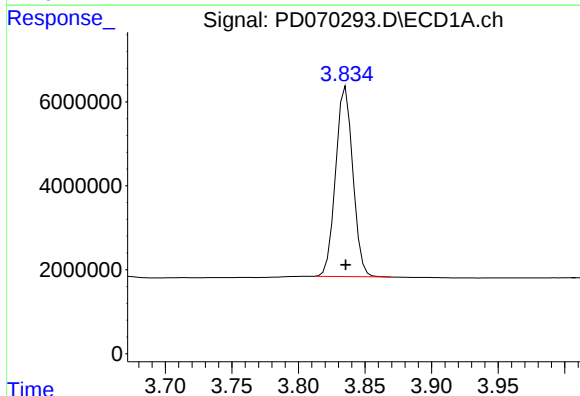


#2 alpha-BHC

R.T.: 3.836 min
Delta R.T.: 0.000 min
Response: 40688959
Conc: 20.00 ng/ml

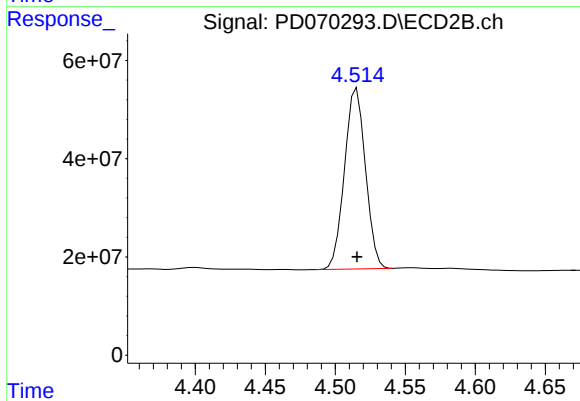

#2 alpha-BHC


R.T.: 4.515 min
Delta R.T.: 0.000 min
Response: 383787452
Conc: 20.00 ng/ml

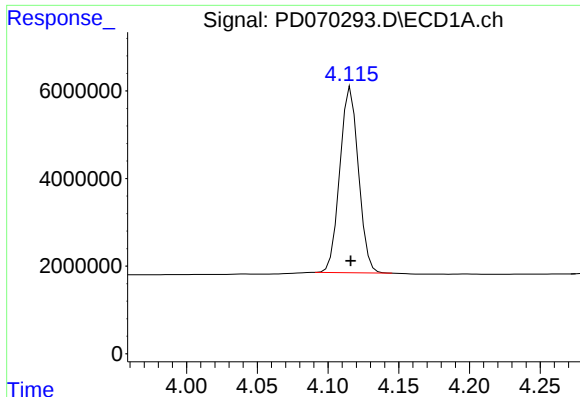

#3 gamma-BHC (Lindane)


R.T.: 4.116 min
Delta R.T.: 0.000 min
Response: 38887343
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

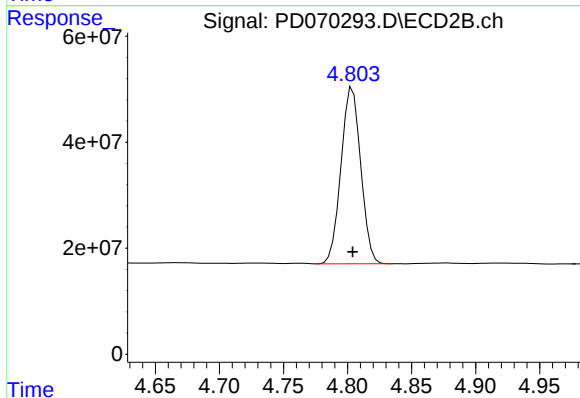


#3 gamma-BHC (Lindane)

R.T.: 4.804 min
Delta R.T.: 0.000 min
Response: 356330446
Conc: 20.00 ng/ml

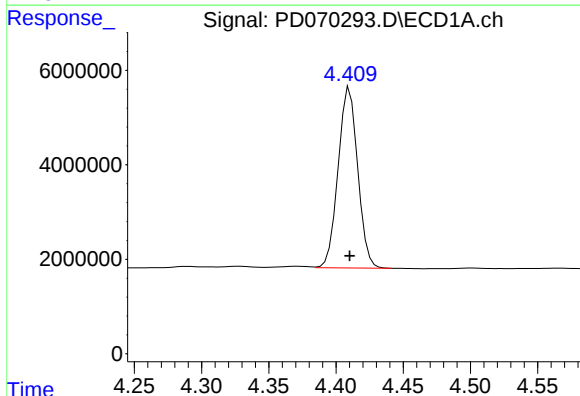


#4 Heptachlor

R.T.: 4.410 min
Delta R.T.: 0.000 min
Response: 38548097
Conc: 20.00 ng/ml

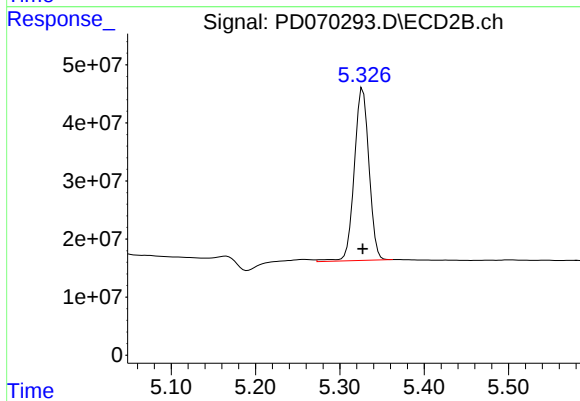

#4 Heptachlor


R.T.: 5.327 min
Delta R.T.: 0.000 min
Response: 359155693
Conc: 20.00 ng/ml

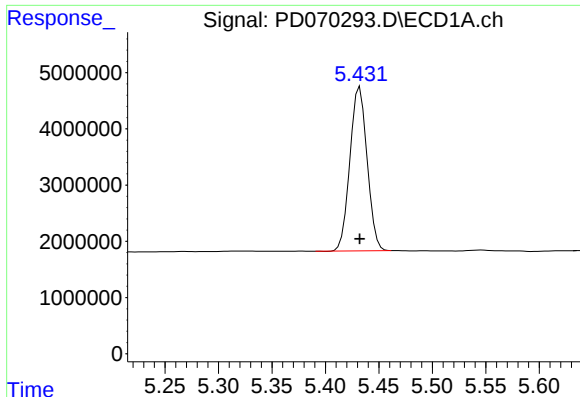

#9 Endosulfan I


R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 32723343
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

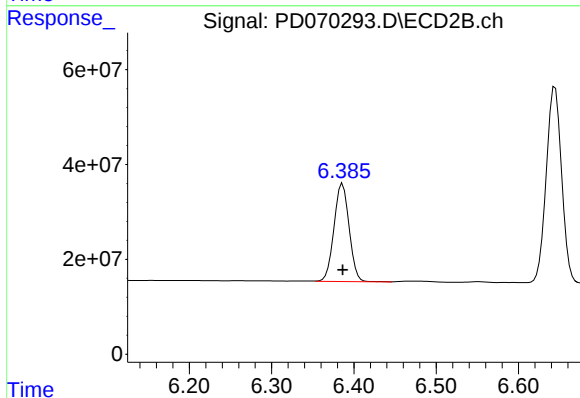


#9 Endosulfan I

R.T.: 6.386 min
Delta R.T.: 0.000 min
Response: 264057164
Conc: 20.00 ng/ml

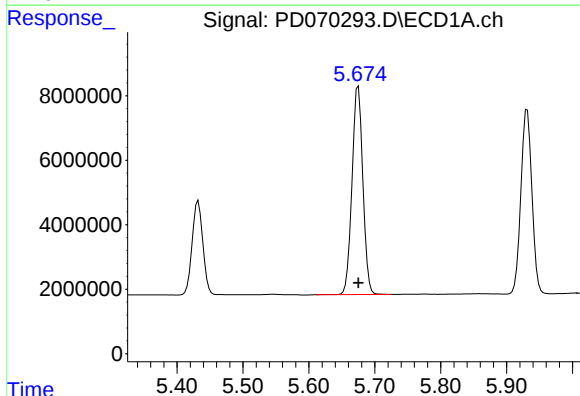


#13 Dieldrin

R.T.: 5.675 min
Delta R.T.: 0.000 min
Response: 74007251
Conc: 40.00 ng/ml

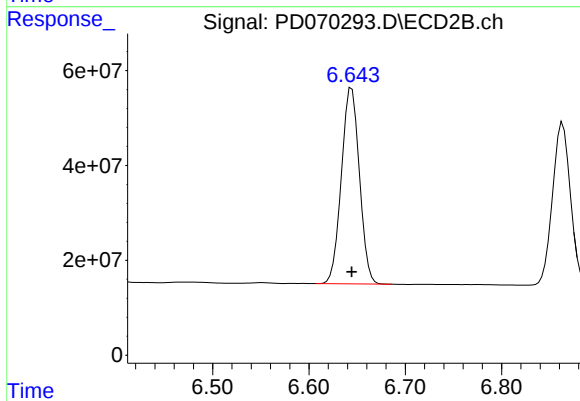

#13 Dieldrin


R.T.: 6.644 min
Delta R.T.: 0.000 min
Response: 536302602
Conc: 40.00 ng/ml

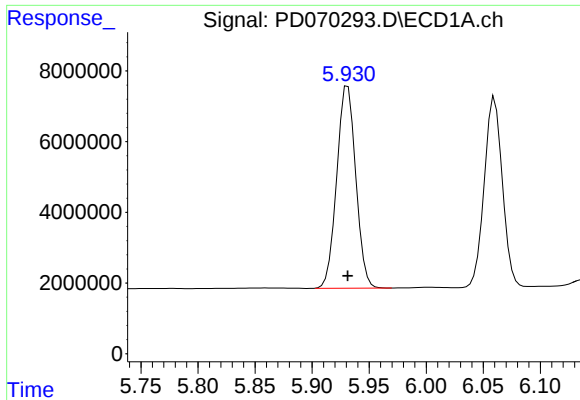

#14 Endrin


R.T.: 5.931 min
Delta R.T.: 0.000 min
Response: 66450642
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

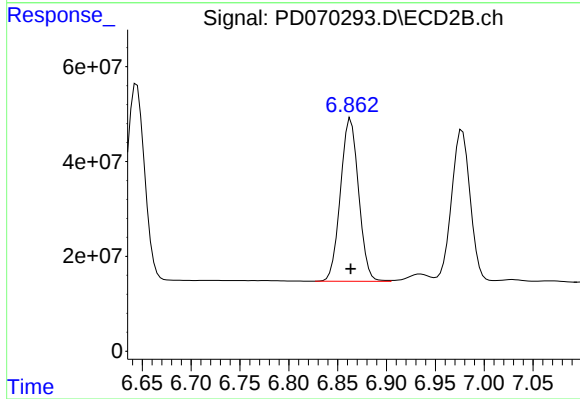


#14 Endrin

R.T.: 6.863 min
Delta R.T.: 0.000 min
Response: 444872440
Conc: 40.00 ng/ml

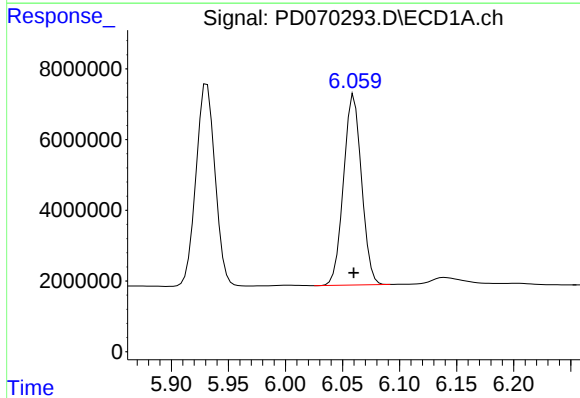


#16 4,4'-DDD

R.T.: 6.060 min
Delta R.T.: 0.000 min
Response: 59140870
Conc: 40.00 ng/ml

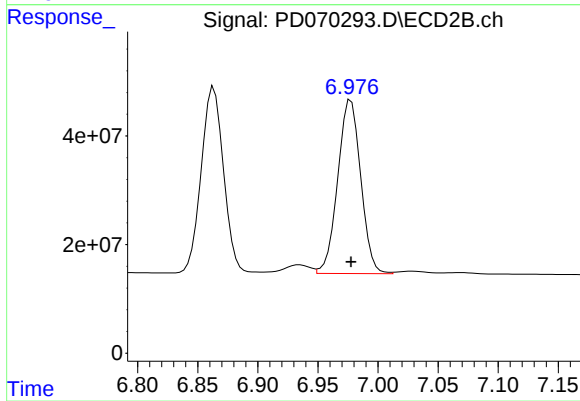

#16 4,4'-DDD


R.T.: 6.978 min
Delta R.T.: 0.000 min
Response: 427327576
Conc: 40.00 ng/ml

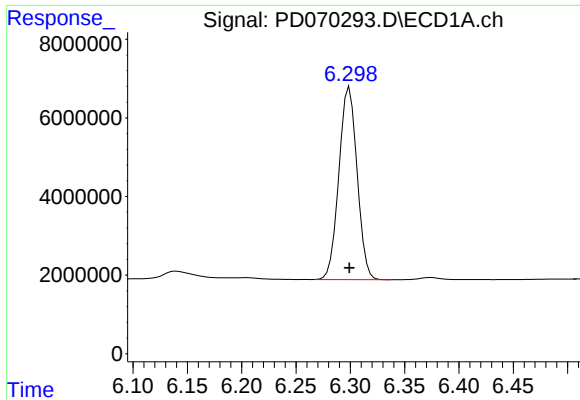

#17 4,4'-DDT


R.T.: 6.299 min
Delta R.T.: 0.000 min
Response: 57138759
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

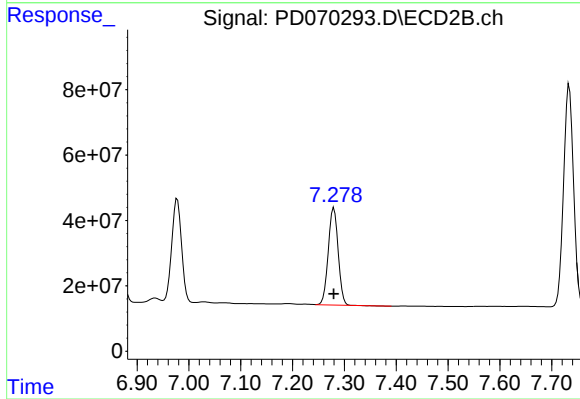


#17 4,4'-DDT

R.T.: 7.280 min
Delta R.T.: 0.000 min
Response: 396267849
Conc: 40.00 ng/ml

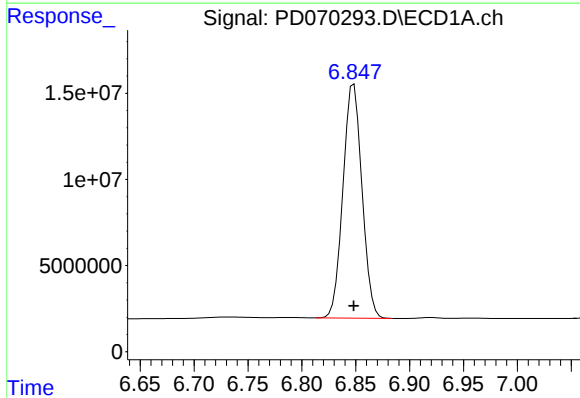


#20 Methoxychlor

R.T.: 6.848 min
Delta R.T.: 0.000 min
Response: 166856090
Conc: 200.00 ng/ml

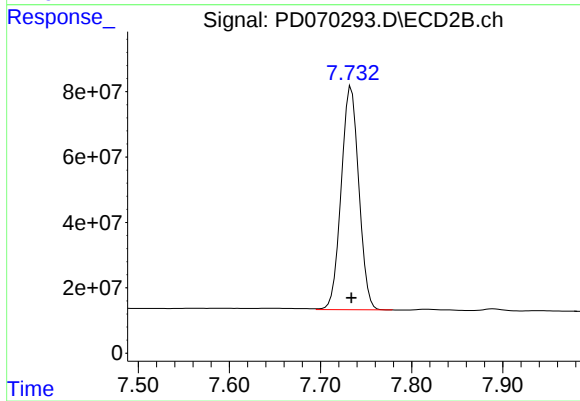

#20 Methoxychlor

R.T.: 7.734 min
Delta R.T.: 0.000 min
Response: 917896012
Conc: 200.00 ng/ml

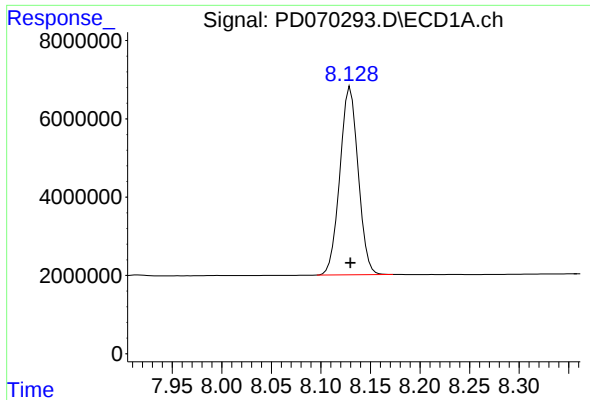

#27 Decachlorobiphenyl


R.T.: 8.130 min

Delta R.T.: 0.000 min

Response: 61649166

Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

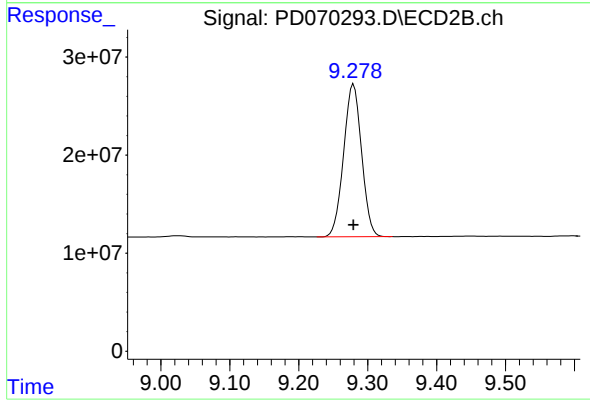

#27 Decachlorobiphenyl

R.T.: 9.280 min

Delta R.T.: 0.000 min

Response: 281726626

Conc: 40.00 ng/ml