

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061422\
 Data File : PD070295.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2022 13:59
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 15:20:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 14 15:17:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.401	4.122	56479715	518.3E6	40.149	39.053
27)	SA Decachlor...	8.130	9.280	121.3E6	520.2E6	78.682	73.862
Target Compounds							
2)	A alpha-BHC	3.836	4.516	85540618	765.1E6	42.046	39.873
3)	MA gamma-BHC...	4.117	4.804	80496015	700.4E6	41.400	39.312
4)	MA Heptachlor	4.411	5.327	78017447	689.0E6	40.478	38.369
9)	A Endosulfan I	5.433	6.387	66694549	510.8E6	40.763	38.685
13)	MA Dieldrin	5.675	6.644	154.1E6	1053.3E6	83.264	78.558
14)	MA Endrin	5.932	6.863	137.5E6	875.0E6	82.776	78.672
16)	A 4,4'-DDD	6.061	6.978	122.9E6	861.7E6	83.144	80.663
17)	MA 4,4'-DDT	6.299	7.280	122.2E6	784.8E6	85.518	79.224
20)	A Methoxychlor	6.849	7.734	331.6E6	1781.7E6	397.438	388.217


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061422\
Data File : PD070295.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2022 13:59
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 15:20:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 14 15:17:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

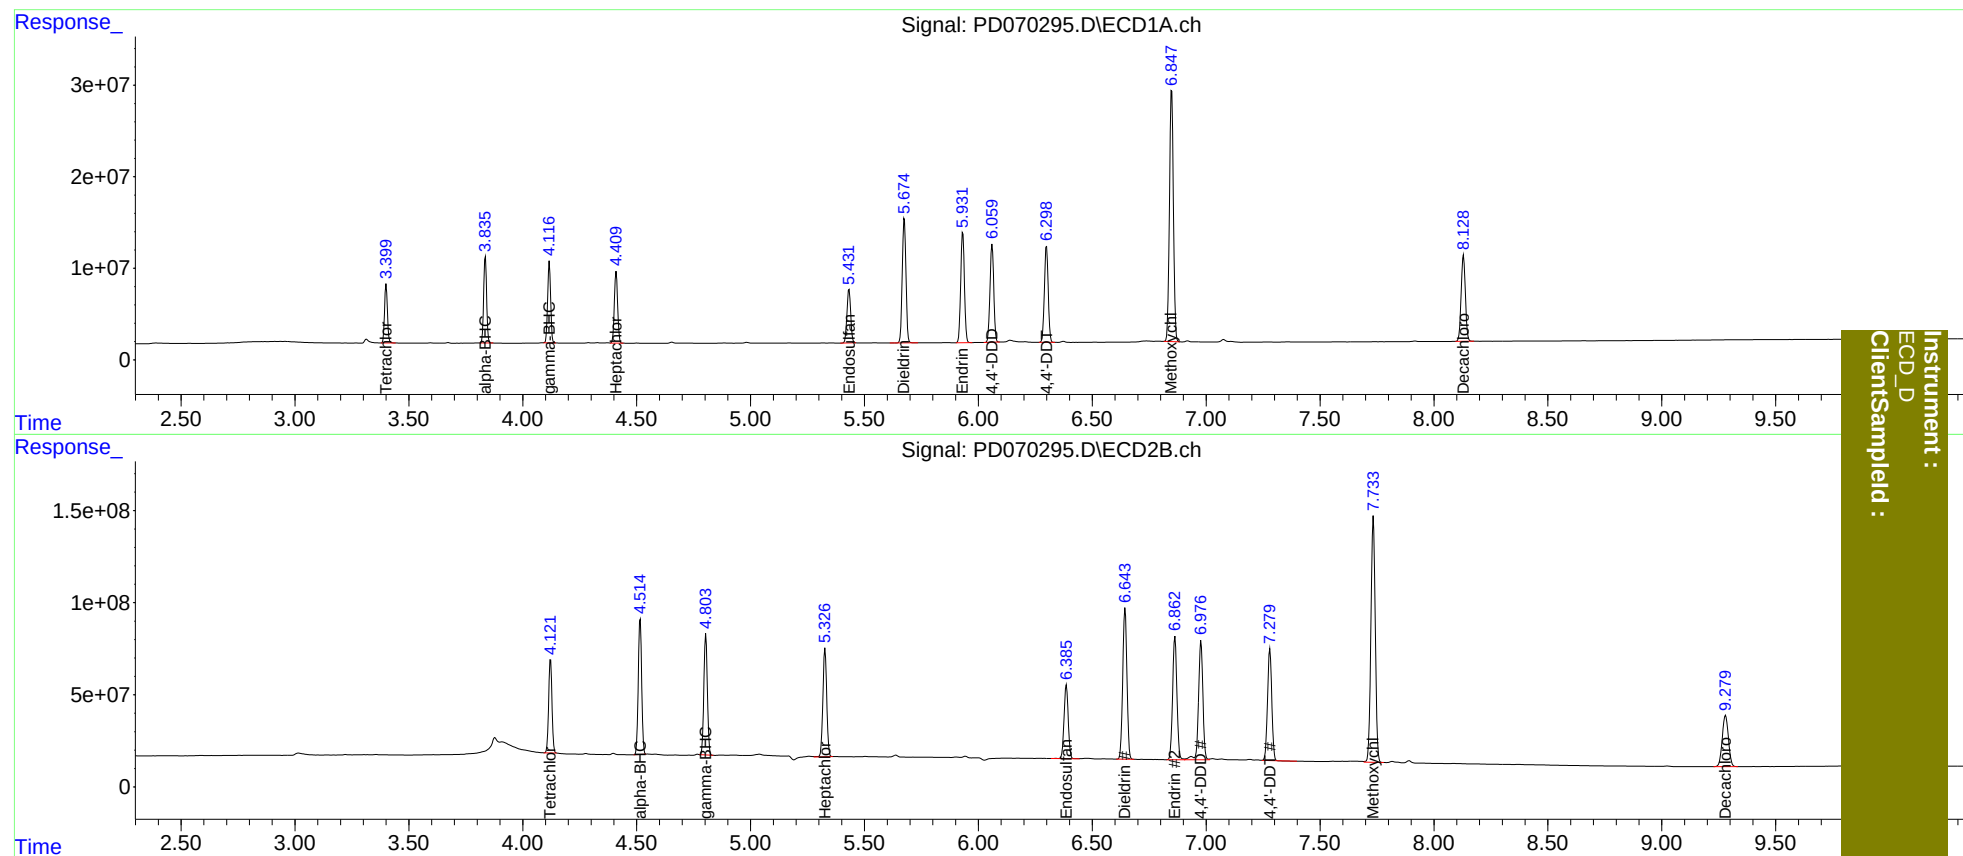


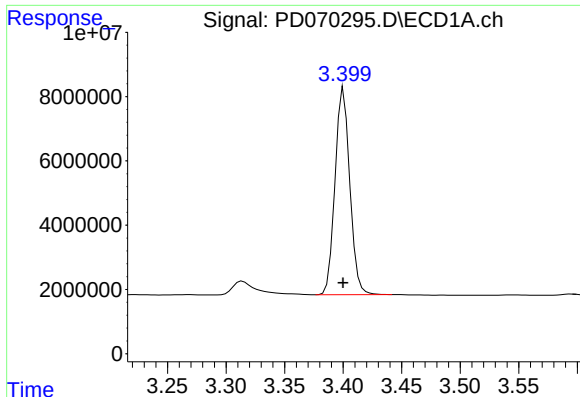

#1 Tetrachloro-m-xylene


R.T.: 3.401 min
Delta R.T.: 0.000 min
Response: 56479715
Conc: 40.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

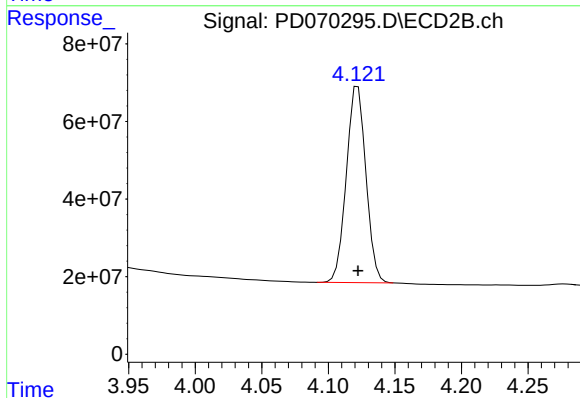


#1 Tetrachloro-m-xylene

R.T.: 4.122 min
Delta R.T.: 0.000 min
Response: 518339752
Conc: 39.05 ng/ml

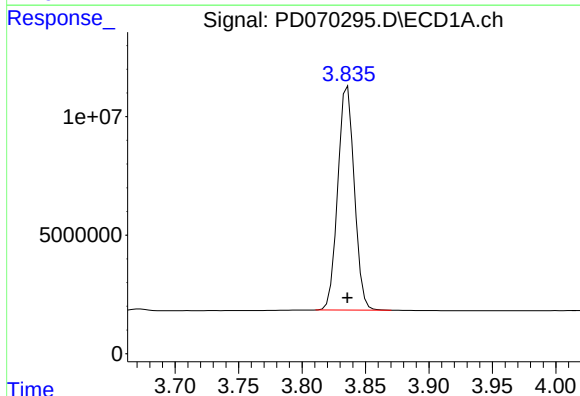


#2 alpha-BHC

R.T.: 3.836 min
Delta R.T.: 0.000 min
Response: 85540618
Conc: 42.05 ng/ml

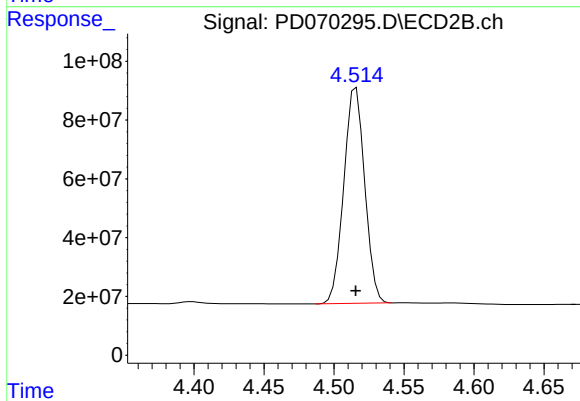

#2 alpha-BHC


R.T.: 4.516 min
Delta R.T.: 0.000 min
Response: 765146808
Conc: 39.87 ng/ml

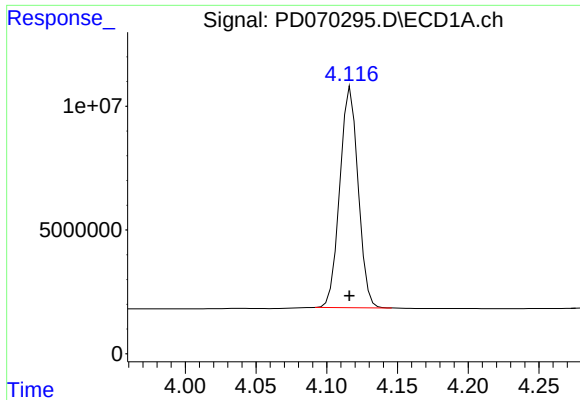

#3 gamma-BHC (Lindane)


R.T.: 4.117 min
Delta R.T.: 0.000 min
Response: 80496015
Conc: 41.40 ng/ml

Instrument :
ECD_D
ClientSampleId :

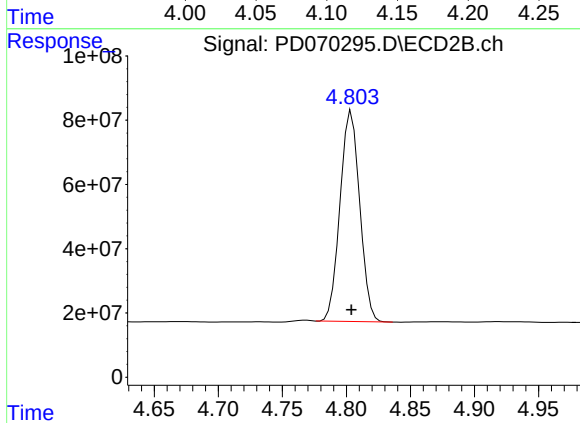


#3 gamma-BHC (Lindane)

R.T.: 4.804 min
Delta R.T.: 0.000 min
Response: 700410303
Conc: 39.31 ng/ml

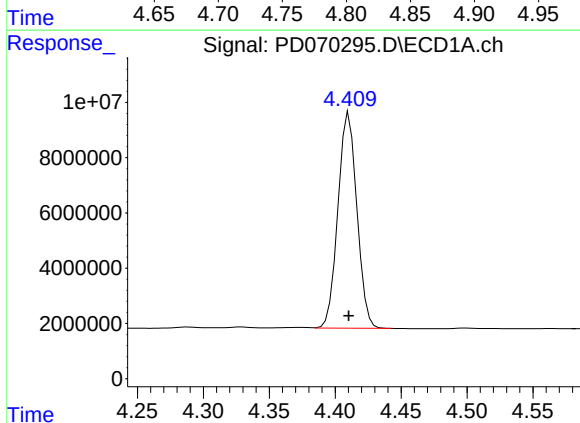


#4 Heptachlor

R.T.: 4.411 min
Delta R.T.: 0.000 min
Response: 78017447
Conc: 40.48 ng/ml

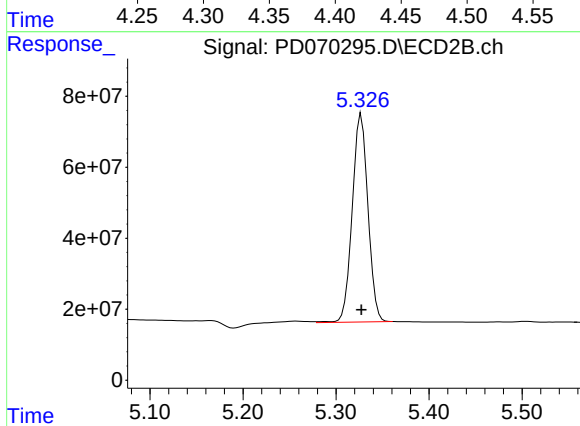

#4 Heptachlor


R.T.: 5.327 min
Delta R.T.: 0.000 min
Response: 689028658
Conc: 38.37 ng/ml

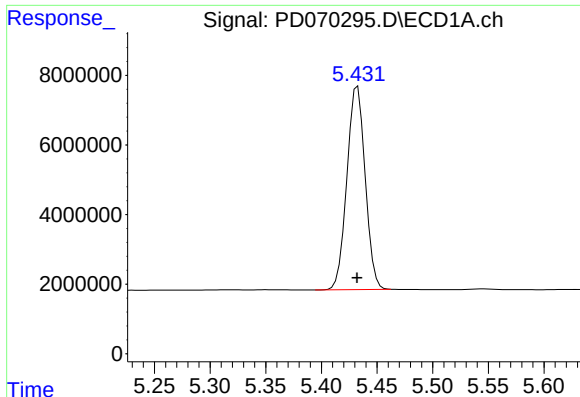

#9 Endosulfan I


R.T.: 5.433 min
Delta R.T.: 0.000 min
Response: 66694549
Conc: 40.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

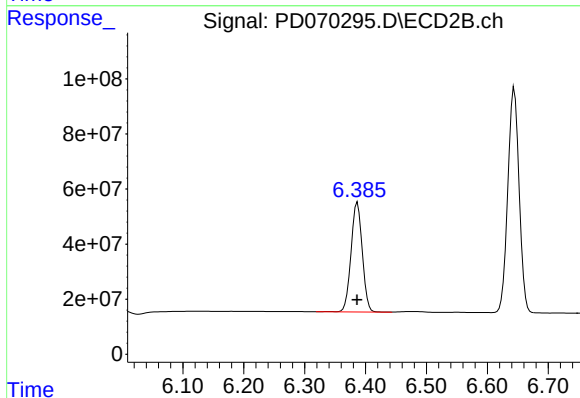


#9 Endosulfan I

R.T.: 6.387 min
Delta R.T.: 0.000 min
Response: 510753646
Conc: 38.69 ng/ml

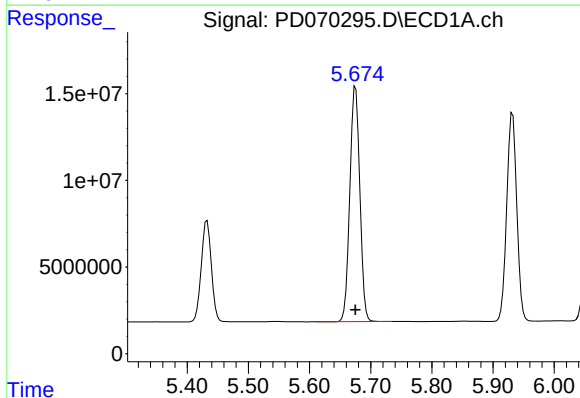


#13 Dieldrin

R.T.: 5.675 min
Delta R.T.: 0.000 min
Response: 154053394
Conc: 83.26 ng/ml

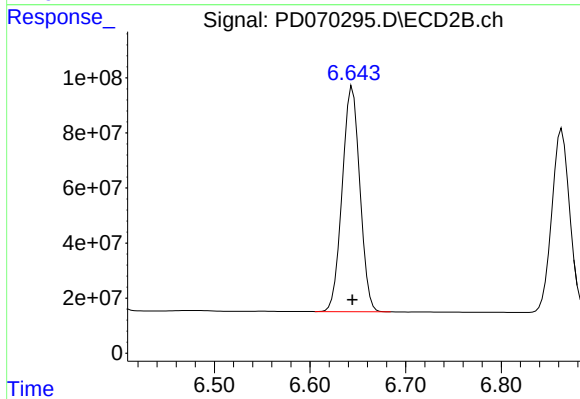

#13 Dieldrin


R.T.: 6.644 min
Delta R.T.: 0.000 min
Response: 1053269305
Conc: 78.56 ng/ml

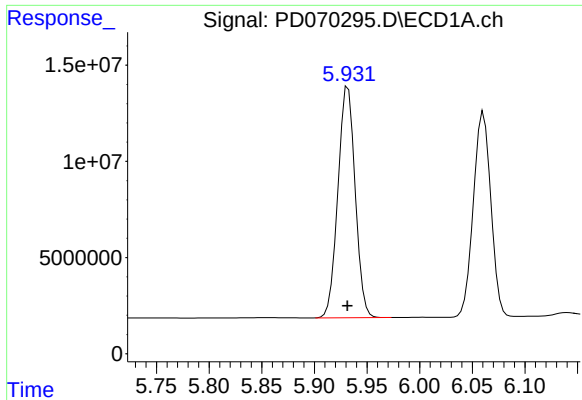

#14 Endrin


R.T.: 5.932 min
Delta R.T.: 0.000 min
Response: 137513164
Conc: 82.78 ng/ml

Instrument :
ECD_D
ClientSampleId :

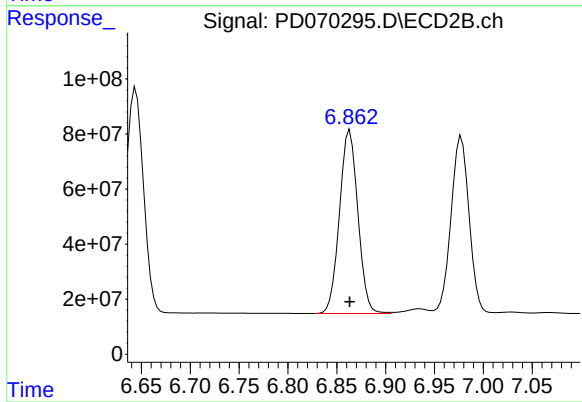


#14 Endrin

R.T.: 6.863 min
Delta R.T.: 0.000 min
Response: 874977367
Conc: 78.67 ng/ml

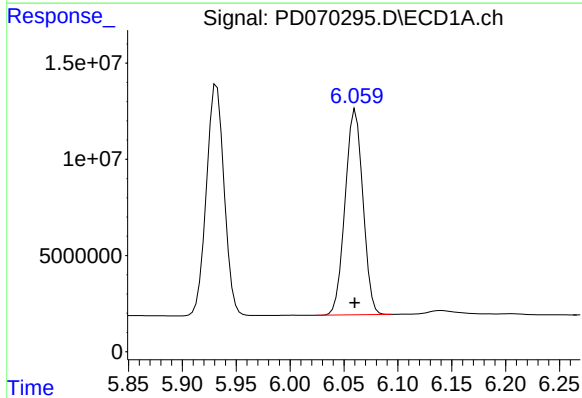


#16 4,4'-DDD

R.T.: 6.061 min
Delta R.T.: 0.000 min
Response: 122929708
Conc: 83.14 ng/ml

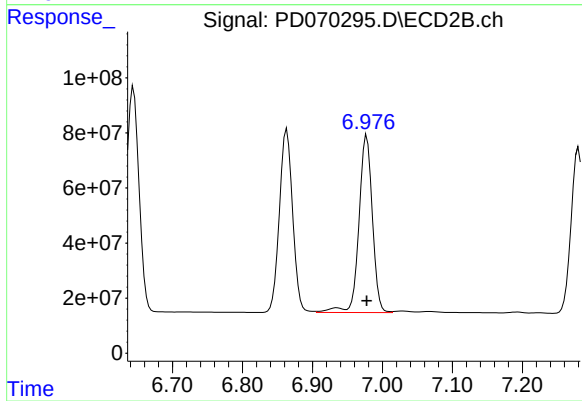

#16 4,4'-DDD


R.T.: 6.978 min
Delta R.T.: 0.000 min
Response: 861732873
Conc: 80.66 ng/ml

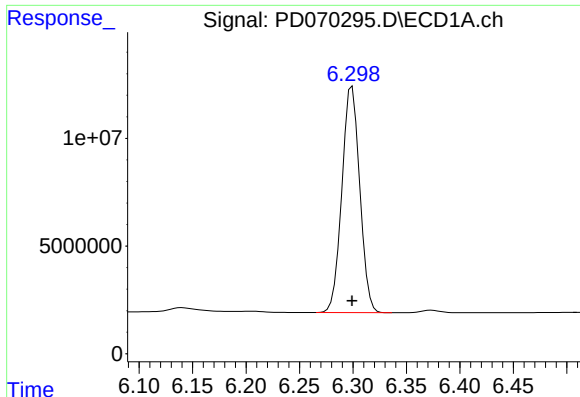

#17 4,4'-DDT


R.T.: 6.299 min
Delta R.T.: 0.000 min
Response: 122159465
Conc: 85.52 ng/ml

Instrument :
ECD_D
ClientSampleId :

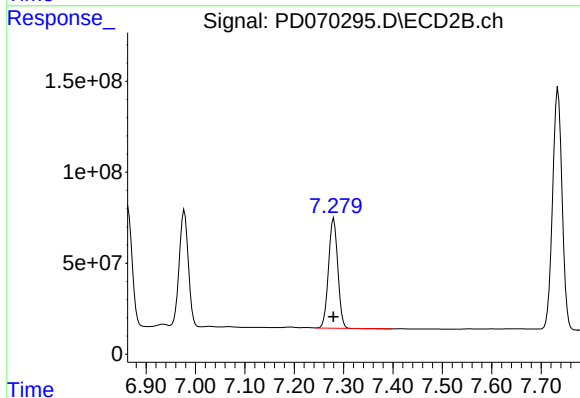


#17 4,4'-DDT

R.T.: 7.280 min
Delta R.T.: 0.000 min
Response: 784849900
Conc: 79.22 ng/ml

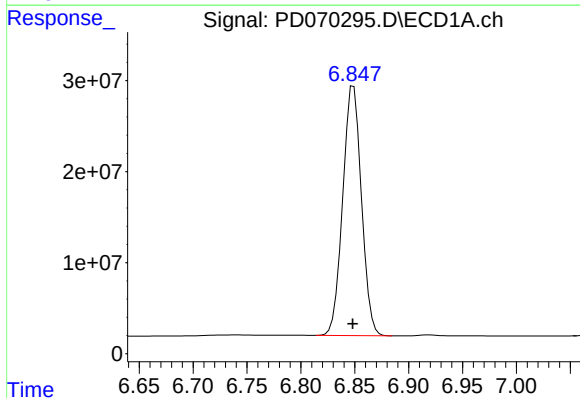


#20 Methoxychlor

R.T.: 6.849 min
Delta R.T.: 0.000 min
Response: 331574782
Conc: 397.44 ng/ml

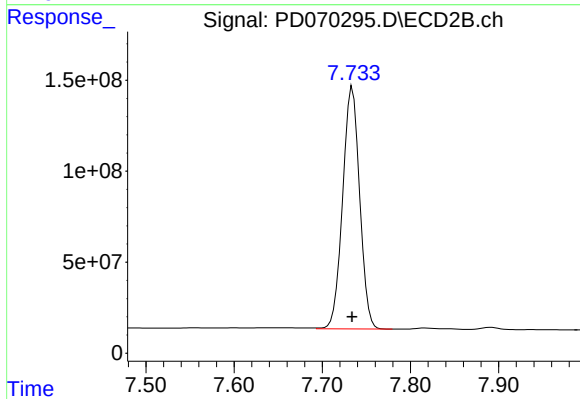

#20 Methoxychlor


R.T.: 7.734 min
Delta R.T.: 0.000 min
Response: 1781712232
Conc: 388.22 ng/ml

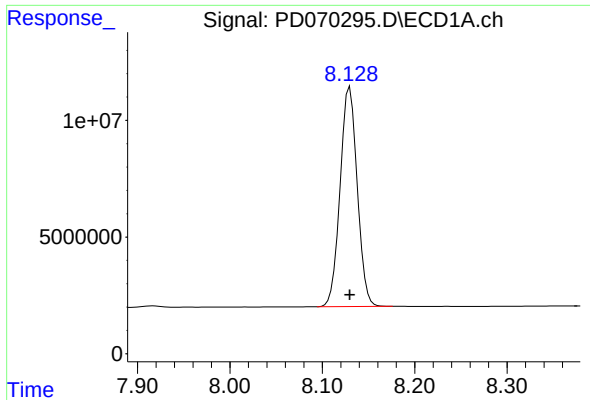

#27 Decachlorobiphenyl

R.T.: 8.130 min
Delta R.T.: 0.000 min
Response: 121267725
Conc: 78.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

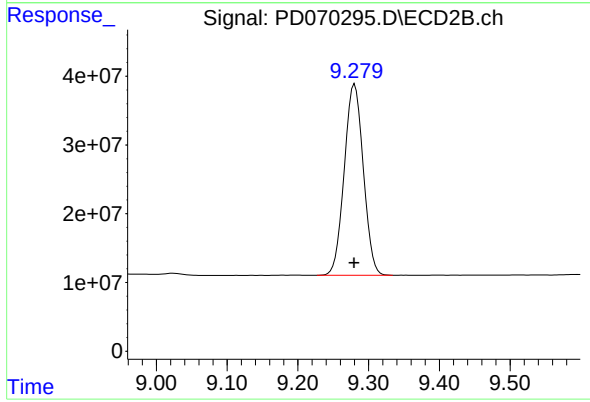

#27 Decachlorobiphenyl

R.T.: 9.280 min
Delta R.T.: 0.000 min
Response: 520222120
Conc: 73.86 ng/ml