

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061422\
 Data File : PD070297.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2022 14:27
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 15:20:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 14 15:17:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.400	4.123	116.3E6	998.3E6	82.666	75.218
27)	SA Decachlor...	8.129	9.279	239.8E6	1028.1E6	155.560	145.971
Target Compounds							
2)	A alpha-BHC	3.836	4.516	183.8E6	1510.1E6	90.347	78.696
3)	MA gamma-BHC...	4.116	4.805	171.8E6	1377.8E6	88.376	77.331
4)	MA Heptachlor	4.410	5.327	164.9E6	1315.5E6	85.537	73.252
9)	A Endosulfan I	5.432	6.387	137.2E6	973.7E6	83.846	73.746
13)	MA Dieldrin	5.675	6.644	320.5E6	2040.7E6	173.216	152.205
14)	MA Endrin	5.931	6.864	285.3E6	1694.4E6	171.766	152.351
16)	A 4,4'-DDD	6.060	6.978	255.6E6	1605.9E6	172.875	150.325
17)	MA 4,4'-DDT	6.299	7.280	259.8E6	1540.7E6	181.872	155.520
20)	A Methoxychlor	6.848	7.733	652.3E6	3372.2E6	781.832	734.777


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061422\
Data File : PD070297.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2022 14:27
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 15:20:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 14 15:17:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

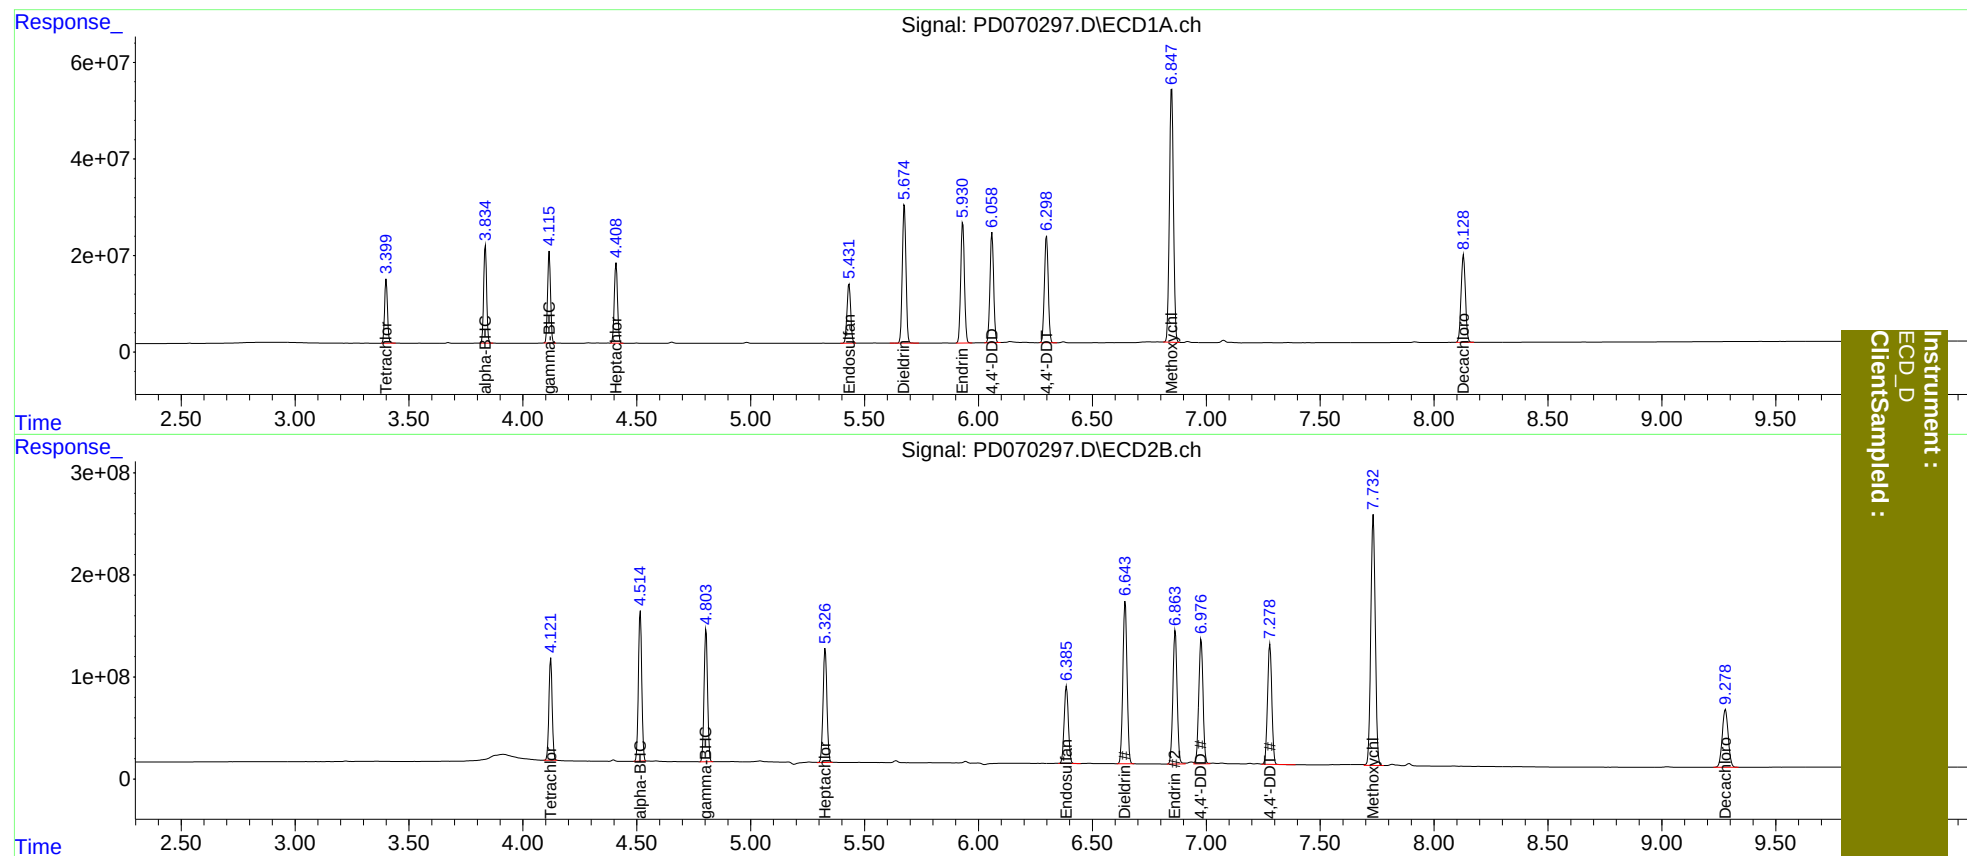


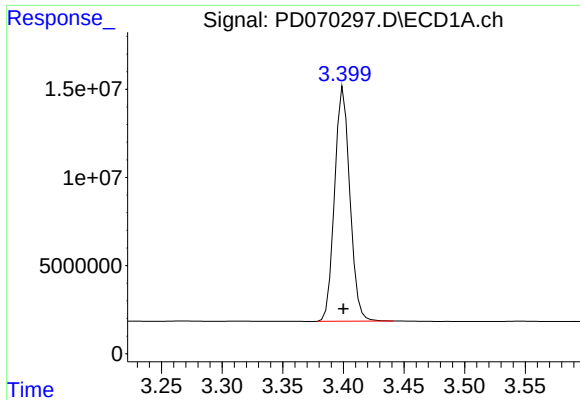

#1 Tetrachloro-m-xylene


R.T.: 3.400 min
Delta R.T.: 0.000 min
Response: 116289629
Conc: 82.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

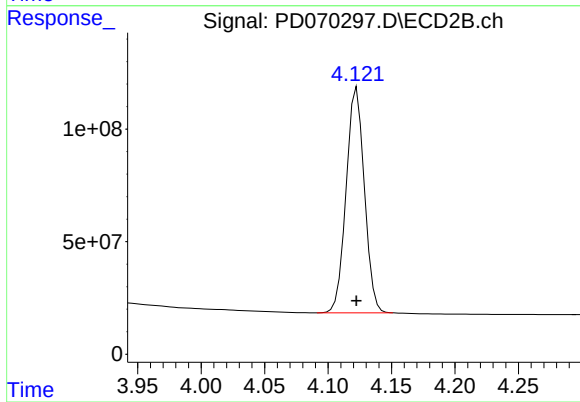


#1 Tetrachloro-m-xylene

R.T.: 4.123 min
Delta R.T.: 0.000 min
Response: 998345100
Conc: 75.22 ng/ml

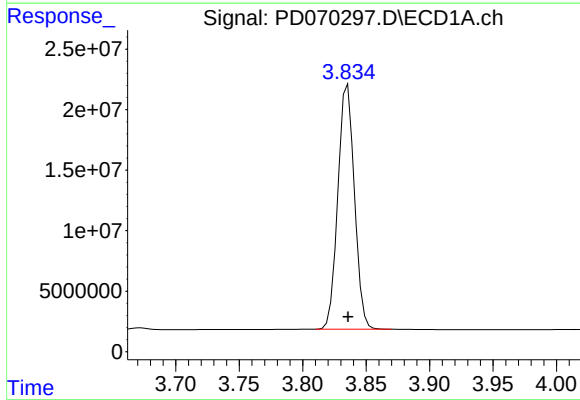


#2 alpha-BHC

R.T.: 3.836 min
Delta R.T.: 0.000 min
Response: 183807013
Conc: 90.35 ng/ml

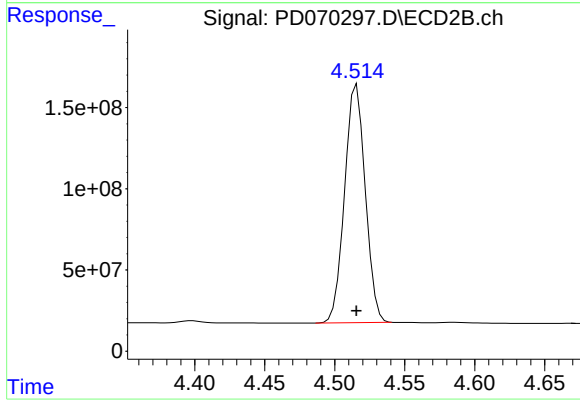

#2 alpha-BHC


R.T.: 4.516 min
Delta R.T.: 0.000 min
Response: 1510121274
Conc: 78.70 ng/ml

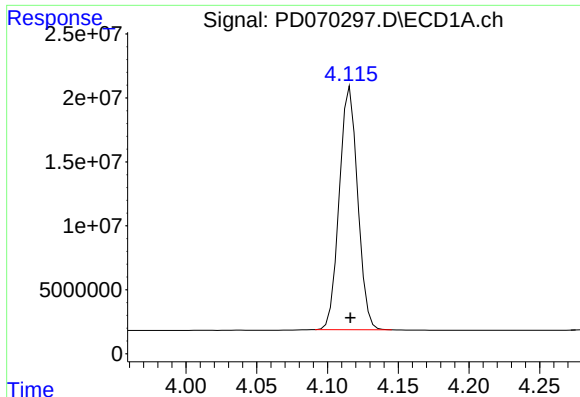

#3 gamma-BHC (Lindane)


R.T.: 4.116 min
Delta R.T.: 0.000 min
Response: 171835566
Conc: 88.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

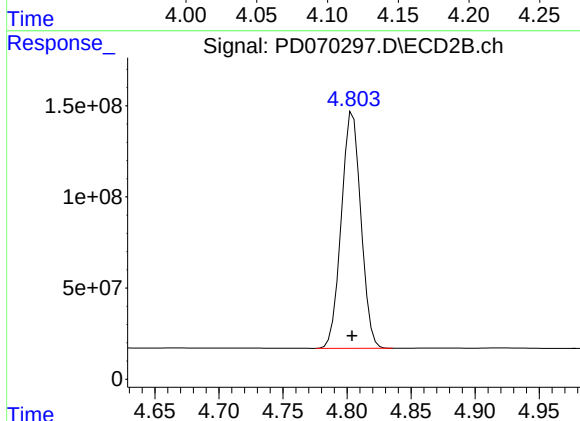


#3 gamma-BHC (Lindane)

R.T.: 4.805 min
Delta R.T.: 0.000 min
Response: 1377777929
Conc: 77.33 ng/ml

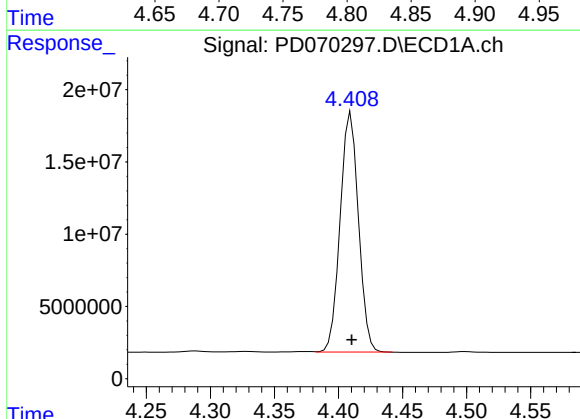


#4 Heptachlor

R.T.: 4.410 min
Delta R.T.: 0.000 min
Response: 164864246
Conc: 85.54 ng/ml

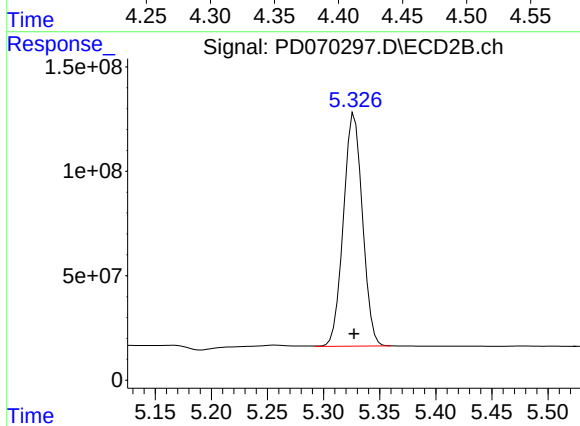

#4 Heptachlor


R.T.: 5.327 min
Delta R.T.: 0.000 min
Response: 1315451142
Conc: 73.25 ng/ml

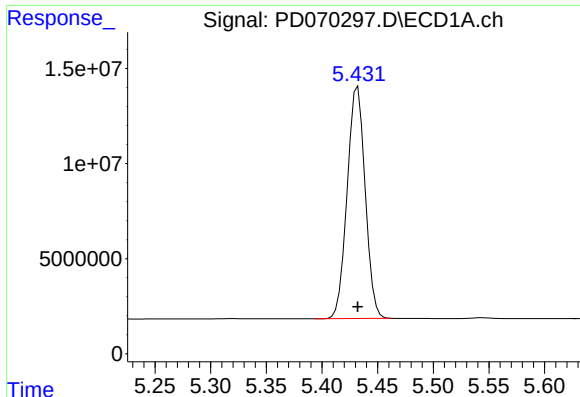

#9 Endosulfan I


R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 137186485
Conc: 83.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

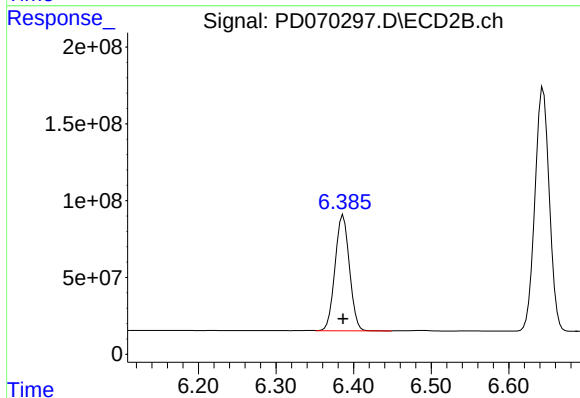


#9 Endosulfan I

R.T.: 6.387 min
Delta R.T.: 0.000 min
Response: 973659391
Conc: 73.75 ng/ml

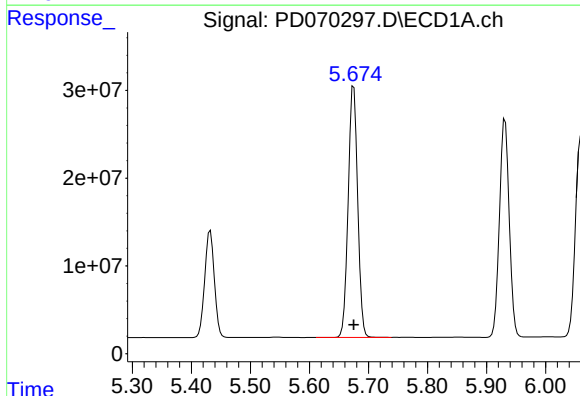


#13 Dieldrin

R.T.: 5.675 min
Delta R.T.: 0.000 min
Response: 320481586
Conc: 173.22 ng/ml

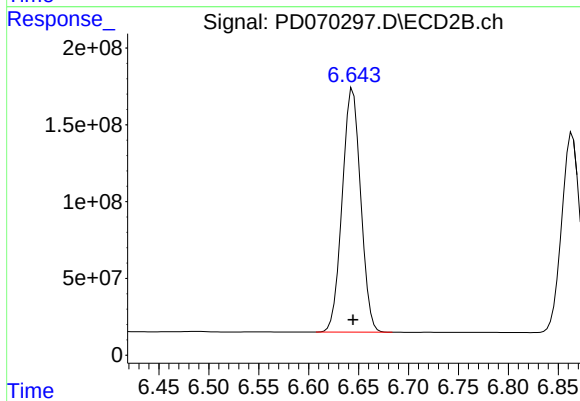

#13 Dieldrin


R.T.: 6.644 min
Delta R.T.: 0.000 min
Response: 2040699035
Conc: 152.21 ng/ml

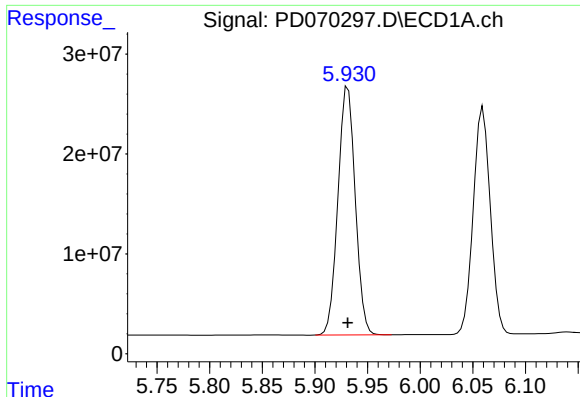

#14 Endrin


R.T.: 5.931 min
Delta R.T.: 0.000 min
Response: 285349319
Conc: 171.77 ng/ml

Instrument :
ECD_D
ClientSampleId :

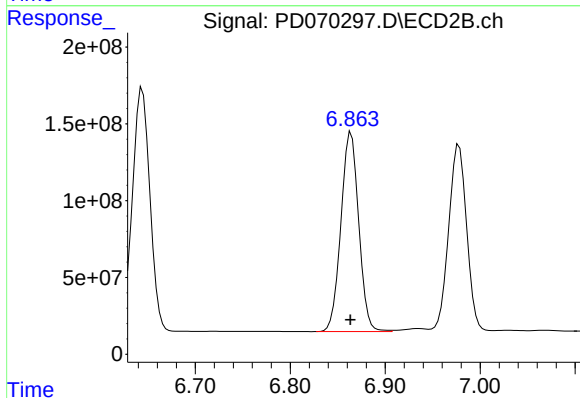


#14 Endrin

R.T.: 6.864 min
Delta R.T.: 0.000 min
Response: 1694420914
Conc: 152.35 ng/ml

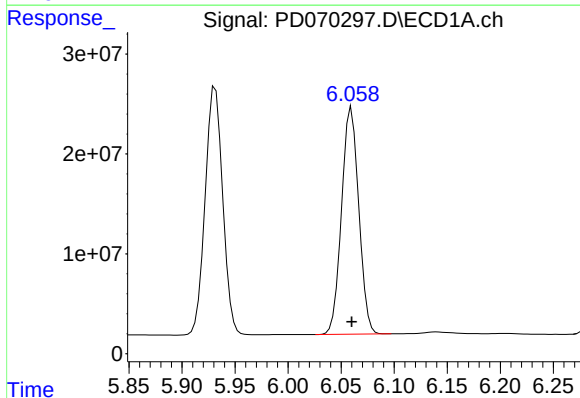


#16 4,4'-DDD

R.T.: 6.060 min
Delta R.T.: 0.000 min
Response: 255599643
Conc: 172.88 ng/ml

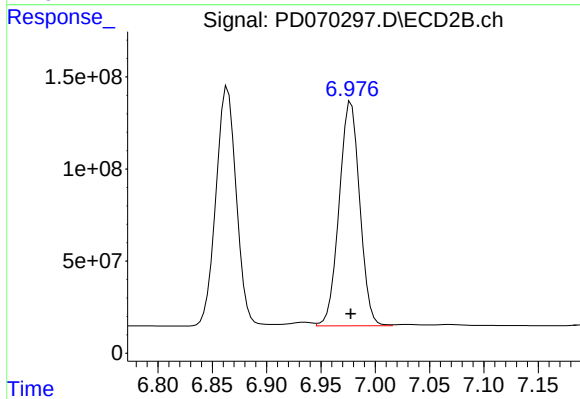

#16 4,4'-DDD


R.T.: 6.978 min
Delta R.T.: 0.000 min
Response: 1605945768
Conc: 150.32 ng/ml

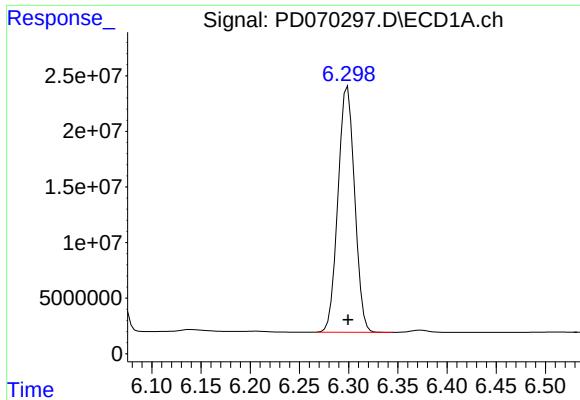

#17 4,4'-DDT


R.T.: 6.299 min
Delta R.T.: 0.000 min
Response: 259798875
Conc: 181.87 ng/ml

Instrument :
ECD_D
ClientSampleId :

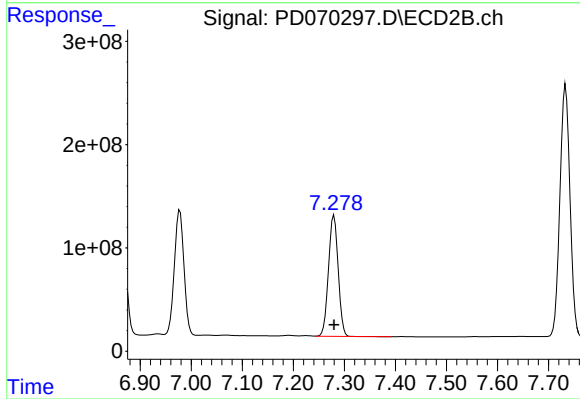


#17 4,4'-DDT

R.T.: 7.280 min
Delta R.T.: 0.000 min
Response: 1540687693
Conc: 155.52 ng/ml

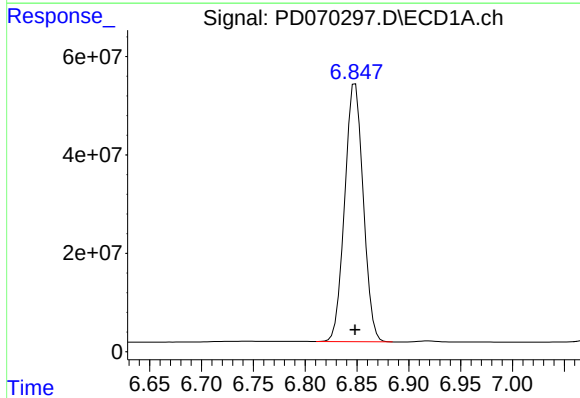


#20 Methoxychlor

R.T.: 6.848 min
Delta R.T.: 0.000 min
Response: 652266912
Conc: 781.83 ng/ml

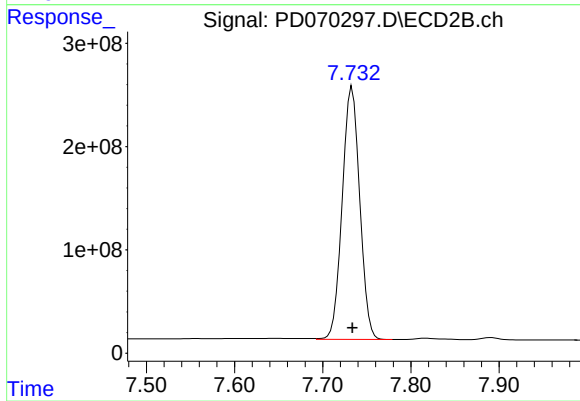

#20 Methoxychlor


R.T.: 7.733 min
Delta R.T.: 0.000 min
Response: 3372244254
Conc: 734.78 ng/ml

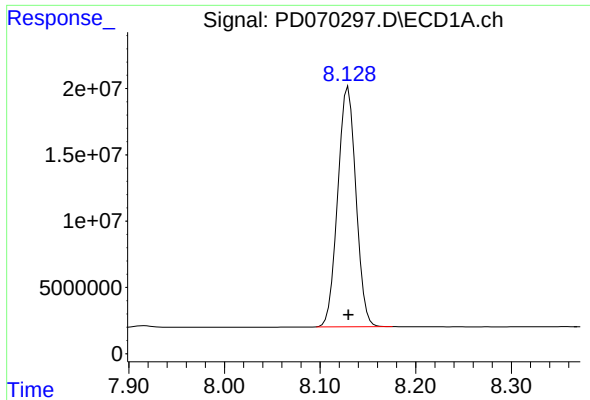

#27 Decachlorobiphenyl

R.T.: 8.129 min
Delta R.T.: 0.000 min
Response: 239753840
Conc: 155.56 ng/ml

Instrument :
ECD_D
ClientSampleId :

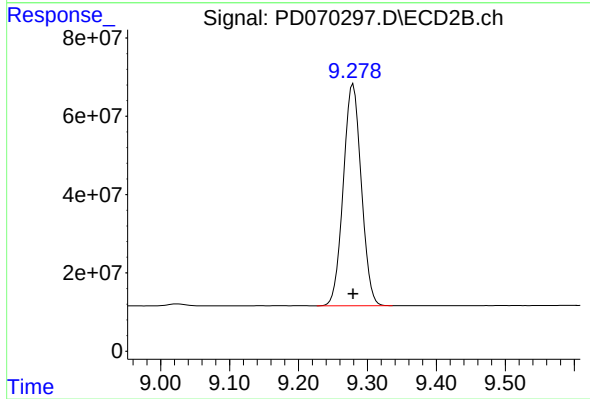

#27 Decachlorobiphenyl

R.T.: 9.279 min
Delta R.T.: 0.000 min
Response: 1028098632
Conc: 145.97 ng/ml