

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061422\
 Data File : PD070298.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2022 14:41
 Operator : AR\AJ
 Sample : INDB501
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 15:50:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 14 15:48:54 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.400	4.122	112.7E6	964.1E6	80.667	72.030
27)	SA Decachlor...	8.130	9.279	231.2E6	989.6E6	149.485	138.362
Target Compounds							
5)	MB Aldrin	4.655	5.638	158.7E6	1211.1E6	84.037	72.187
6)	B beta-BHC	4.366	4.968	64907645	561.5E6	72.311	69.948
7)	B delta-BHC	4.567	5.192	172.3E6	1083.5E6	86.401	80.823
8)	B Heptachlo...	5.096	6.025	140.6E6	913.7E6	81.078	75.037
10)	B trans-Chl...	5.320	6.261	146.3E6	1046.1E6	82.508	71.630
11)	B cis-Chlor...	5.379	6.335	141.5E6	1002.9E6	80.921	70.600
12)	B 4,4'-DDE	5.545	6.487	286.0E6	1908.0E6	170.378	146.322
15)	B Endosulfa...	6.205	7.069	262.0E6	1574.9E6	161.884	142.425
18)	B Endrin al...	6.375	7.193	193.8E6	1161.6E6	155.690	138.130
19)	B Endosulfa...	6.586	7.418	253.2E6	1424.7E6	160.154	142.244
21)	B Endrin ke...	7.077	7.891	290.7E6	1473.6E6	161.781	142.753


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061422\
Data File : PD070298.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2022 14:41
Operator : AR\AJ
Sample : INDB501
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 15:50:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 14 15:48:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

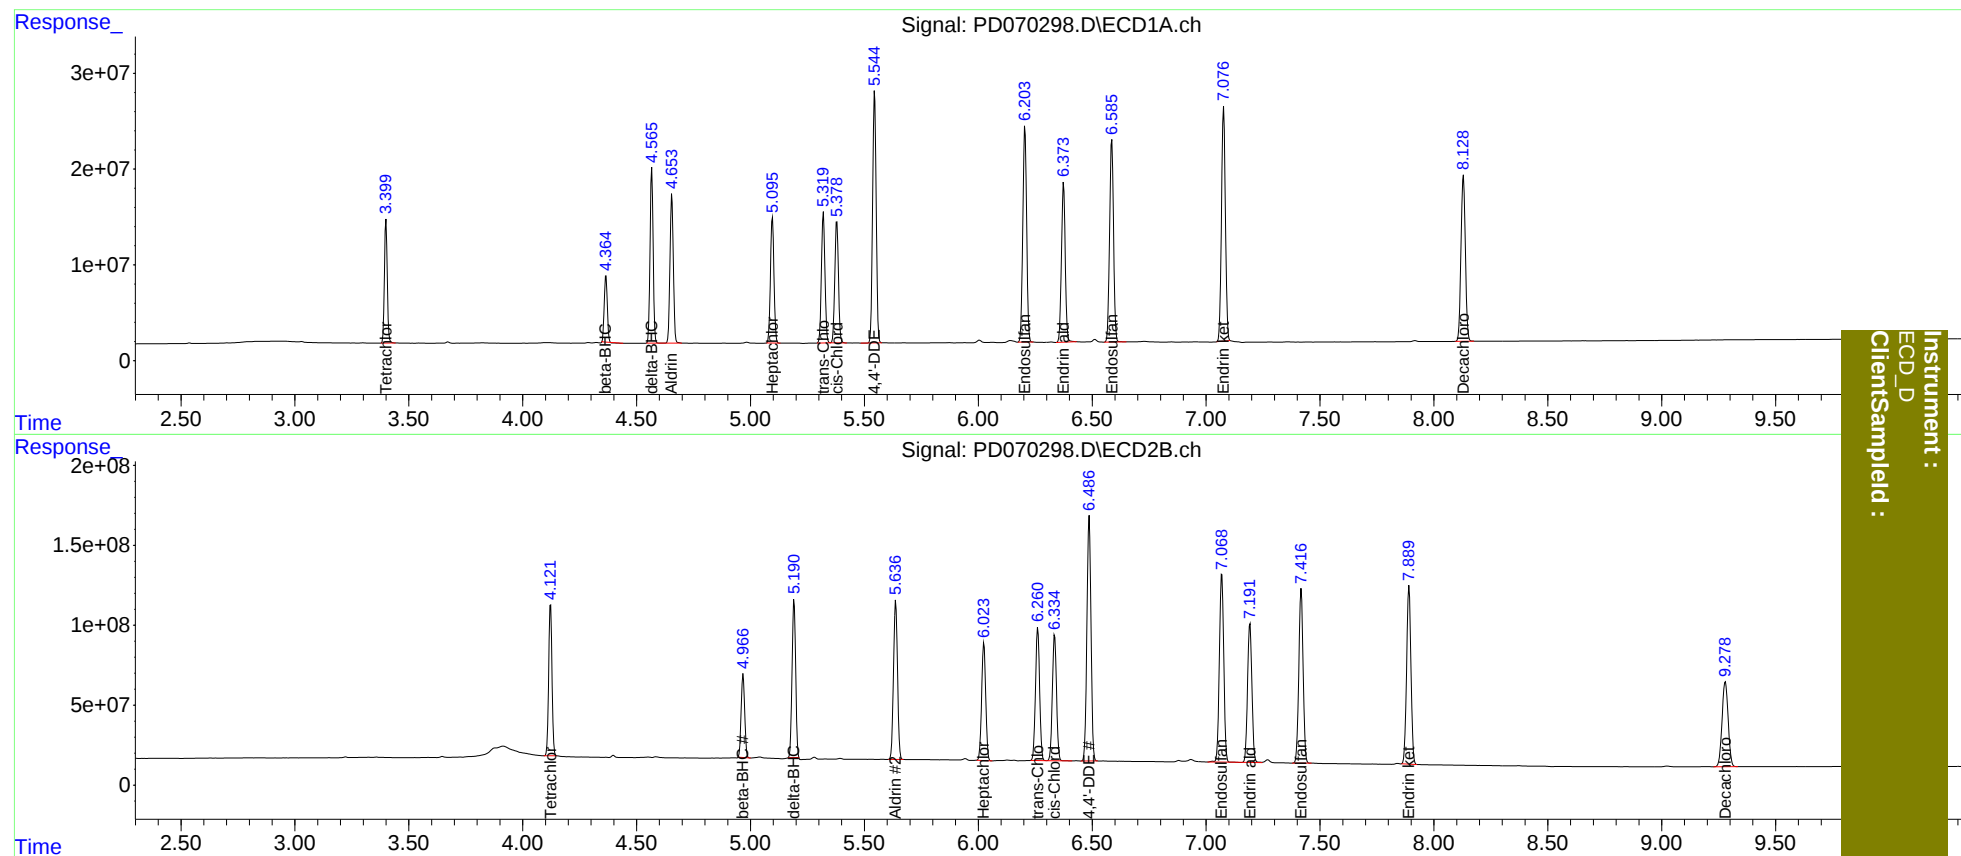


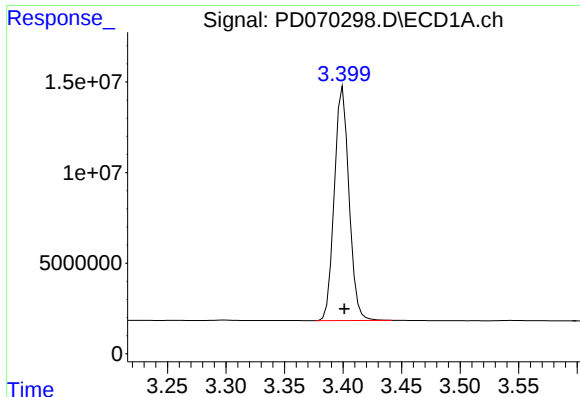

#1 Tetrachloro-m-xylene


R.T.: 3.400 min
Delta R.T.: 0.000 min
Response: 112663322
Conc: 80.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

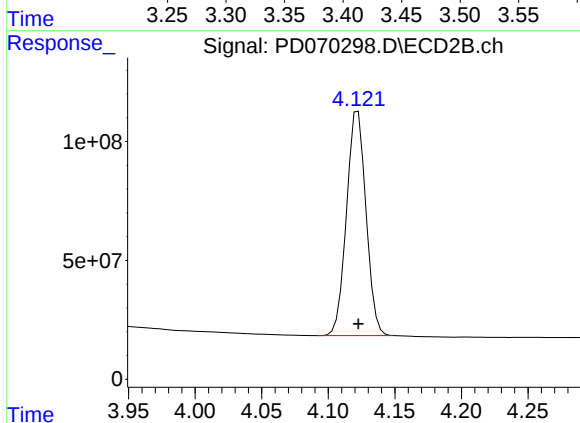


#1 Tetrachloro-m-xylene

R.T.: 4.122 min
Delta R.T.: 0.000 min
Response: 964050165
Conc: 72.03 ng/ml

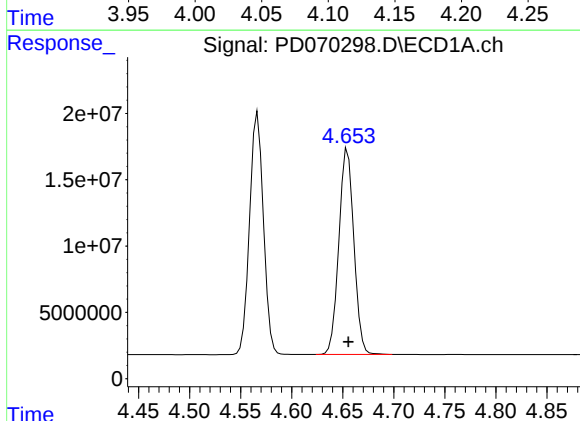


#5 Aldrin

R.T.: 4.655 min
Delta R.T.: 0.000 min
Response: 158705087
Conc: 84.04 ng/ml

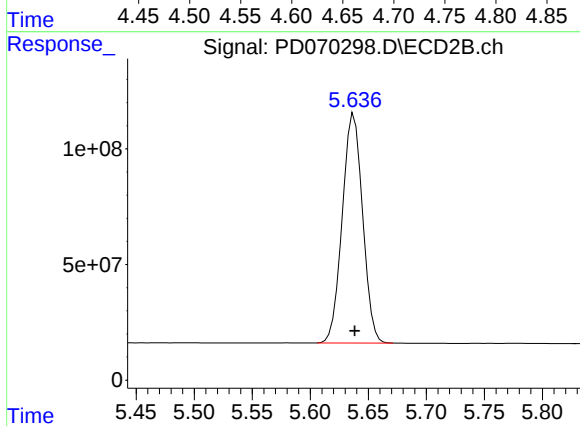

#5 Aldrin


R.T.: 5.638 min
Delta R.T.: 0.000 min
Response: 1211114302
Conc: 72.19 ng/ml

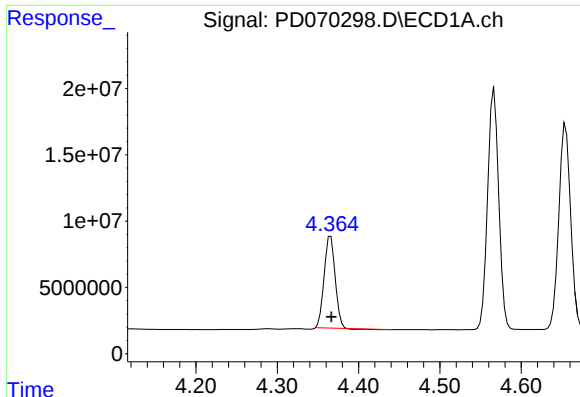

#6 beta-BHC


R.T.: 4.366 min
Delta R.T.: 0.000 min
Response: 64907645
Conc: 72.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

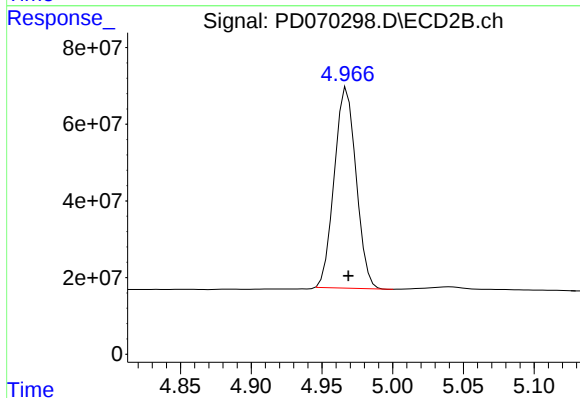


#6 beta-BHC

R.T.: 4.968 min
Delta R.T.: 0.000 min
Response: 561512493
Conc: 69.95 ng/ml

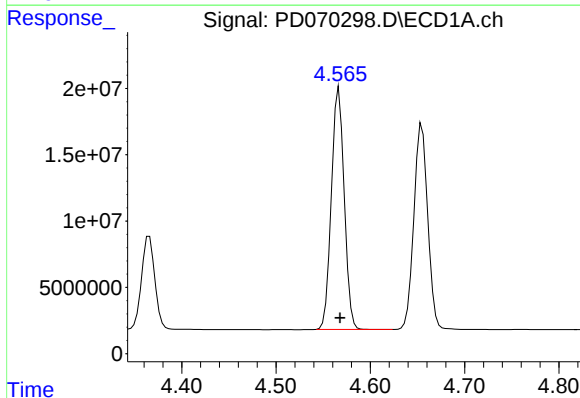


#7 delta-BHC

R.T.: 4.567 min
Delta R.T.: 0.000 min
Response: 172307093
Conc: 86.40 ng/ml

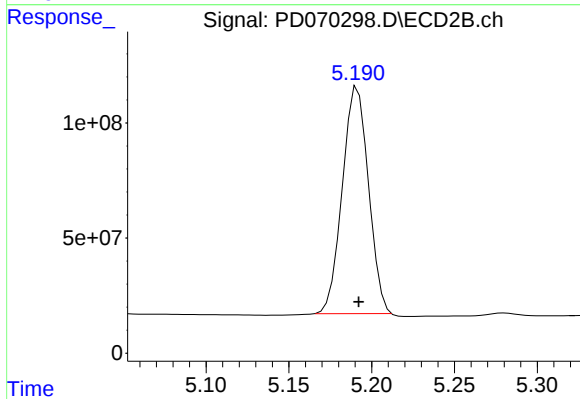

#7 delta-BHC


R.T.: 5.192 min
Delta R.T.: 0.000 min
Response: 1083470306
Conc: 80.82 ng/ml

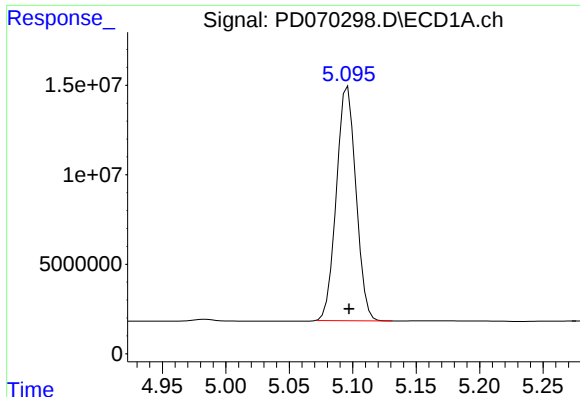

#8 Heptachlor epoxide


R.T.: 5.096 min
Delta R.T.: -0.001 min
Response: 140550887
Conc: 81.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

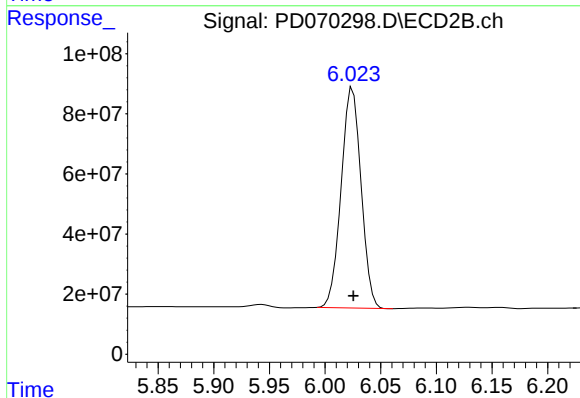


#8 Heptachlor epoxide

R.T.: 6.025 min
Delta R.T.: 0.000 min
Response: 913660899
Conc: 75.04 ng/ml

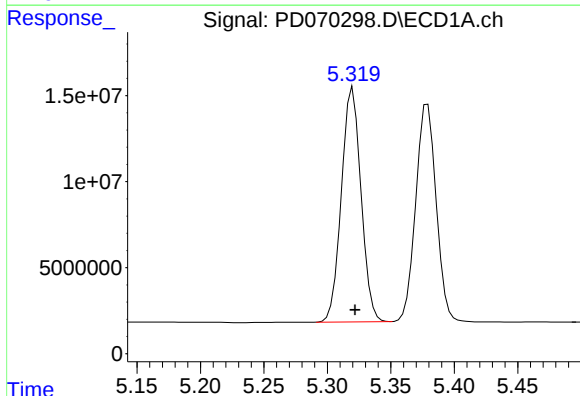


#10 trans-Chlordane

R.T.: 5.320 min
Delta R.T.: -0.002 min
Response: 146311003
Conc: 82.51 ng/ml

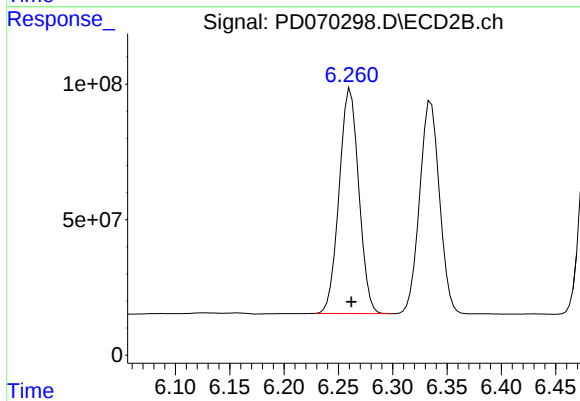

#10 trans-Chlordane


R.T.: 6.261 min
Delta R.T.: 0.000 min
Response: 1046100847
Conc: 71.63 ng/ml

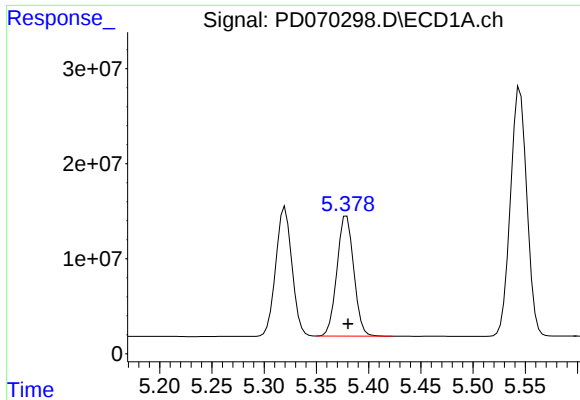

#11 cis-Chlordane


R.T.: 5.379 min
Delta R.T.: -0.001 min
Response: 141516869
Conc: 80.92 ng/ml

Instrument :
ECD_D
ClientSampleId :

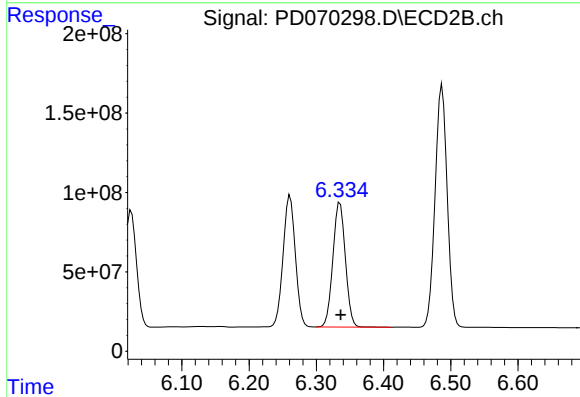


#11 cis-Chlordane

R.T.: 6.335 min
Delta R.T.: -0.001 min
Response: 1002910959
Conc: 70.60 ng/ml

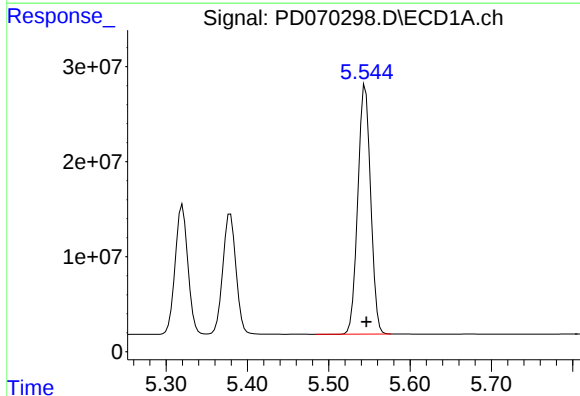


#12 4,4'-DDE

R.T.: 5.545 min
Delta R.T.: -0.001 min
Response: 286000908
Conc: 170.38 ng/ml

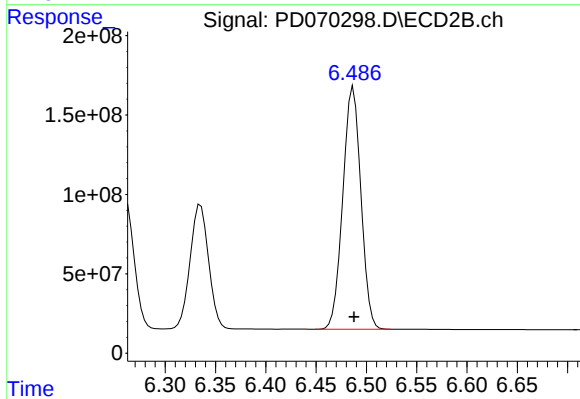

#12 4,4'-DDE


R.T.: 6.487 min
Delta R.T.: 0.000 min
Response: 1907979577
Conc: 146.32 ng/ml

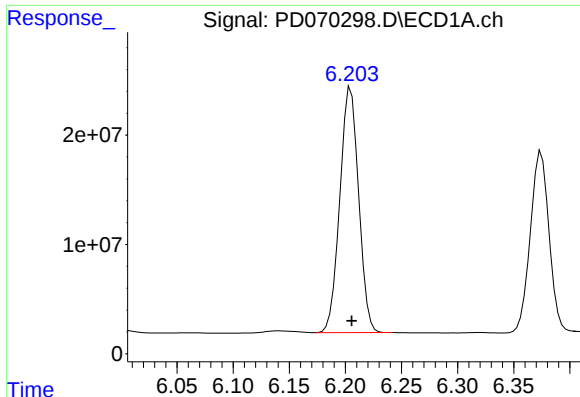

#15 Endosulfan II


R.T.: 6.205 min
Delta R.T.: 0.000 min
Response: 261963990
Conc: 161.88 ng/ml

Instrument :
ECD_D
ClientSampleId :

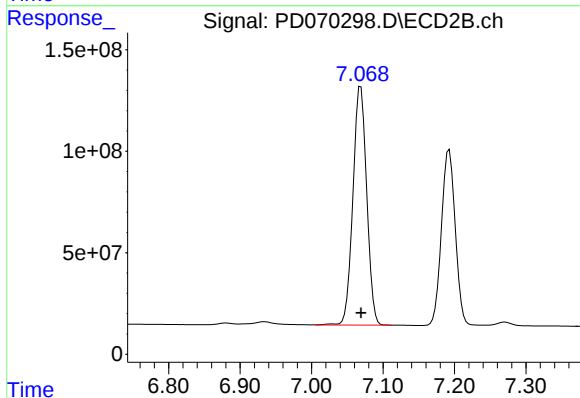


#15 Endosulfan II

R.T.: 7.069 min
Delta R.T.: 0.000 min
Response: 1574923207
Conc: 142.43 ng/ml

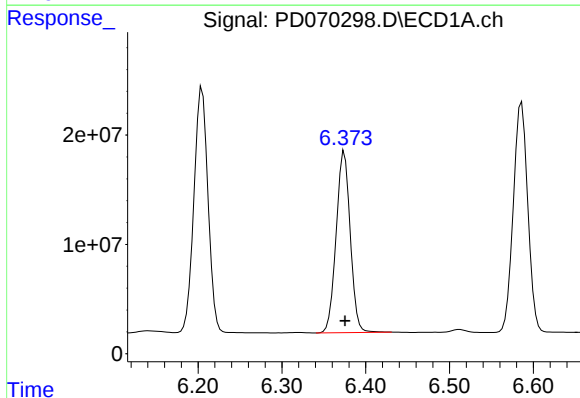


#18 Endrin aldehyde

R.T.: 6.375 min
Delta R.T.: 0.000 min
Response: 193758642
Conc: 155.69 ng/ml

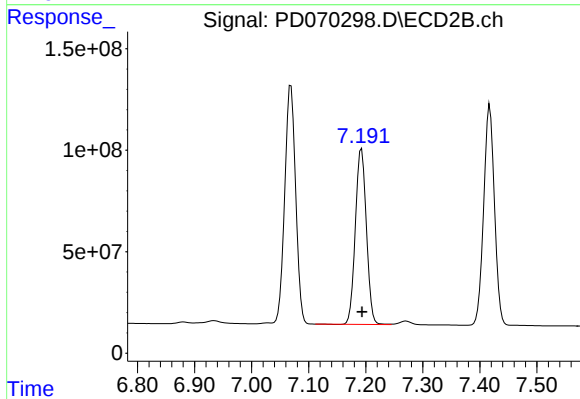

#18 Endrin aldehyde


R.T.: 7.193 min
Delta R.T.: 0.000 min
Response: 1161616872
Conc: 138.13 ng/ml

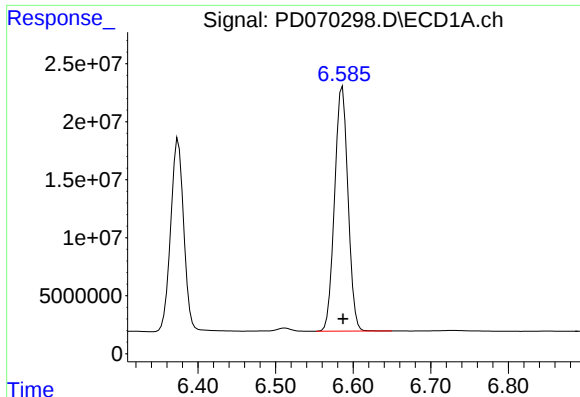

#19 Endosulfan Sulfate


R.T.: 6.586 min
Delta R.T.: 0.000 min
Response: 253186700
Conc: 160.15 ng/ml

Instrument :
ECD_D
ClientSampleId :

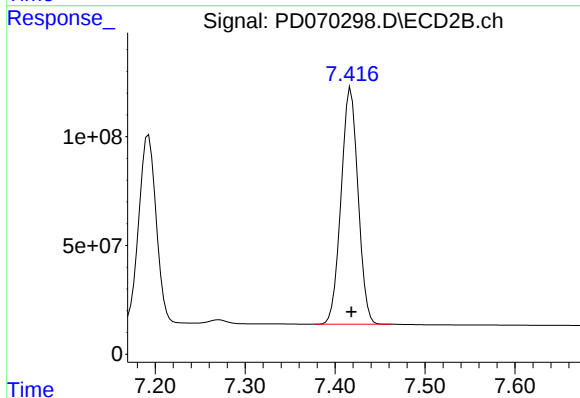


#19 Endosulfan Sulfate

R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 1424749655
Conc: 142.24 ng/ml

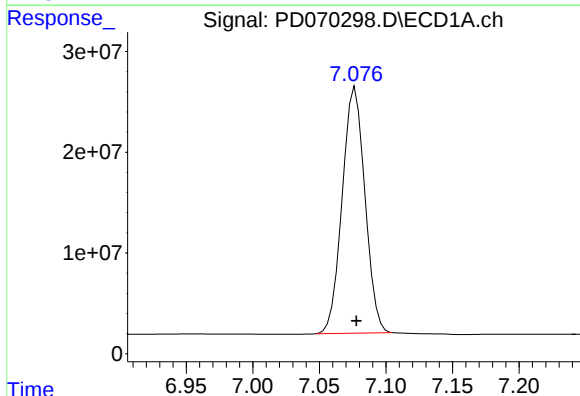


#21 Endrin ketone

R.T.: 7.077 min
Delta R.T.: 0.000 min
Response: 290717543
Conc: 161.78 ng/ml

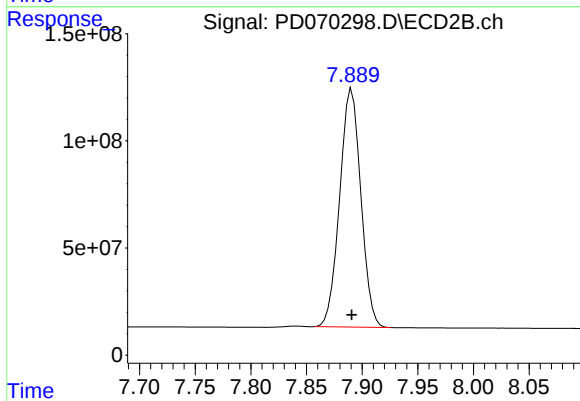

#21 Endrin ketone


R.T.: 7.891 min
Delta R.T.: 0.000 min
Response: 1473628840
Conc: 142.75 ng/ml

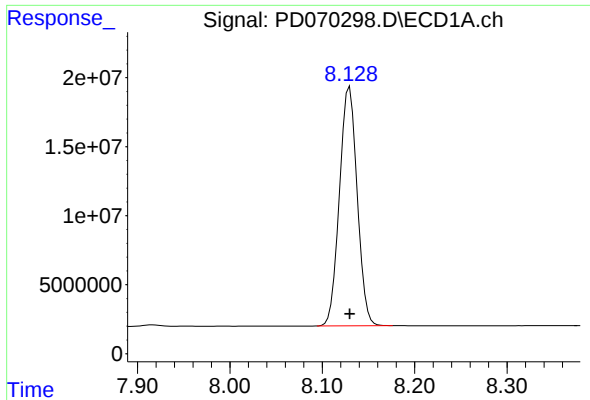

#27 Decachlorobiphenyl

R.T.: 8.130 min
Delta R.T.: 0.000 min
Response: 231177556
Conc: 149.49 ng/ml

Instrument :
ECD_D
ClientSampleId :

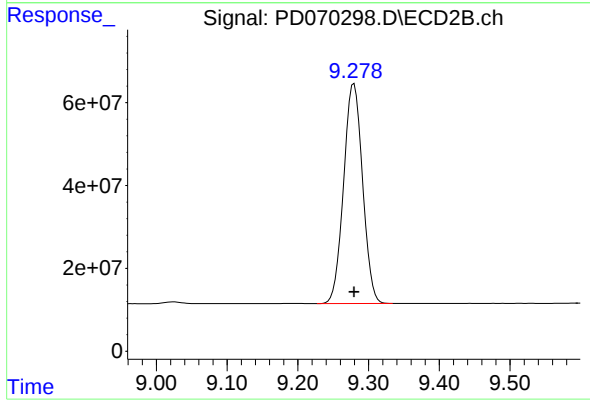

#27 Decachlorobiphenyl

R.T.: 9.279 min
Delta R.T.: 0.000 min
Response: 989567286
Conc: 138.36 ng/ml