

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061422\
 Data File : PD070310.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2022 18:38
 Operator : AR\AJ
 Sample : N3226-24MS
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW4P1MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/15/2022
 Supervised By : Ankita Jodhani 06/15/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 23:25:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 14 16:58:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.401	4.122	19710081	238.8E6	13.590	17.676 #
27)	SA Decachlor...	8.130	9.282	44625165	214.0E6	27.861	29.654
Target Compounds							
2)	A alpha-BHC	3.836	4.516	75293040	630.7E6	35.629	32.215
3)	MA gamma-BHC...	4.117	4.805	76887114	656.0E6	38.289	35.975
4)	MA Heptachlor	4.411	5.328	83156727	693.0E6	42.253	38.680
5)	MB Aldrin	4.655	5.639	81764570	661.1E6	42.865	39.773
6)	B beta-BHC	4.366	4.967	36265110	324.6E6	40.517	41.034m
7)	B delta-BHC	4.567	5.191	8754165	21891281	4.338	1.697m#
8)	B Heptachlo...	5.096	6.026	75613629	470.4E6	43.166	40.315
9)	A Endosulfan I	5.432	6.387	69763347	531.8E6	41.475	39.433
10)	B trans-Chl...	5.321	6.263	78544761	567.9E6	43.669	39.293
11)	B cis-Chlor...	5.380	6.337	73783063	560.2E6	41.715	39.894
12)	B 4,4'-DDE	5.545	6.488	156.6E6	1101.1E6	92.780	84.685
13)	MA Dieldrin	5.675	6.645	163.3E6	1104.7E6	86.069	80.660
14)	MA Endrin	5.932	6.864	150.1E6	933.8E6	88.187	81.161
15)	B Endosulfa...	6.205	7.070	138.7E6	879.5E6	85.468	79.966
16)	A 4,4'-DDD	6.061	6.978	128.6E6	859.3E6	84.925	77.830
17)	MA 4,4'-DDT	6.300	7.280	128.9E6	846.5E6	88.611	82.330
18)	B Endrin al...	6.375	7.194	113.2E6	707.9E6	90.957	84.161
19)	B Endosulfa...	6.587	7.419	95538479	585.1E6	60.316	59.191
20)	A Methoxychlor	6.849	7.735	363.8E6	1936.3E6	429.829	410.133
21)	B Endrin ke...	7.077	7.892	160.6E6	852.9E6	90.030	83.717

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061422\
Data File : PD070310.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2022 18:38
Operator : AR\AJ
Sample : N3226-24MS
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 23:25:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 14 16:58:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

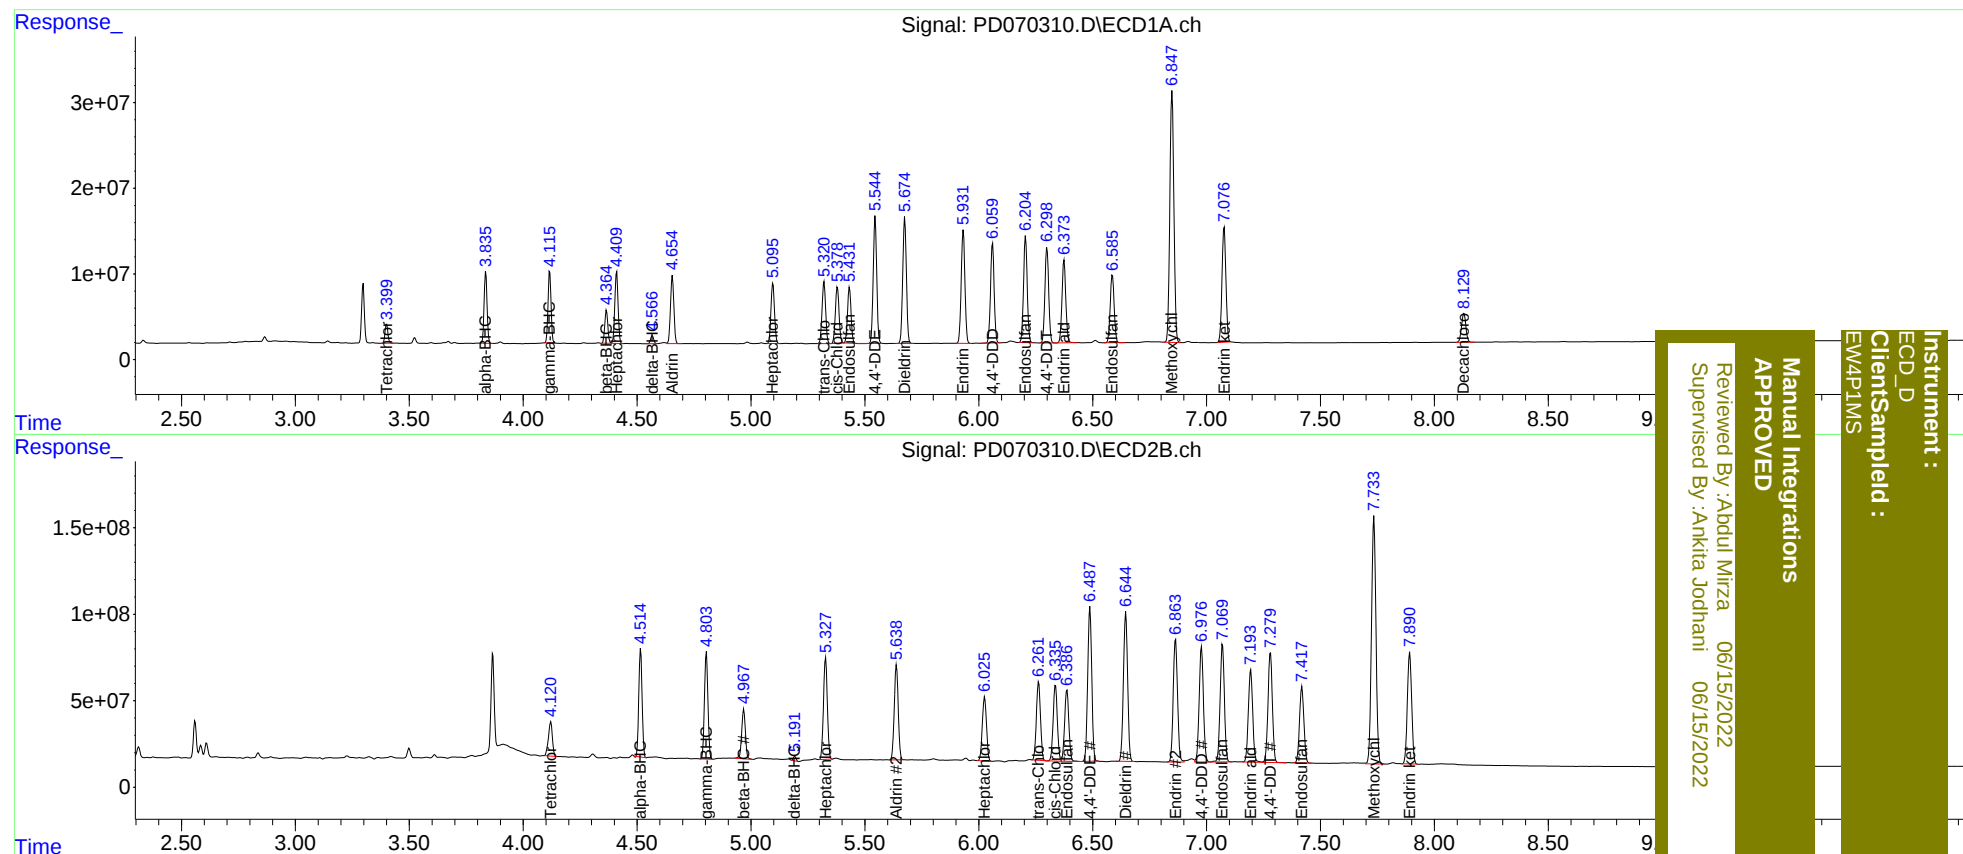

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 06/15/2022
Supervised By: Ankita Jodhani 06/15/2022

Instrument :
ECD_D
ClientSampled :
EW4P1MS