

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061521\
 Data File : PD063845.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2021 07:18
 Operator : AR\AJ
 Sample : M2618-06MSD
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BG5R7MSD

Manual Integrations
 APPROVED

Ankita
 6/18/2021 9:02:55 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 15 07:39:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 15 03:10:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	3.969	17229369	1573.7E6	11.083m	99.365m#
2)	SA Decachlor...	8.193	9.026	78905833	493.3E6	45.585	35.569m
Target Compounds							
2)	A alpha-BHC	3.874	4.358	86944590	1136.0E6	37.171	45.723
3)	MA gamma-BHC...	4.158	4.641	107.7E6	894.9E6	47.343	39.219m
4)	MA Heptachlor	4.458	5.150	85681168	657.7E6	39.245	28.233 #
5)	MB Aldrin	4.705	5.454	75058594	673.4E6	37.033	30.569
6)	B beta-BHC	4.409	4.815	35263017	298.9E6	36.316	30.647m
7)	B delta-BHC	4.612	5.029	81066367	752.5E6	37.556	32.116m
8)	B Heptachlo...	5.148	5.841	66635494	548.4E6	35.140	26.656
9)	A Endosulfan I	5.488	6.196	55937183	517.4E6	30.569m	26.116m
10)	B trans-Chl...	5.376	6.064	96802731	1522.4E6	49.779	72.373m#
11)	B cis-Chlor...	5.434	6.148	83883910	702.2E6	44.150	34.863
12)	B 4,4'-DDE	5.598	6.303	151.0E6	1146.0E6	76.490	56.721 #
13)	MA Dieldrin	5.730	6.453	201.9E6	1322.7E6	96.452m	63.226m#
14)	MA Endrin	5.989	6.670	145.1E6	808.1E6	80.236	46.187m#
15)	B Endosulfa...	6.263	6.880	118.4E6	921.6E6	72.471	56.954m
16)	A 4,4'-DDD	6.116	6.794	106.5E6	1006.7E6	64.517	59.802
17)	MA 4,4'-DDT	6.356	7.094	347.8E6	2683.0E6	206.679	162.977
18)	B Endrin al...	6.432	7.003	73347787	668.3E6	51.375	47.504m
19)	B Endosulfa...	6.645	7.227	108.1E6	820.0E6	69.613	49.821m#
20)	A Methoxychlor	6.901	7.552	294.0E6	1852.9E6	318.920m	239.491
21)	B Endrin ke...	7.136	7.697	95129653	779.0E6	50.145m	49.089m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061521\
Data File : PD063845.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2021 07:18
Operator : AR\AJ
Sample : M2618-06MSD
Misc :
ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 15 07:39:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 15 03:10:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

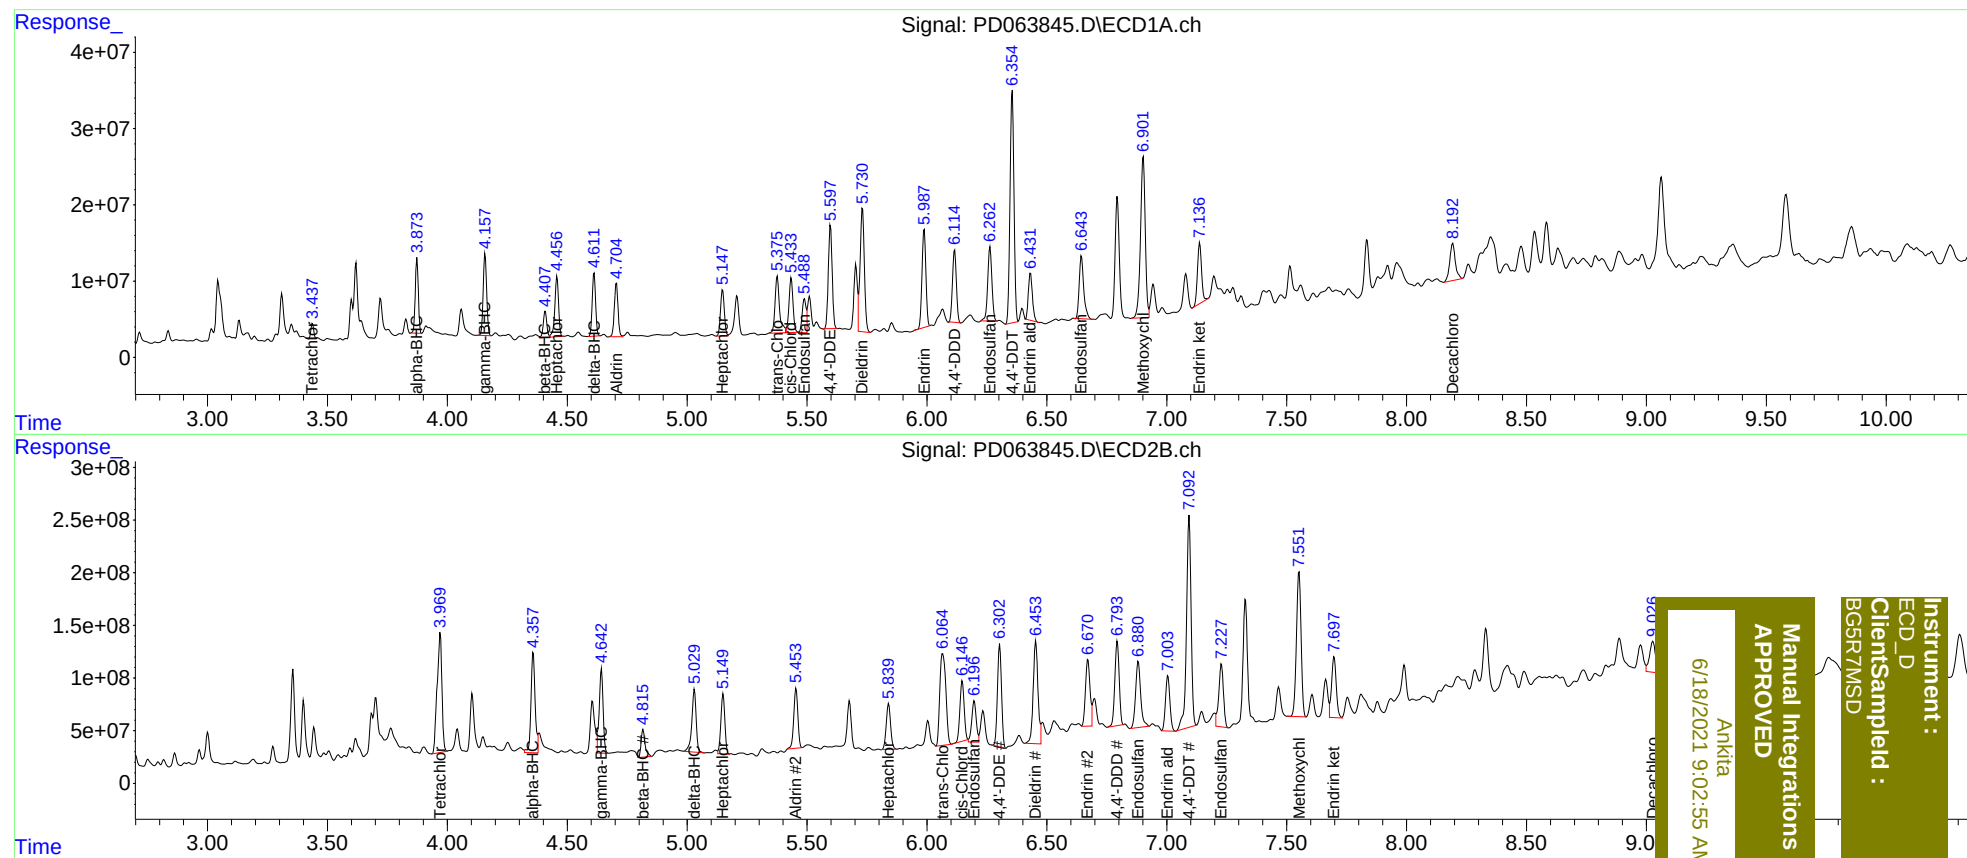

6/18/2021 9:02:55 AM

Manual Integrations
APPROVED

Ankita

Instrument :
ECD_D
Client Sampled :
BG5RTMSD