

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061521\
Data File : PD063853.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2021 12:24
Operator : AR\AJ
Sample : INDA351
Misc :
ALS Vial : 28 Sample Multiplier: 1


Instrument :
ECD_D
LabSampleId :
INDA351

Manual Integrations
APPROVED

Ankita
6/21/2021 11:47:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 04:29:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 15 03:10:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

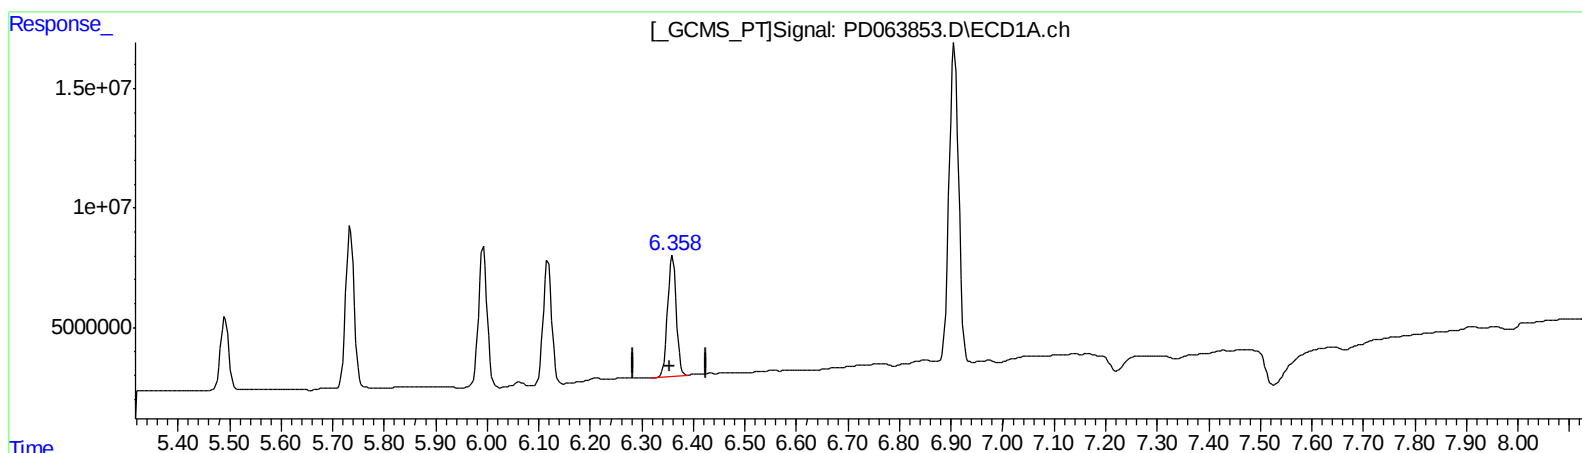

(17) 4,4'-DDT (MA)

6.360min 35.114 ng/ml

response 59097776

(17) 4,4'-DDT #2 (MA)

7.094min 35.992 ng/ml

response 592513216

(+) = Expected Retention Time

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061521\
Data File : PD063853.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2021 12:24
Operator : AR\AJ
Sample : INDA351
Misc :
ALS Vial : 28 Sample Multiplier: 1


Instrument :
ECD_D
LabSampleId :
INDA351

Manual Integrations
APPROVED

Ankita
6/21/2021 11:47:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 04:29:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 15 03:10:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

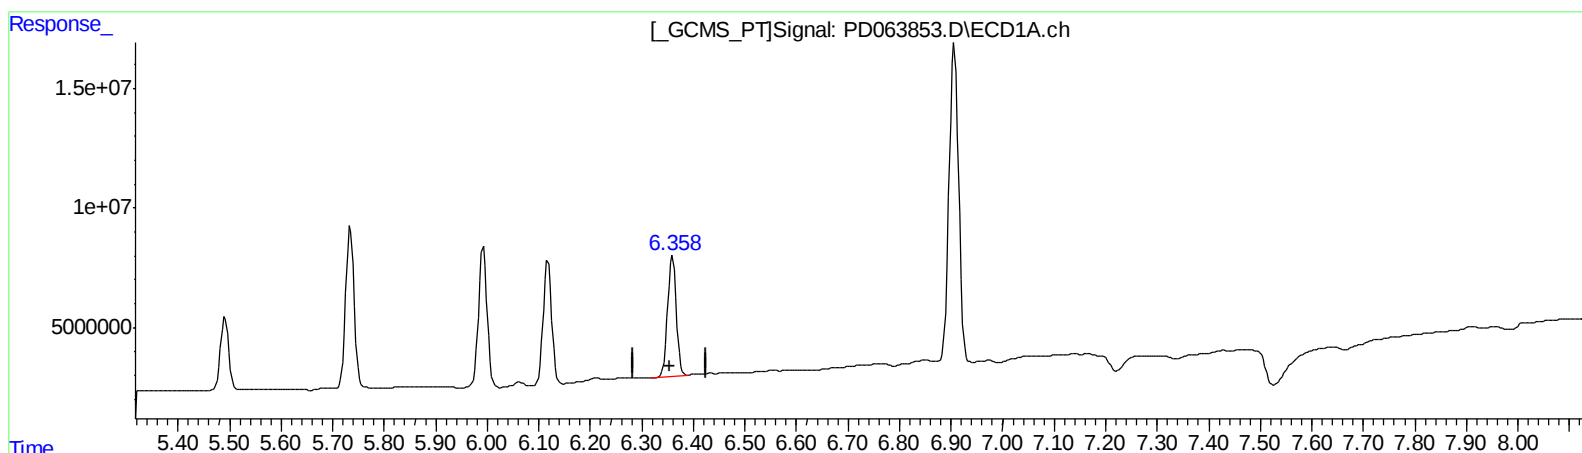

(17) 4,4'-DDT (MA)

6.360min 35.114 ng/ml

response 59097776

(17) 4,4'-DDT #2 (MA)

7.093min 33.725 ng/ml m

response 555187244

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061521\
 Data File : PD063853.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2021 12:24
 Operator : AR\AJ
 Sample : INDA351
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_D
 LabSampleId :
 INDA351

Manual Integrations
 APPROVED

Ankita
 6/21/2021 11:47:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 04:29:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 15 03:10:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.441	3.971	30101378	300.9E6	19.364	18.996
27) SA Decachlor...	8.198	9.027	56350548	514.9E6	32.554	37.130
Target Compounds						
2) A alpha-BHC	3.877	4.359	46177277	512.1E6	19.742	20.610
3) MA gamma-BHC...	4.161	4.643	45471453	443.1E6	19.980	19.418
4) MA Heptachlor	4.461	5.151	42116662	445.9E6	19.291	19.142
9) A Endosulfan I	5.492	6.198	34427633	341.6E6	18.814	17.243
13) MA Dieldrin	5.735	6.455	78009161	709.5E6	37.276	33.916
14) MA Endrin	5.993	6.673	69764770	586.7E6	38.576	33.531
16) A 4,4'-DDD	6.118	6.795	59980162	594.5E6	36.329	35.317
17) MA 4,4'-DDT	6.360	7.093	59097776	555.2E6	35.114	33.725m
20) A Methoxychlor	6.907	7.552	167.2E6	1338.1E6	181.403	172.954

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

AJ
 06/21/21