

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061523\
 Data File : PD075799.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2023 16:49
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 01:26:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 01:24:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.766	217.0E6	125.1E6	103.083	103.744
28)	SA Decachlor...	9.090	7.914	233.9E6	91658751	96.610	97.946
Target Compounds							
23)	Chlordane-1	4.711	3.766	114.1E6	45192781	1022.754	1018.748
24)	Chlordane-2	5.243	4.343	121.7E6	48945722	981.470	975.299
25)	Chlordane-3	5.956	4.974	538.3E6	150.2E6	1062.013	1042.656
26)	Chlordane-4	6.038	5.037	640.0E6	146.7E6	1042.496	1020.630
27)	Chlordane-5	6.890	5.934	102.2E6	51557109	1033.257	1043.250



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061523\
Data File : PD075799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2023 16:49
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 01:26:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 01:24:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

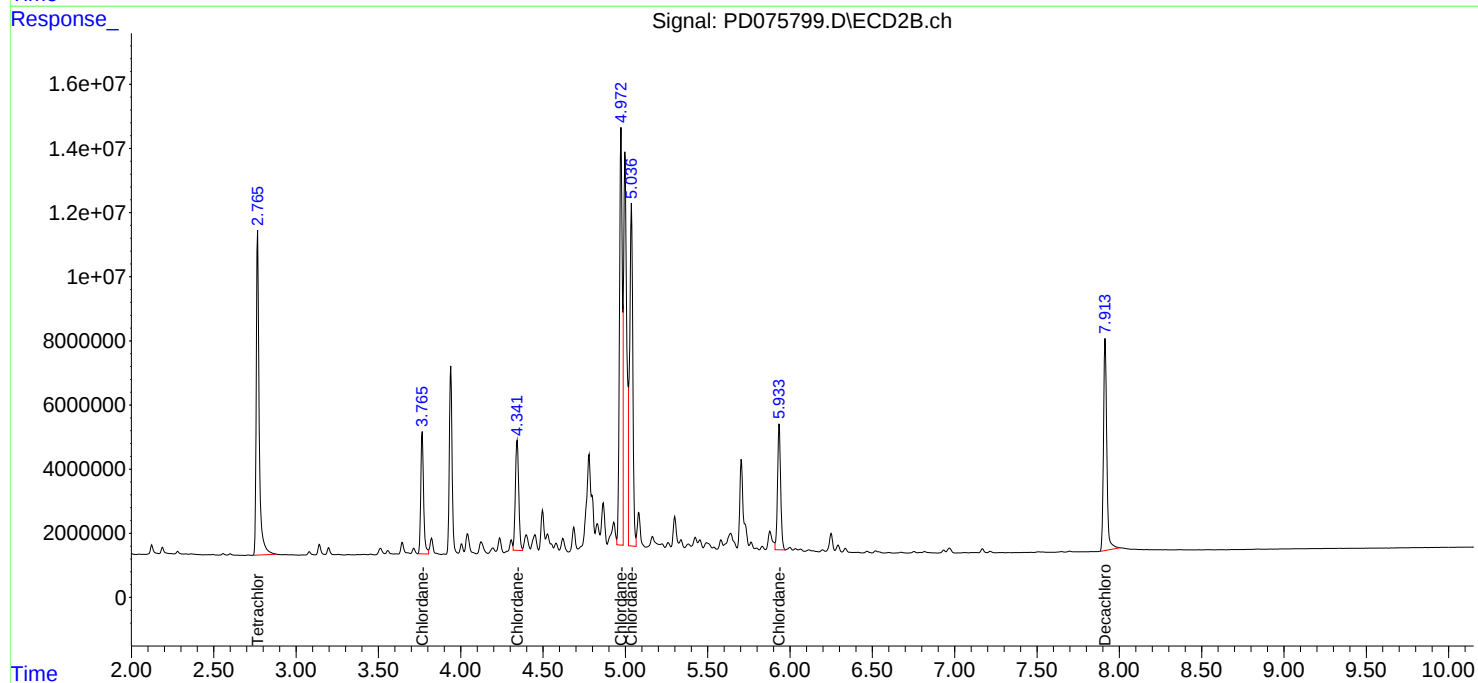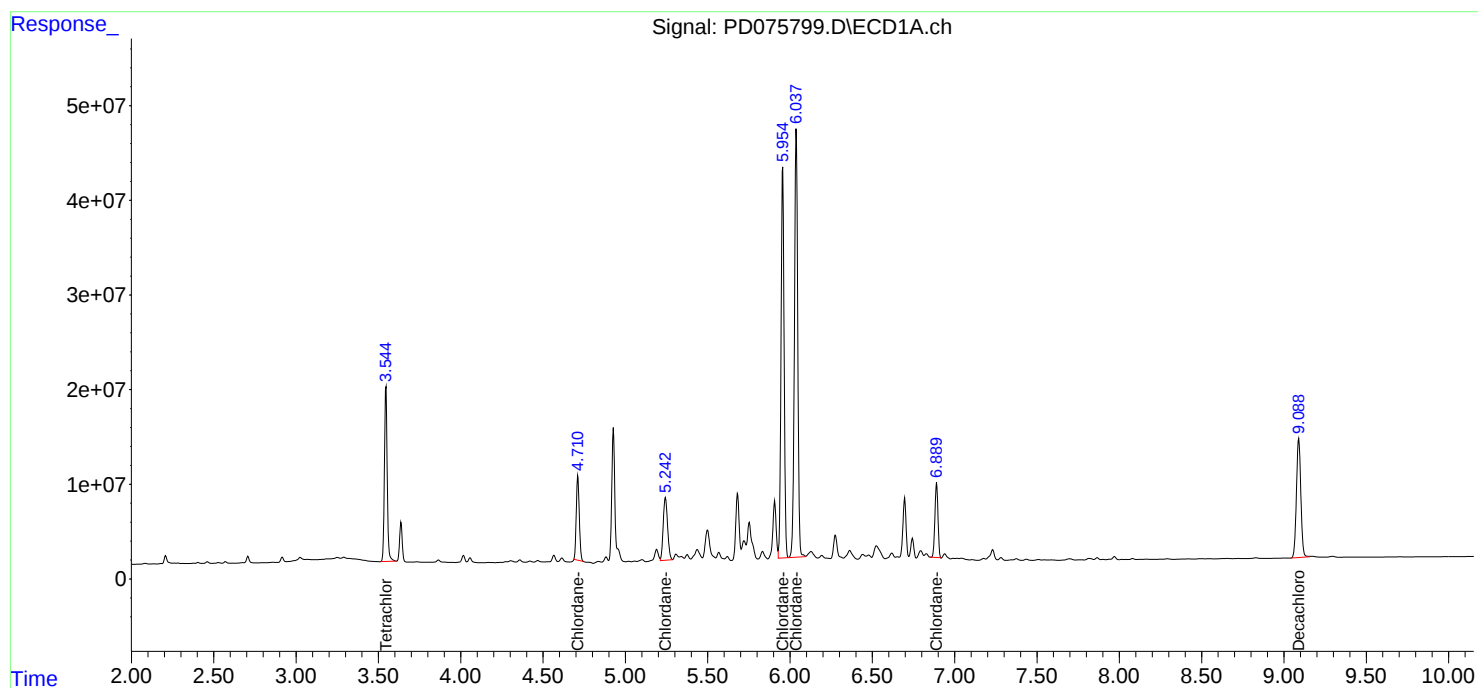


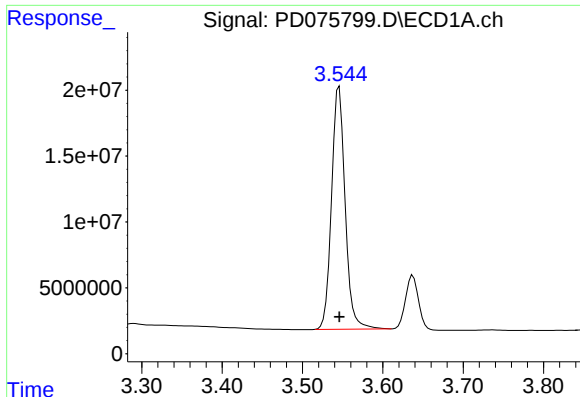

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 217029416
Conc: 103.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

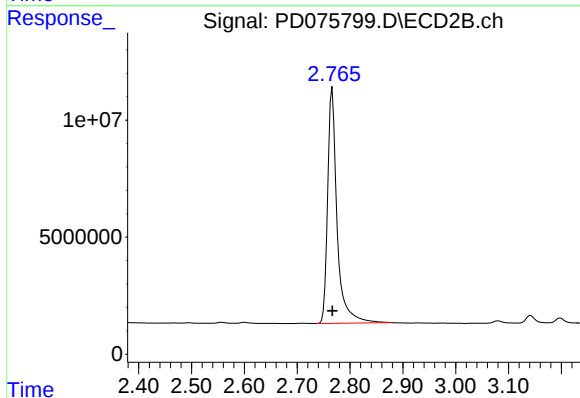


#1 Tetrachloro-m-xylene

R.T.: 2.766 min
Delta R.T.: 0.000 min
Response: 125054958
Conc: 103.74 ng/ml

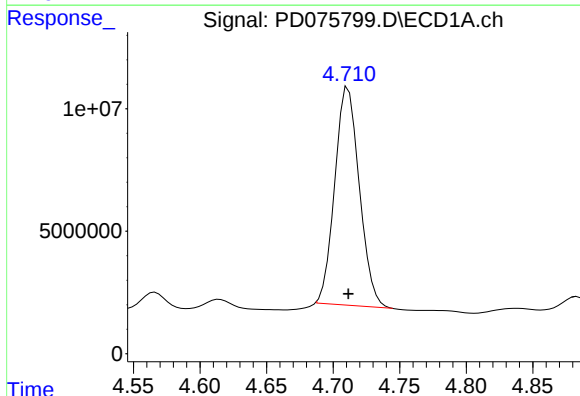


#23 Chlordane-1

R.T.: 4.711 min
Delta R.T.: 0.000 min
Response: 114117340
Conc: 1022.75 ng/ml

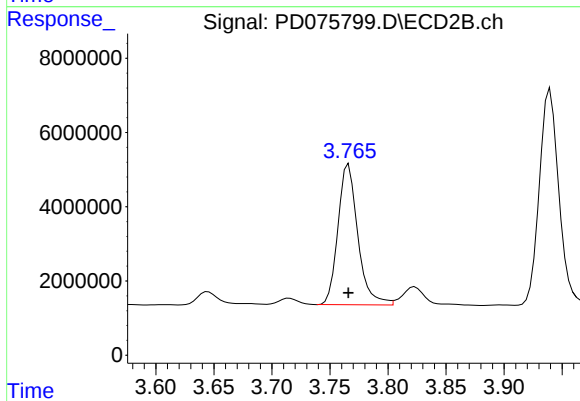

#23 Chlordane-1


R.T.: 3.766 min
Delta R.T.: 0.000 min
Response: 45192781
Conc: 1018.75 ng/ml

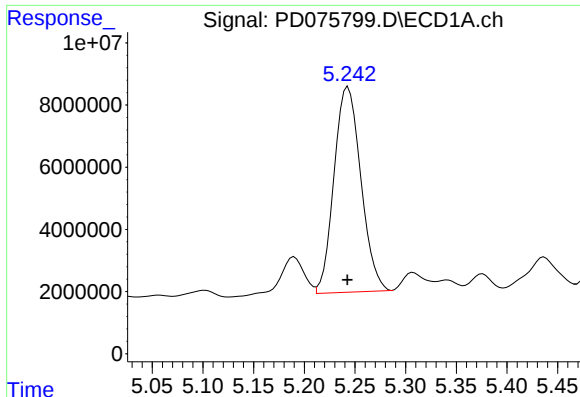

#24 Chlordane-2


R.T.: 5.243 min
Delta R.T.: 0.000 min
Response: 121740253
Conc: 981.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

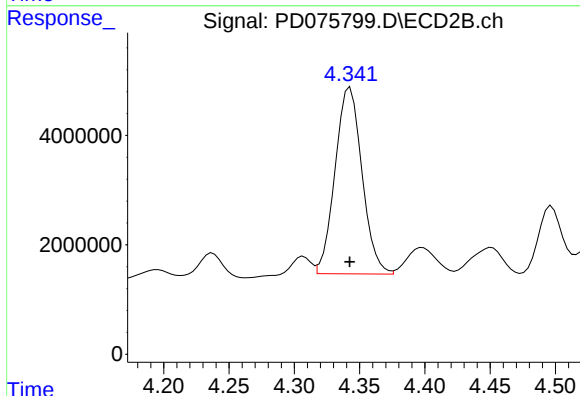


#24 Chlordane-2

R.T.: 4.343 min
Delta R.T.: 0.000 min
Response: 48945722
Conc: 975.30 ng/ml

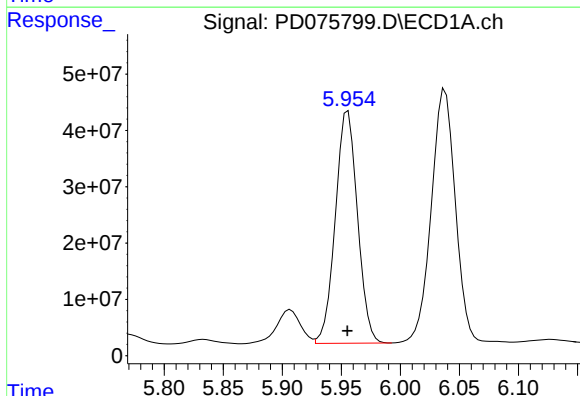


#25 Chlordane-3

R.T.: 5.956 min
Delta R.T.: 0.000 min
Response: 538305343
Conc: 1062.01 ng/ml

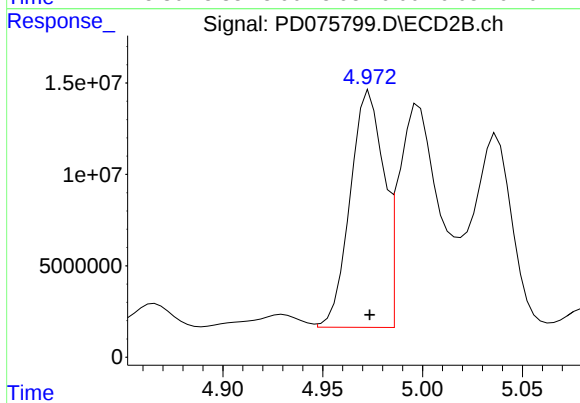

#25 Chlordane-3


R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 150190278
Conc: 1042.66 ng/ml

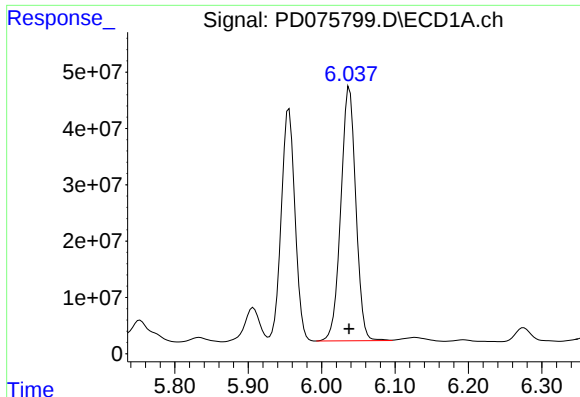

#26 Chlordane-4


R.T.: 6.038 min
Delta R.T.: 0.000 min
Response: 640038999
Conc: 1042.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

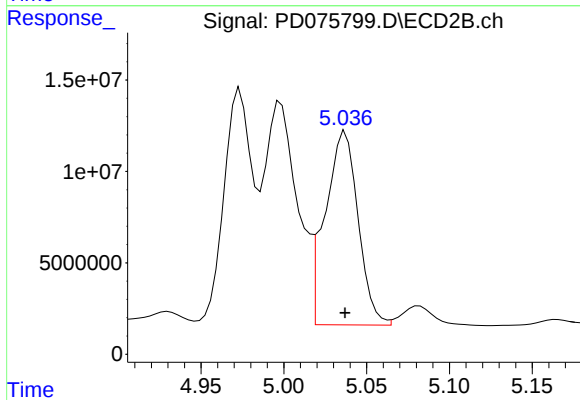


#26 Chlordane-4

R.T.: 5.037 min
Delta R.T.: 0.000 min
Response: 146678425
Conc: 1020.63 ng/ml

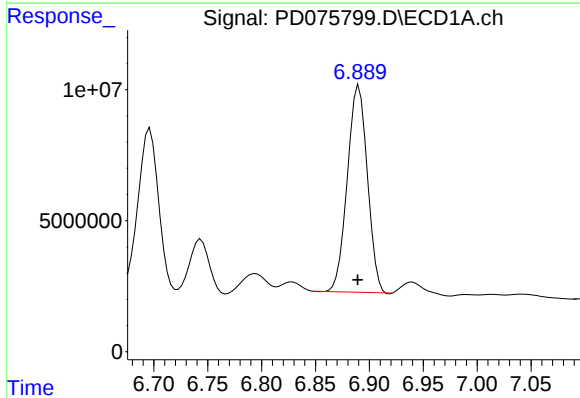


#27 Chlordane-5

R.T.: 6.890 min
Delta R.T.: 0.001 min
Response: 102163414
Conc: 1033.26 ng/ml

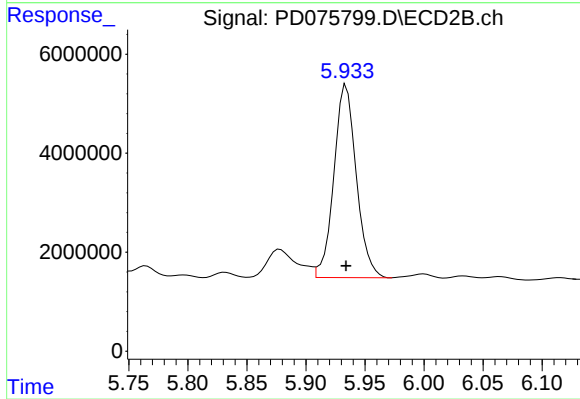

#27 Chlordane-5


R.T.: 5.934 min
Delta R.T.: 0.000 min
Response: 51557109
Conc: 1043.25 ng/ml

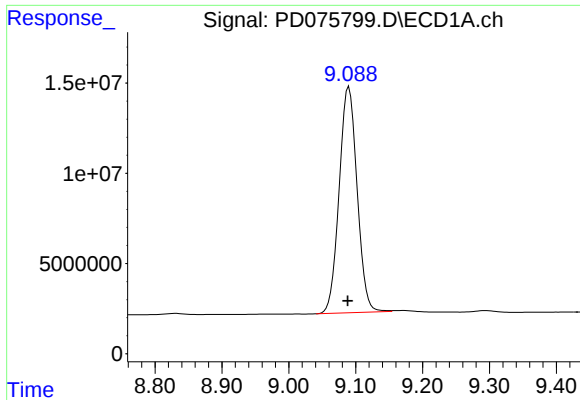

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: 0.002 min
Response: 233931614
Conc: 96.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

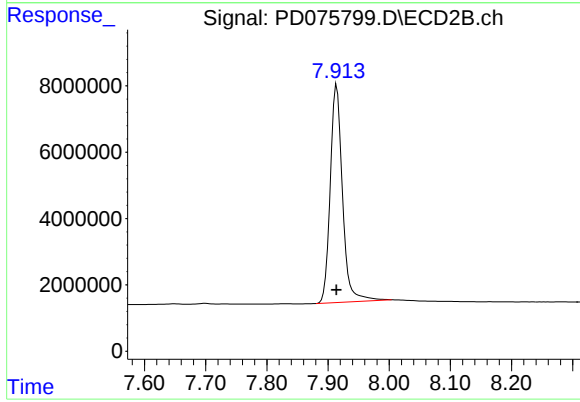

#28 Decachlorobiphenyl

R.T.: 7.914 min
Delta R.T.: 0.000 min
Response: 91658751
Conc: 97.95 ng/ml