

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061523\
 Data File : PD075800.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2023 17:03
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 01:26:33 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 01:24:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.767	159.8E6	91339320	75.882	75.774
28)	SA Decachlor...	9.089	7.914	175.4E6	68049156	72.456	72.717
Target Compounds							
23)	Chlordane-1	4.713	3.767	84232138	33318602	754.913	751.077
24)	Chlordane-2	5.244	4.343	91295147	37129594	736.022	739.849
25)	Chlordane-3	5.956	4.974	390.9E6	109.9E6	771.236	762.852
26)	Chlordane-4	6.038	5.037	467.3E6	106.5E6	761.066	741.386
27)	Chlordane-5	6.890	5.934	74864740	37681238	757.165	762.474



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061523\
Data File : PD075800.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2023 17:03
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 01:26:33 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 01:24:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

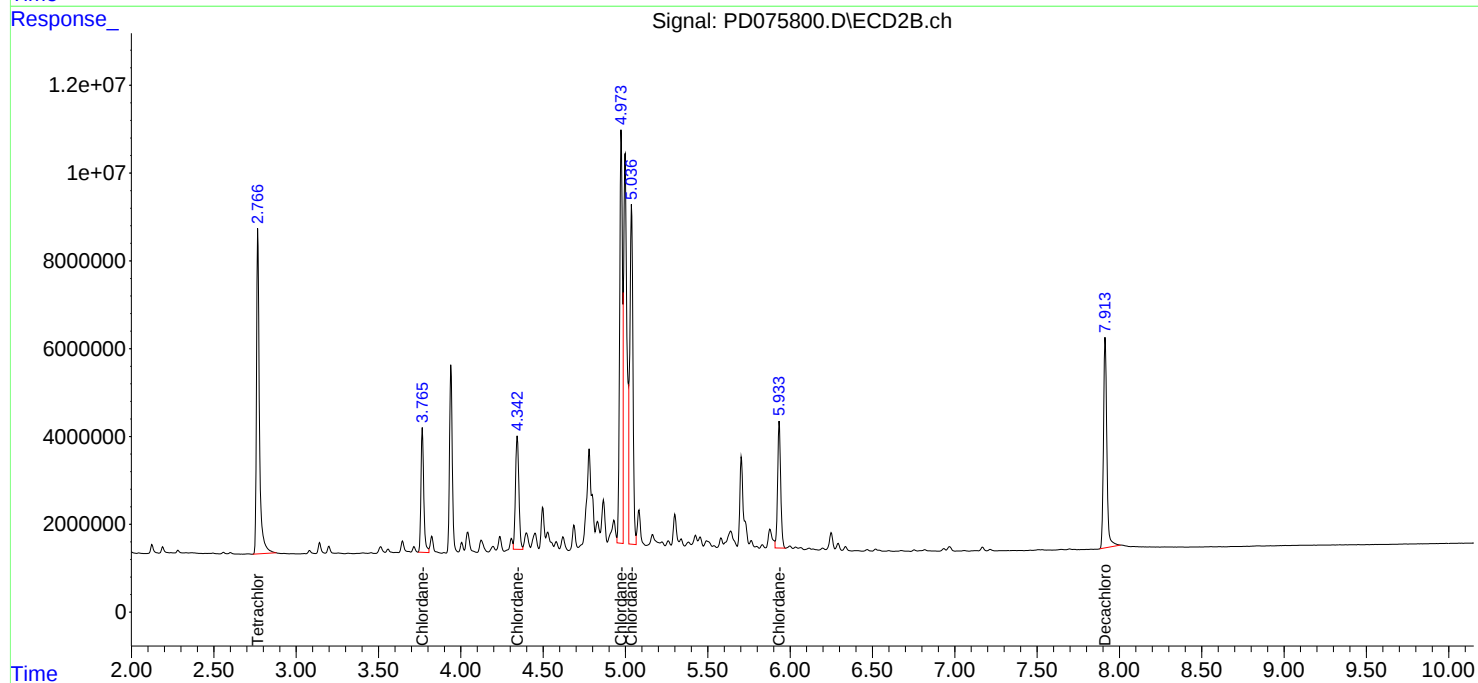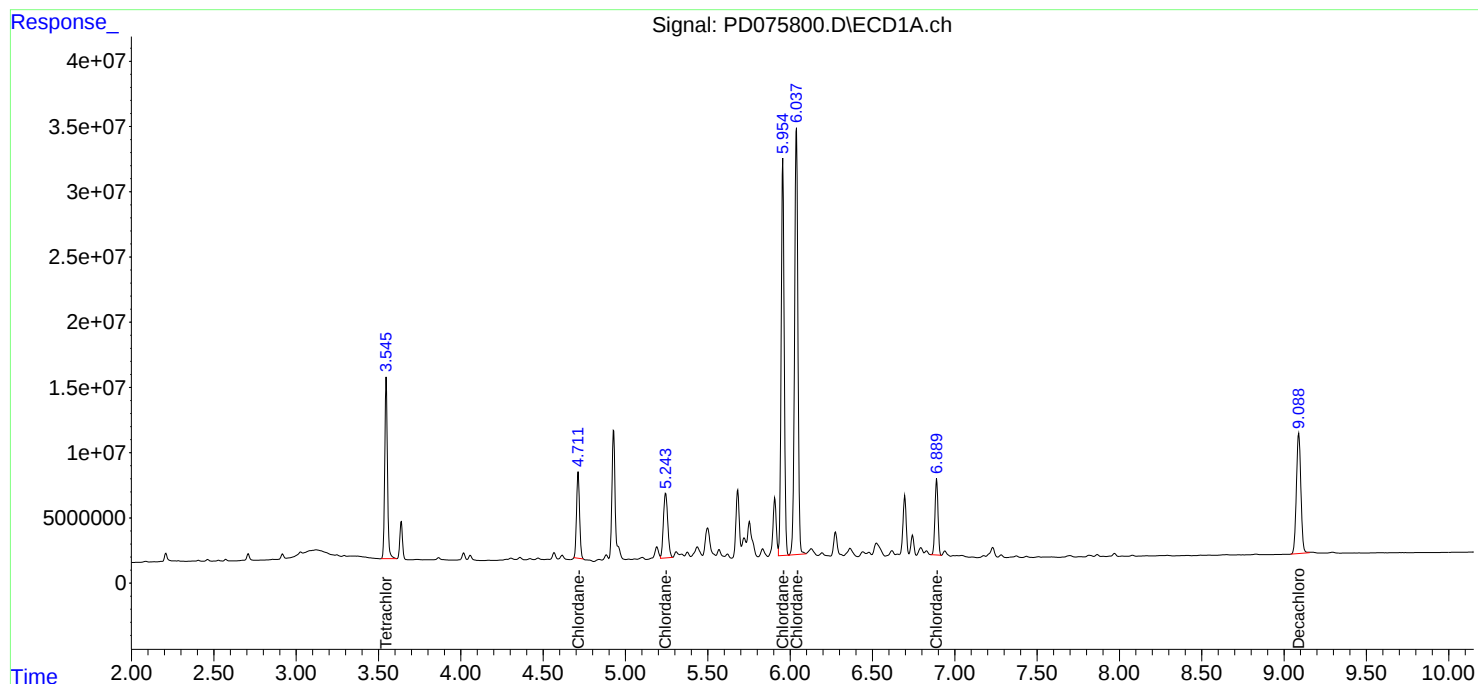


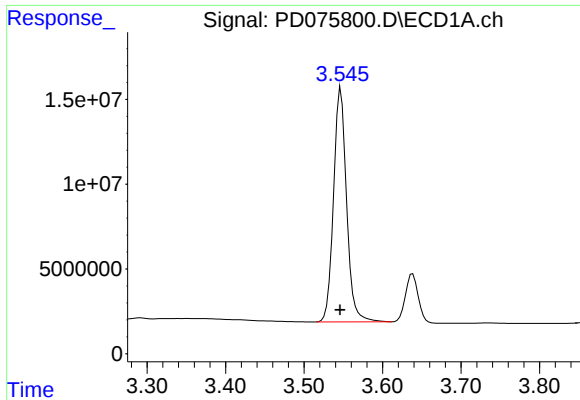

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 159760977
Conc: 75.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

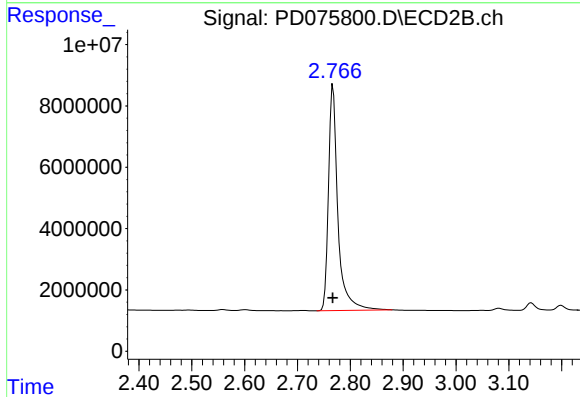


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 91339320
Conc: 75.77 ng/ml

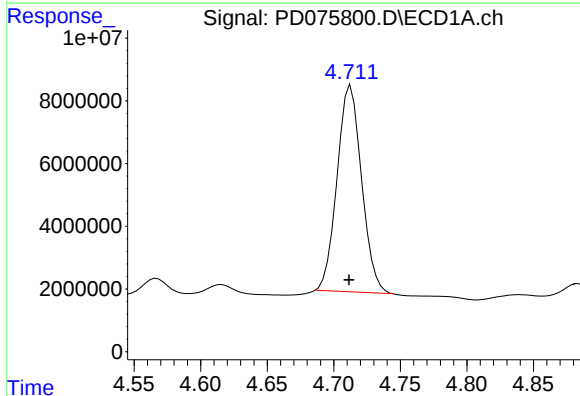


#23 Chlordane-1

R.T.: 4.713 min
Delta R.T.: 0.001 min
Response: 84232138
Conc: 754.91 ng/ml

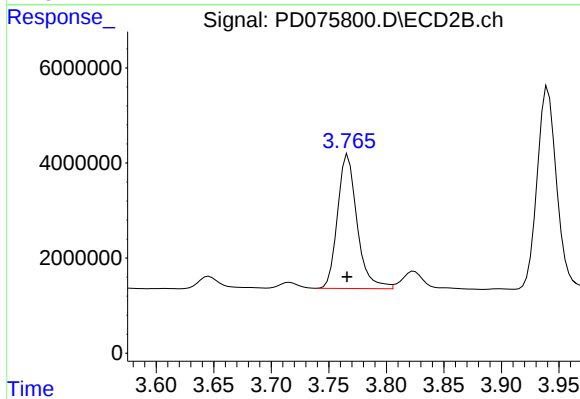

#23 Chlordane-1


R.T.: 3.767 min
Delta R.T.: 0.000 min
Response: 33318602
Conc: 751.08 ng/ml

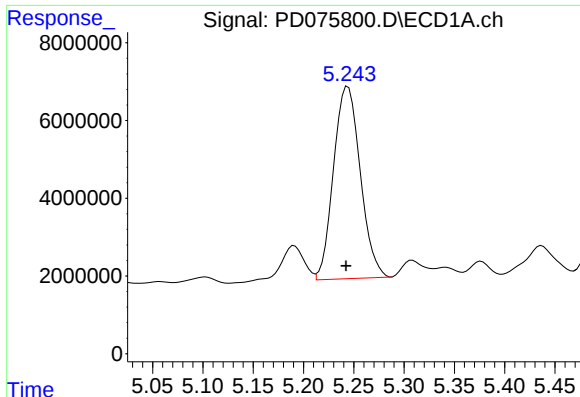

#24 Chlordane-2


R.T.: 5.244 min
Delta R.T.: 0.002 min
Response: 91295147
Conc: 736.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

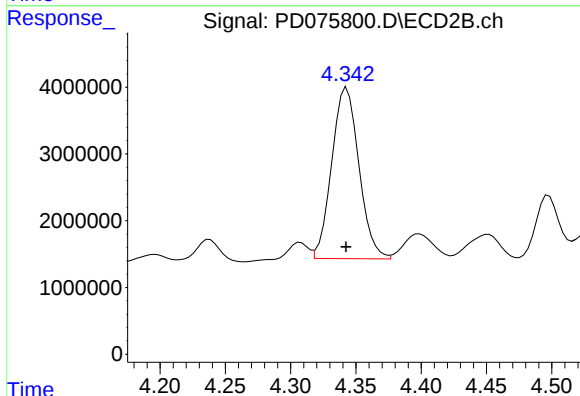


#24 Chlordane-2

R.T.: 4.343 min
Delta R.T.: 0.000 min
Response: 37129594
Conc: 739.85 ng/ml

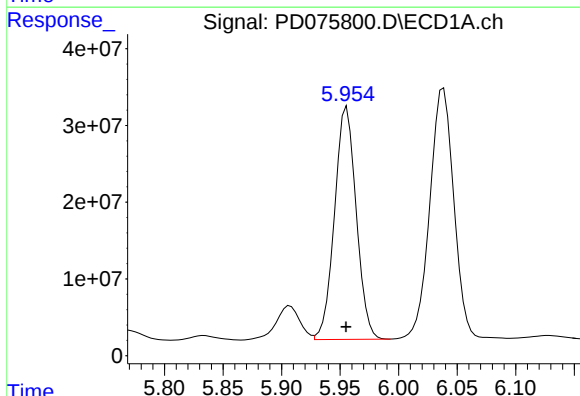


#25 Chlordane-3

R.T.: 5.956 min
Delta R.T.: 0.000 min
Response: 390918541
Conc: 771.24 ng/ml

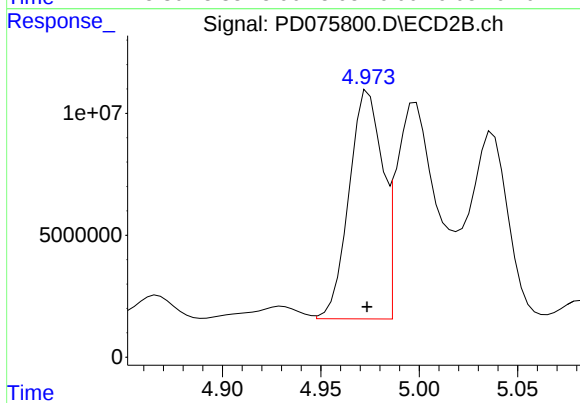

#25 Chlordane-3


R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 109885693
Conc: 762.85 ng/ml

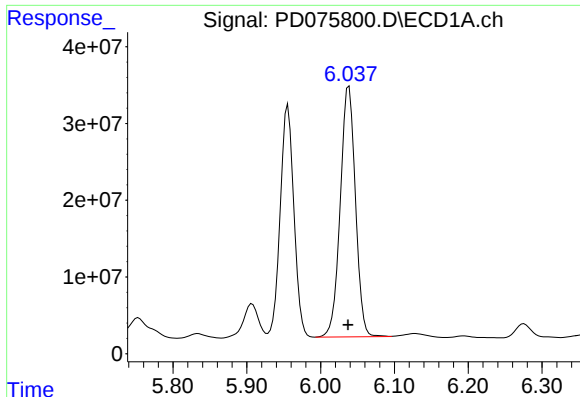

#26 Chlordane-4


R.T.: 6.038 min
Delta R.T.: 0.001 min
Response: 467255667
Conc: 761.07 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

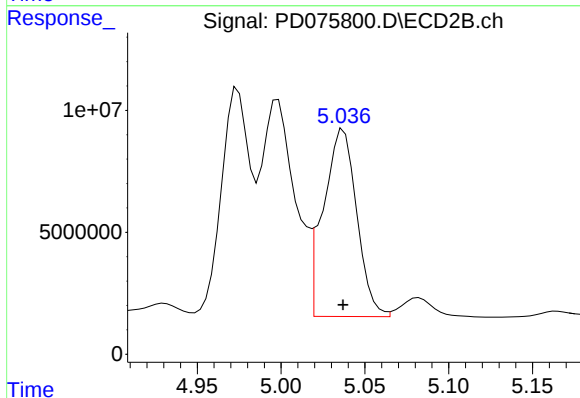


#26 Chlordane-4

R.T.: 5.037 min
Delta R.T.: 0.000 min
Response: 106547360
Conc: 741.39 ng/ml

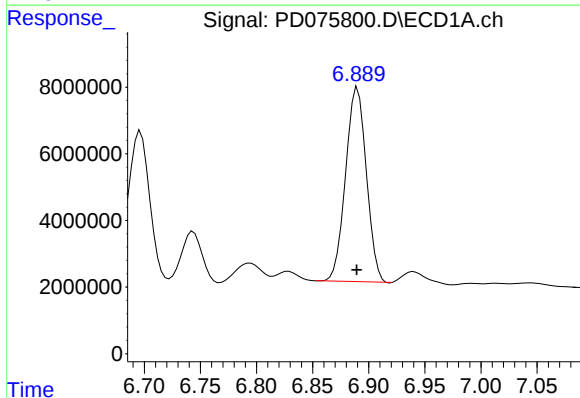


#27 Chlordane-5

R.T.: 6.890 min
Delta R.T.: 0.000 min
Response: 74864740
Conc: 757.16 ng/ml

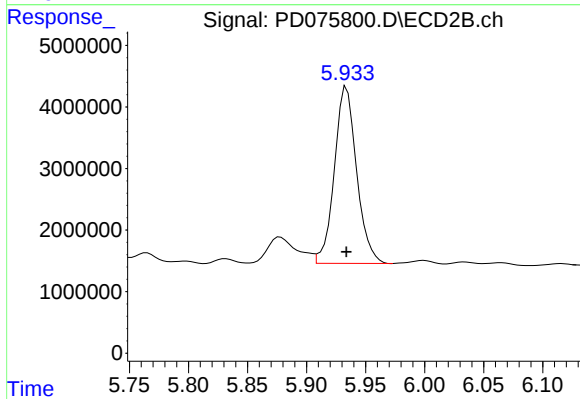

#27 Chlordane-5


R.T.: 5.934 min
Delta R.T.: 0.000 min
Response: 37681238
Conc: 762.47 ng/ml

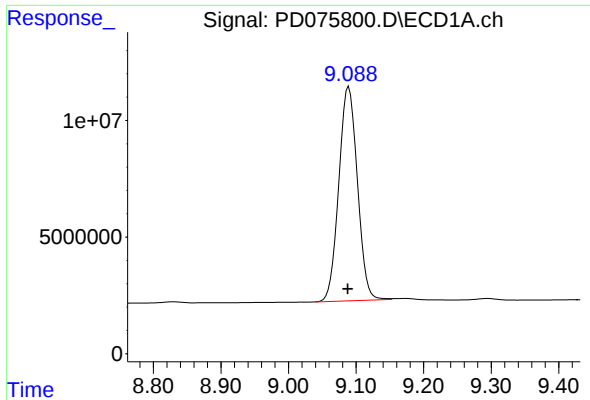

#28 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: 0.002 min
Response: 175444479
Conc: 72.46 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

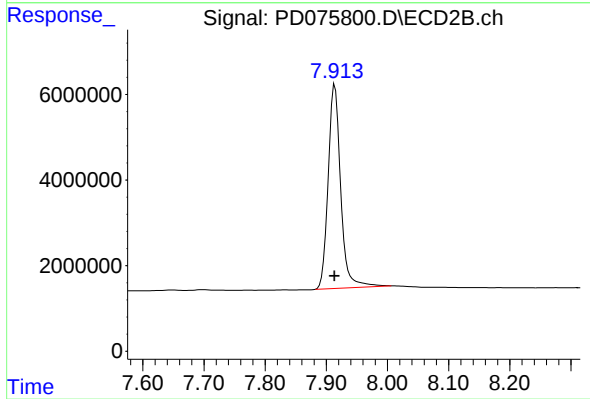

#28 Decachlorobiphenyl

R.T.: 7.914 min
Delta R.T.: 0.000 min
Response: 68049156
Conc: 72.72 ng/ml