

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061523\
 Data File : PD075812.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2023 20:16
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 03:51:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 03:47:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.767	53668416	27195630	25.195	25.067
28)	SA Decachlor...	9.090	7.914	65348085	24918017	25.795	25.484
Target Compounds							
6)	B beta-BHC	0.000	3.905	0	222239	N.D.	0.349 #
7)	B delta-BHC	4.765f	0.000	1754225	0	0.526	N.D. #
8)	B Heptachlo...	5.692	0.000	1083516	0	0.336	N.D. #
9)	A Endosulfan I	6.083	0.000	285919	0	0.095	N.D. #
10)	B gamma-Chl...	5.941	0.000	248359	0	0.077	N.D. #
11)	B alpha-Chl...	6.035	0.000	259349	0	0.080	N.D. #
15)	B Endosulfa...	6.787f	0.000	698920	0	0.271	N.D. #
19)	B Endosulfa...	0.000	6.320	0	940568	N.D.	0.870 #
21)	B Endrin ke...	7.692f	0.000	1033764	0	0.371	N.D. #
25)	Chlordane-3	5.941	0.000	248359	0	0.478	N.D. #
26)	Chlordane-4	6.035	0.000	259349	0	0.412	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061523\
Data File : PD075812.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2023 20:16
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 03:51:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 03:47:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

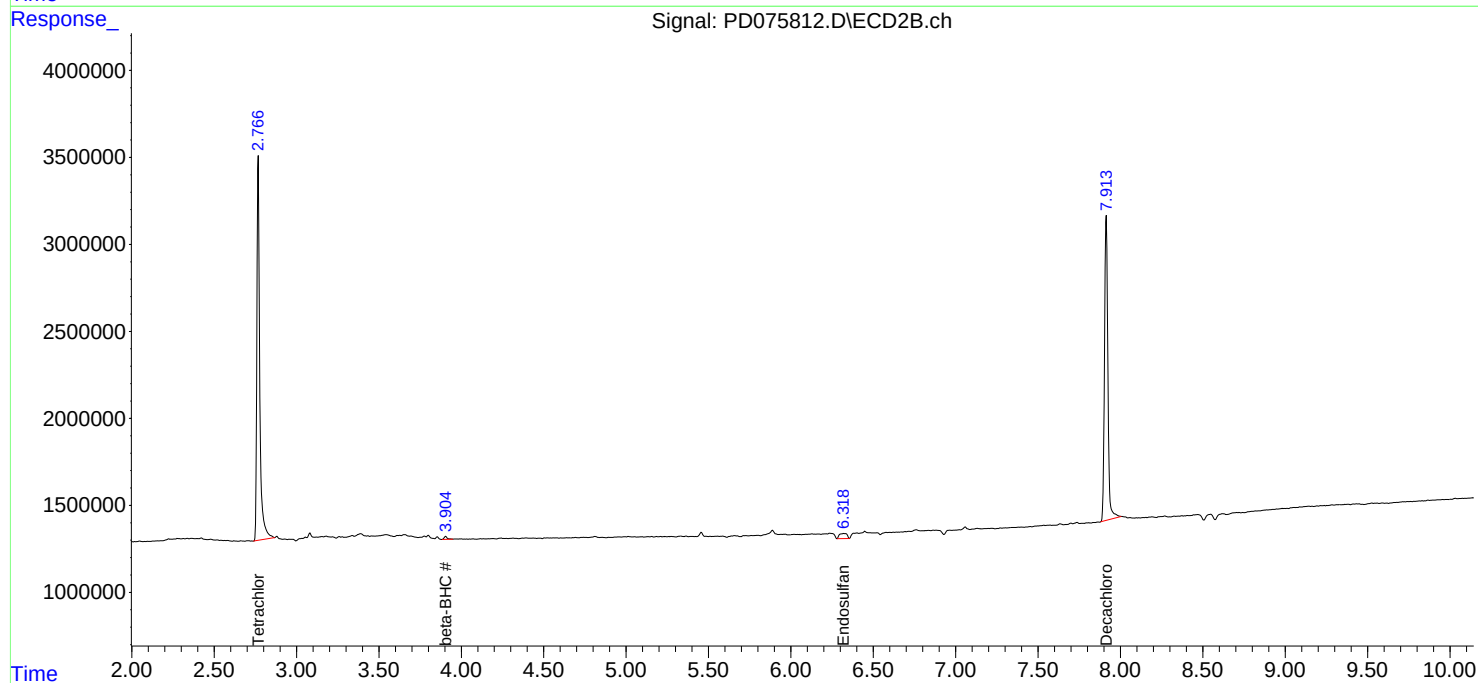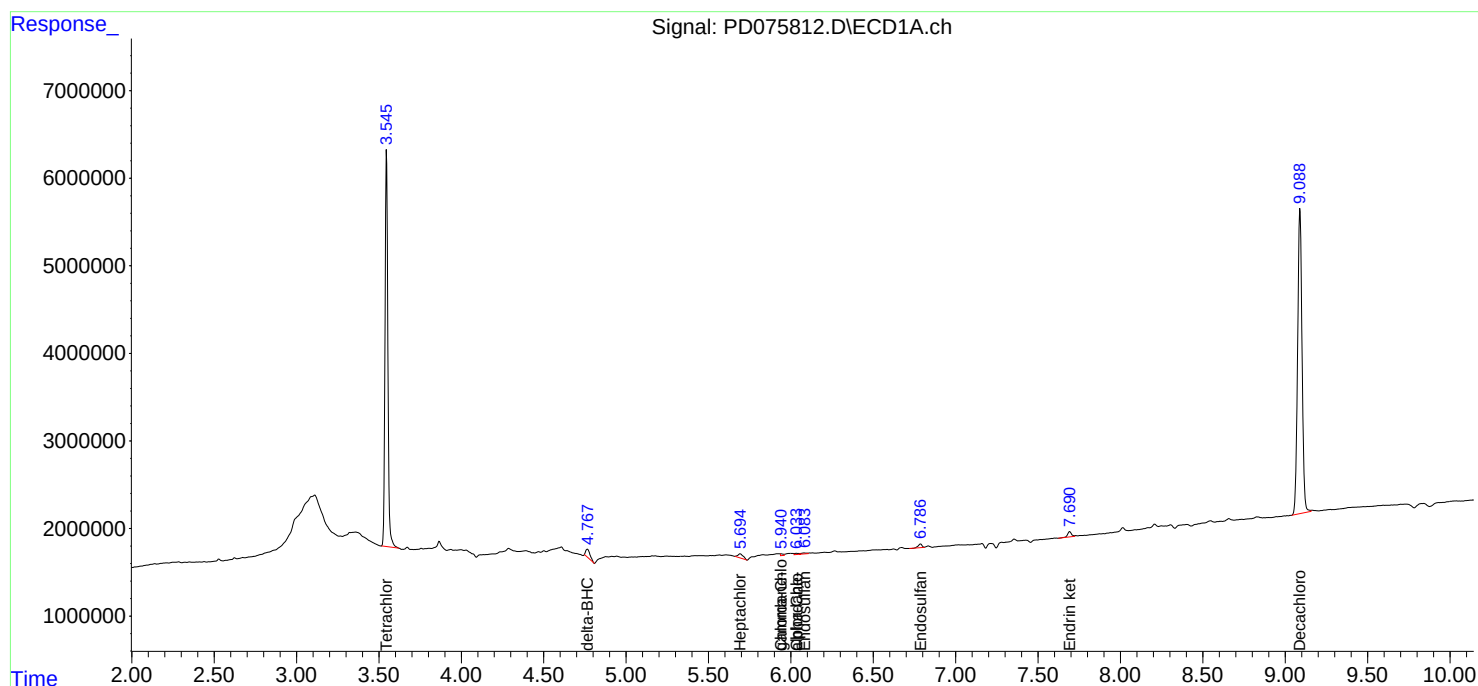


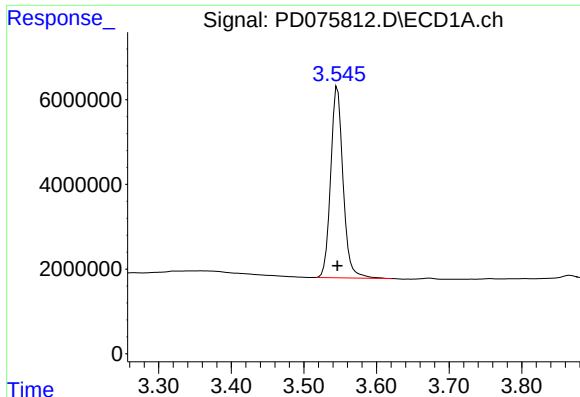

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 53668416
Conc: 25.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

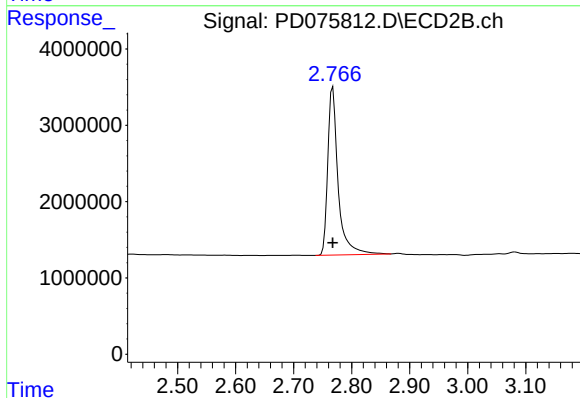


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 27195630
Conc: 25.07 ng/ml

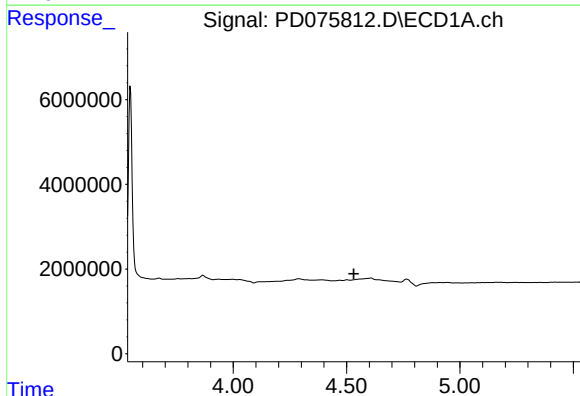


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.532 min
Response: 0
Conc: N.D.

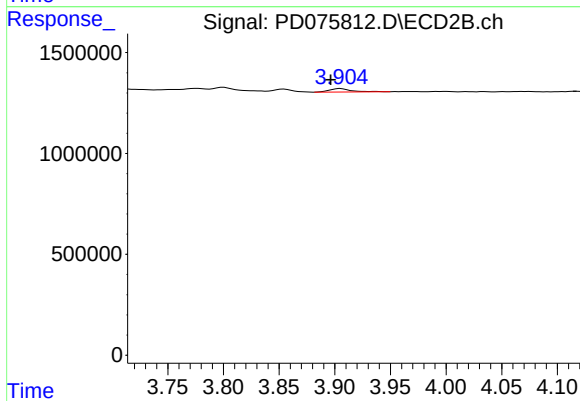

#6 beta-BHC


R.T.: 3.905 min
Delta R.T.: 0.009 min
Response: 222239
Conc: 0.35 ng/ml

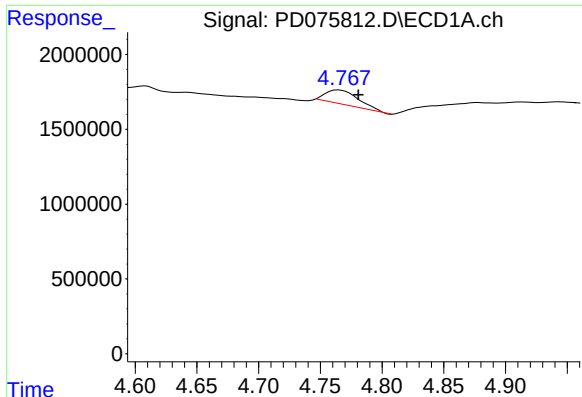

#7 delta-BHC


R.T.: 4.765 min
Delta R.T.: -0.016 min
Response: 1754225
Conc: 0.53 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

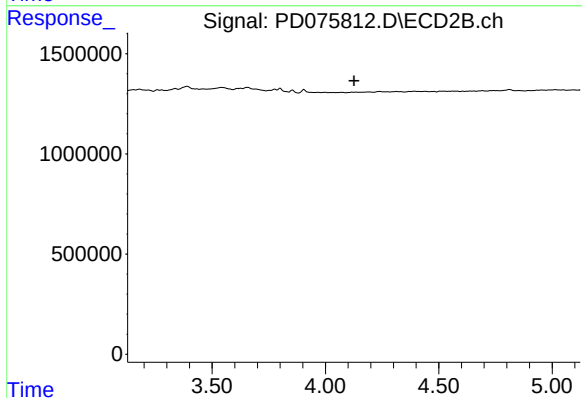


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.127 min
Response: 0
Conc: N.D.

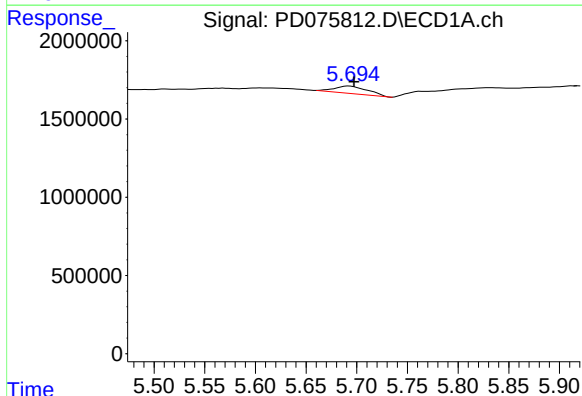


#8 Heptachlor epoxide

R.T.: 5.692 min
Delta R.T.: -0.005 min
Response: 1083516
Conc: 0.34 ng/ml

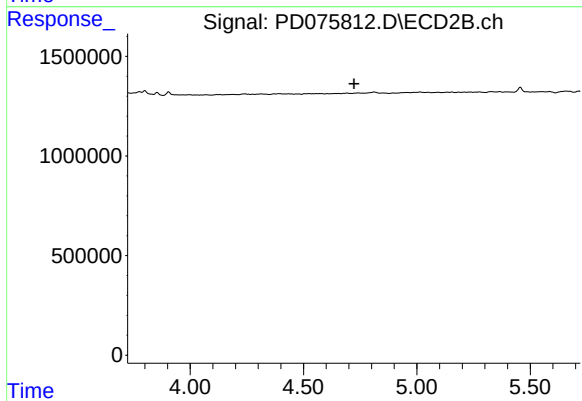

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

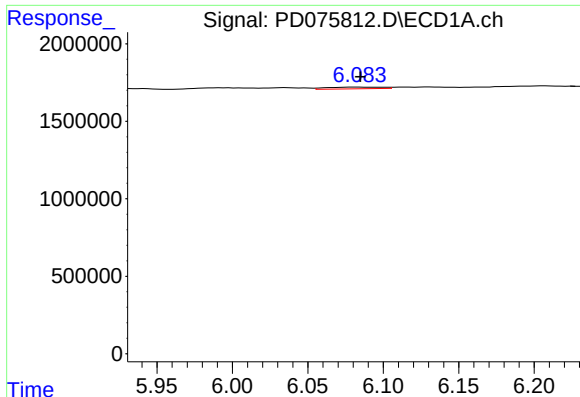

#9 Endosulfan I


R.T.: 6.083 min
Delta R.T.: -0.002 min
Response: 285919
Conc: 0.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

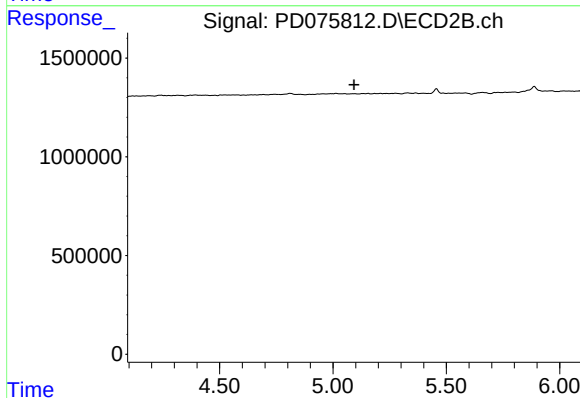


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.093 min
Response: 0
Conc: N.D.

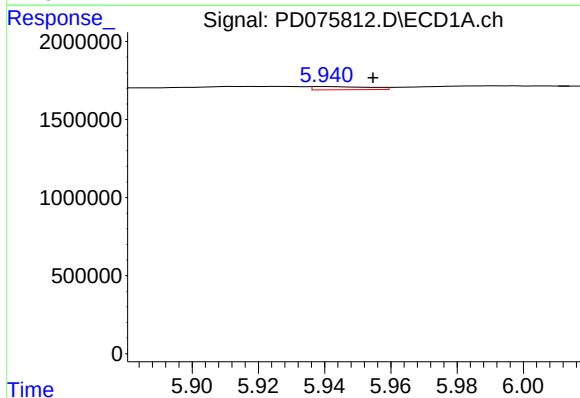


#10 gamma-Chlordane

R.T.: 5.941 min
Delta R.T.: -0.014 min
Response: 248359
Conc: 0.08 ng/ml

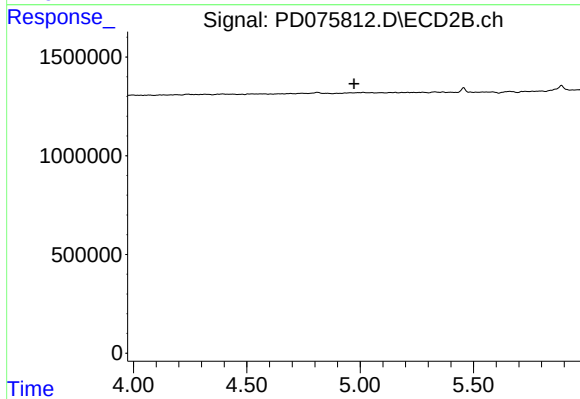

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.973 min
Response: 0
Conc: N.D.

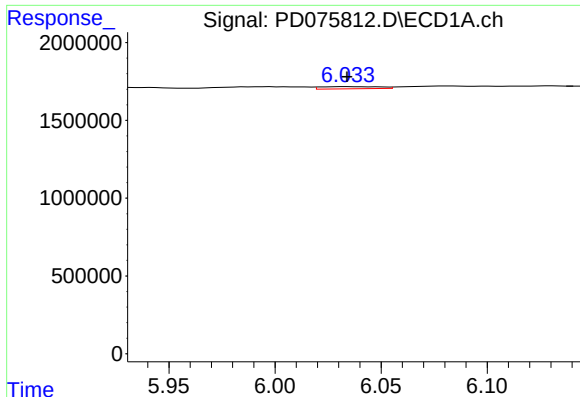

#11 alpha-Chlordane


R.T.: 6.035 min
Delta R.T.: 0.000 min
Response: 259349
Conc: 0.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

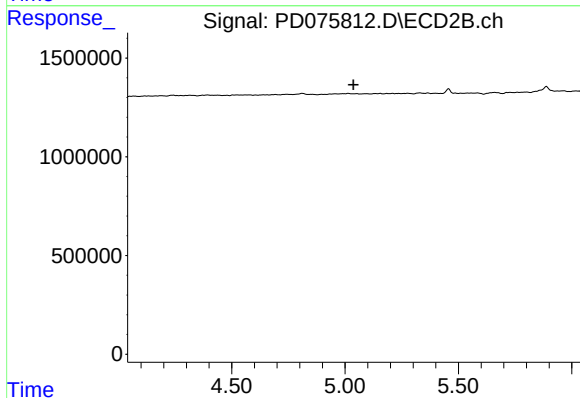


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

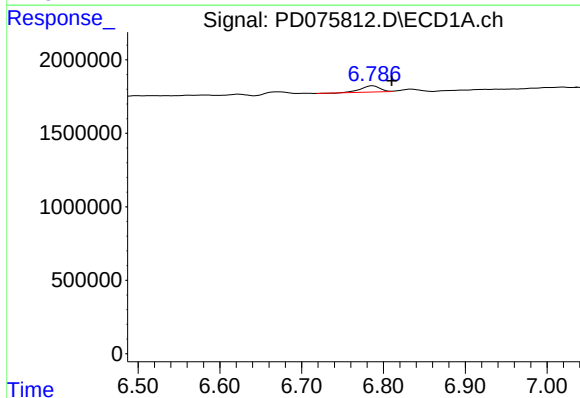


#15 Endosulfan II

R.T.: 6.787 min
Delta R.T.: -0.023 min
Response: 698920
Conc: 0.27 ng/ml

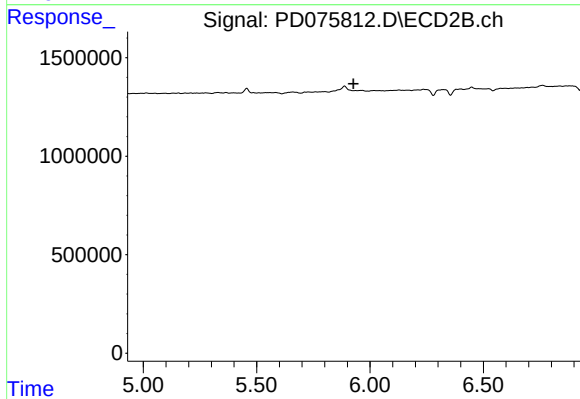

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.928 min
Response: 0
Conc: N.D.

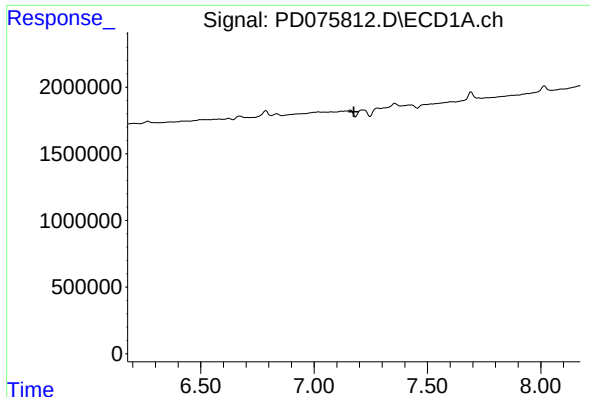

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.175 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
I.BLK

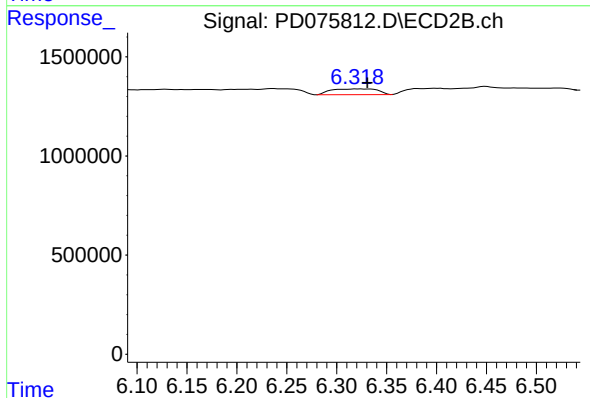


#19 Endosulfan Sulfate

R.T.: 6.320 min
Delta R.T.: -0.011 min
Response: 940568
Conc: 0.87 ng/ml

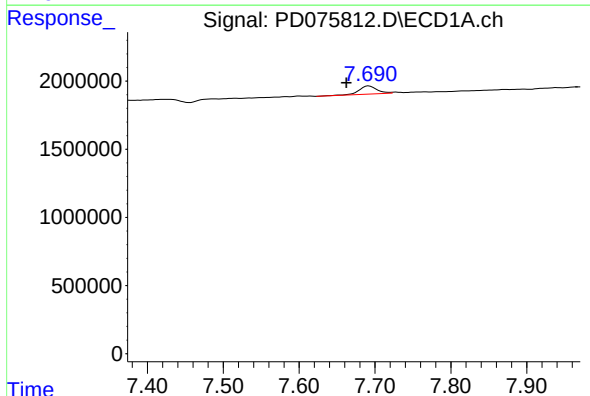


#21 Endrin ketone

R.T.: 7.692 min
Delta R.T.: 0.029 min
Response: 1033764
Conc: 0.37 ng/ml

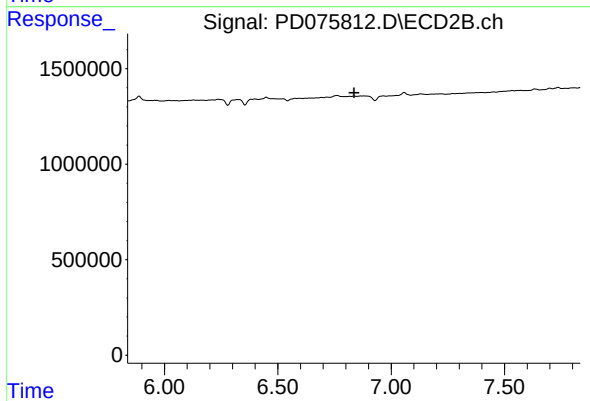

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.837 min
Response: 0
Conc: N.D.

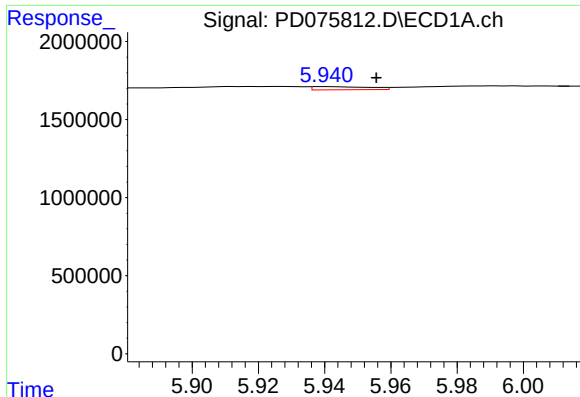

#25 Chlordane-3


R.T.: 5.941 min
Delta R.T.: -0.015 min
Response: 248359
Conc: 0.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

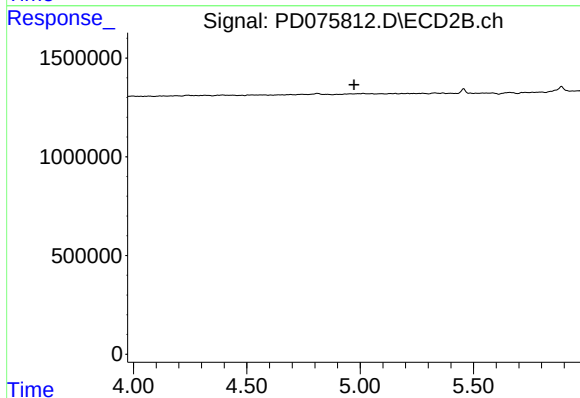


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.974 min
Response: 0
Conc: N.D.

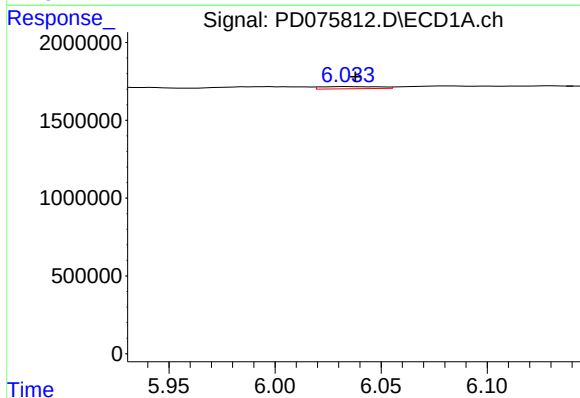


#26 Chlordane-4

R.T.: 6.035 min
Delta R.T.: -0.003 min
Response: 259349
Conc: 0.41 ng/ml

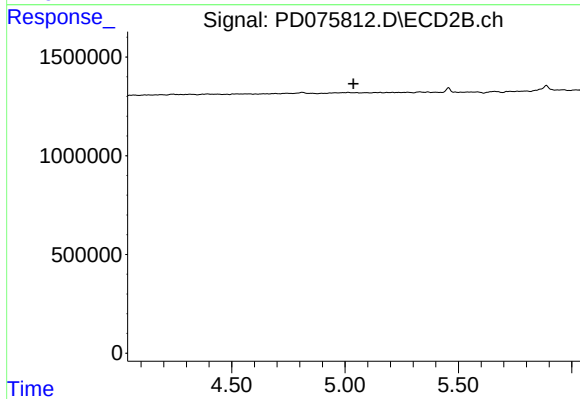

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

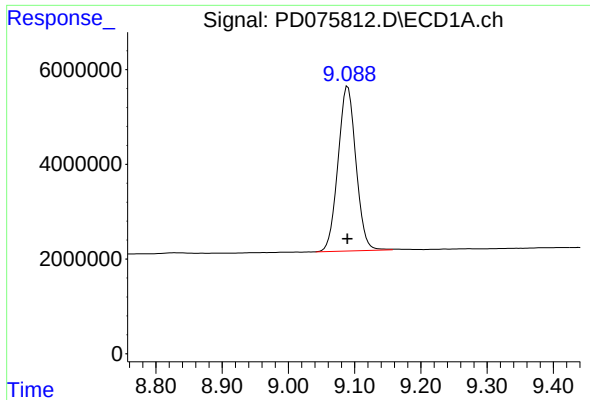

#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: 0.000 min
Response: 65348085
Conc: 25.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

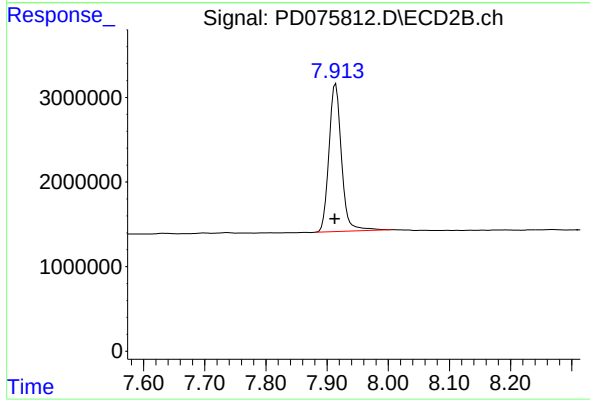

#28 Decachlorobiphenyl

R.T.: 7.914 min
Delta R.T.: 0.001 min
Response: 24918017
Conc: 25.48 ng/ml