

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061523\
 Data File : PD075807.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2023 19:07
 Operator : AR\AJ
 Sample : PTOXICC250
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 04:24:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 04:23:57 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.546	2.768	52889780	26192233	25.025	25.526
7) SA Decachlor...	9.089	7.914	63086446	24841246	25.837	25.851
Target Compounds						
2) Toxaphene-1	6.253	4.999	5988232	1880580	259.675	246.122
3) Toxaphene-2	7.168	5.683	13063683	1892780	233.170	251.988
4) Toxaphene-3	7.265	6.598	8071178	4222264	235.739	219.418
5) Toxaphene-4	7.590	6.725	9840699	7728345	239.236	240.091
6) Toxaphene-5	7.954	7.041	9120221	2855812	227.139	225.107


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061523\
Data File : PD075807.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2023 19:07
Operator : AR\AJ
Sample : PTOXICC250
Misc :
ALS Vial : 18 Sample Multiplier: 1


Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 04:24:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX061523.M
Quant Title : GC Extractables
Qlast Update : Fri Jun 16 04:23:57 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x0.25µm

Response_ Time 2.00 2.50 3.00 3.50 4.00 4.50 5.00 5.50 6.00 6.50 7.00 7.50 8.00 8.50 9.00 9.50 10.00
Signal: PD075807.D\ECD1A.ch

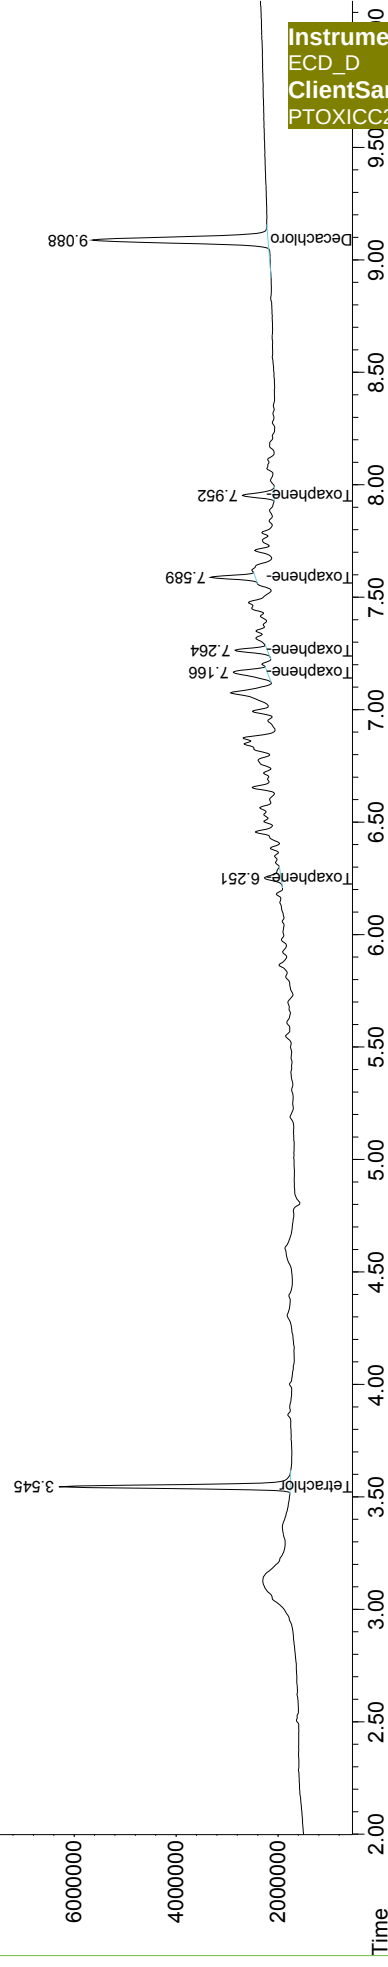

Response_ Time 2.00 2.50 3.00 3.50 4.00 4.50 5.00 5.50 6.00 6.50 7.00 7.50 8.00 8.50 9.00 9.50 10.00
Signal: PD075807.D\ECD2B.ch

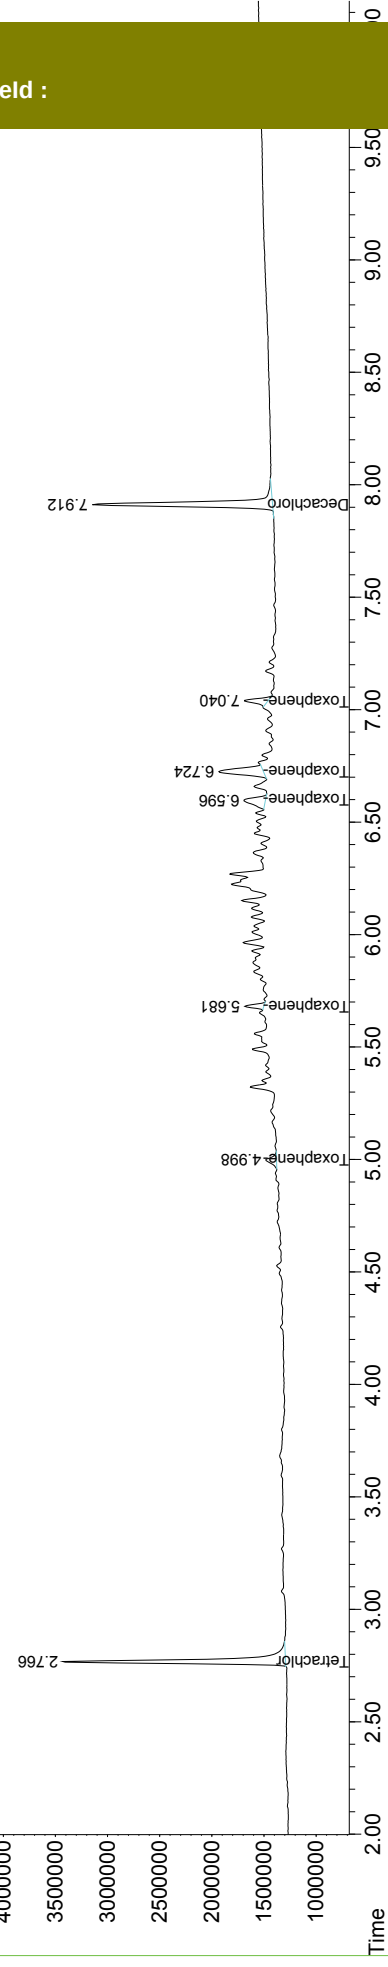

Instrument :
ECD_D
ClientSampleId :
PTOXICC250