

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061523\
 Data File : PD075799.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2023 16:49
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 01:31:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 01:31:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.766	217.0E6	125.1E6	101.518	101.837
28)	SA Decachlor...	9.090	7.914	233.9E6	91658751	98.276	98.962
Target Compounds							
23)	Chlordane-1	4.711	3.766	114.1E6	45192781	1011.249	1009.287
24)	Chlordane-2	5.243	4.343	121.7E6	48945722	990.649	987.495
25)	Chlordane-3	5.956	4.974	538.3E6	150.2E6	1030.074	1020.883
26)	Chlordane-4	6.038	5.037	640.0E6	146.7E6	1020.806	1010.209
27)	Chlordane-5	6.890	5.934	102.2E6	51557109	1016.357	1021.167



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061523\
Data File : PD075799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2023 16:49
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 01:31:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 01:31:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

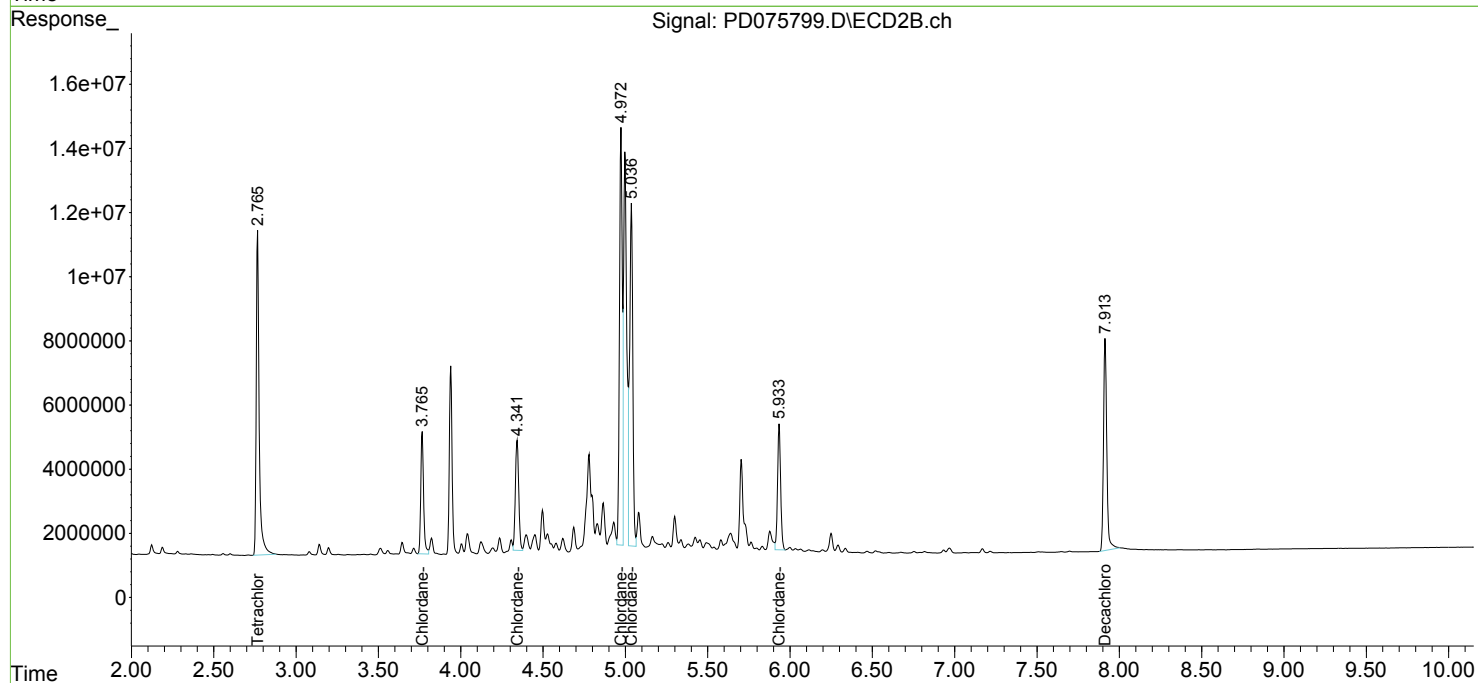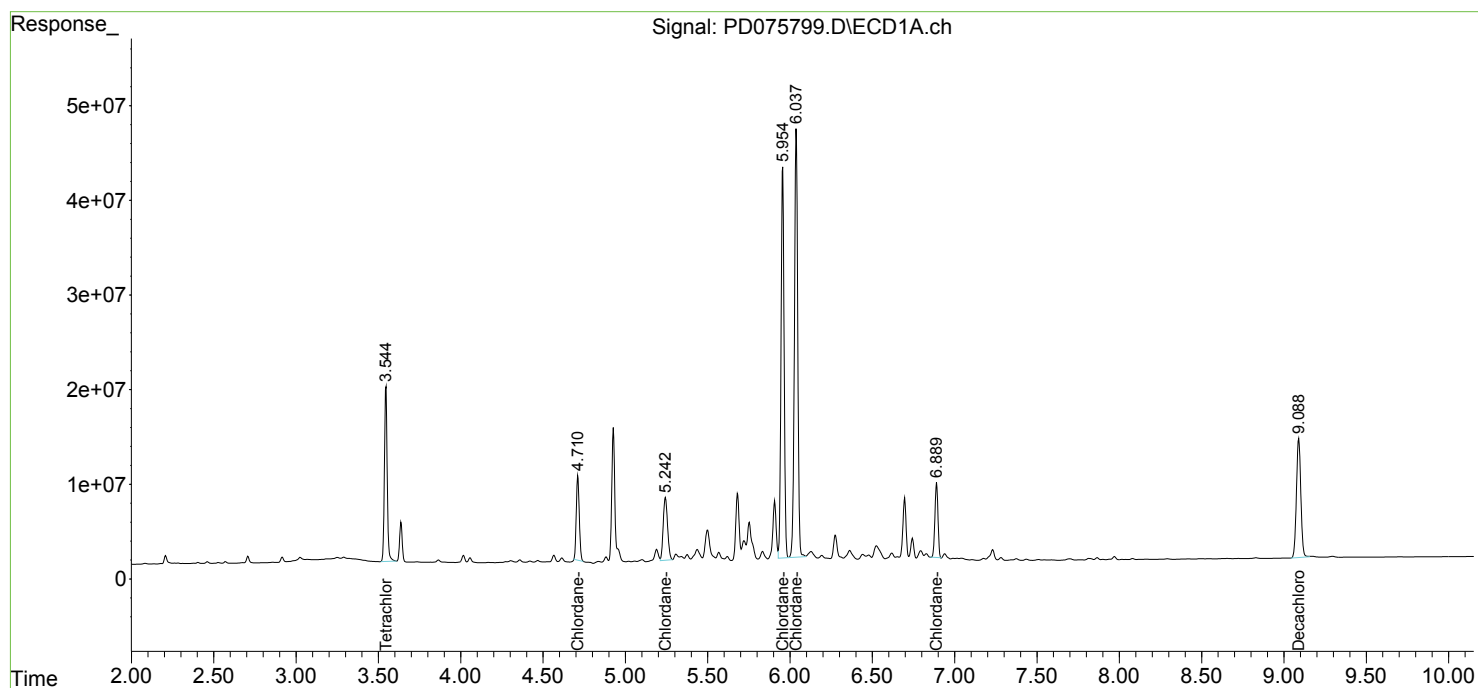


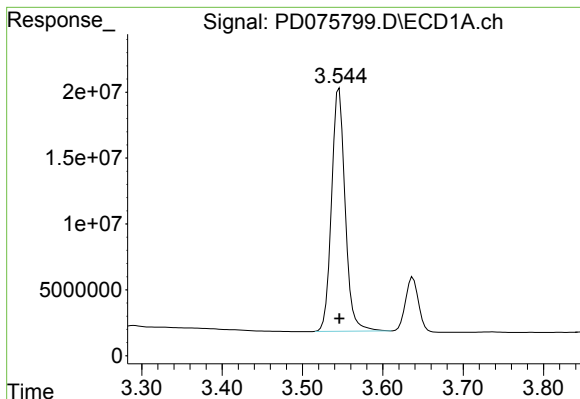

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 217029416
Conc: 101.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

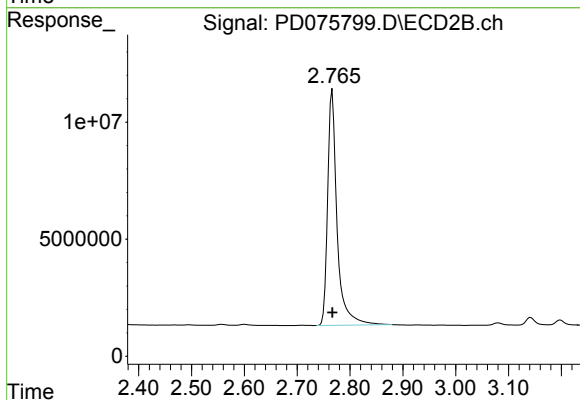


#1 Tetrachloro-m-xylene

R.T.: 2.766 min
Delta R.T.: 0.000 min
Response: 125054958
Conc: 101.84 ng/ml

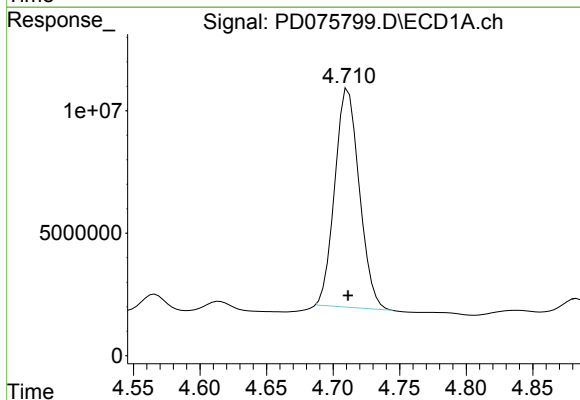


#23 Chlordane-1

R.T.: 4.711 min
Delta R.T.: 0.000 min
Response: 114117340
Conc: 1011.25 ng/ml

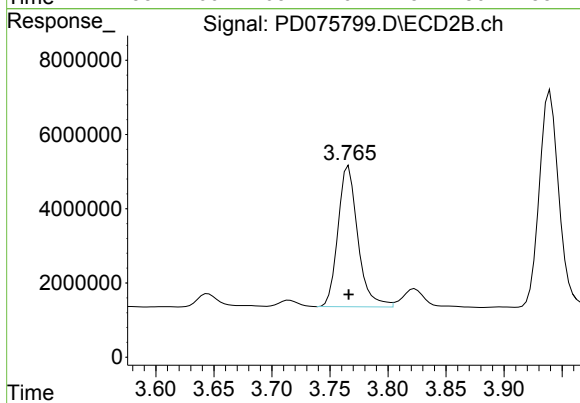

#23 Chlordane-1


R.T.: 3.766 min
Delta R.T.: 0.000 min
Response: 45192781
Conc: 1009.29 ng/ml

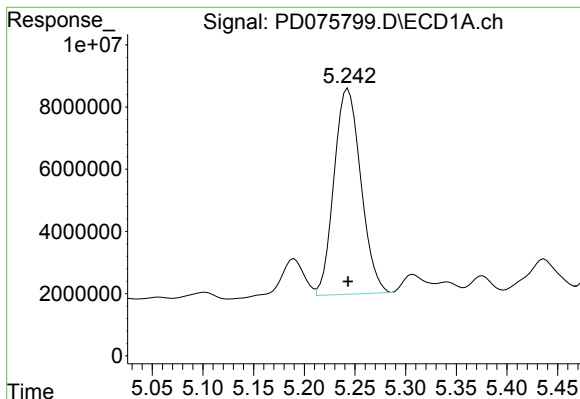

#24 Chlordane-2


R.T.: 5.243 min
Delta R.T.: 0.000 min
Response: 121740253
Conc: 990.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

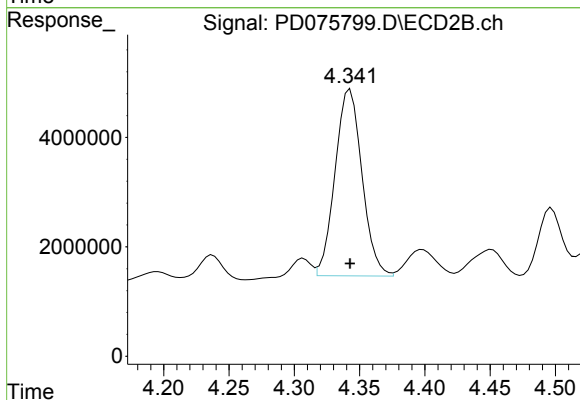


#24 Chlordane-2

R.T.: 4.343 min
Delta R.T.: 0.000 min
Response: 48945722
Conc: 987.49 ng/ml

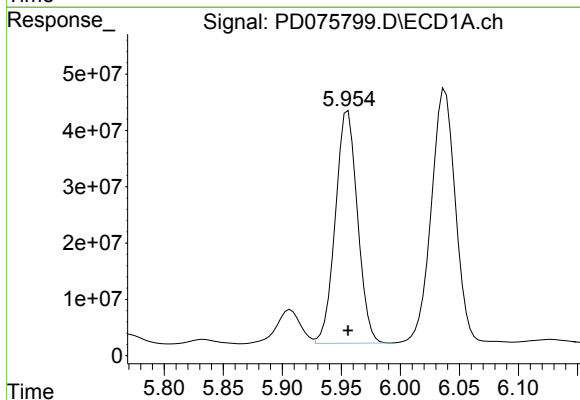


#25 Chlordane-3

R.T.: 5.956 min
Delta R.T.: 0.000 min
Response: 538305343
Conc: 1030.07 ng/ml

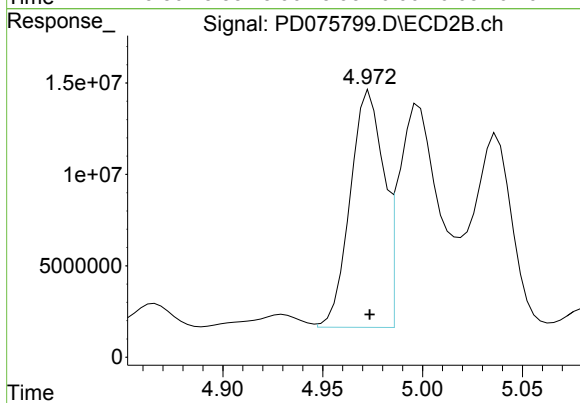

#25 Chlordane-3


R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 150190278
Conc: 1020.88 ng/ml

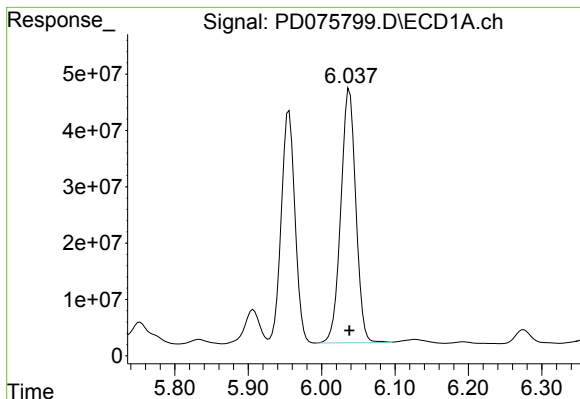

#26 Chlordane-4


R.T.: 6.038 min
Delta R.T.: 0.000 min
Response: 640038999
Conc: 1020.81 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

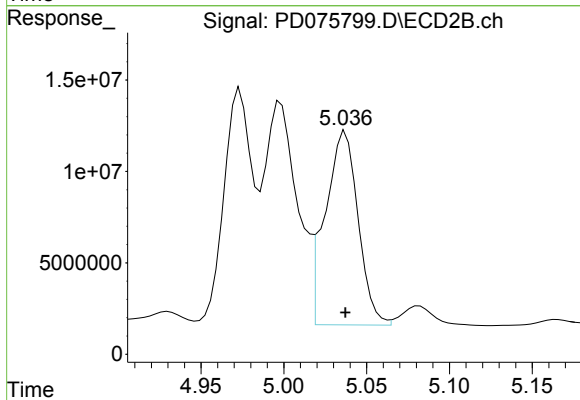


#26 Chlordane-4

R.T.: 5.037 min
Delta R.T.: 0.000 min
Response: 146678425
Conc: 1010.21 ng/ml

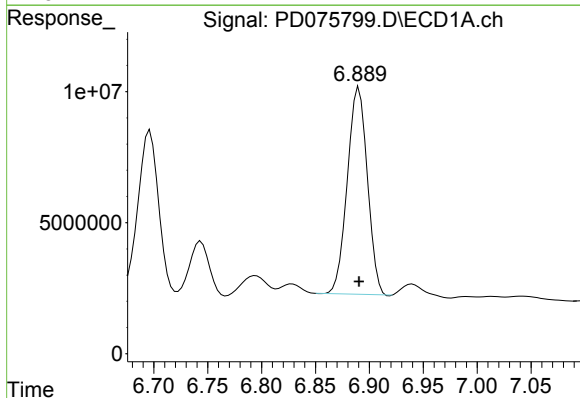


#27 Chlordane-5

R.T.: 6.890 min
Delta R.T.: 0.000 min
Response: 102163414
Conc: 1016.36 ng/ml

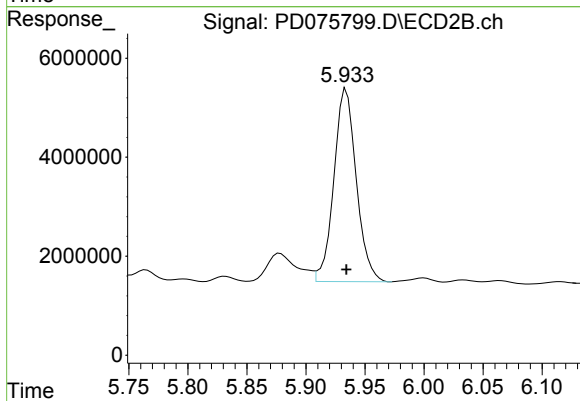

#27 Chlordane-5

R.T.: 5.934 min
Delta R.T.: 0.000 min
Response: 51557109
Conc: 1021.17 ng/ml

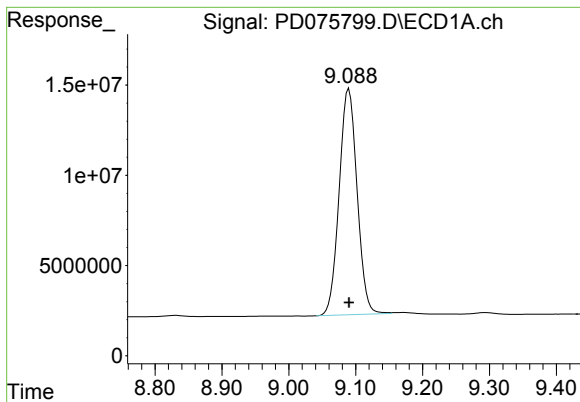

#28 Decachlorobiphenyl


R.T.: 9.090 min

Delta R.T.: 0.000 min

Response: 233931614

Conc: 98.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC1000

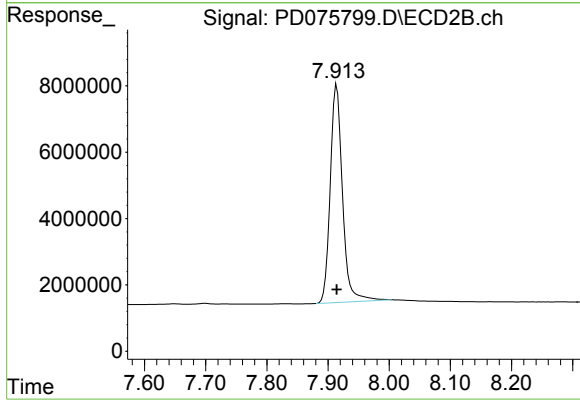

#28 Decachlorobiphenyl

R.T.: 7.914 min

Delta R.T.: 0.000 min

Response: 91658751

Conc: 98.96 ng/ml