

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061523\
 Data File : PD075801.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2023 17:16
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 01:26:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 01:24:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.767	105.3E6	60271127	50.000	50.000
28)	SA Decachlor...	9.088	7.914	121.1E6	46790503	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.711	3.766	55789268	22180541	500.000	500.000
24)	Chlordane-2	5.242	4.342	62019315	25092686	500.000	500.000
25)	Chlordane-3	5.955	4.974	253.4E6	72022937	500.000	500.000
26)	Chlordane-4	6.037	5.037	307.0E6	71856835	500.000	500.000
27)	Chlordane-5	6.889	5.934	49437563	24709849	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061523\
Data File : PD075801.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2023 17:16
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 01:26:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 01:24:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

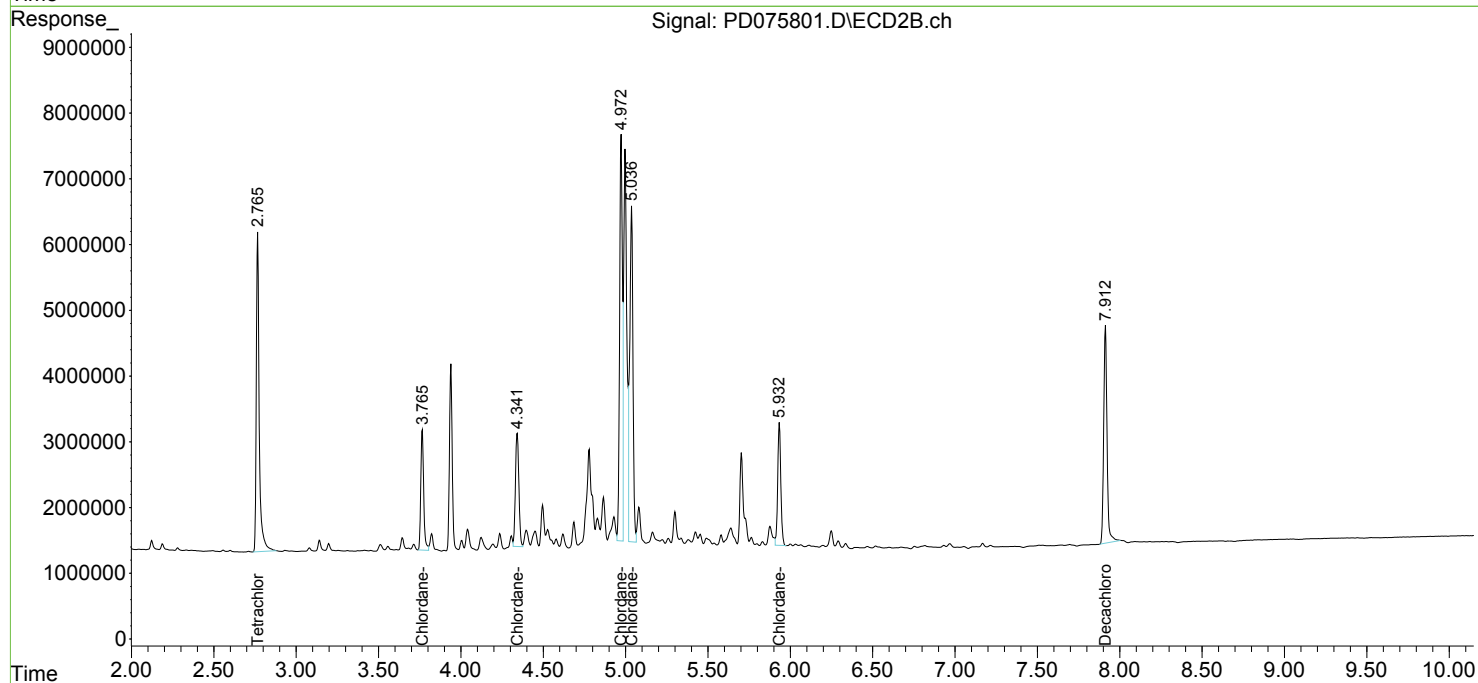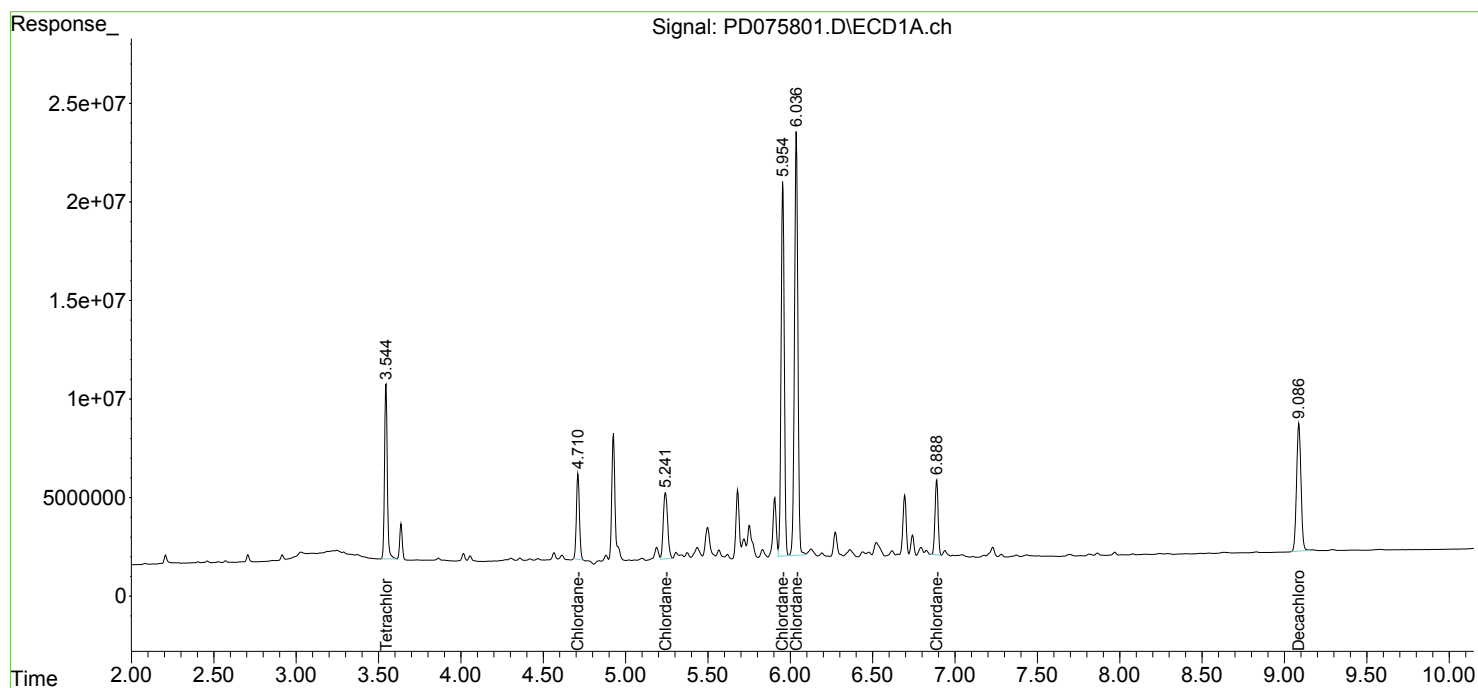


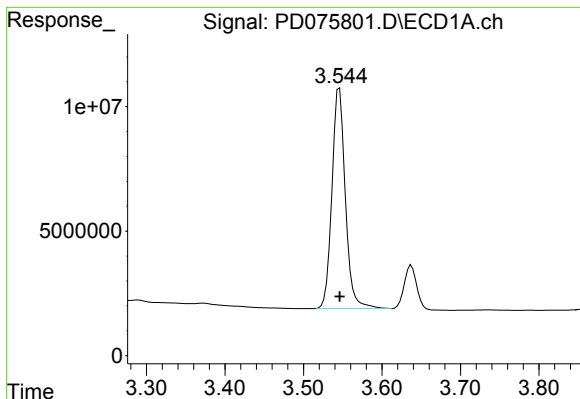

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 105268948
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

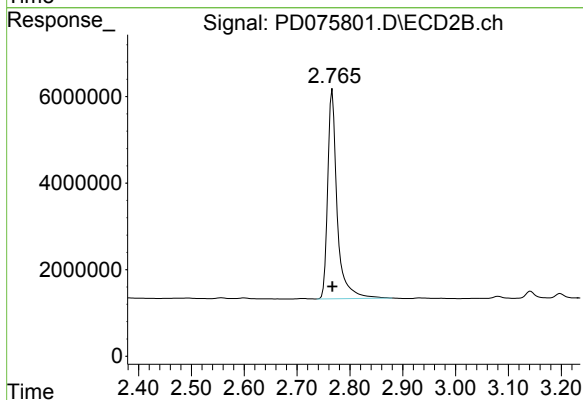


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 60271127
Conc: 50.00 ng/ml

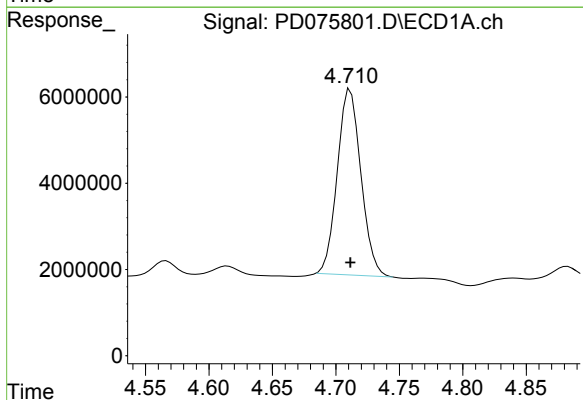


#23 Chlordane-1

R.T.: 4.711 min
Delta R.T.: 0.000 min
Response: 55789268
Conc: 500.00 ng/ml

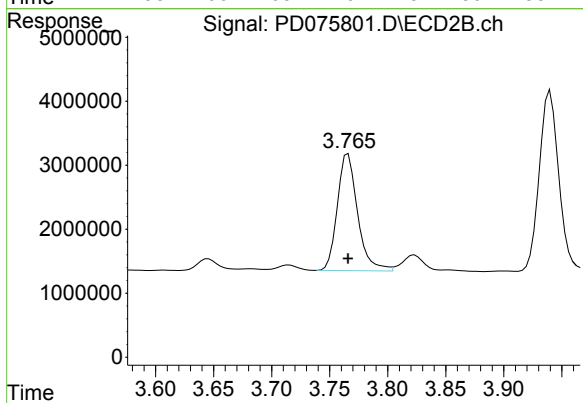

#23 Chlordane-1


R.T.: 3.766 min
Delta R.T.: 0.000 min
Response: 22180541
Conc: 500.00 ng/ml

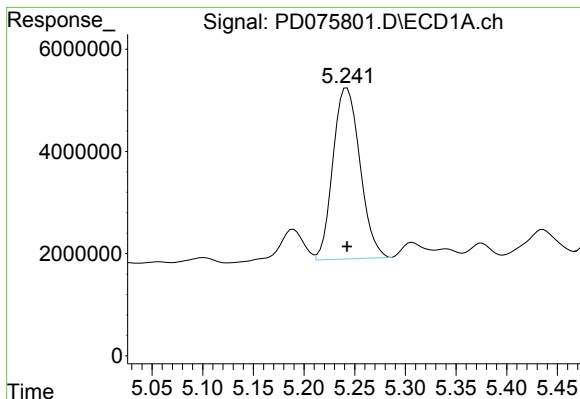

#24 Chlordane-2


R.T.: 5.242 min
Delta R.T.: 0.000 min
Response: 62019315
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

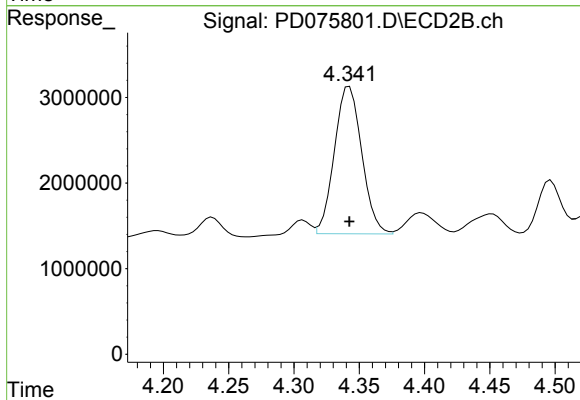


#24 Chlordane-2

R.T.: 4.342 min
Delta R.T.: 0.000 min
Response: 25092686
Conc: 500.00 ng/ml

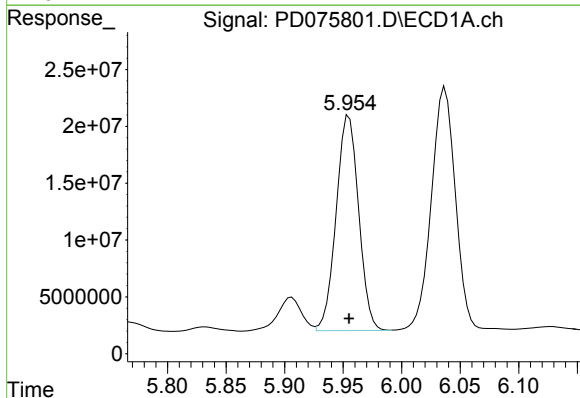


#25 Chlordane-3

R.T.: 5.955 min
Delta R.T.: 0.000 min
Response: 253436273
Conc: 500.00 ng/ml

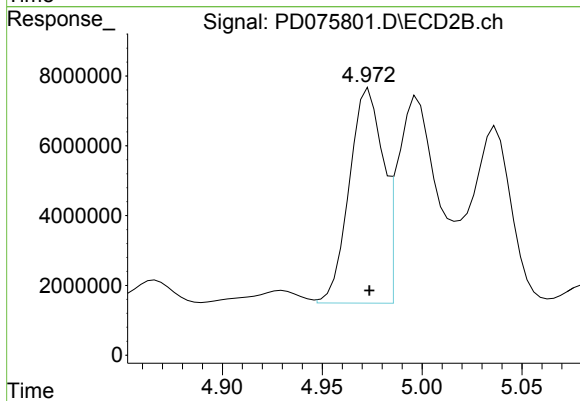

#25 Chlordane-3


R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 72022937
Conc: 500.00 ng/ml

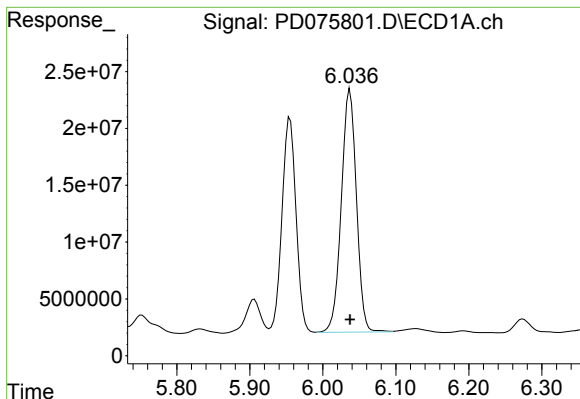

#26 Chlordane-4


R.T.: 6.037 min
Delta R.T.: 0.000 min
Response: 306974359
Conc: 500.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

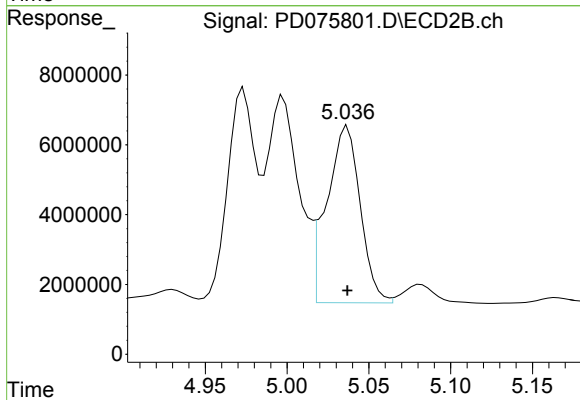


#26 Chlordane-4

R.T.: 5.037 min
Delta R.T.: 0.000 min
Response: 71856835
Conc: 500.00 ng/ml

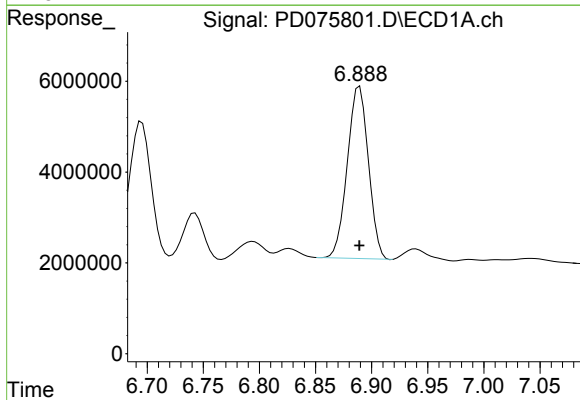


#27 Chlordane-5

R.T.: 6.889 min
Delta R.T.: 0.000 min
Response: 49437563
Conc: 500.00 ng/ml

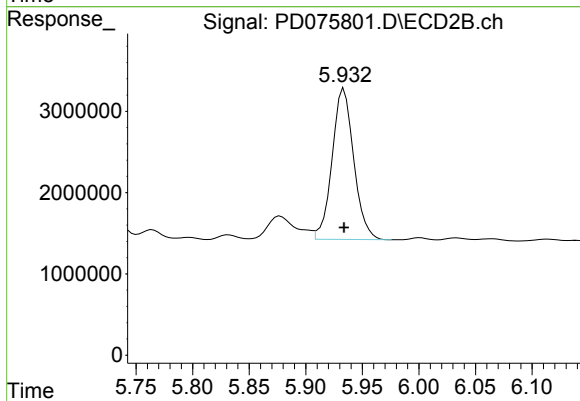

#27 Chlordane-5


R.T.: 5.934 min
Delta R.T.: 0.000 min
Response: 24709849
Conc: 500.00 ng/ml

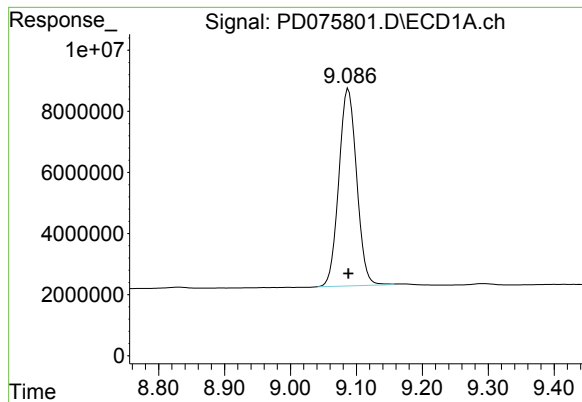

#28 Decachlorobiphenyl

R.T.: 9.088 min
Delta R.T.: 0.000 min
Response: 121070355
Conc: 50.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

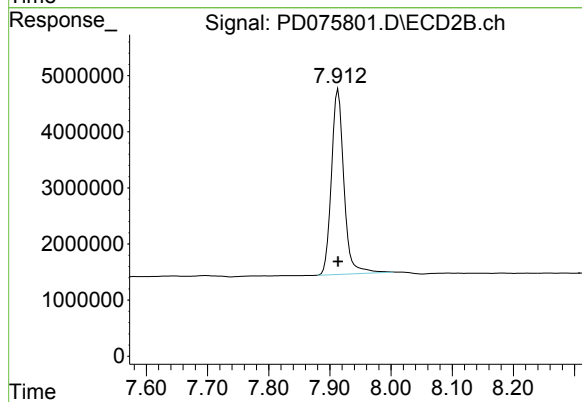

#28 Decachlorobiphenyl

R.T.: 7.914 min
Delta R.T.: 0.000 min
Response: 46790503
Conc: 50.00 ng/ml