

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061523\
 Data File : PD075802.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Jun 2023 17:30
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 01:44:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 01:44:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.767	51462591	28822995	24.320	23.886
28)	SA Decachlor...	9.089	7.914	61118956	23888244	25.614	25.719
Target Compounds							
23)	Chlordane-1	4.712	3.766	27079242	11023053	242.688	247.610
24)	Chlordane-2	5.242	4.343	31566643	13134058	255.718	261.149
25)	Chlordane-3	5.955	4.974	118.9E6	34739007	232.869	239.701
26)	Chlordane-4	6.038	5.037	145.7E6	33862883	236.950	238.510
27)	Chlordane-5	6.889	5.934	22878542	11655518	233.233	235.655



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061523\
Data File : PD075802.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Jun 2023 17:30
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 01:44:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 01:44:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

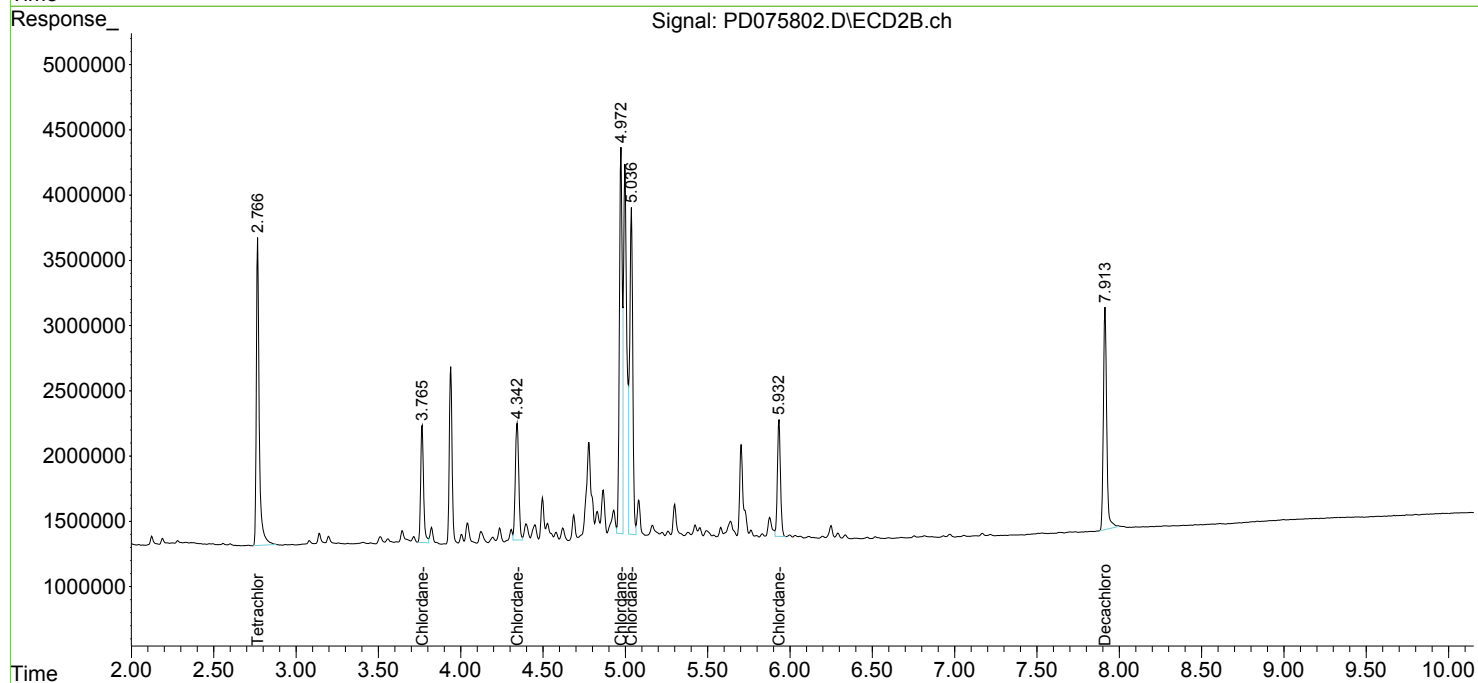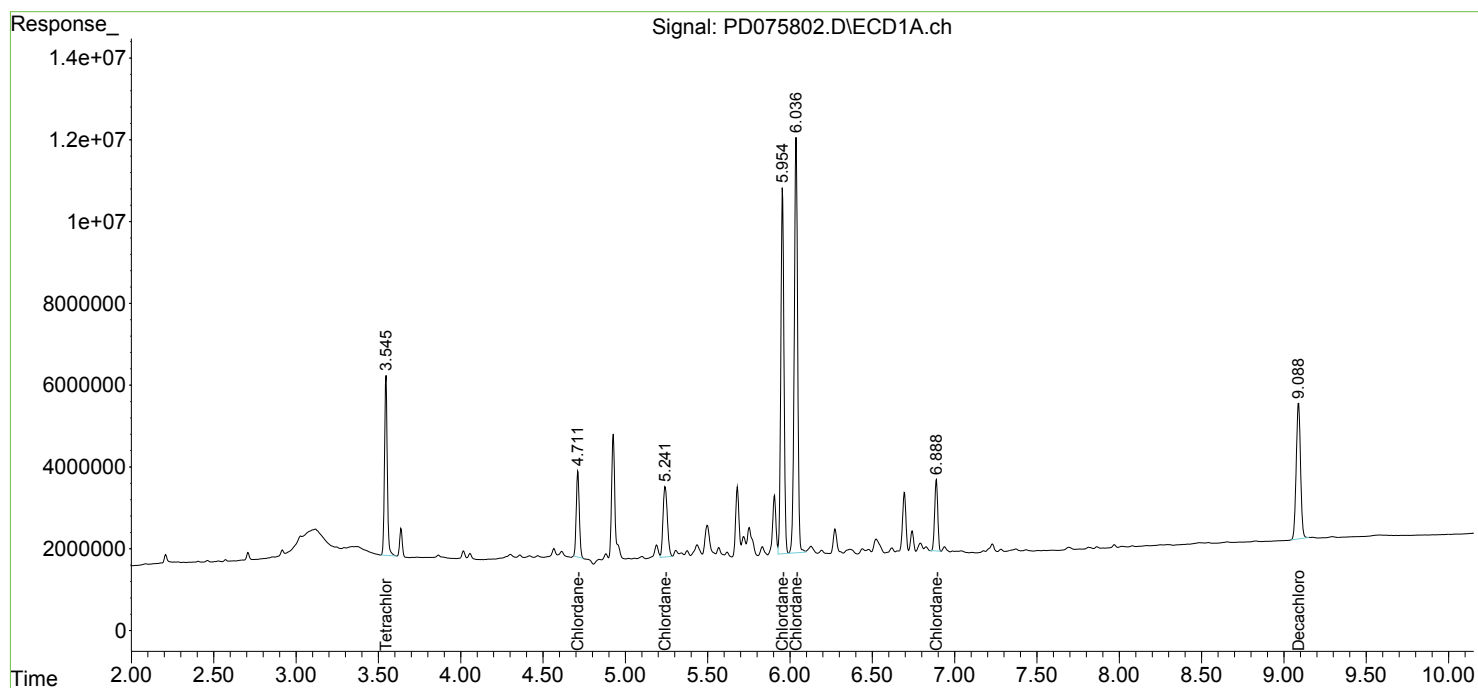


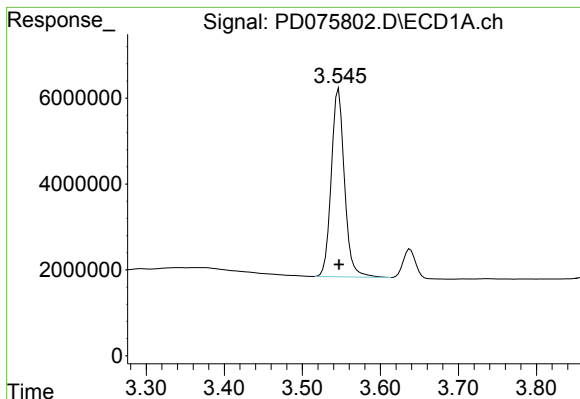

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 51462591
Conc: 24.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

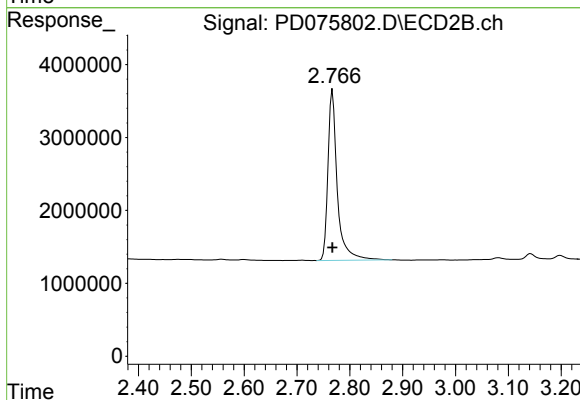


#1 Tetrachloro-m-xylene

R.T.: 2.767 min
Delta R.T.: 0.000 min
Response: 28822995
Conc: 23.89 ng/ml

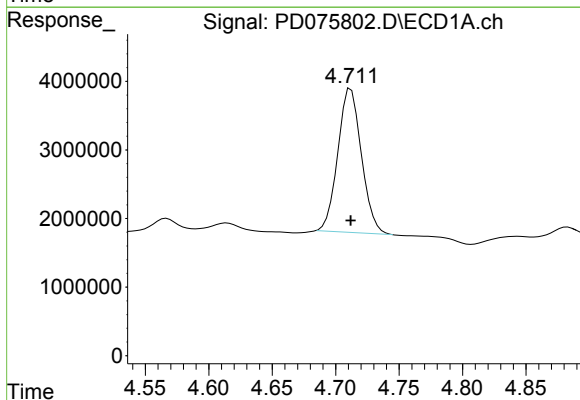


#23 Chlordane-1

R.T.: 4.712 min
Delta R.T.: 0.000 min
Response: 27079242
Conc: 242.69 ng/ml

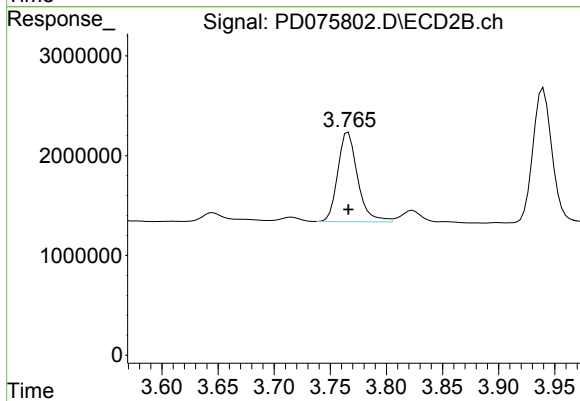

#23 Chlordane-1


R.T.: 3.766 min
Delta R.T.: 0.000 min
Response: 11023053
Conc: 247.61 ng/ml

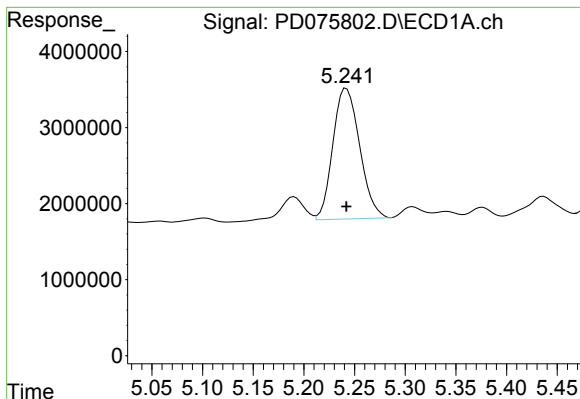

#24 Chlordane-2


R.T.: 5.242 min
Delta R.T.: 0.000 min
Response: 31566643
Conc: 255.72 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

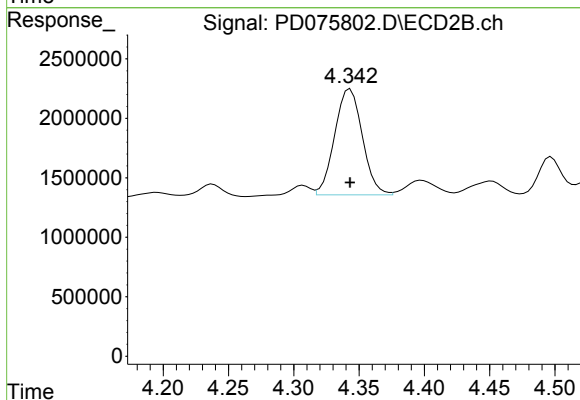


#24 Chlordane-2

R.T.: 4.343 min
Delta R.T.: 0.000 min
Response: 13134058
Conc: 261.15 ng/ml

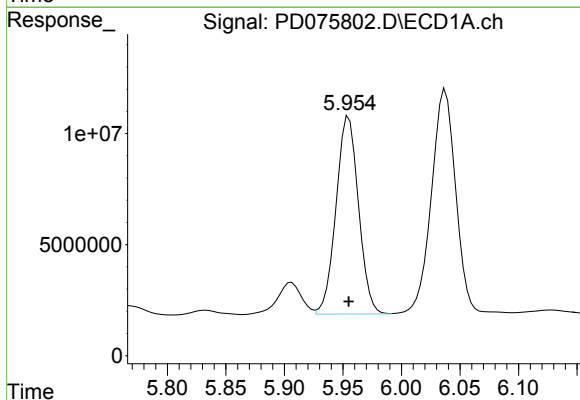


#25 Chlordane-3

R.T.: 5.955 min
Delta R.T.: 0.000 min
Response: 118873728
Conc: 232.87 ng/ml

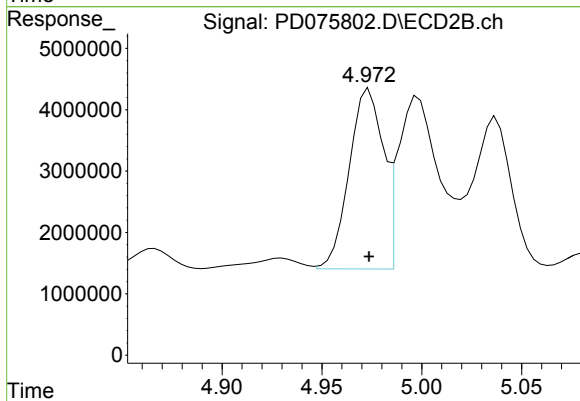

#25 Chlordane-3


R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 34739007
Conc: 239.70 ng/ml

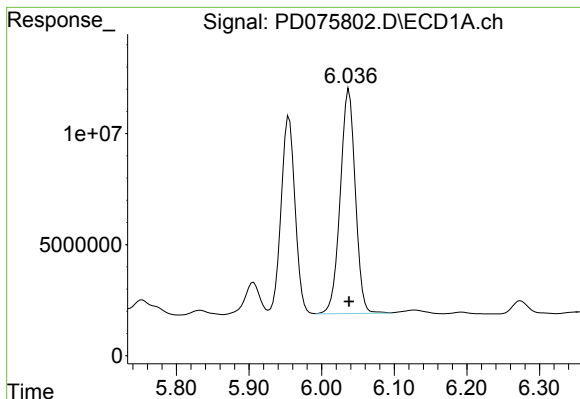

#26 Chlordane-4


R.T.: 6.038 min
Delta R.T.: 0.000 min
Response: 145716039
Conc: 236.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

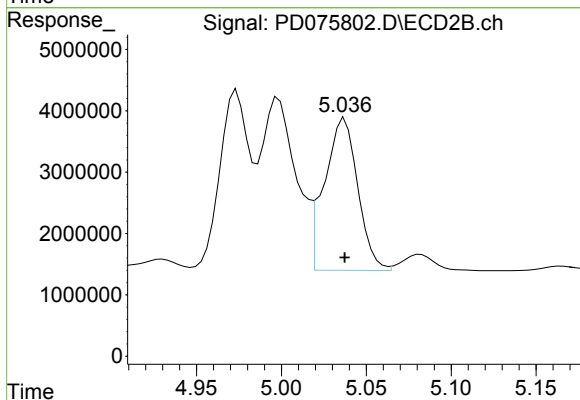


#26 Chlordane-4

R.T.: 5.037 min
Delta R.T.: 0.000 min
Response: 33862883
Conc: 238.51 ng/ml

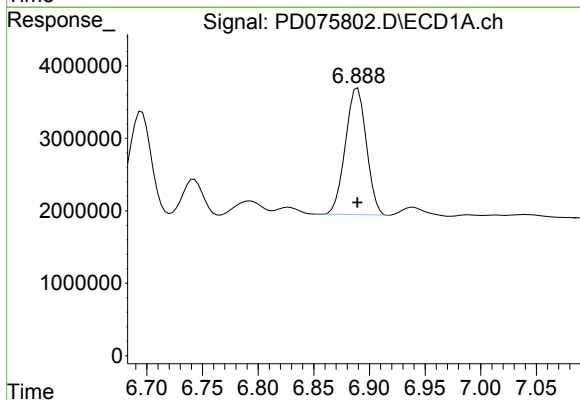


#27 Chlordane-5

R.T.: 6.889 min
Delta R.T.: 0.000 min
Response: 22878542
Conc: 233.23 ng/ml

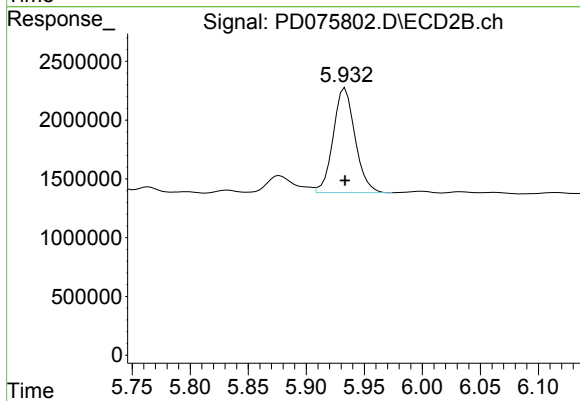

#27 Chlordane-5


R.T.: 5.934 min
Delta R.T.: 0.000 min
Response: 11655518
Conc: 235.65 ng/ml

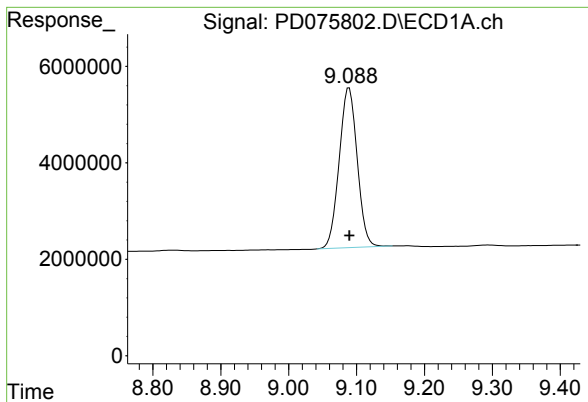

#28 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: 0.000 min
Response: 61118956
Conc: 25.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

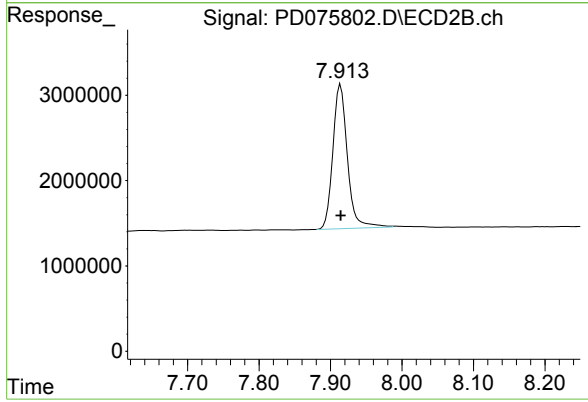

#28 Decachlorobiphenyl

R.T.: 7.914 min
Delta R.T.: 0.000 min
Response: 23888244
Conc: 25.72 ng/ml