

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061621\
 Data File : PD063882.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jun 2021 11:52
 Operator : AR\AJ
 Sample : M2690-06
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 08:07:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds


6) B	beta-BHC	0.000	4.764f	0	27038028	N.D.	3.023
7) B	delta-BHC	0.000	5.026	0	10863525	N.D.	0.492
8) B	Heptachlo...	0.000	5.850	0	12158395	N.D.	0.611
13) MA	Dieldrin	0.000	6.494f	0	3472211	N.D.	0.181
15) B	Endosulfa...	0.000	6.897	0	7319580	N.D.	0.484
16) A	4,4'-DDD	0.000	6.752f	0	8596630	N.D.	0.566
19) B	Endosulfa...	6.596f	7.252	497181	6384550	0.346	0.410
20) A	Methoxychlor	6.928	0.000	462592	0	0.561	N.D. #
26)	Toxaphene-5	7.059	0.000	607134	0	17.722	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061621\
Data File : PD063882.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jun 2021 11:52
Operator : AR\AJ
Sample : M2690-06
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 08:07:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

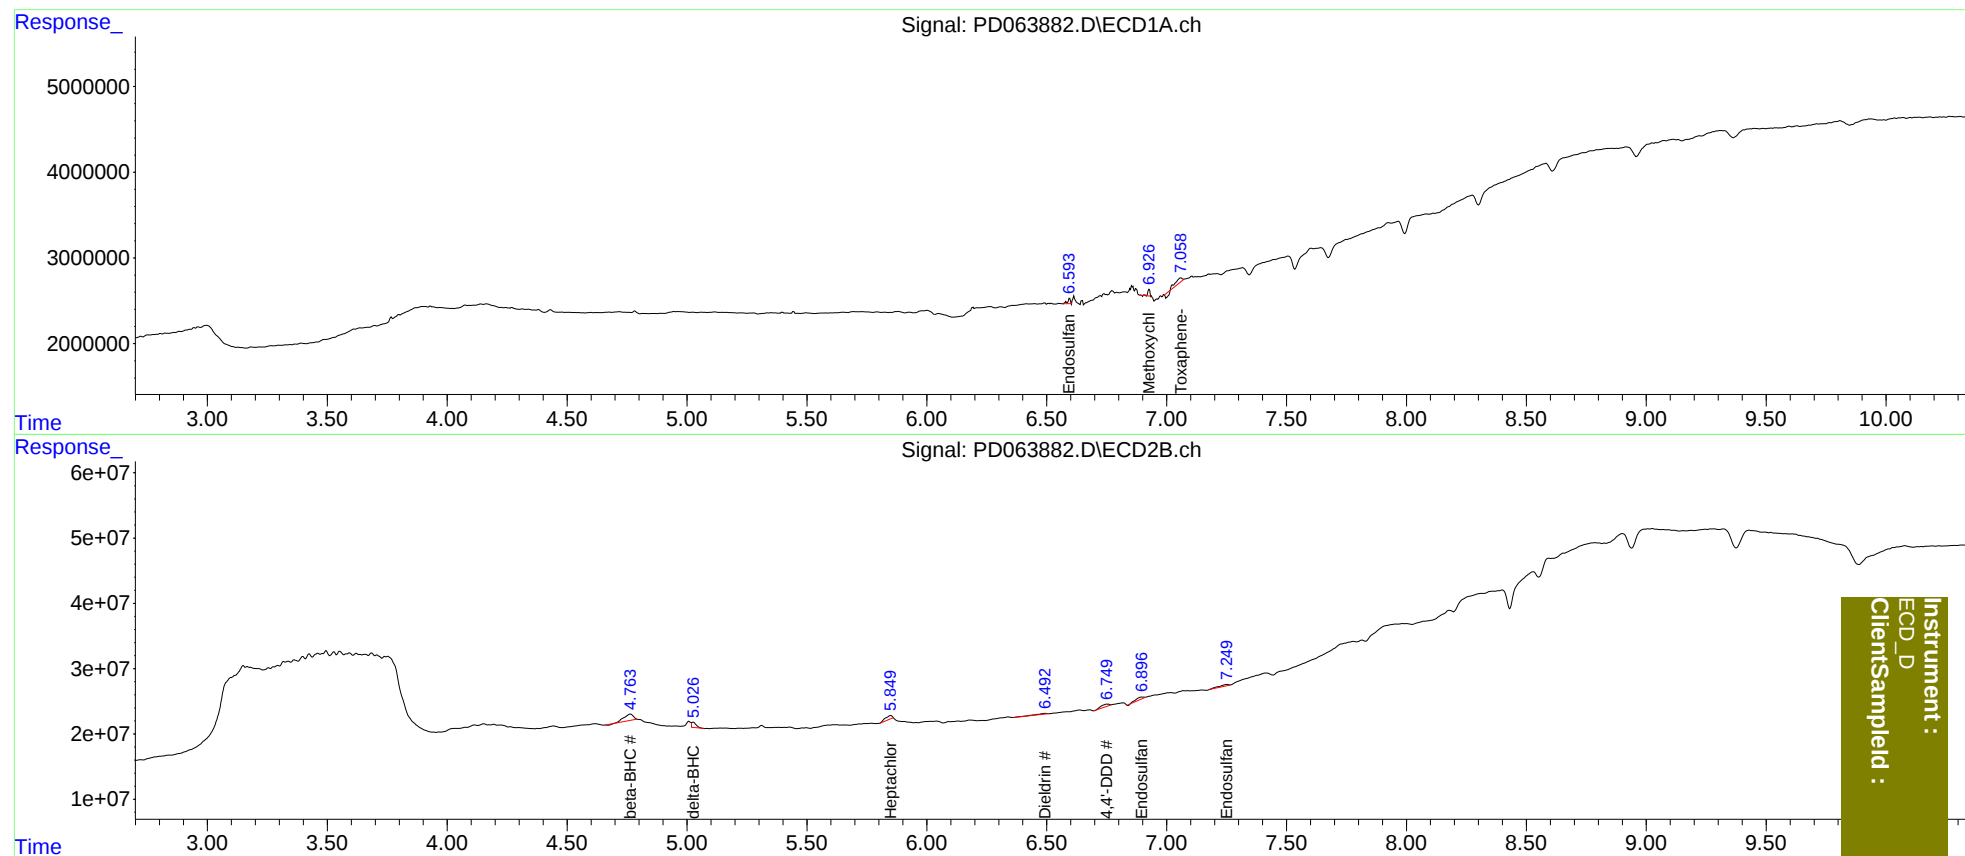


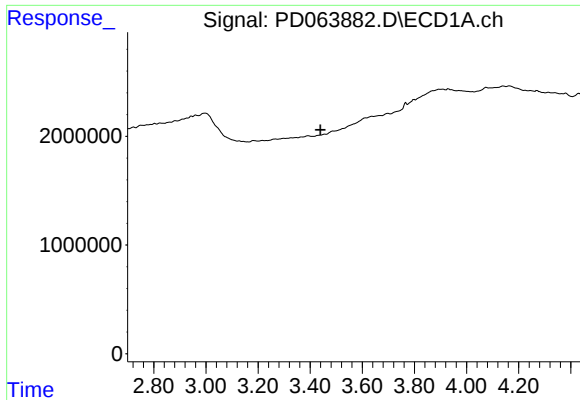

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.439 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

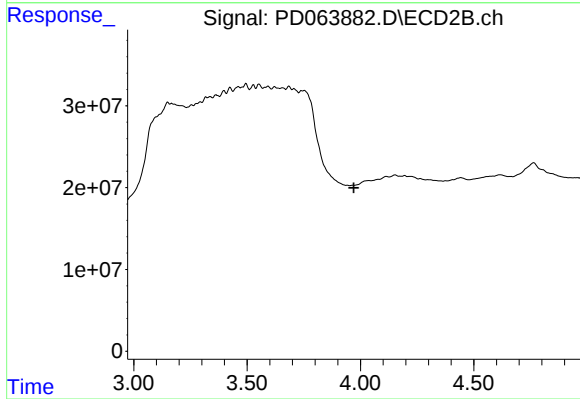


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.970 min
Response: 0
Conc: N.D.

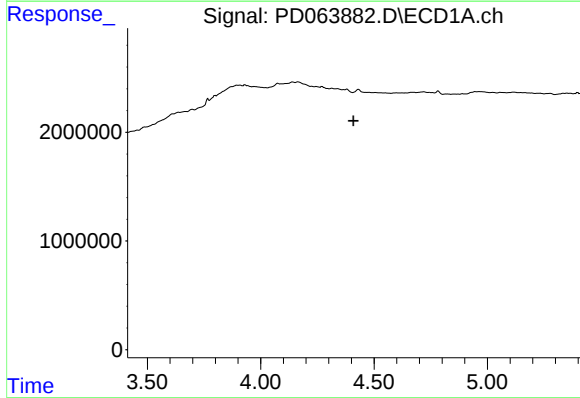


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.409 min
Response: 0
Conc: N.D.

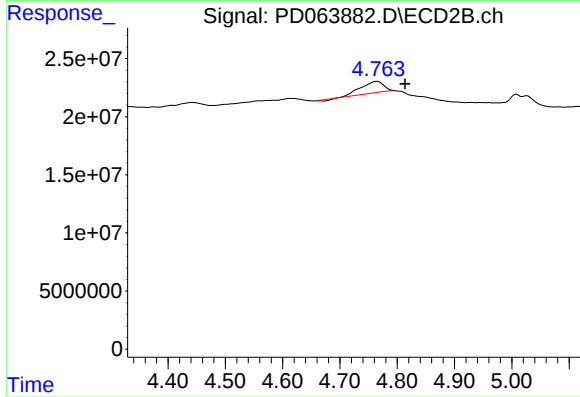

#6 beta-BHC


R.T.: 4.764 min
Delta R.T.: -0.049 min
Response: 27038028
Conc: 3.02 ng/ml

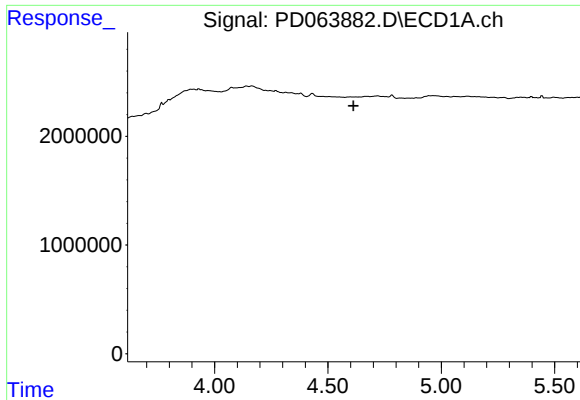

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.613 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

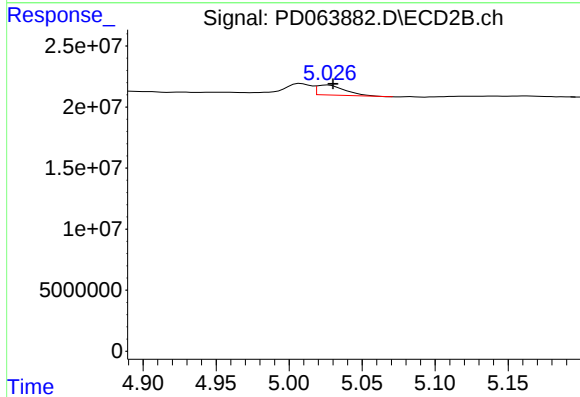


#7 delta-BHC

R.T.: 5.026 min
Delta R.T.: -0.004 min
Response: 10863525
Conc: 0.49 ng/ml

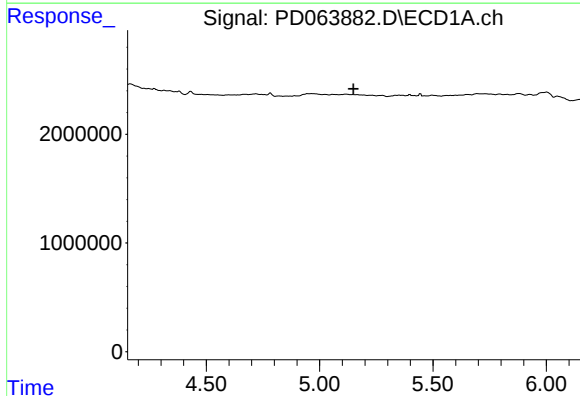


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.150 min
Response: 0
Conc: N.D.

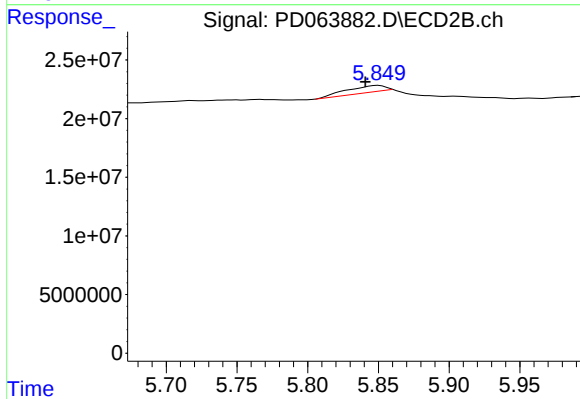

#8 Heptachlor epoxide


R.T.: 5.850 min
Delta R.T.: 0.009 min
Response: 12158395
Conc: 0.61 ng/ml

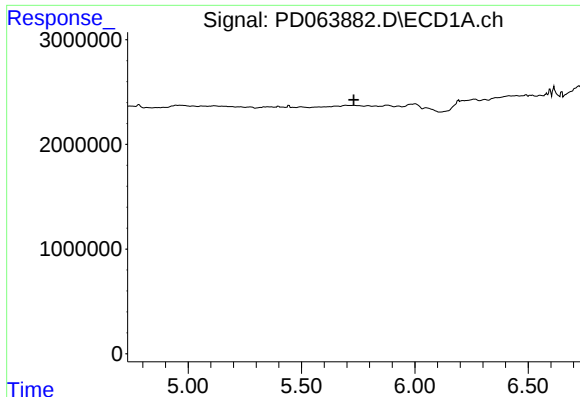

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.731 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

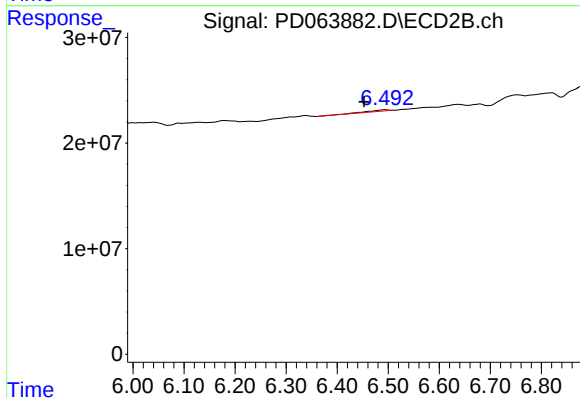


#13 Dieldrin

R.T.: 6.494 min
Delta R.T.: 0.041 min
Response: 3472211
Conc: 0.18 ng/ml

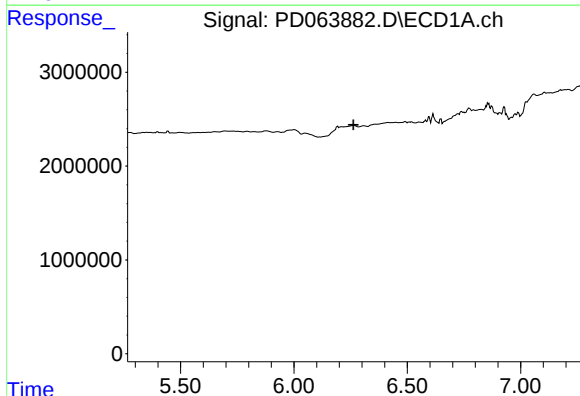


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.263 min
Response: 0
Conc: N.D.

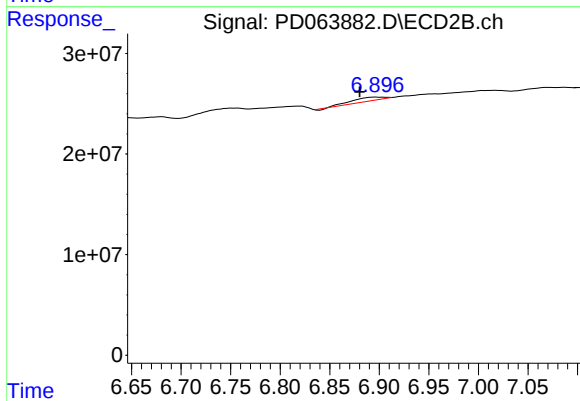

#15 Endosulfan II


R.T.: 6.897 min
Delta R.T.: 0.016 min
Response: 7319580
Conc: 0.48 ng/ml

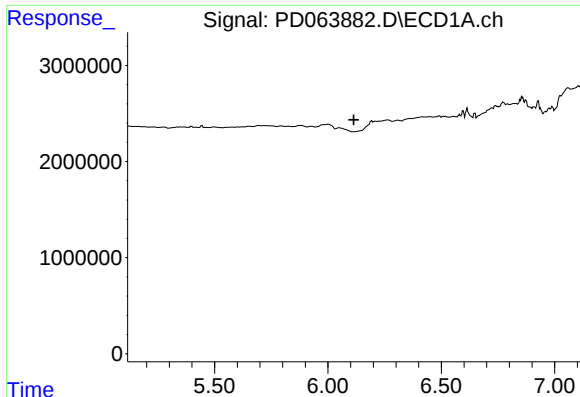

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.115 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

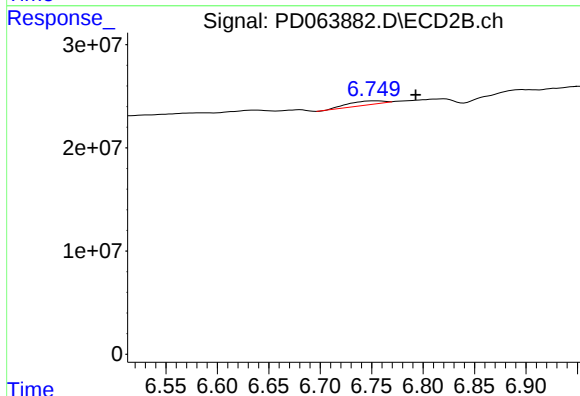


#16 4,4'-DDD

R.T.: 6.752 min
Delta R.T.: -0.041 min
Response: 8596630
Conc: 0.57 ng/ml

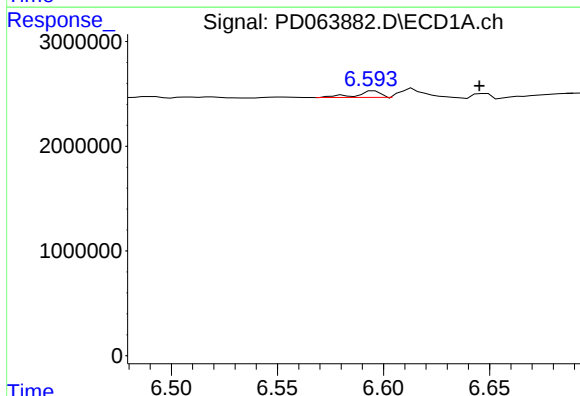


#19 Endosulfan Sulfate

R.T.: 6.596 min
Delta R.T.: -0.049 min
Response: 497181
Conc: 0.35 ng/ml

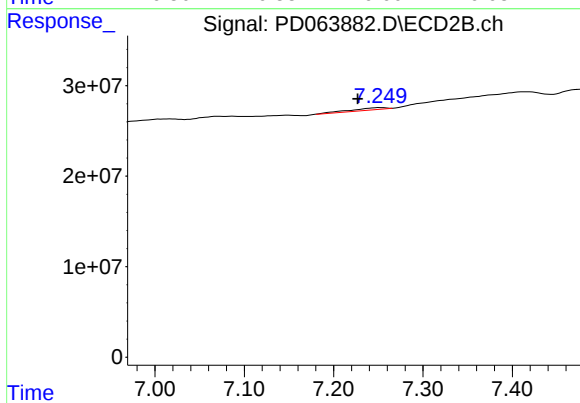

#19 Endosulfan Sulfate


R.T.: 7.252 min
Delta R.T.: 0.025 min
Response: 6384550
Conc: 0.41 ng/ml

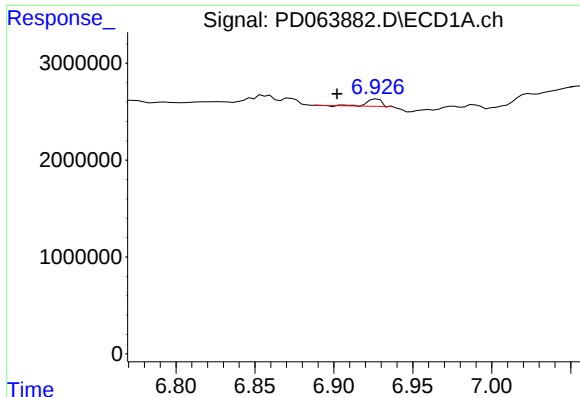

#20 Methoxychlor


R.T.: 6.928 min
Delta R.T.: 0.025 min
Response: 462592
Conc: 0.56 ng/ml

Instrument :
ECD_D
ClientSampleId :

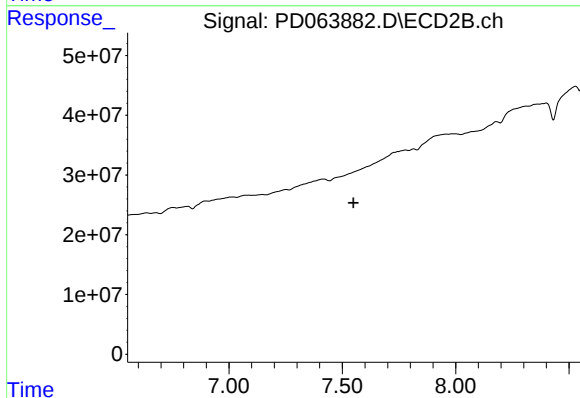


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.550 min
Response: 0
Conc: N.D.

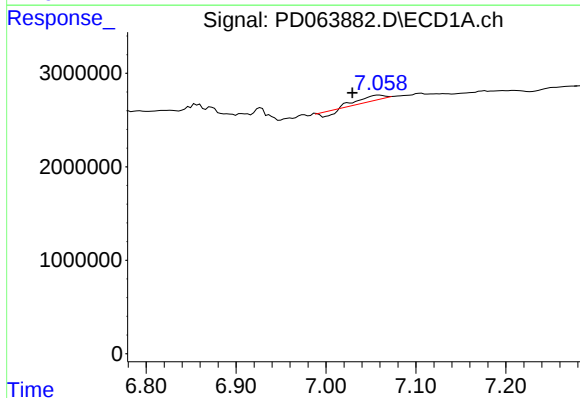


#26 Toxaphene-5

R.T.: 7.059 min
Delta R.T.: 0.030 min
Response: 607134
Conc: 17.72 ng/ml

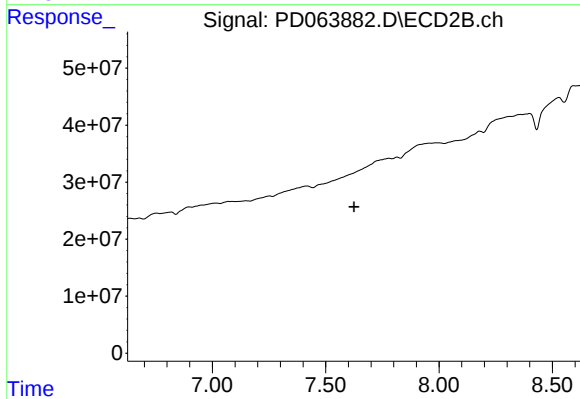

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T. : 7.625 min
Response: 0
Conc: N.D.

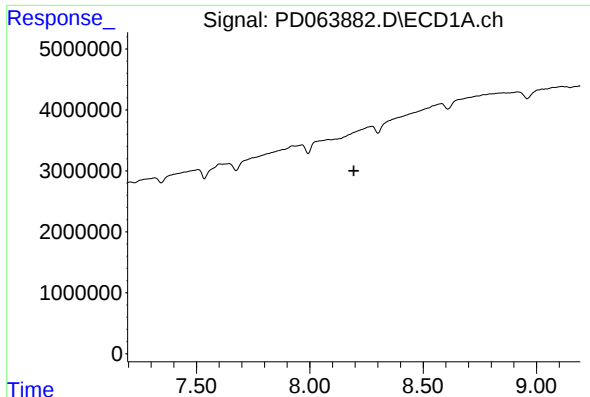

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.194 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

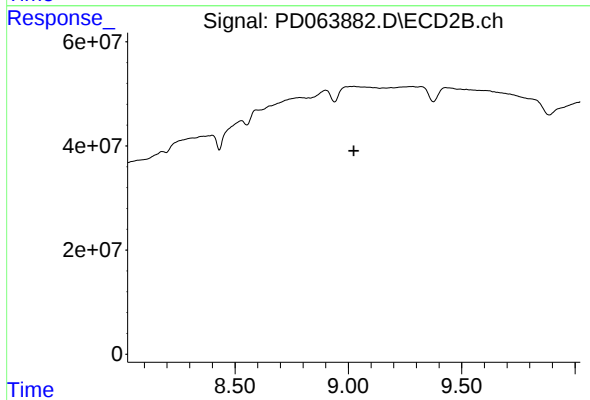

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.024 min
Response: 0
Conc: N.D.