

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061621\
Data File : PD063887.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jun 2021 14:34
Operator : AR\AJ
Sample : INDA303
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
ECD_D
LabSampleId :
INDA303

Manual Integrations
APPROVED

Ankita
6/17/2021 3:17:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 08:08:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

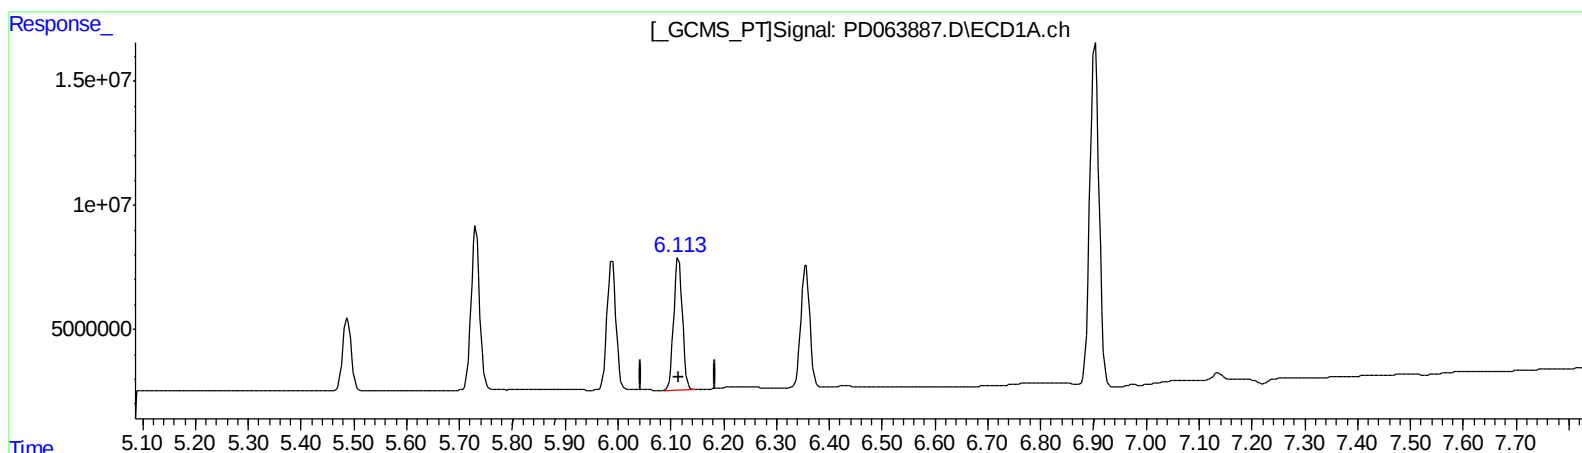

(16) 4,4'-DDD (A)
6.115min 40.866 ng/ml
response 60389435

(16) 4,4'-DDD #2 (A)
6.793min 40.637 ng/ml
response 617334800

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061621\
Data File : PD063887.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jun 2021 14:34
Operator : AR\AJ
Sample : INDA303
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_D
LabSampleId :
INDA303

Manual Integrations
APPROVED

Ankita
6/17/2021 3:17:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 08:08:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

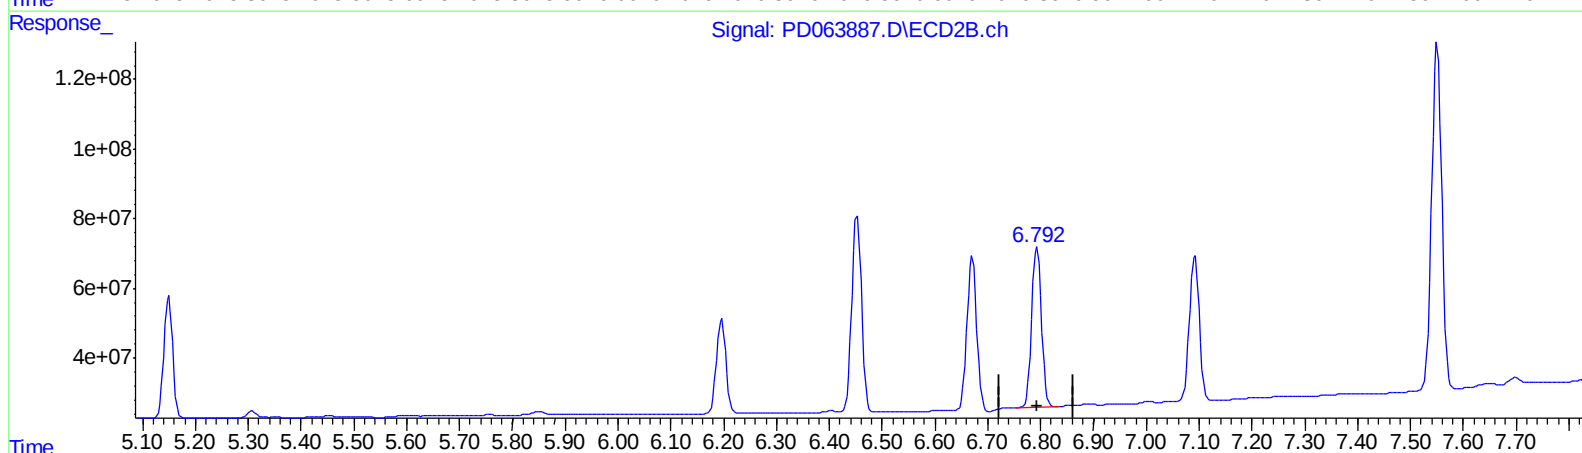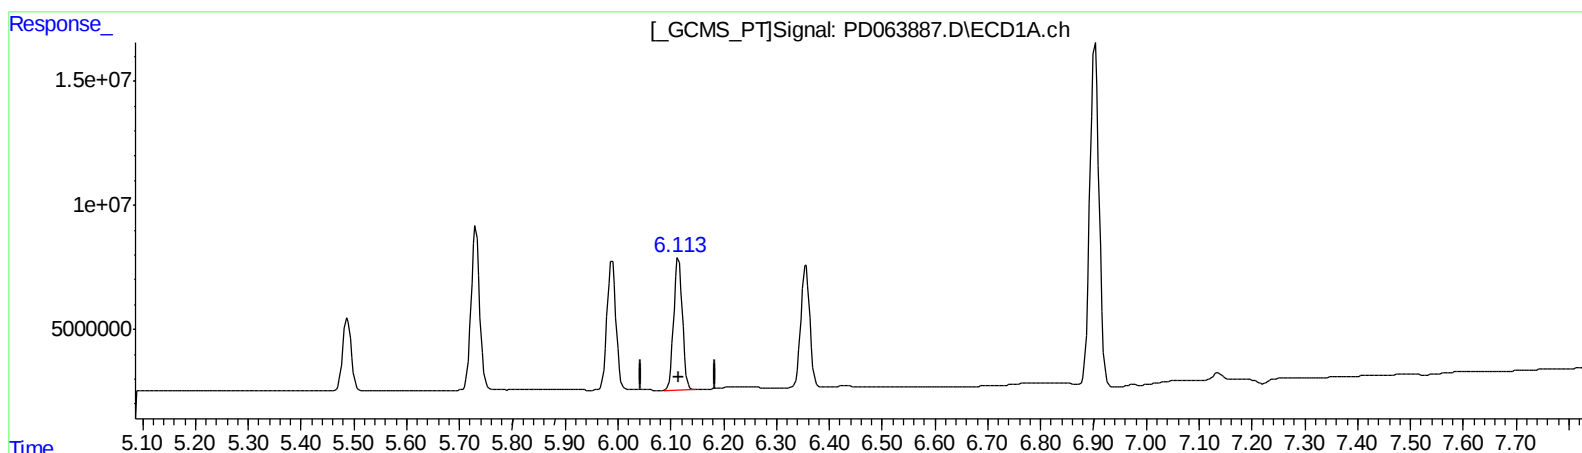

QEdit

(16) 4,4'-DDD (A)

6.115min 40.866 ng/ml

response 60389435

(16) 4,4'-DDD #2 (A)

6.792min 38.881 ng/ml m

response 590652863

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061621\
 Data File : PD063887.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jun 2021 14:34
 Operator : AR\AJ
 Sample : INDA303
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 LabSampleId :
 INDA303

Manual Integrations
 APPROVED

Ankita
 6/17/2021 3:17:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 08:08:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061421CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.438	3.970	28189667	281.3E6	20.537	19.980
27) SA Decachlor...	8.195	9.025	59762060	488.4E6	36.783	33.289
Target Compounds						
2) A alpha-BHC	3.874	4.358	42321987	446.6E6	20.728	20.206
3) MA gamma-BHC...	4.157	4.642	41311163	405.9E6	20.520	19.869
4) MA Heptachlor	4.458	5.150	39329957	408.4E6	20.212	19.655
9) A Endosulfan I	5.488	6.196	33072661	342.8E6	20.116	19.193
13) MA Dieldrin	5.731	6.453	75194537	731.8E6	40.142	38.248
14) MA Endrin	5.989	6.671	61775947	579.5E6	38.223	36.595
16) A 4,4'-DDD	6.115	6.792	60389435	590.7E6	40.866	38.881m
17) MA 4,4'-DDT	6.356	7.092	58081964	550.9E6	38.256	35.841
20) A Methoxychlor	6.903	7.551	168.3E6	1323.3E6	203.996	183.414

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

AJ
 06/21/21