

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061625\
 Data File : PD088976.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jun 2025 15:28
 Operator : AR\AJ
 Sample : Q2325-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 TP-8

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/17/2025
 Supervised By :mohammad ahmed 06/18/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 02:29:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051925.M
 Quant Title : GC Extractables
 QLast Update : Mon May 19 15:27:28 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.549	2.879	42217201	265.2E6	19.511	17.531
28) SA Decachlor...	9.071	8.070	33103868	132.6E6	9.673	7.261
Target Compounds						
20) A Methoxychlor	7.489	6.750	1257954	10964857	0.753m	1.145m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061625\
Data File : PD088976.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jun 2025 15:28
Operator : AR\AJ
Sample : Q2325-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
TP-8


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 06/17/2025
Supervised By : mohammad ahmed 06/18/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 02:29:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051925.M
Quant Title : GC Extractables
QLast Update : Mon May 19 15:27:28 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

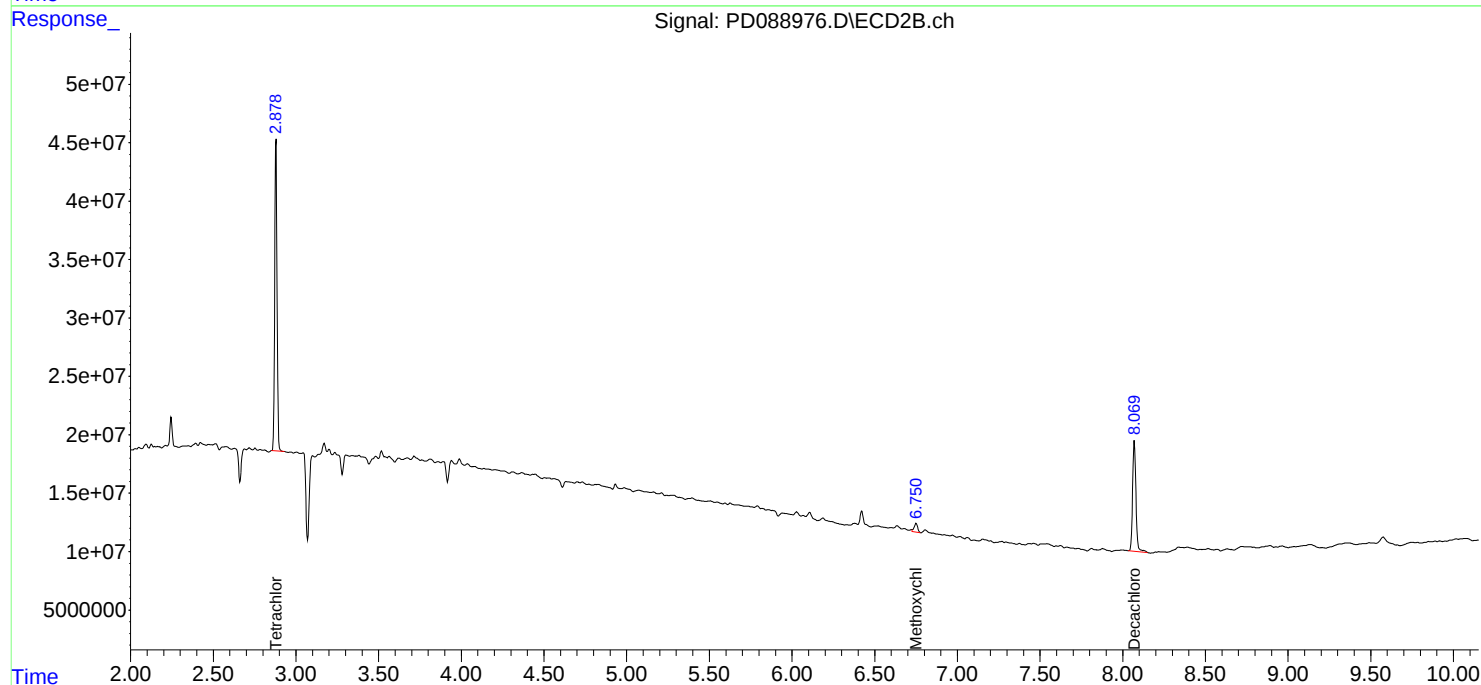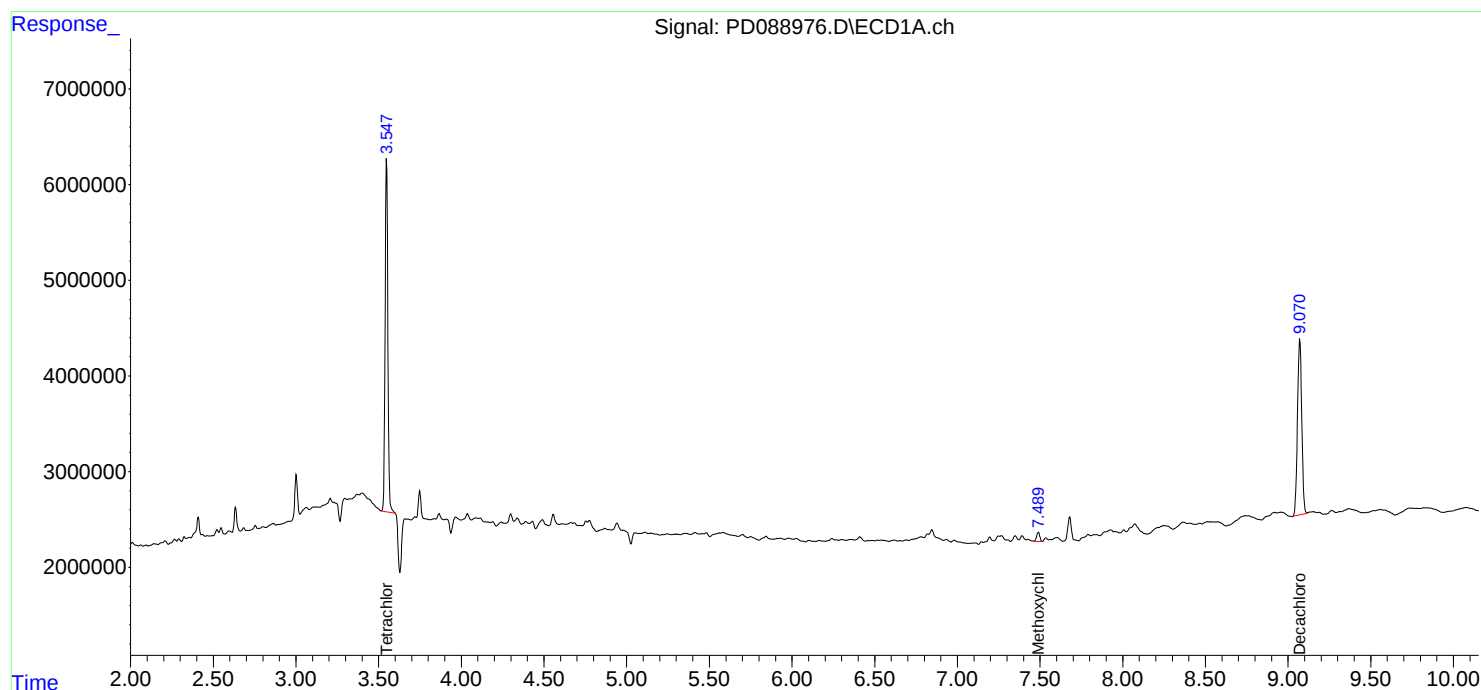

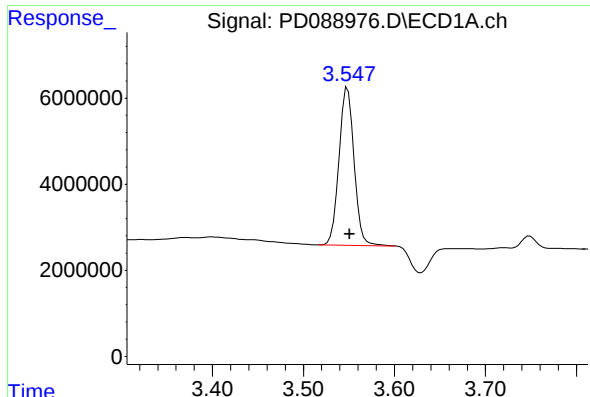


#1 Tetrachloro-m-xylene

R.T.: 3.549 min
Delta R.T.: -0.002 min
Response: 42217201
Conc: 19.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-8


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/17/2025
Supervised By :mohammad ahmed 06/18/2025

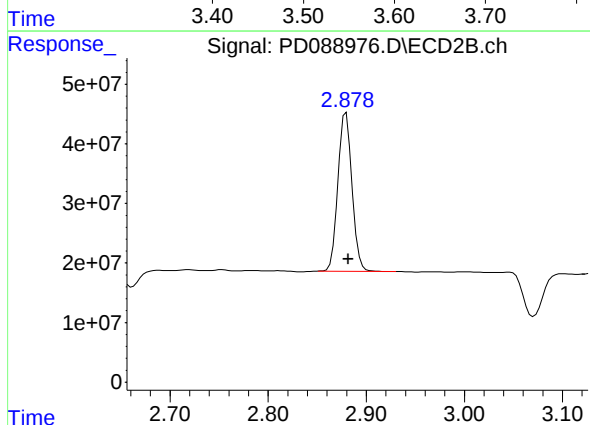


#1 Tetrachloro-m-xylene

R.T.: 2.879 min
Delta R.T.: -0.002 min
Response: 265188808
Conc: 17.53 ng/ml

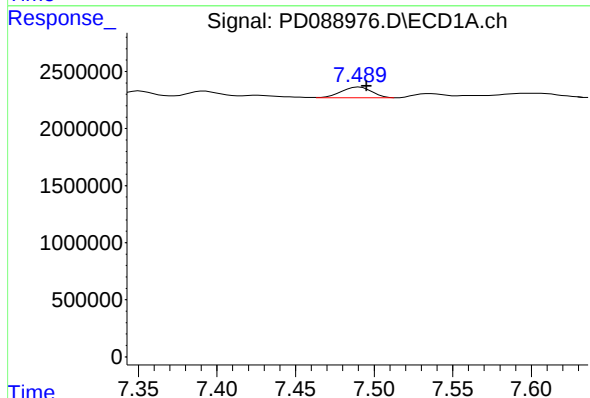


#20 Methoxychlor

R.T.: 7.489 min
Delta R.T.: -0.006 min
Response: 1257954
Conc: 0.75 ng/ml m

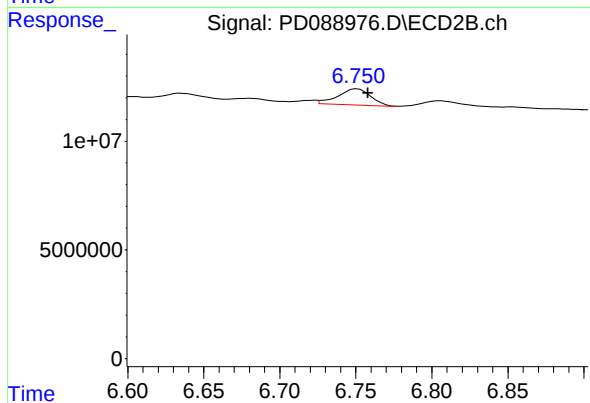

#20 Methoxychlor

R.T.: 6.750 min
Delta R.T.: -0.008 min
Response: 10964857
Conc: 1.15 ng/ml m

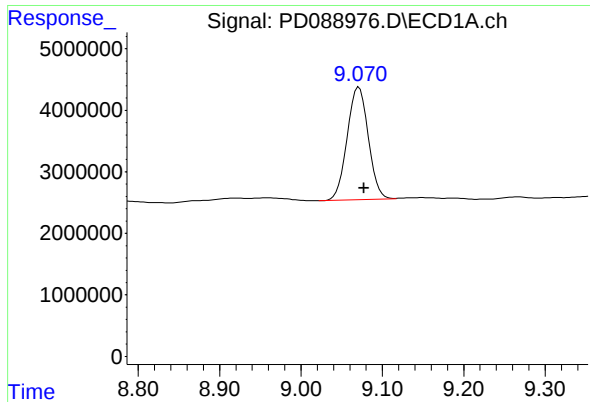


#28 Decachlorobiphenyl

R.T.: 9.071 min
Delta R.T.: -0.006 min
Response: 33103868
Conc: 9.67 ng/ml

Instrument :
ECD_D
ClientSampleId :
TP-8

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 06/17/2025
Supervised By :mohammad ahmed 06/18/2025

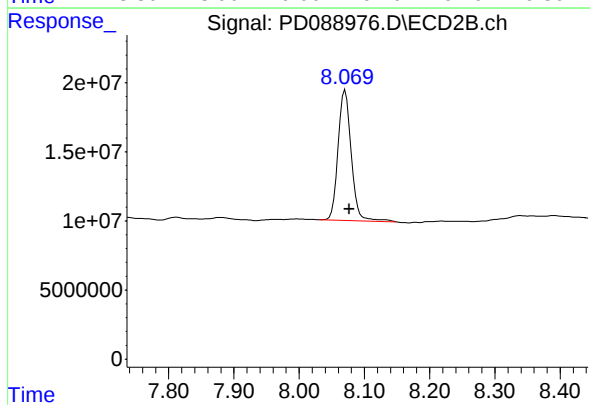

#28 Decachlorobiphenyl

R.T.: 8.070 min
Delta R.T.: -0.006 min
Response: 132556872
Conc: 7.26 ng/ml