

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061723\
 Data File : PD075869.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jun 2023 19:57
 Operator : AR\AJ
 Sample : PB153487BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB153487BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 16 22:13:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.768	51793557	25351720	24.315	23.367
28)	SA Decachlor...	9.089	7.913	59246074	23507316	23.386	24.041
Target Compounds							
7)	B delta-BHC	4.772	0.000	1045075	0	0.314	N.D. #
8)	B Heptachlo...	5.693	0.000	831094	0	0.258	N.D. #
9)	A Endosulfan I	6.095	0.000	127383	0	0.042	N.D. #
10)	B gamma-Chl...	5.978f	0.000	256908	0	0.080	N.D. #
11)	B alpha-Chl...	6.025	0.000	124779	0	0.039	N.D. #
14)	MA Endrin	6.619f	0.000	264728	0	0.099	N.D. #
15)	B Endosulfa...	6.783f	0.000	104099	0	0.040	N.D. #
21)	B Endrin ke...	7.692f	0.000	656117	0	0.236	N.D. #
25)	Chlordane-3	5.978f	0.000	256908	0	0.495	N.D. #
26)	Chlordane-4	6.025	0.000	124779	0	0.198	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061723\
Data File : PD075869.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jun 2023 19:57
Operator : AR\AJ
Sample : PB153487BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB153487BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 16 22:13:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

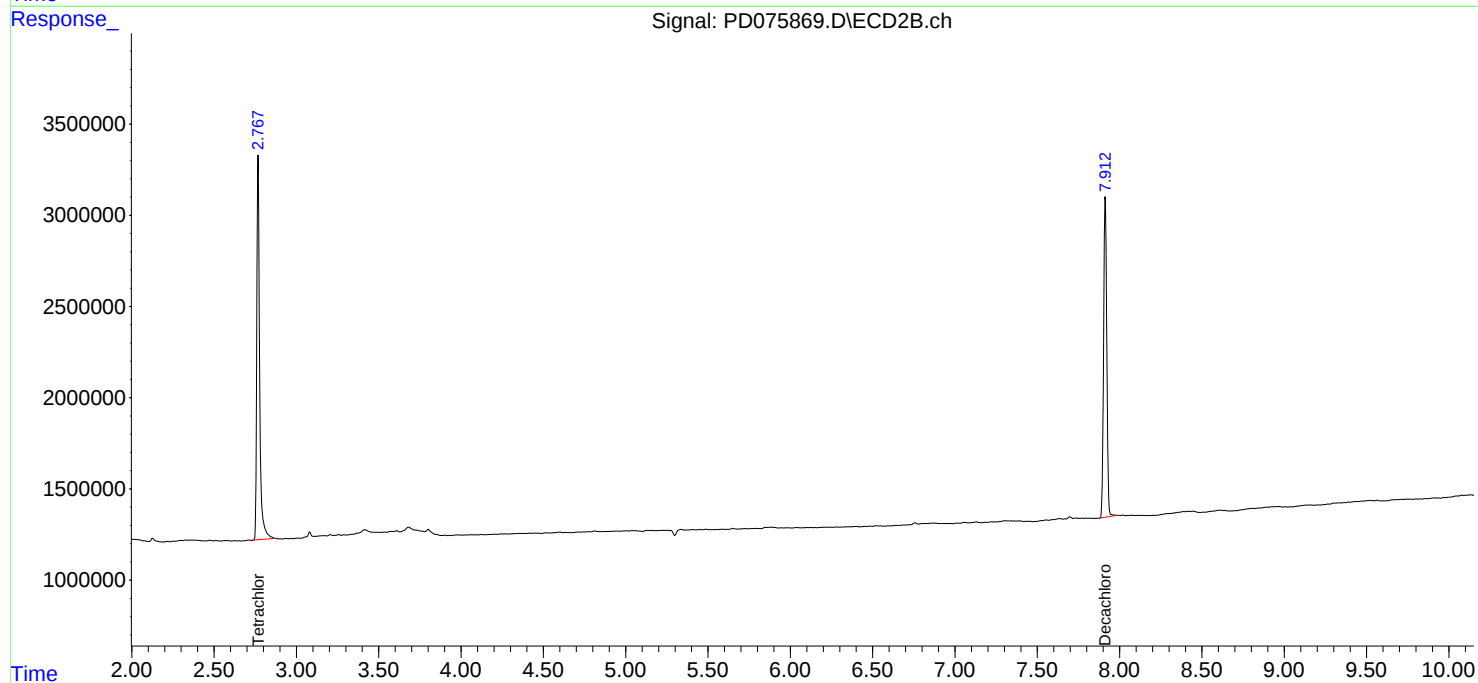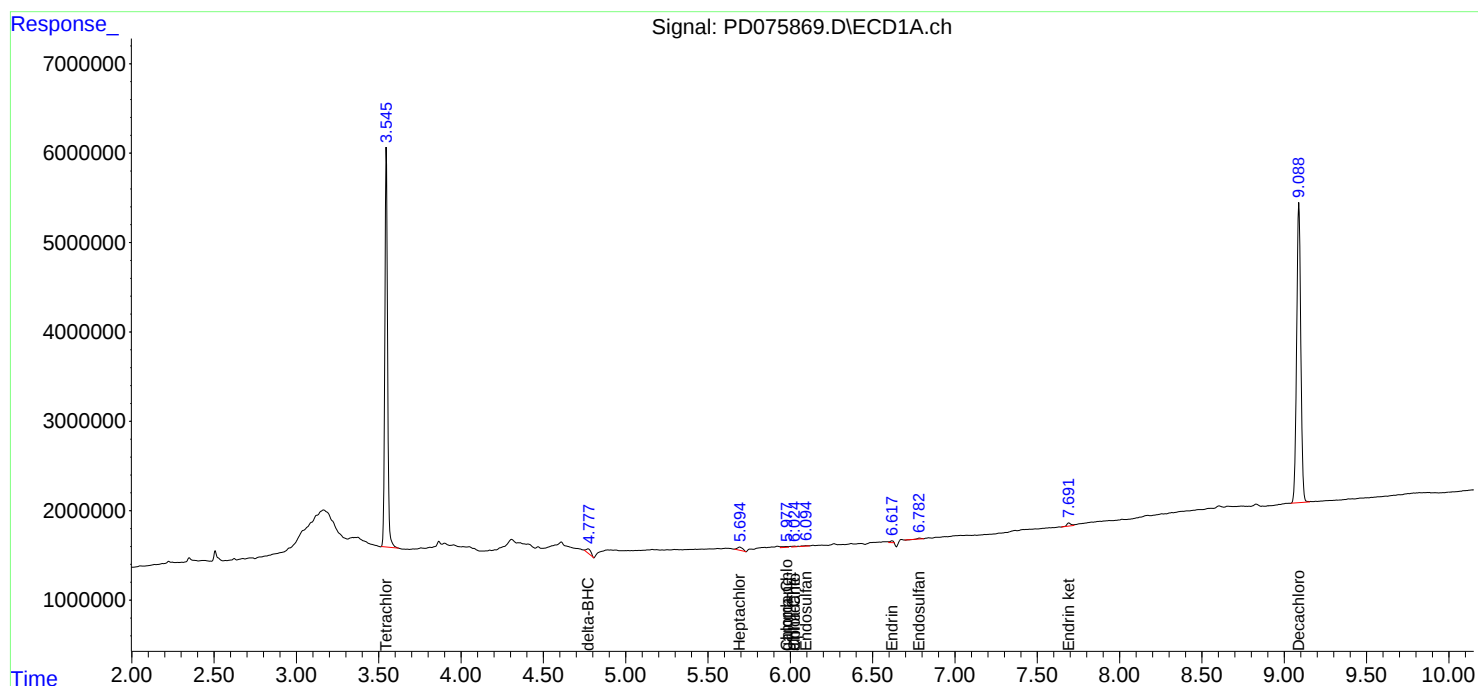


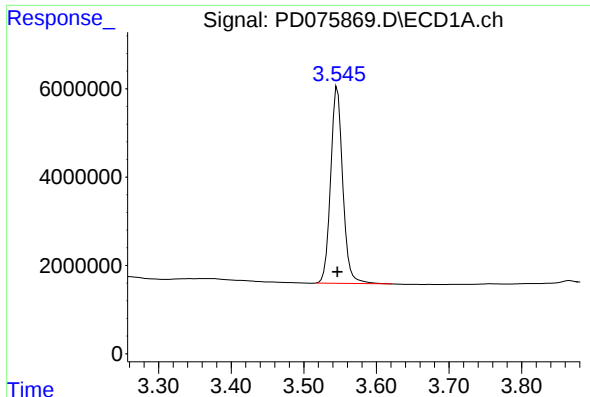

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 51793557
Conc: 24.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153487BL

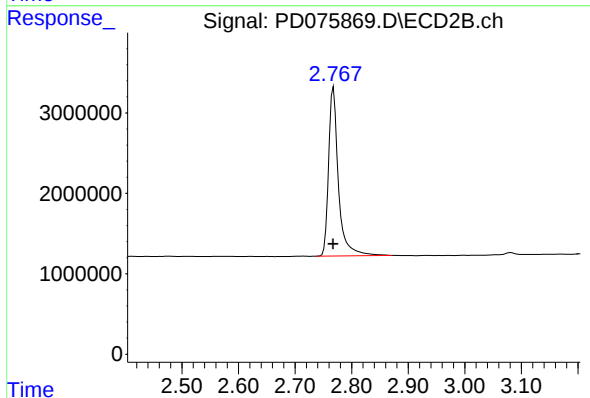


#1 Tetrachloro-m-xylene

R.T.: 2.768 min
Delta R.T.: 0.000 min
Response: 25351720
Conc: 23.37 ng/ml

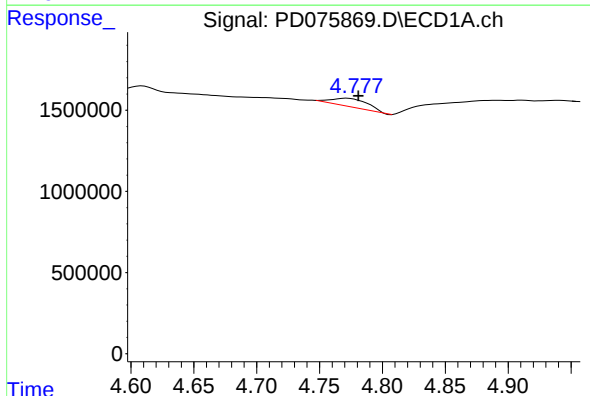


#7 delta-BHC

R.T.: 4.772 min
Delta R.T.: -0.009 min
Response: 1045075
Conc: 0.31 ng/ml

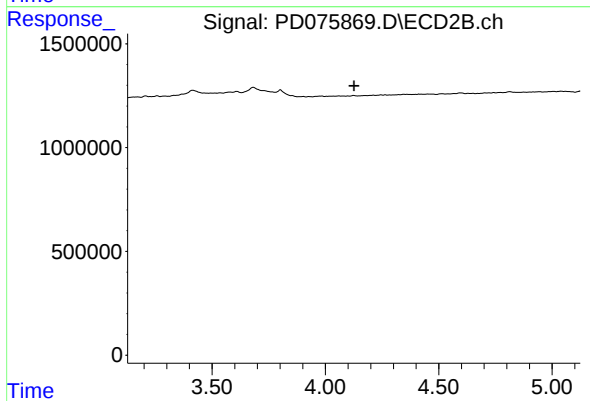

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.127 min
Response: 0
Conc: N.D.

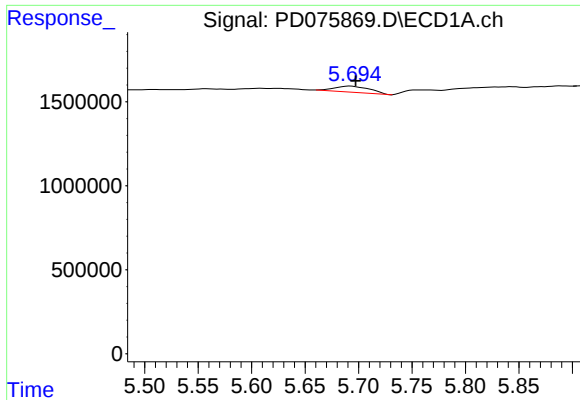

#8 Heptachlor epoxide


R.T.: 5.693 min
Delta R.T.: -0.005 min
Response: 831094
Conc: 0.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153487BL

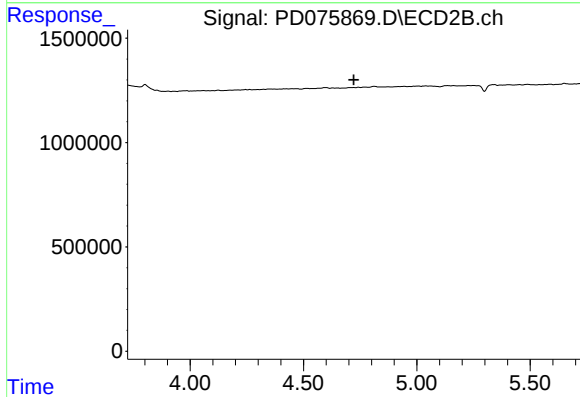


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

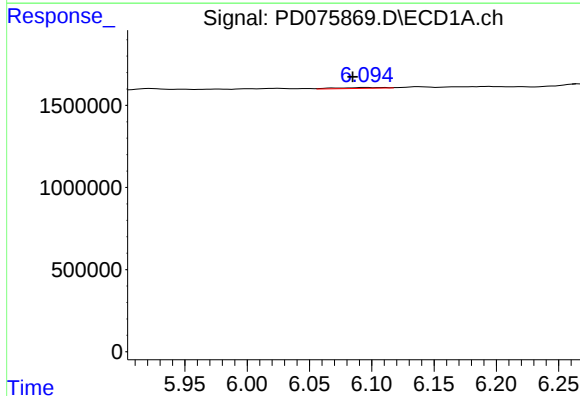


#9 Endosulfan I

R.T.: 6.095 min
Delta R.T.: 0.010 min
Response: 127383
Conc: 0.04 ng/ml

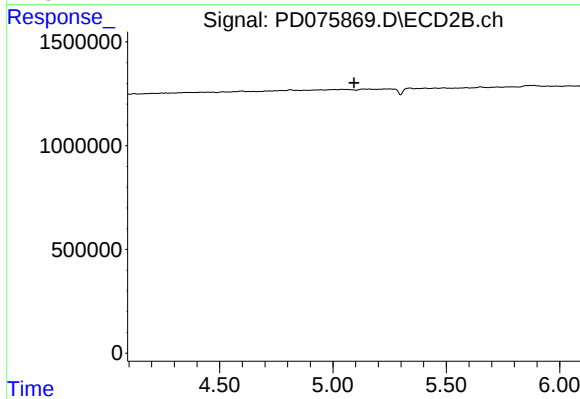

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.093 min
Response: 0
Conc: N.D.

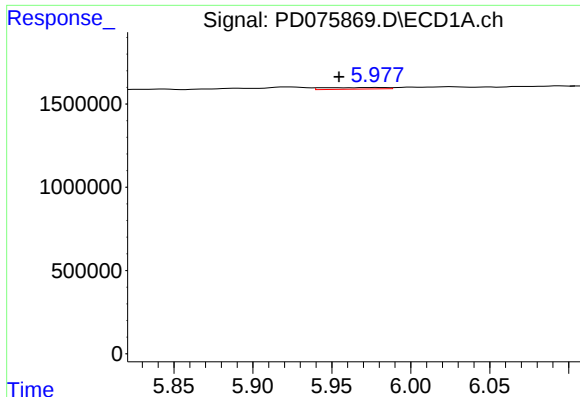

#10 gamma-Chlordane


R.T.: 5.978 min
Delta R.T.: 0.024 min
Response: 256908
Conc: 0.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153487BL

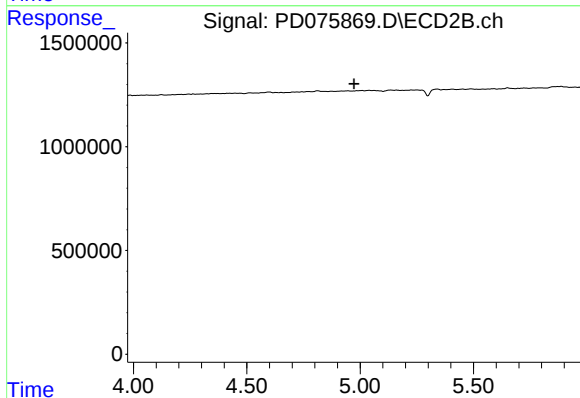


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.973 min
Response: 0
Conc: N.D.

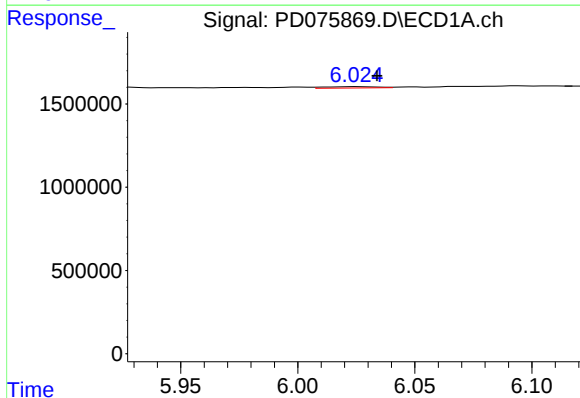


#11 alpha-Chlordane

R.T.: 6.025 min
Delta R.T.: -0.009 min
Response: 124779
Conc: 0.04 ng/ml

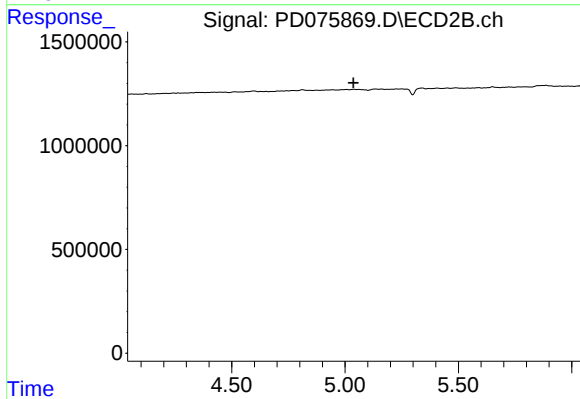

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

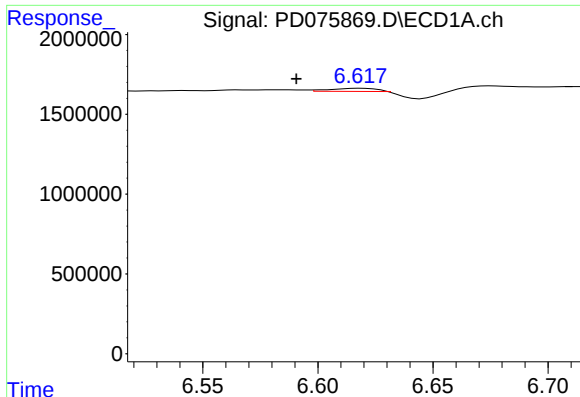

#14 Endrin


R.T.: 6.619 min
Delta R.T.: 0.028 min
Response: 264728
Conc: 0.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153487BL

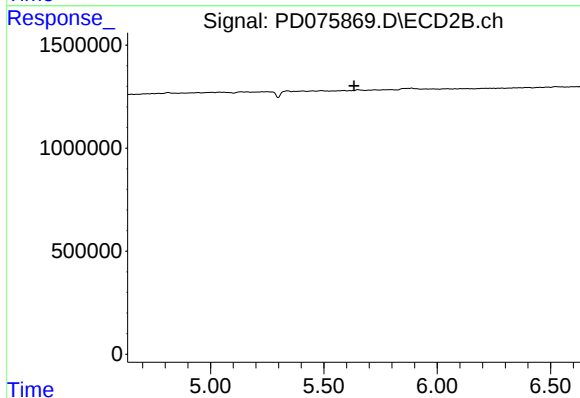


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.633 min
Response: 0
Conc: N.D.

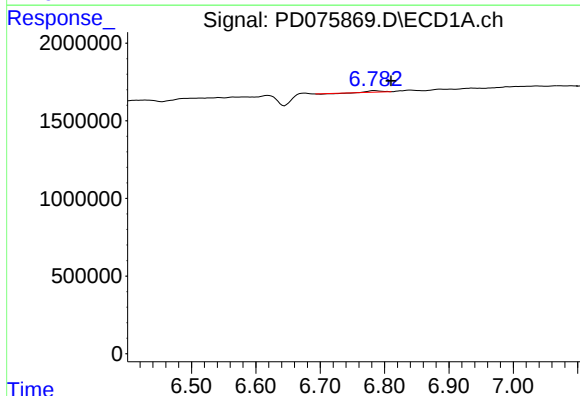


#15 Endosulfan II

R.T.: 6.783 min
Delta R.T.: -0.027 min
Response: 104099
Conc: 0.04 ng/ml

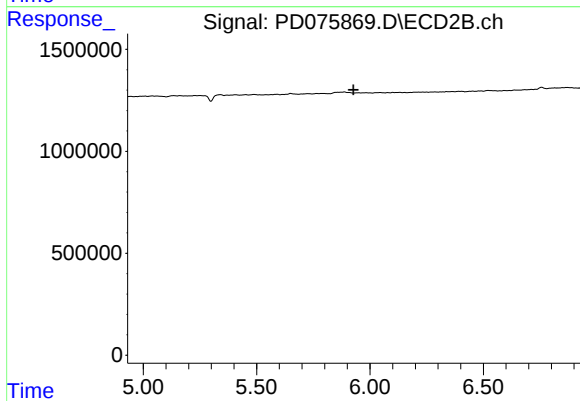

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.928 min
Response: 0
Conc: N.D.

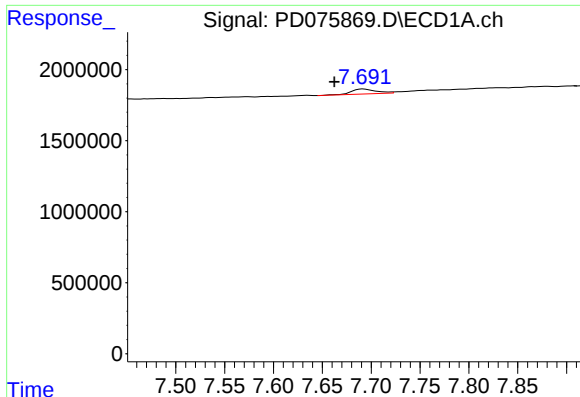

#21 Endrin ketone


R.T.: 7.692 min
Delta R.T.: 0.029 min
Response: 656117
Conc: 0.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153487BL

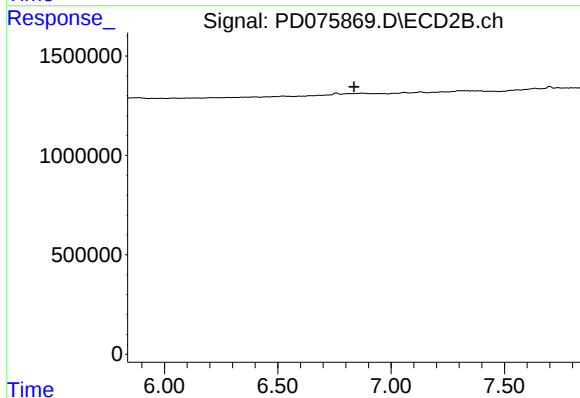


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.

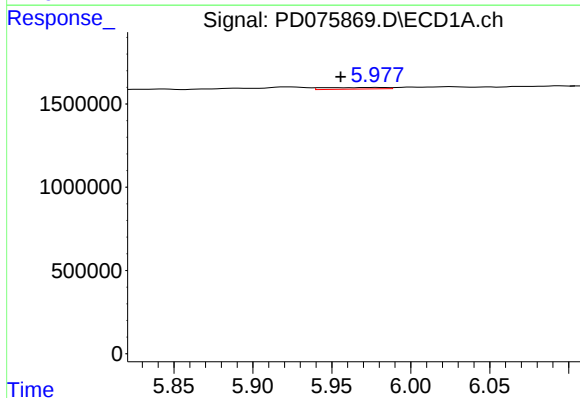


#25 Chlordane-3

R.T.: 5.978 min
Delta R.T.: 0.023 min
Response: 256908
Conc: 0.49 ng/ml

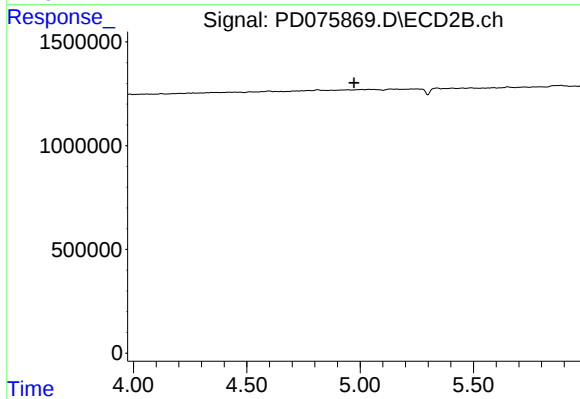

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 4.974 min
Response: 0
Conc: N.D.

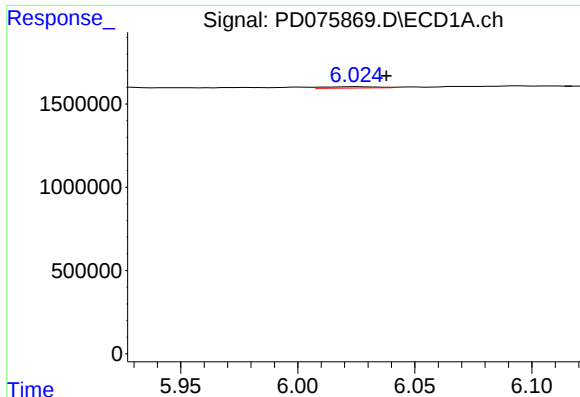

#26 Chlordane-4


R.T.: 6.025 min
Delta R.T.: -0.013 min
Response: 124779
Conc: 0.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB153487BL

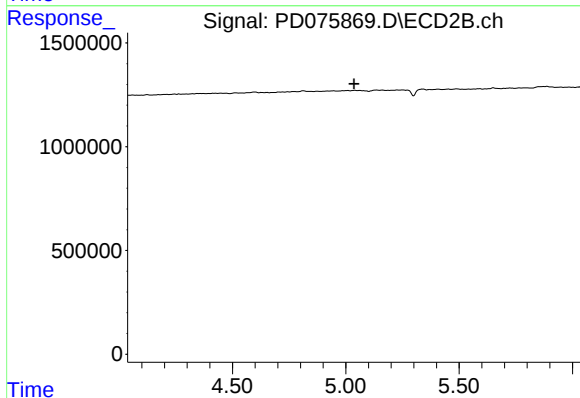


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

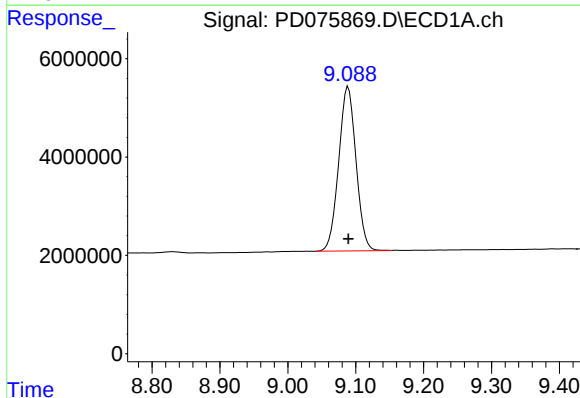

#28 Decachlorobiphenyl

R.T.: 9.089 min
Delta R.T.: 0.000 min
Response: 59246074
Conc: 23.39 ng/ml

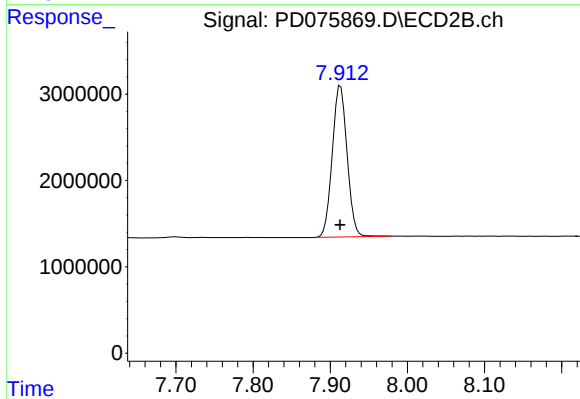

#28 Decachlorobiphenyl

R.T.: 7.913 min
Delta R.T.: 0.000 min
Response: 23507316
Conc: 24.04 ng/ml