

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD061723\  
 Data File : PD075831.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 16 Jun 2023 09:33  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jun 16 11:02:07 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD061523.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Jun 16 10:43:19 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|-------|-------|----------|----------|--------|--------|
| -----                       |                 |       |       |          |          |        |        |
| System Monitoring Compounds |                 |       |       |          |          |        |        |
| 1)                          | SA Tetrachlo... | 3.552 | 2.765 | 49202801 | 23860491 | 23.098 | 21.993 |
| 28)                         | SA Decachlor... | 9.098 | 7.915 | 61298390 | 23188031 | 24.196 | 23.715 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD061723\  
Data File : PD075831.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 16 Jun 2023 09:33  
Operator : AR\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_D  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jun 16 11:02:07 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD061523.M  
Quant Title : GC Extractables  
QLast Update : Fri Jun 16 10:43:19 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

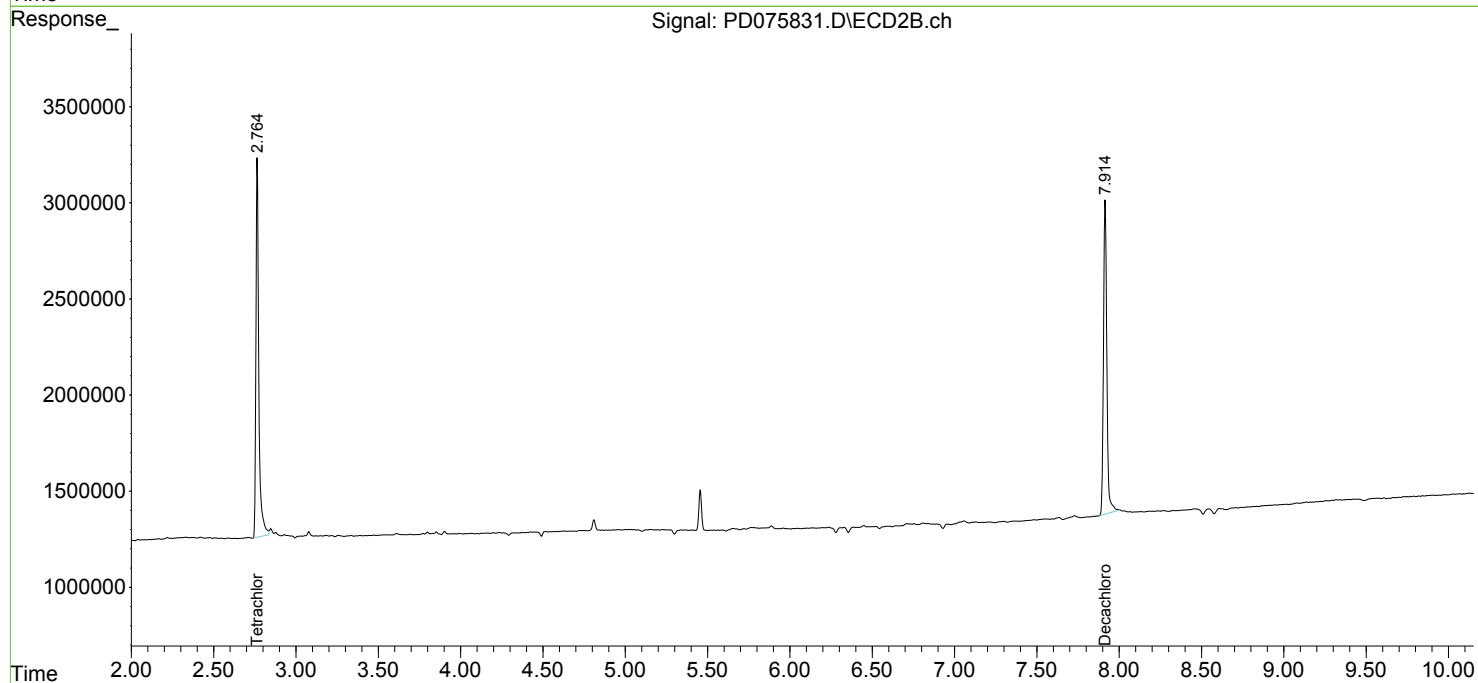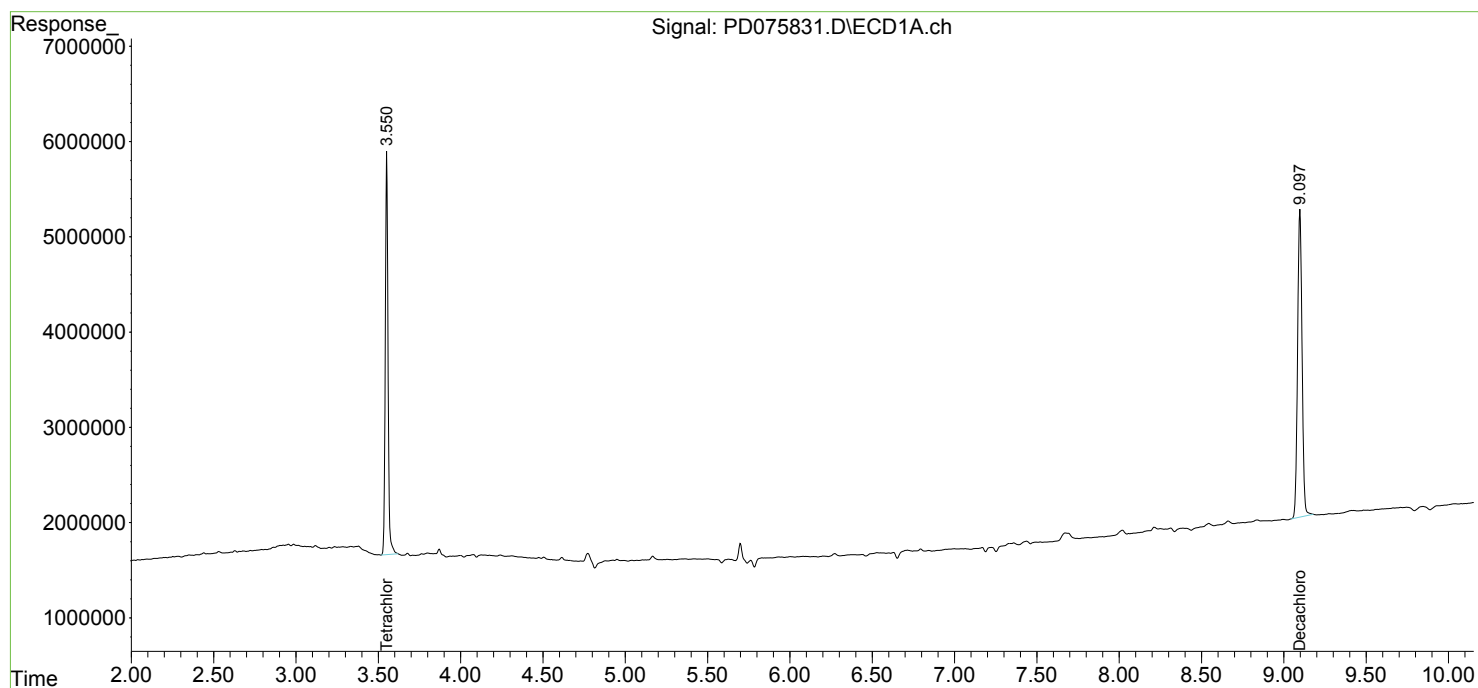


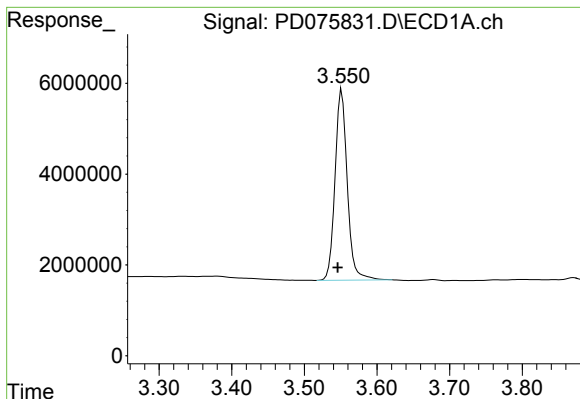

#1 Tetrachloro-m-xylene


R.T.: 3.552 min  
Delta R.T.: 0.006 min  
Response: 49202801  
Conc: 23.10 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :  
I.BLK

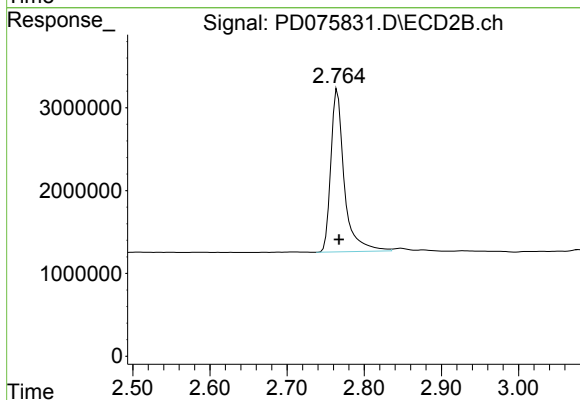


#1 Tetrachloro-m-xylene

R.T.: 2.765 min  
Delta R.T.: -0.002 min  
Response: 23860491  
Conc: 21.99 ng/ml

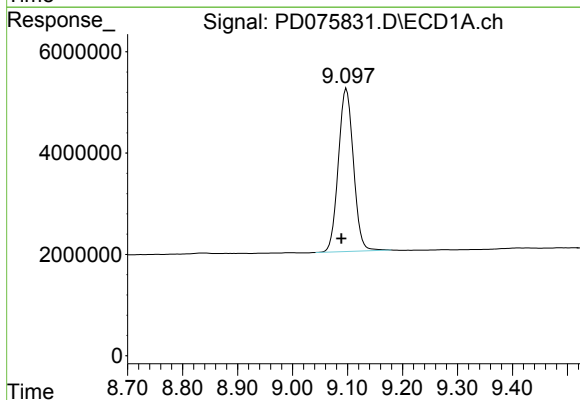

#28 Decachlorobiphenyl

R.T.: 9.098 min  
Delta R.T.: 0.009 min  
Response: 61298390  
Conc: 24.20 ng/ml

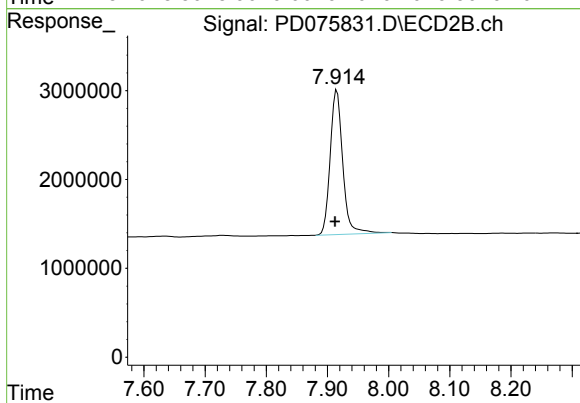

#28 Decachlorobiphenyl

R.T.: 7.915 min  
Delta R.T.: 0.003 min  
Response: 23188031  
Conc: 23.71 ng/ml